


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN021320\
 Data File : VN060081.D
 Acq On : 13 Feb 2020 9:15
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N021220W.M
 Title : SW846 8260
 Last Update : Wed Feb 12 14:12:21 2020

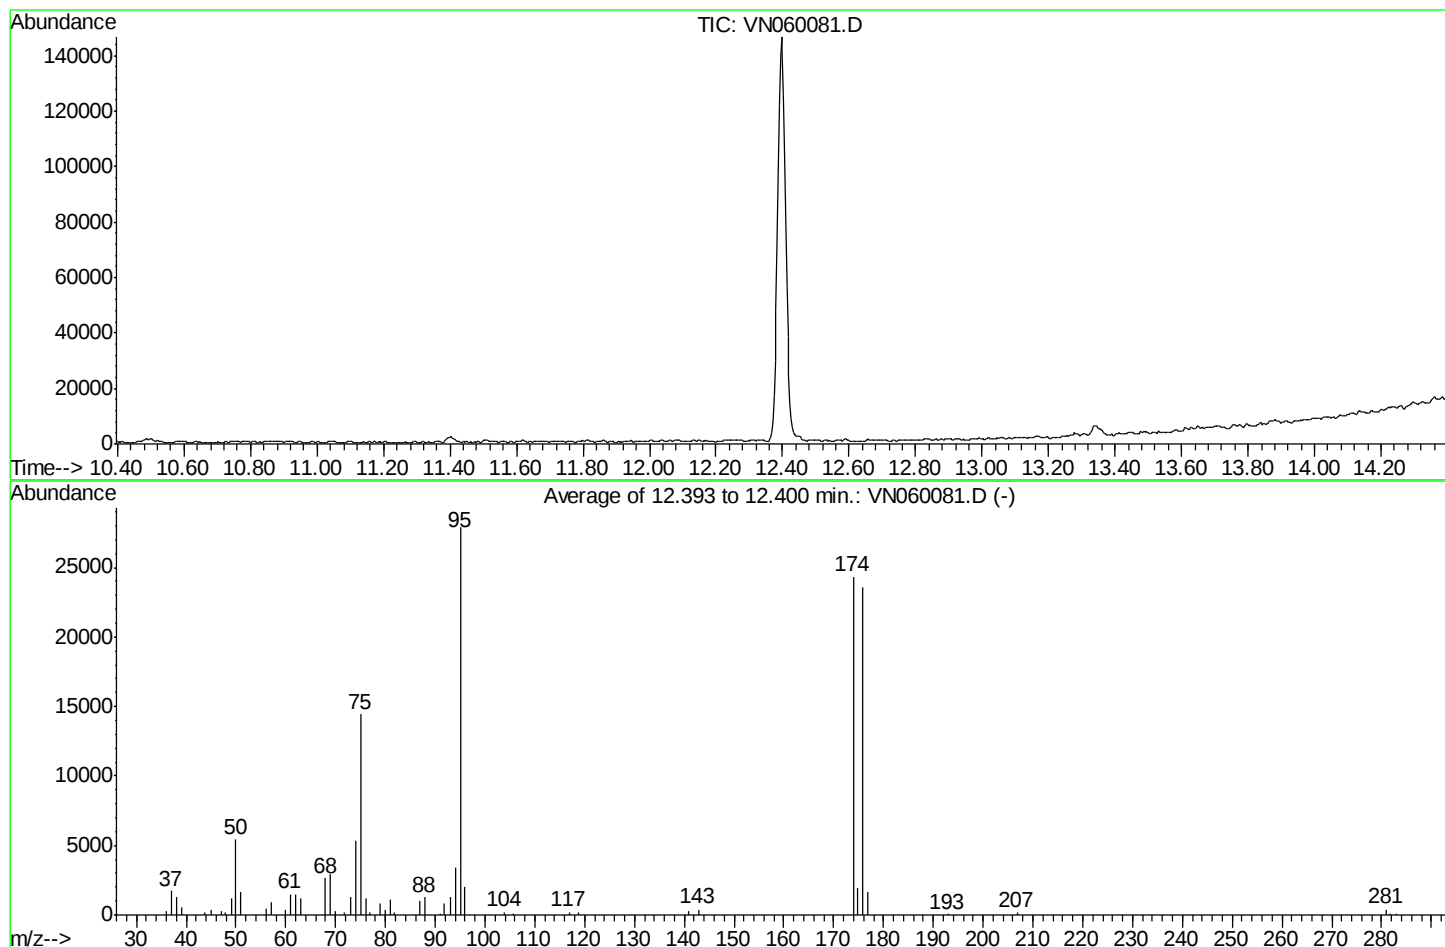

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	5409	PASS
75	95	30	60	51.8	14452	PASS
95	95	100	100	100.0	27885	PASS
96	95	5	9	7.4	2052	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.3	24344	PASS
175	174	5	9	8.0	1940	PASS
176	174	95	101	96.8	23570	PASS
177	176	5	9	6.9	1623	PASS