

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021323\
 Data File : VN076631.D
 Acq On : 13 Feb 2023 16:22
 Operator : JC\MD
 Sample : VN0213WBL01
 Misc : 5.0mL/MSVOA_N/Water
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0213WBL01

Quant Time: Feb 14 05:23:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 14 01:44:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.231	168	326493	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.107	114	573745	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	508047	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.795	152	202045	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	222696	49.396	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	98.800%
35) Dibromofluoromethane	8.172	113	177201	47.161	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.320%
50) Toluene-d8	10.572	98	693126	49.396	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	98.800%
62) 4-Bromofluorobenzene	12.854	95	203698	43.830	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	87.660%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021323\
Data File : VN076631.D
Acq On : 13 Feb 2023 16:22
Operator : JC\MD
Sample : VN0213WBL01
Misc : 5.0mL/MSVOA_N/Water
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0213WBL01

Quant Time: Feb 14 05:23:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 14 01:44:47 2023
Response via : Initial Calibration




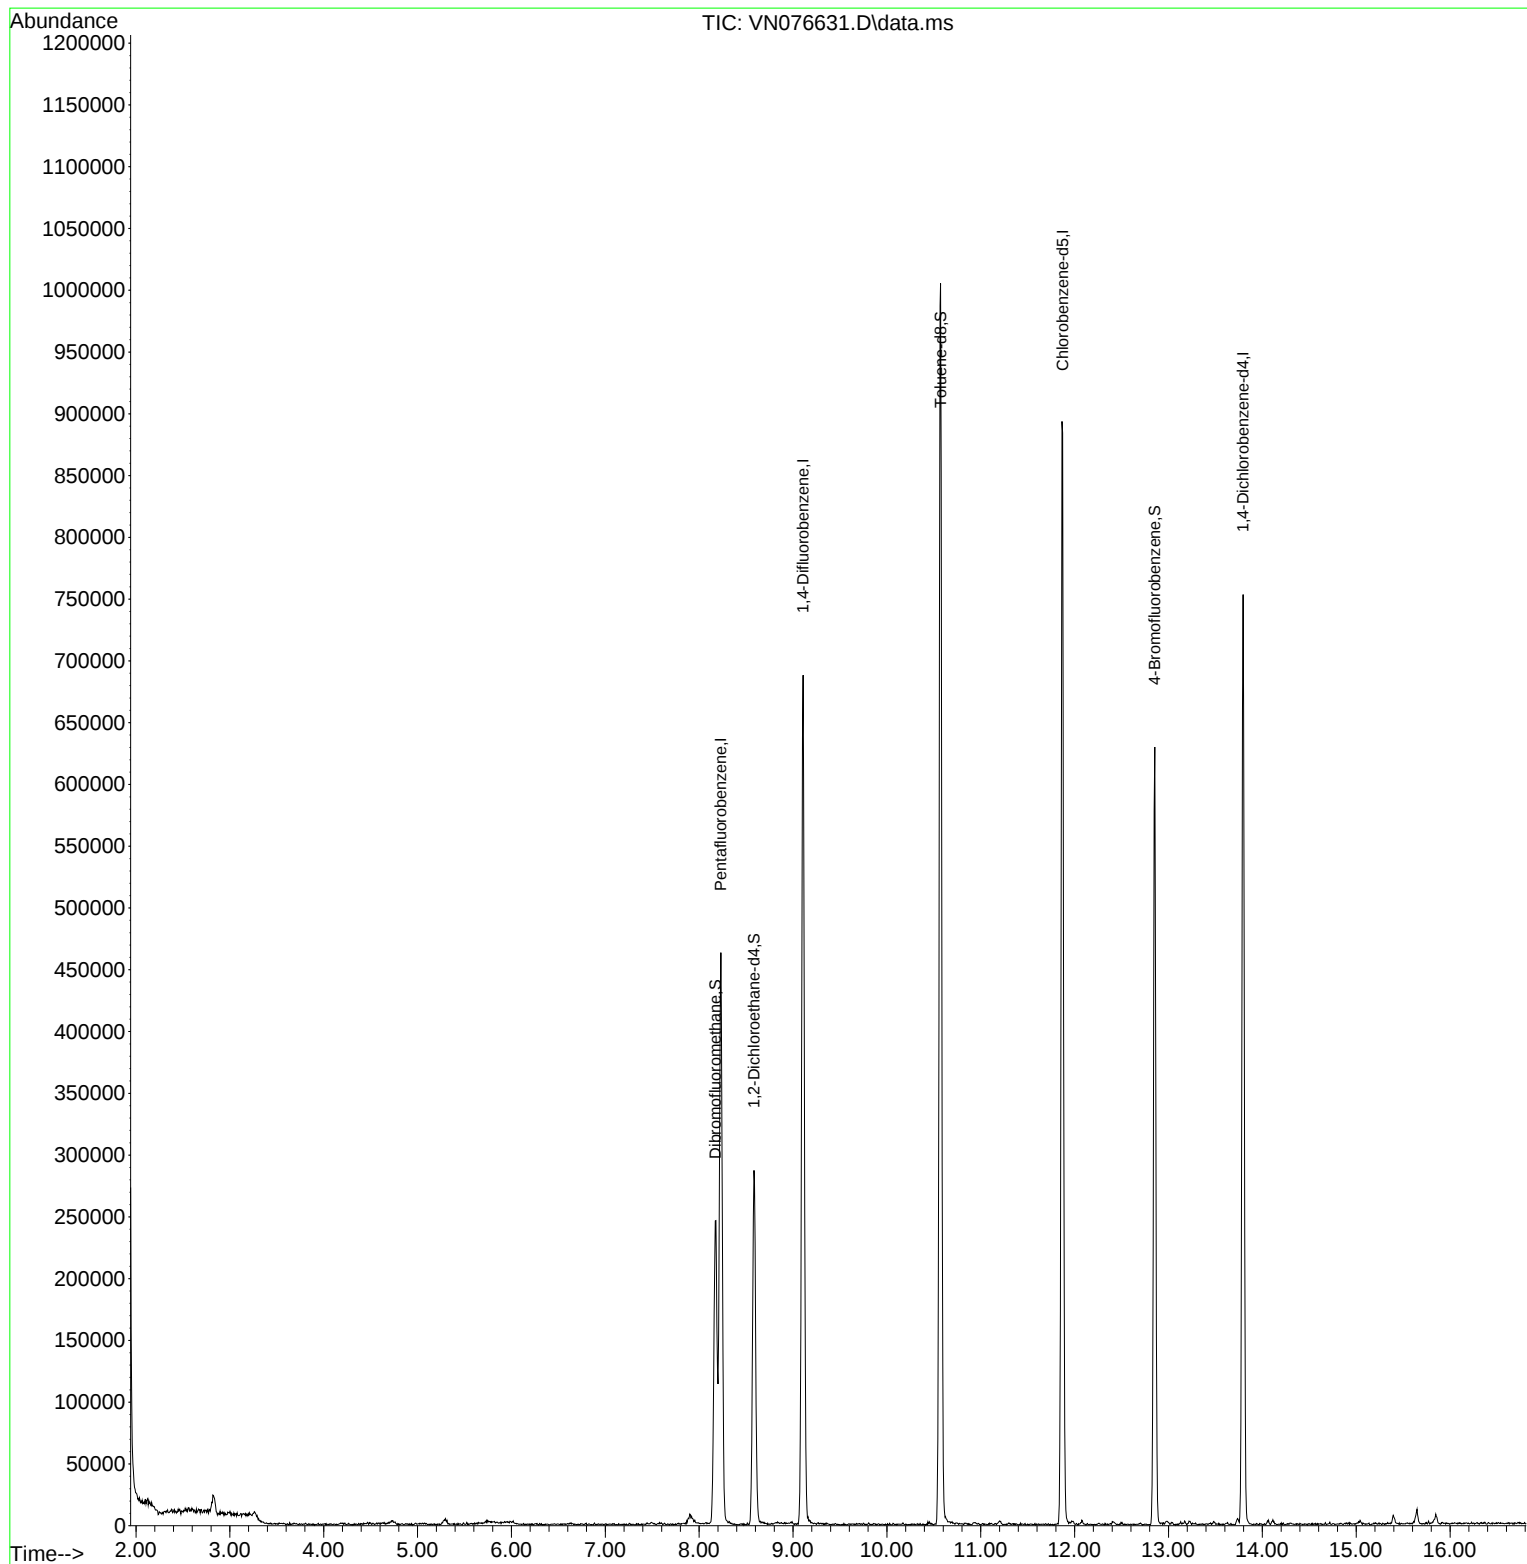


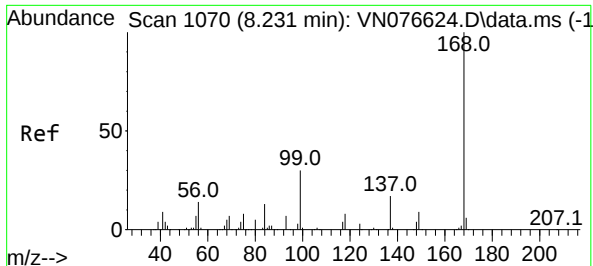

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.231 min Scan# 1070
Delta R.T. -0.000 min
Lab File: VN076631.D
Acq: 13 Feb 2023 16:22




Instrument :
MSVOA_N
ClientSampleId :
VN0213WBL01


Tgt Ion:168 Resp: 326493
Ion Ratio Lower Upper
168 100
99 58.8 44.8 67.2

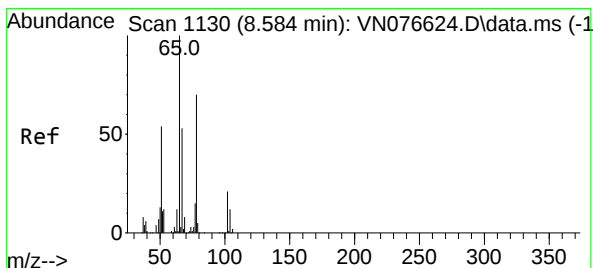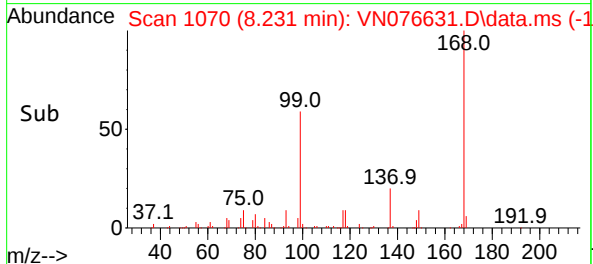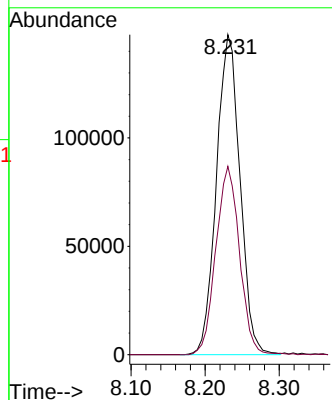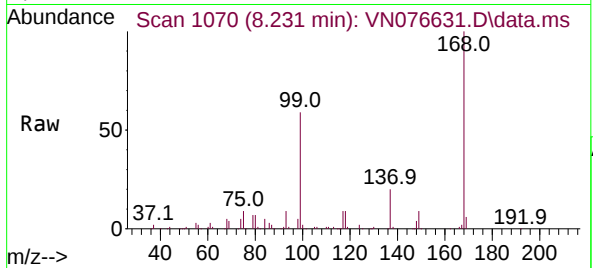

#33
1,2-Dichloroethane-d4
Concen: 49.396 ug/l
RT: 8.583 min Scan# 1130
Delta R.T. -0.000 min
Lab File: VN076631.D
Acq: 13 Feb 2023 16:22

Tgt Ion: 65 Resp: 222696
Ion Ratio Lower Upper
65 100
67 52.9 0.0 105.6

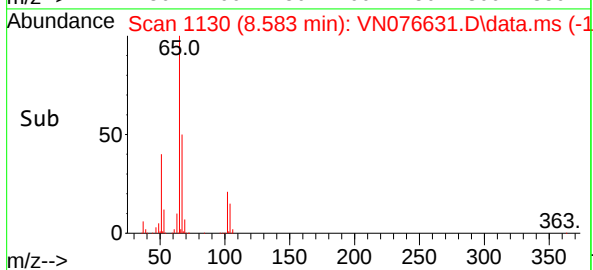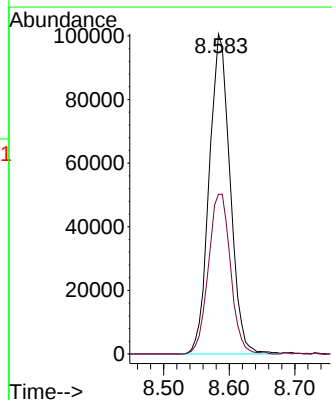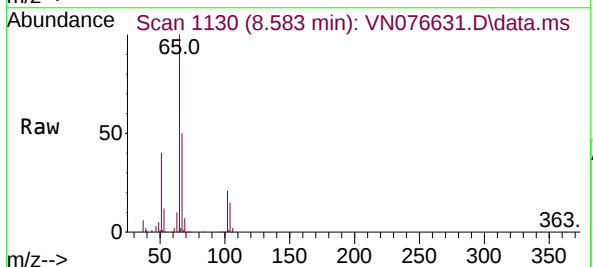

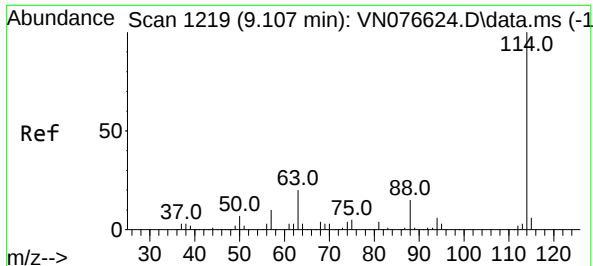

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.107 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN076631.D

Acq: 13 Feb 2023 16:22

Instrument :

MSVOA_N

ClientSampleId :

VN0213WBL01





Tgt Ion:114 Resp: 573745

Ion Ratio Lower Upper

114 100

63 21.5 0.0 40.0

88 15.2 0.0 29.6

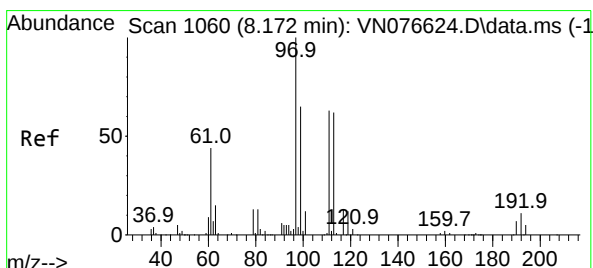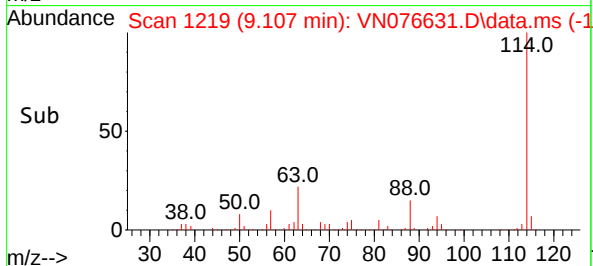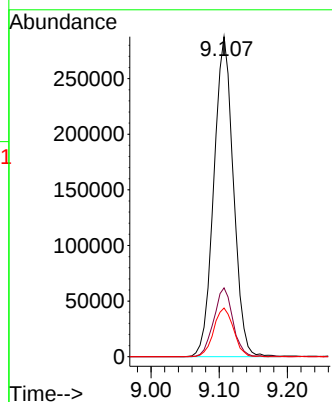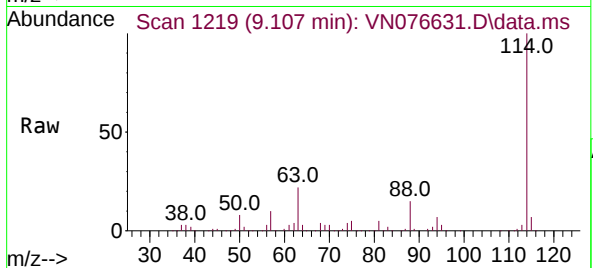

#35

Dibromofluoromethane

Concen: 47.161 ug/l

RT: 8.172 min Scan# 1060

Delta R.T. -0.000 min

Lab File: VN076631.D

Acq: 13 Feb 2023 16:22




Tgt Ion:113 Resp: 177201


Ion Ratio Lower Upper

113 100

111 103.1 83.1 124.7

192 16.9 15.6 23.4


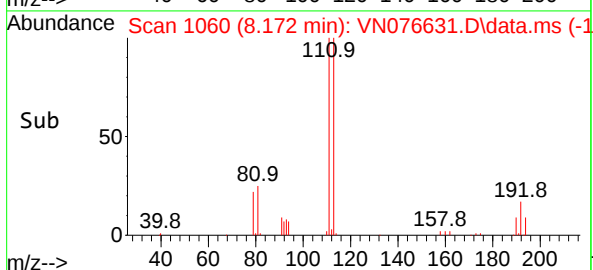
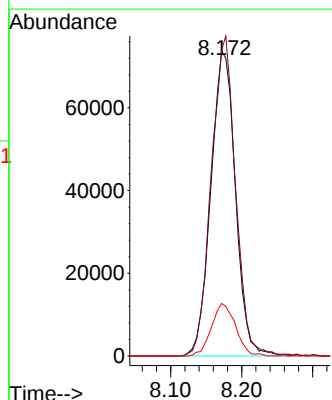
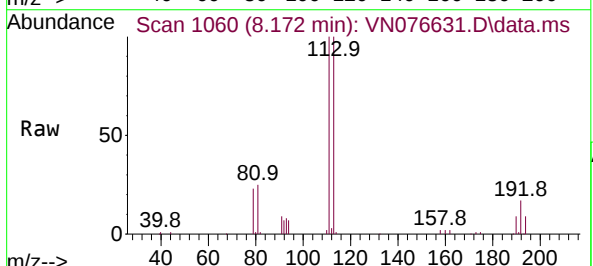


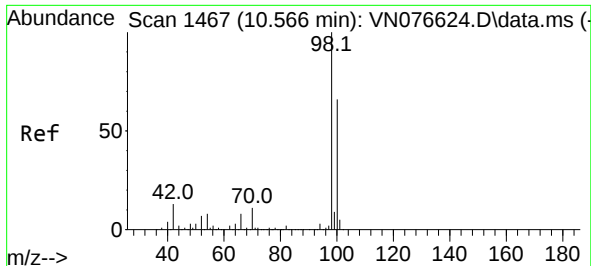

#50
Toluene-d8
Concen: 49.396 ug/l
RT: 10.572 min Scan# 1468
Delta R.T. 0.006 min
Lab File: VN076631.D
Acq: 13 Feb 2023 16:22




Instrument :
MSVOA_N
ClientSampleId :
VN0213WBL01


Tgt Ion: 98 Resp: 693126
Ion Ratio Lower Upper
98 100
100 65.1 52.9 79.3

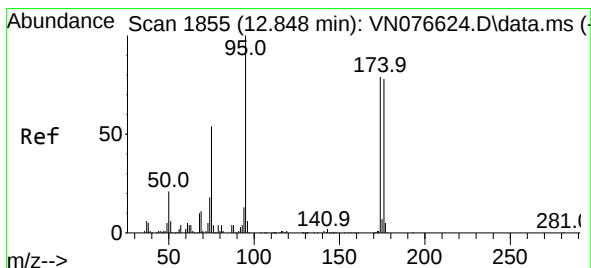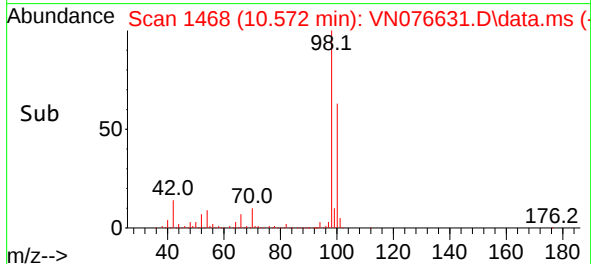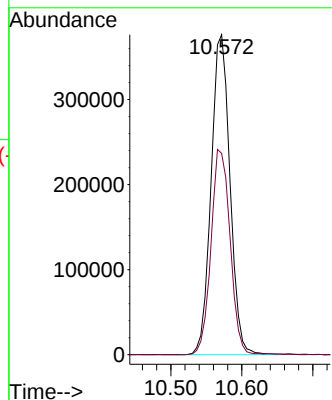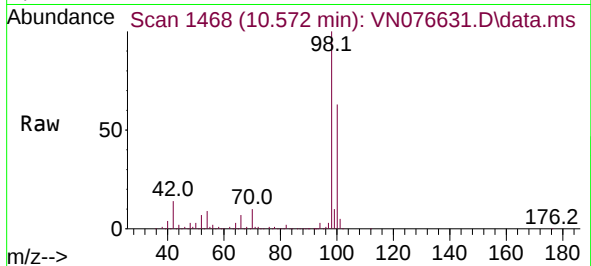

#62
4-Bromofluorobenzene
Concen: 43.830 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.006 min
Lab File: VN076631.D
Acq: 13 Feb 2023 16:22

Tgt Ion: 95 Resp: 203698
Ion Ratio Lower Upper
95 100
174 81.2 0.0 169.2
176 75.9 0.0 163.4


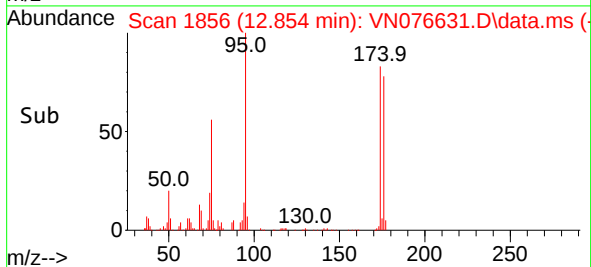
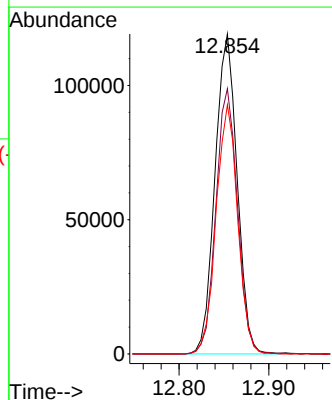
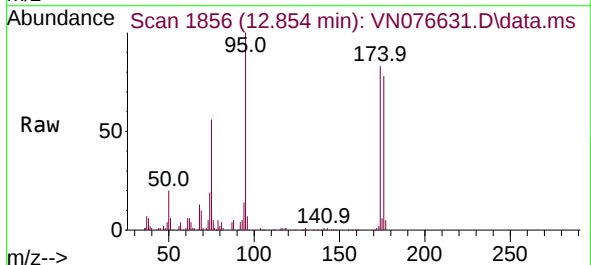


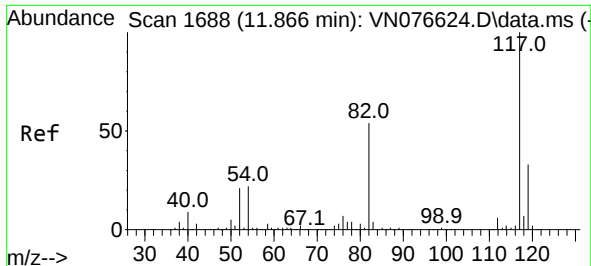

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN076631.D
Acq: 13 Feb 2023 16:22

Instrument :
MSVOA_N
ClientSampleId :
VN0213WBL01

Tgt Ion:117 Resp: 508047
Ion Ratio Lower Upper
117 100
82 54.1 43.4 65.2
119 32.2 26.1 39.1

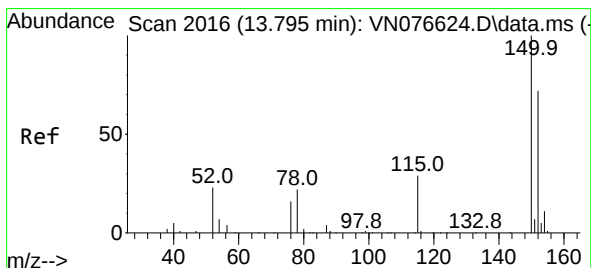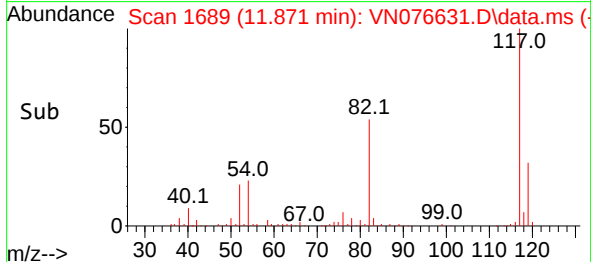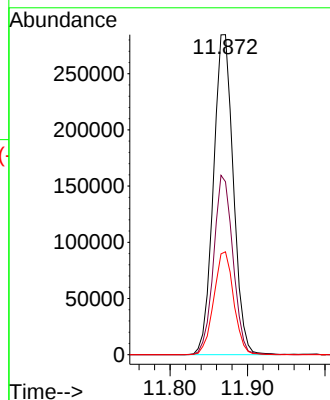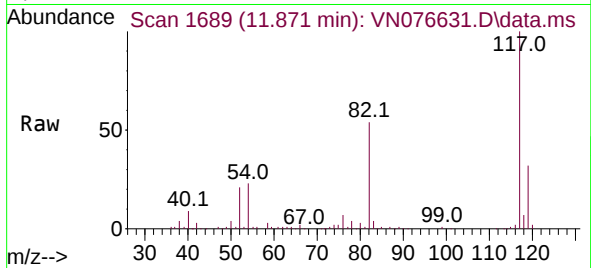

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.795 min Scan# 2016
Delta R.T. -0.000 min
Lab File: VN076631.D
Acq: 13 Feb 2023 16:22

Tgt Ion:152 Resp: 202045
Ion Ratio Lower Upper
152 100
115 58.5 29.3 87.9
150 156.1 0.0 349.8

