

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN021323\  
Data File : VN076634.D  
Acq On : 13 Feb 2023 17:55  
Operator : JC\MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N021323W.M

Title : SW846 8260

Signal : TIC: VN076634.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.831       | 145           | 152         | 162          | rVB9     | 19226          | 61802         | 3.26%           | 0.636%        |
| 2         | 7.901       | 1006          | 1014        | 1019         | rBV      | 9197           | 23978         | 1.26%           | 0.247%        |
| 3         | 8.172       | 1049          | 1060        | 1065         | rBV      | 247868         | 618787        | 32.60%          | 6.366%        |
| 4         | 8.231       | 1065          | 1070        | 1082         | rVB      | 452976         | 1006663       | 53.03%          | 10.357%       |
| 5         | 8.583       | 1120          | 1130        | 1142         | rBV      | 286371         | 643534        | 33.90%          | 6.621%        |
| 6         | 9.107       | 1210          | 1219        | 1233         | rBV      | 682247         | 1391241       | 73.29%          | 14.314%       |
| 7         | 10.572      | 1458          | 1468        | 1482         | rBV      | 1006138        | 1898383       | 100.00%         | 19.531%       |
| 8         | 11.866      | 1680          | 1688        | 1699         | rBV      | 894942         | 1614290       | 85.04%          | 16.608%       |
| 9         | 12.854      | 1847          | 1856        | 1866         | rBV      | 658026         | 1122751       | 59.14%          | 11.551%       |
| 10        | 13.795      | 2009          | 2016        | 2027         | rVB      | 781482         | 1338333       | 70.50%          | 13.769%       |




Sum of corrected areas: 9719762

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN021323\  
Data File : VN076634.D  
Acq On : 13 Feb 2023 17:55  
Operator : JC\MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N021323W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

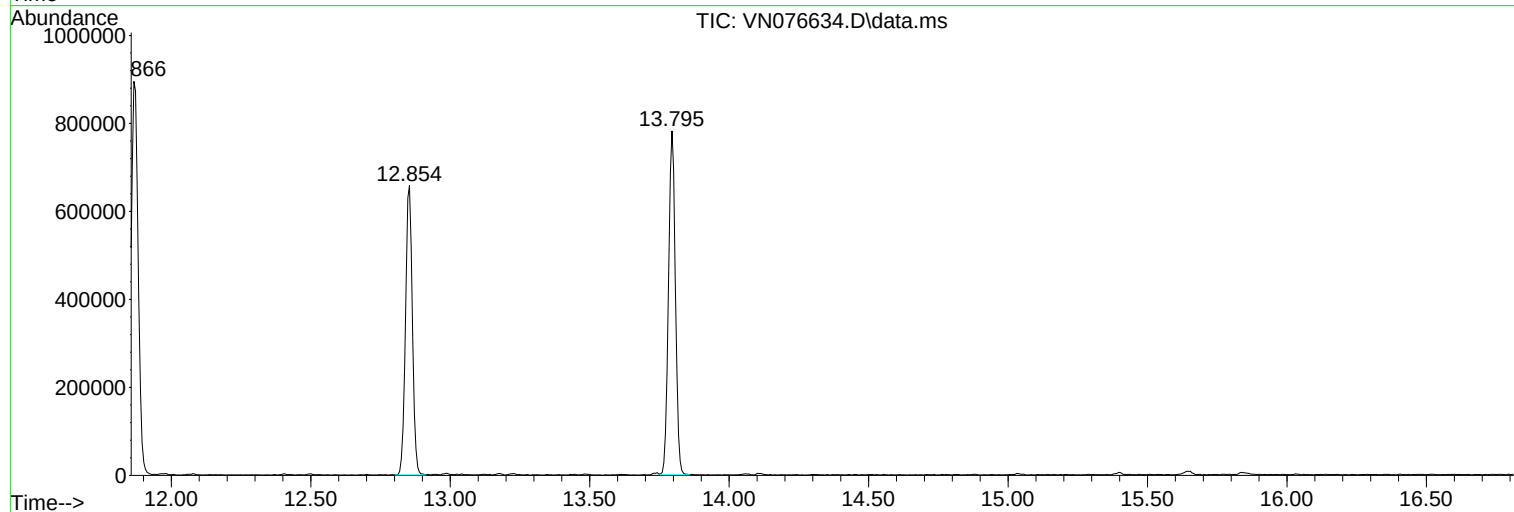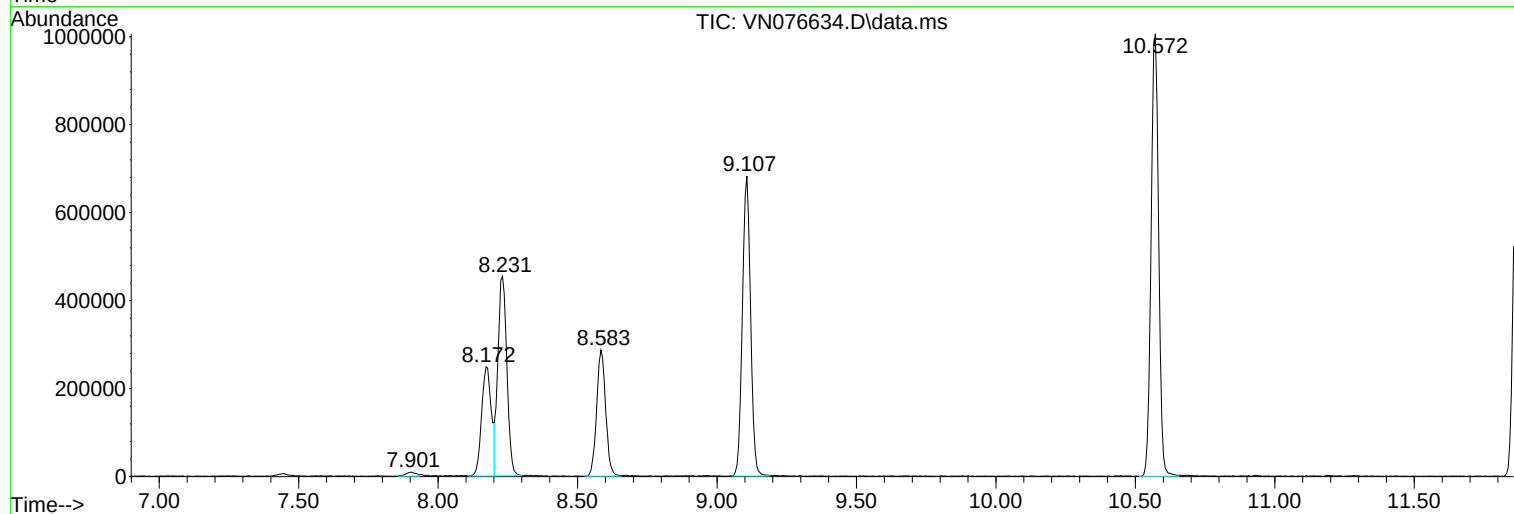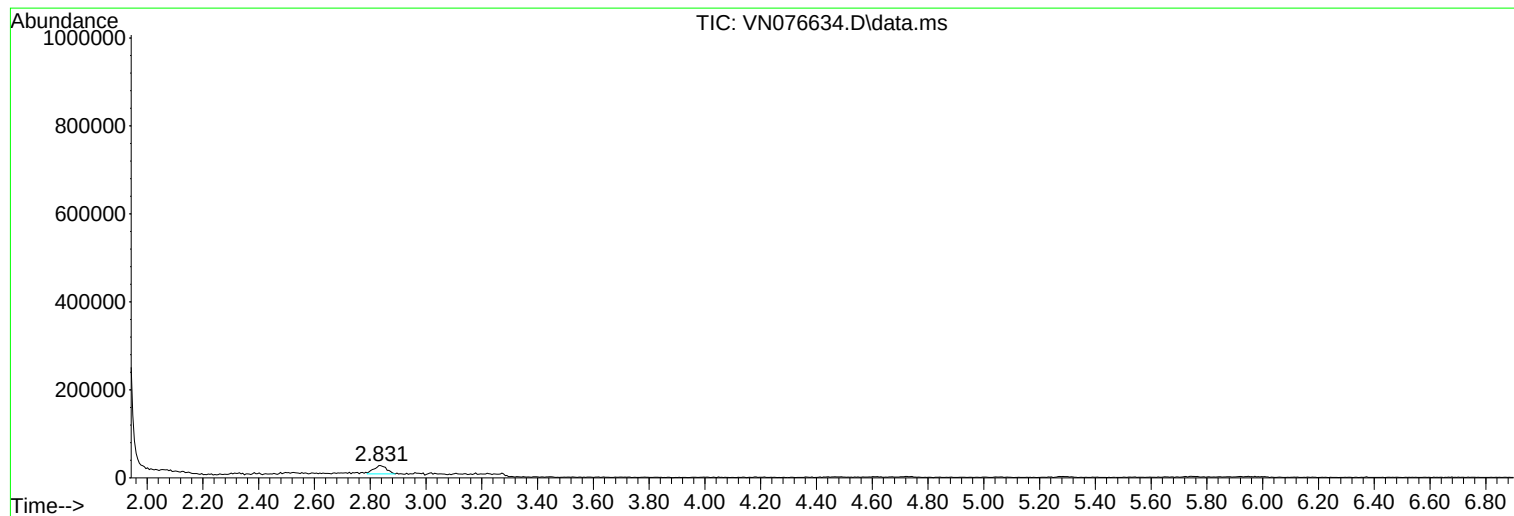

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN021323\  
Data File : VN076634.D  
Acq On : 13 Feb 2023 17:55  
Operator : JC\MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N021323W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN021323\  
Data File : VN076634.D  
Acq On : 13 Feb 2023 17:55  
Operator : JC\MD  
Sample : IBLK  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N021323W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|