
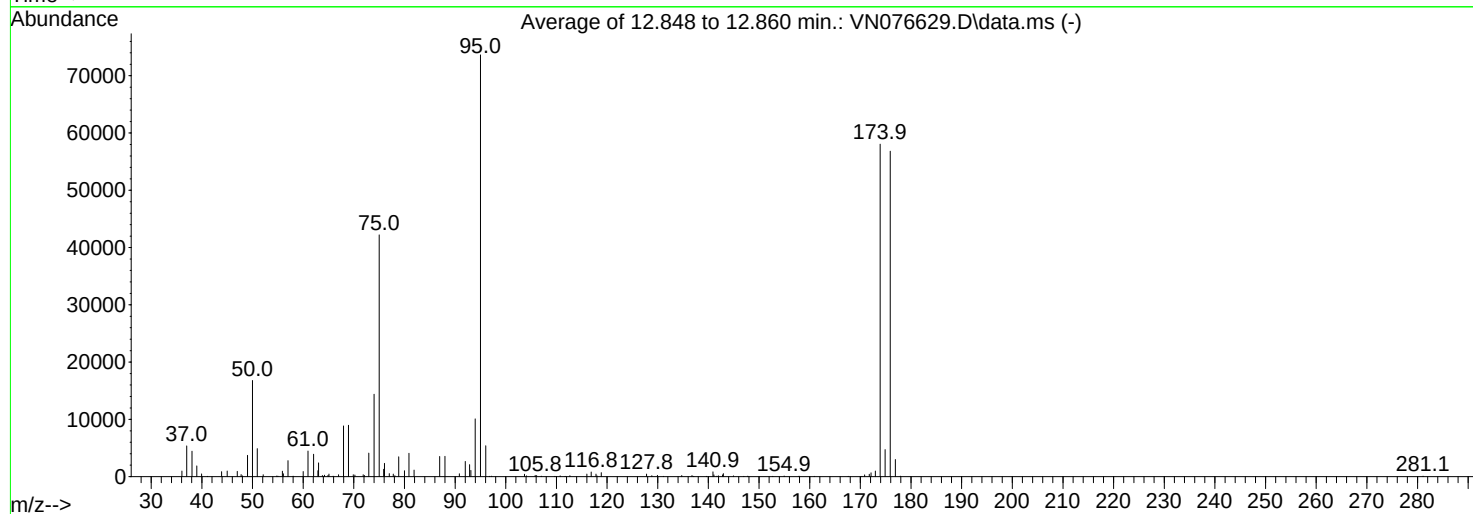


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021323\
Data File : VN076629.D
Acq On : 13 Feb 2023 15:14
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
Title : SW846 8260
Last Update : Tue Feb 14 01:44:47 2023

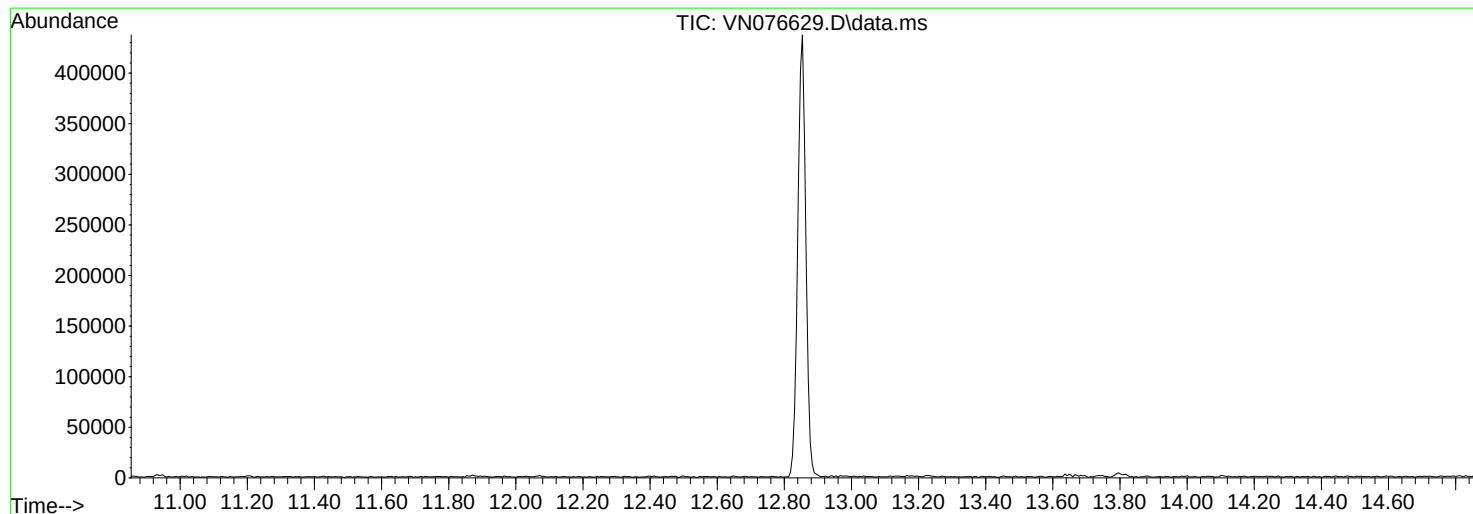

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.8	16784	PASS
75	95	30	60	57.3	42219	PASS
95	95	100	100	100.0	73651	PASS
96	95	5	9	7.3	5395	PASS
173	174	0.00	2	1.7	992	PASS
174	95	50	100	78.8	58056	PASS
175	174	5	9	8.2	4732	PASS
176	174	95	101	97.9	56827	PASS
177	176	5	9	5.3	3001	PASS

Average of 12.848 to 12.860 min.: VN076629.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	978	49.00	3723	60.95	4476	68.95	896
37.00	5377	50.00	16784	62.05	3920	69.90	32
38.05	4447	50.95	4894	62.90	1025	70.20	27
39.00	1874	52.10	340	63.05	2400	71.85	32
39.95	474	54.80	114	63.80	211	72.10	199
41.10	64	55.00	93	64.20	257	72.95	4102
43.90	869	55.90	957	64.90	218	74.00	14377
45.00	970	56.10	516	65.10	460	75.00	42219
47.00	936	57.00	2810	65.90	82	75.90	1299
47.75	376	58.00	99	67.00	325	76.05	2315
48.00	152	60.00	896	67.95	8863	77.00	530

Average of 12.848 to 12.860 min.: VN076629.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.80	438	93.10	1099	109.70	70	129.95	228
78.10	177	93.95	10099	110.75	136	131.10	67
78.85	3471	95.00	73651	111.70	60	134.75	209
80.00	1041	96.05	5395	112.65	161	136.75	205
80.90	4077	96.80	68	116.00	442	137.10	60
81.90	1139	97.20	93	116.85	800	139.60	56
86.95	3530	103.70	428	117.80	440	140.90	842
88.00	3545	104.10	155	118.00	148	141.10	298
90.85	504	105.80	221	118.85	702	141.70	95
92.00	2654	106.10	208	127.80	442	142.00	142
92.85	2090	107.00	72	128.85	160	142.80	314

Average of 12.848 to 12.860 min.: VN076629.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
142.95	544	171.75	424				
144.95	155	172.10	672				
147.00	68	172.95	992				
147.80	90	173.90	58056				
152.70	70	174.90	4732				
154.95	108	175.90	56827				
157.90	91	176.90	3001				
160.90	59	177.90	81				
167.60	58	281.10	94				
170.30	71						
170.85	312						

Instrument :

MSVOA_N

ClientSampleId :

BFB