


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN021419\
Data File : VN053768.D
Acq On : 14 Feb 2019 9:46
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
Title : SW846 8260
Last Update : Fri Feb 01 09:11:52 2019

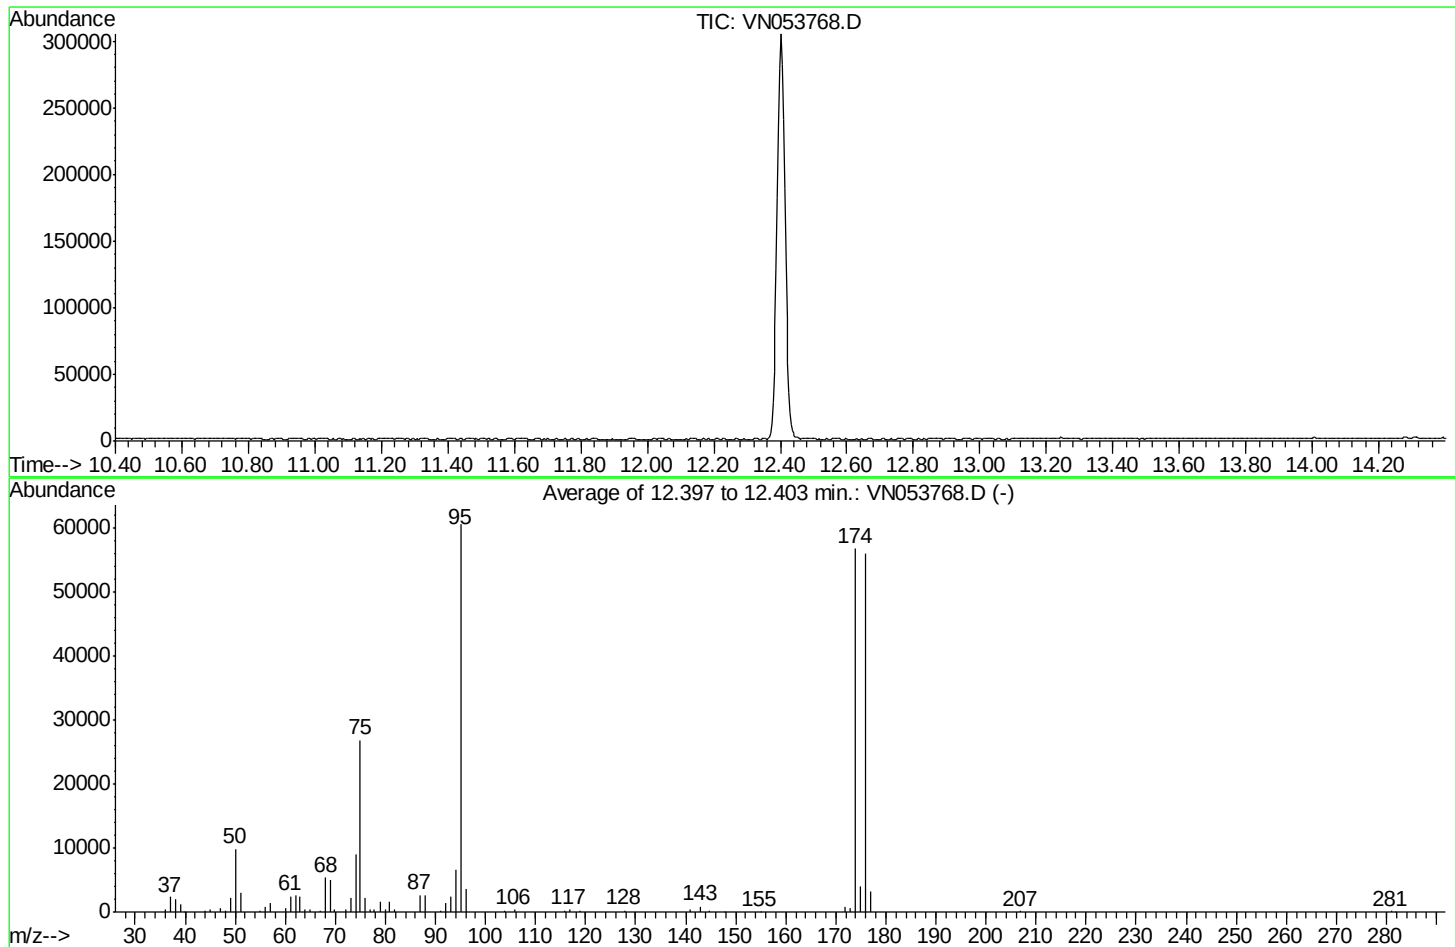

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	9803	PASS
75	95	30	60	44.4	26858	PASS
95	95	100	100	100.0	60520	PASS
96	95	5	9	6.1	3701	PASS
173	174	0.00	2	1.0	546	PASS
174	95	50	100	93.7	56712	PASS
175	174	5	9	7.0	3955	PASS
176	174	95	101	98.7	55981	PASS
177	176	5	9	5.7	3217	PASS