


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN021420\
 Data File : VN060097.D
 Acq On : 14 Feb 2020 8:59
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N021220W.M
 Title : SW846 8260
 Last Update : Wed Feb 12 14:12:21 2020

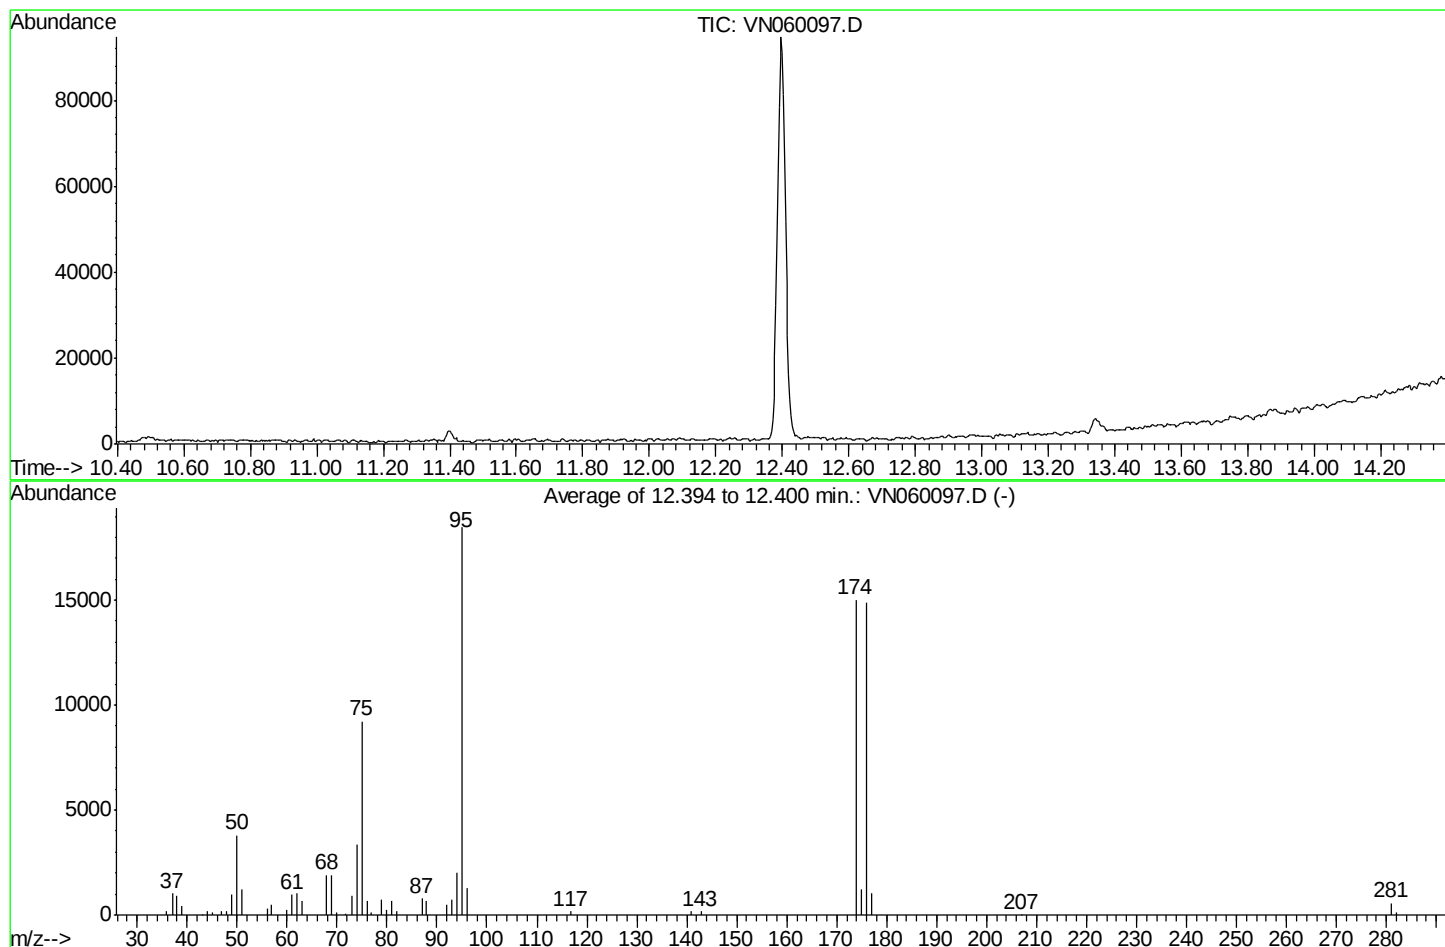

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	3794	PASS
75	95	30	60	49.9	9218	PASS
95	95	100	100	100.0	18472	PASS
96	95	5	9	7.0	1288	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.3	15020	PASS
175	174	5	9	8.2	1238	PASS
176	174	95	101	99.1	14891	PASS
177	176	5	9	7.0	1044	PASS