



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021423\
Data File : VN076651.D
Acq On : 14 Feb 2023 10:19
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
Title : SW846 8260
Last Update : Tue Feb 14 01:44:47 2023

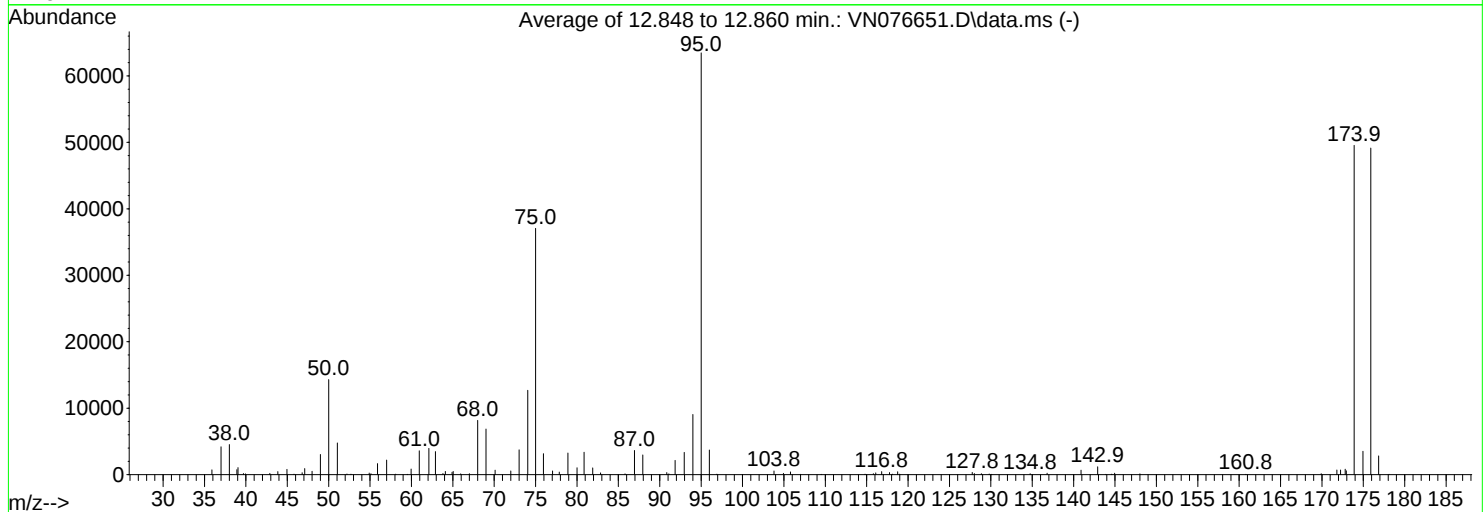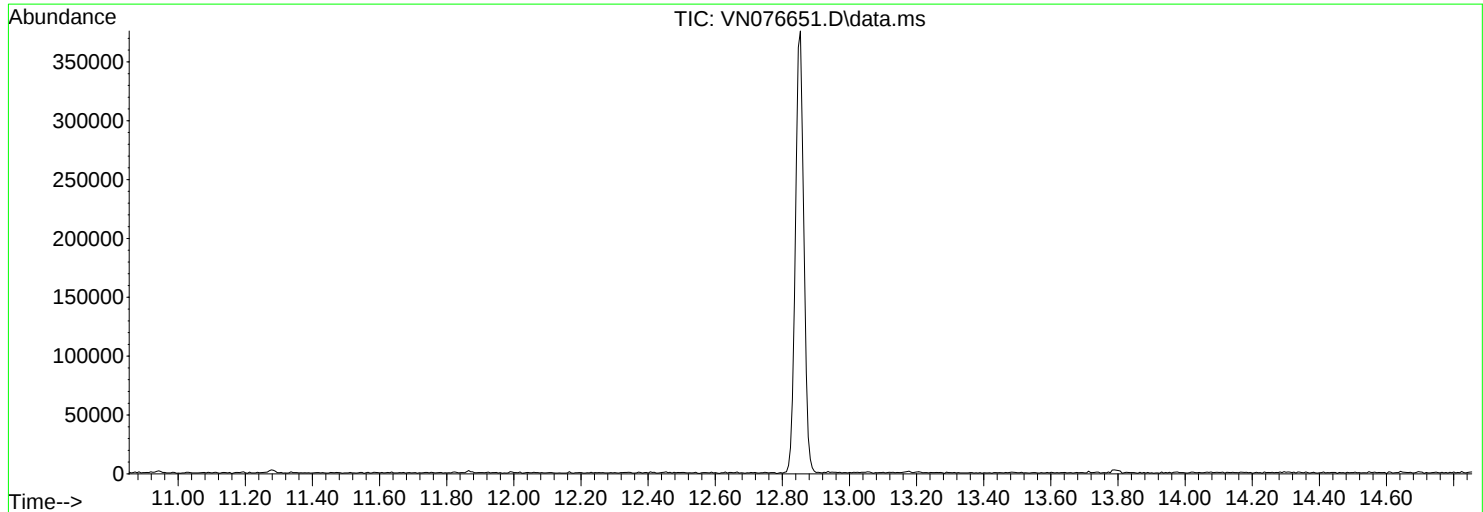

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	14297	PASS
75	95	30	60	58.4	37045	PASS
95	95	100	100	100.0	63472	PASS
96	95	5	9	5.9	3715	PASS
173	174	0.00	2	1.7	824	PASS
174	95	50	100	78.1	49549	PASS
175	174	5	9	7.1	3526	PASS
176	174	95	101	99.2	49133	PASS
177	176	5	9	5.7	2813	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	720	46.80	280	57.00	2182	65.95	12
37.00	4194	47.10	910	58.10	80	67.00	13
38.00	4527	48.00	498	59.50	52	68.00	816
38.90	759	49.00	3027	59.95	854	69.00	687
39.05	1062	50.00	14297	60.95	3589	70.10	680
39.70	168	51.05	4758	62.10	3960	72.00	544
39.95	112	52.20	108	62.90	3477	73.00	3742
42.90	186	52.70	75	63.80	181	74.05	12683
43.85	465	54.90	255	64.10	478	75.00	37045
44.95	787	55.10	141	64.90	362	75.95	3160
45.80	65	55.90	1665	65.05	484	77.05	556

Average of 12.848 to 12.860 min.: VN076651.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.85	386	91.85	2137	114.80	84	129.80	102
78.90	3252	92.95	3355	115.80	144	130.10	53
80.00	1037	94.00	9050	116.10	264	134.75	147
80.85	3364	95.00	63472	116.80	461	136.80	228
81.90	1017	96.00	3715	117.75	323	140.90	686
82.85	262	96.90	71	118.10	83	142.90	1190
85.80	134	103.80	563	118.75	424	143.90	60
86.95	3638	104.95	204	119.00	87	144.60	74
87.95	2954	105.80	416	127.75	334	144.95	221
90.85	313	107.00	52	128.00	169	148.00	126
91.10	129	109.50	51	128.85	159	160.80	54

Average of 12.848 to 12.860 min.: VN076651.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
169.90	145						
171.80	706						
172.25	702						
172.80	824						
172.95	568						
173.90	49549						
174.95	3526						
175.90	49133						
176.85	2813						
178.10	61						

Instrument :

MSVOA_N

ClientSampleId :

BFB