
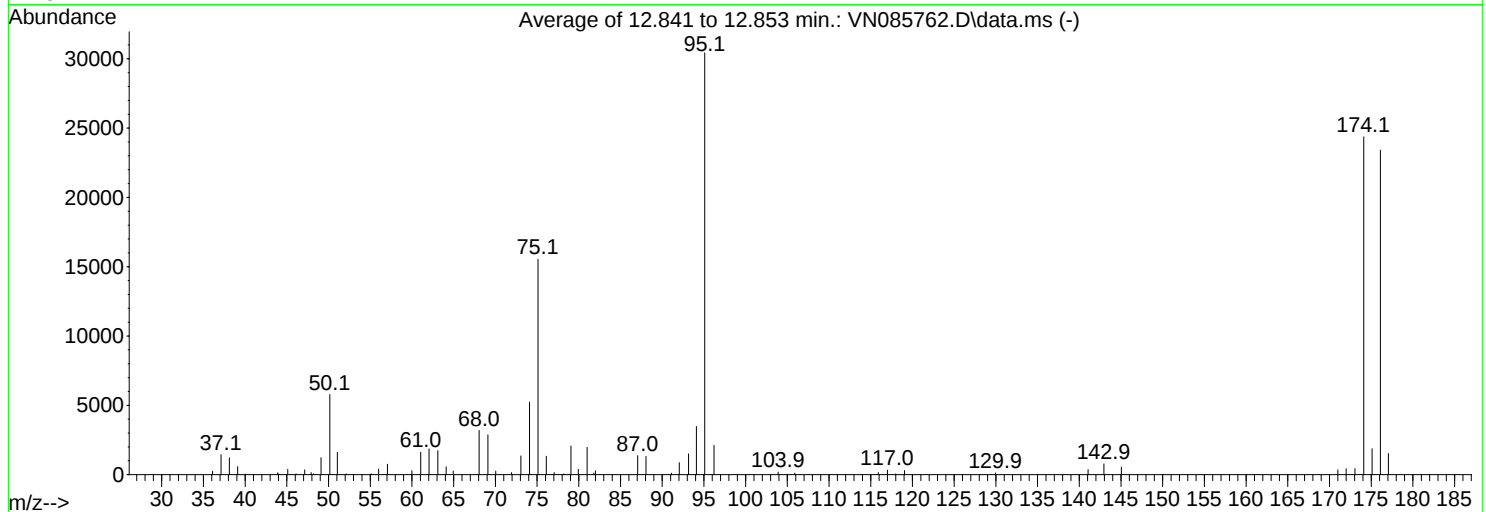


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021425\
Data File : VN085762.D
Acq On : 14 Feb 2025 09:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N011425W.M
Title : SW846 8260
Last Update : Wed Jan 15 02:16:08 2025

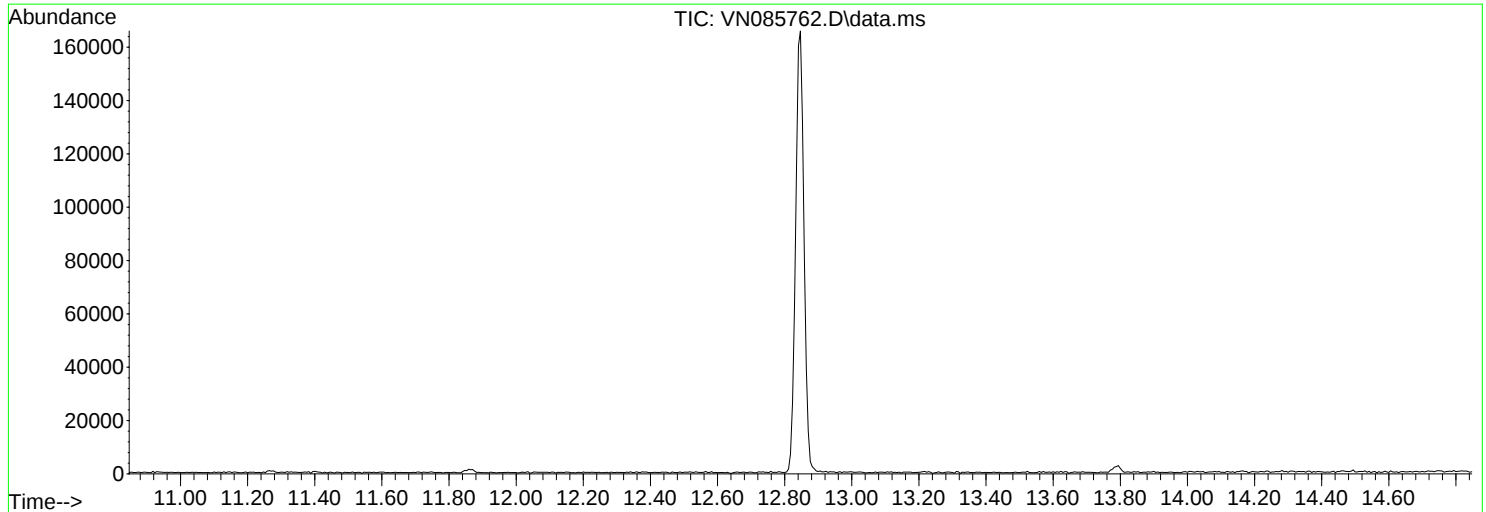

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	5779	PASS
75	95	30	60	51.1	15538	PASS
95	95	100	100	100.0	30429	PASS
96	95	5	9	6.9	2108	PASS
173	174	0.00	2	1.8	442	PASS
174	95	50	100	80.1	24365	PASS
175	174	5	9	7.7	1873	PASS
176	174	95	101	96.1	23411	PASS
177	176	5	9	6.5	1519	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	239	48.20	53	63.10	1726	77.05	144
37.10	1448	49.10	1225	64.10	565	78.20	5
38.10	1208	50.15	5779	64.95	261	79.05	206
39.10	575	51.05	1617	68.05	3193	79.95	38
40.05	30	52.10	53	69.10	2879	81.00	1978
43.90	142	55.10	57	70.05	253	81.80	114
44.05	49	56.00	402	71.95	151	82.00	273
45.10	376	57.05	750	73.05	1346	87.05	1375
46.10	56	60.00	288	74.10	5237	88.05	1318
47.15	345	61.05	1615	75.10	15538	91.10	110
47.90	153	62.05	1863	76.10	1329	92.05	861

Average of 12.841 to 12.853 min.: VN085762.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.15	1504	141.05	371				
94.10	3479	142.95	778				
95.10	30429	145.05	544				
96.20	2108	171.00	347				
103.90	189	172.00	428				
105.90	116	173.05	442				
115.90	154	174.10	24365				
117.00	323	175.10	1873				
118.00	56	176.10	23411				
119.05	299	177.05	1519				
129.95	132						

Instrument :

MSVOA_N

ClientSampleId :

BFB