


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN021519\
Data File : VN053814.D
Acq On : 15 Feb 2019 21:33
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
Title : SW846 8260
Last Update : Fri Feb 01 09:11:52 2019

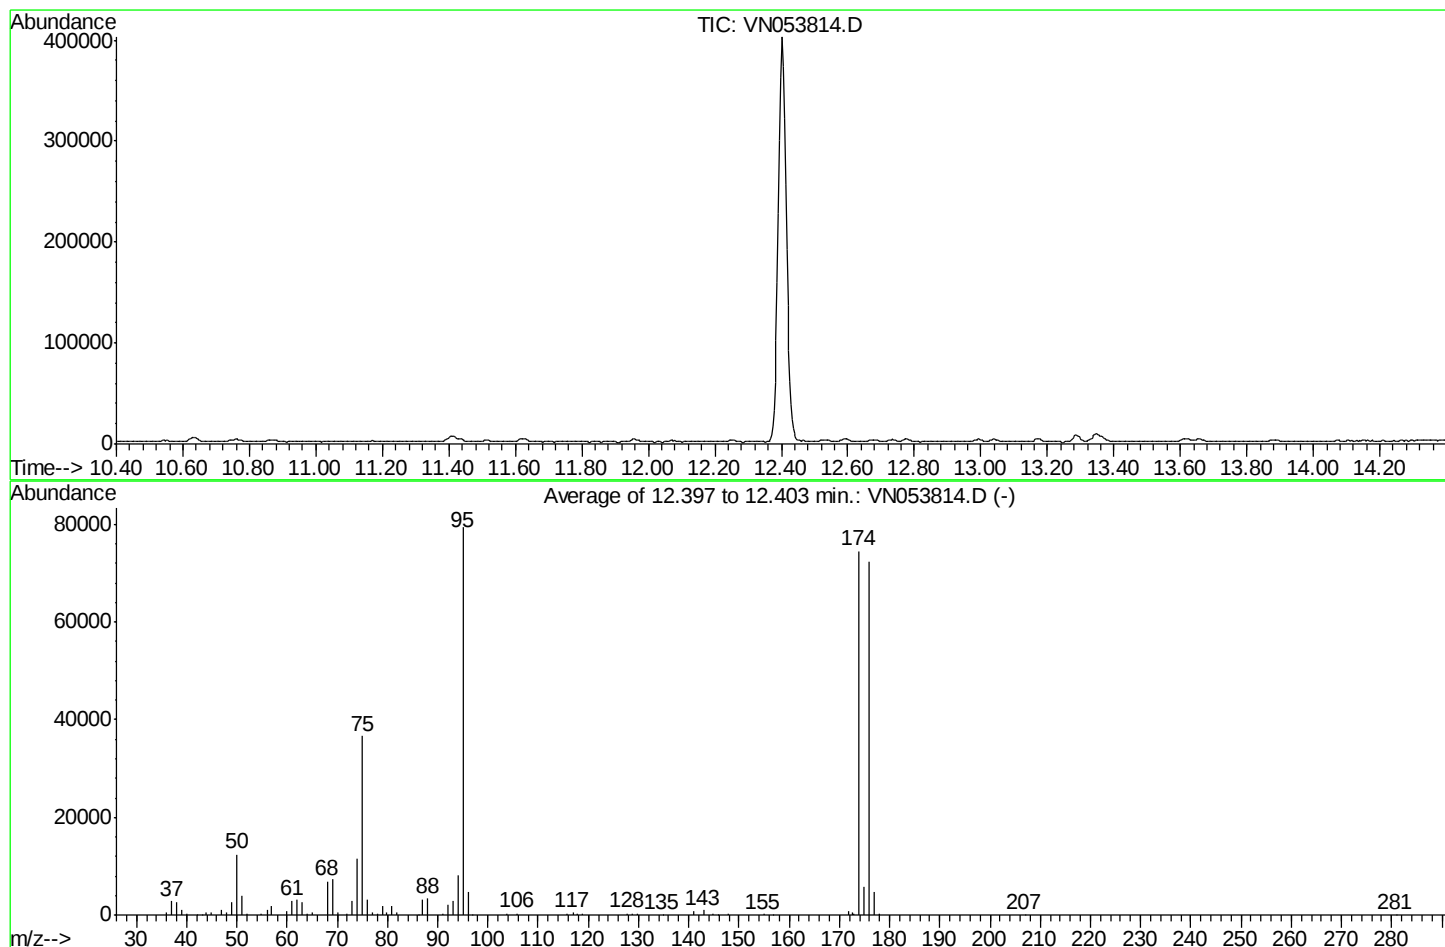

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	12464	PASS
75	95	30	60	46.2	36685	PASS
95	95	100	100	100.0	79421	PASS
96	95	5	9	6.1	4810	PASS
173	174	0.00	2	0.6	451	PASS
174	95	50	100	93.8	74490	PASS
175	174	5	9	7.6	5658	PASS
176	174	95	101	97.3	72480	PASS
177	176	5	9	6.6	4808	PASS