
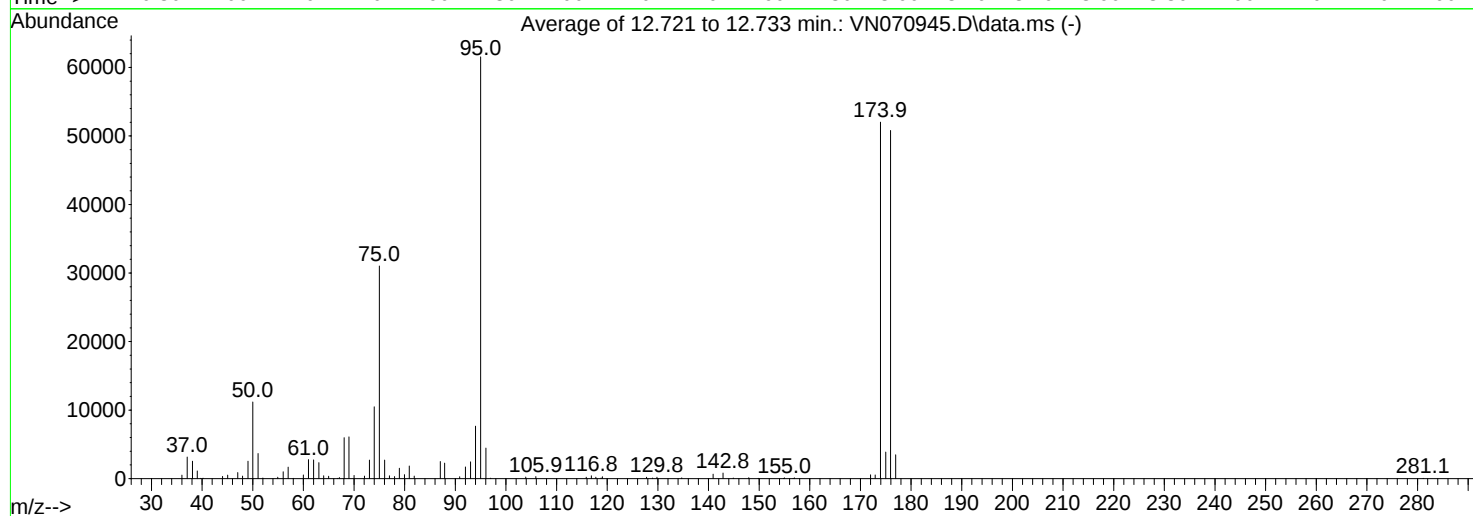


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021522\
 Data File : VN070945.D
 Acq On : 15 Feb 2022 11:11
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
 Title : SW846 8260
 Last Update : Mon Feb 21 07:57:15 2022

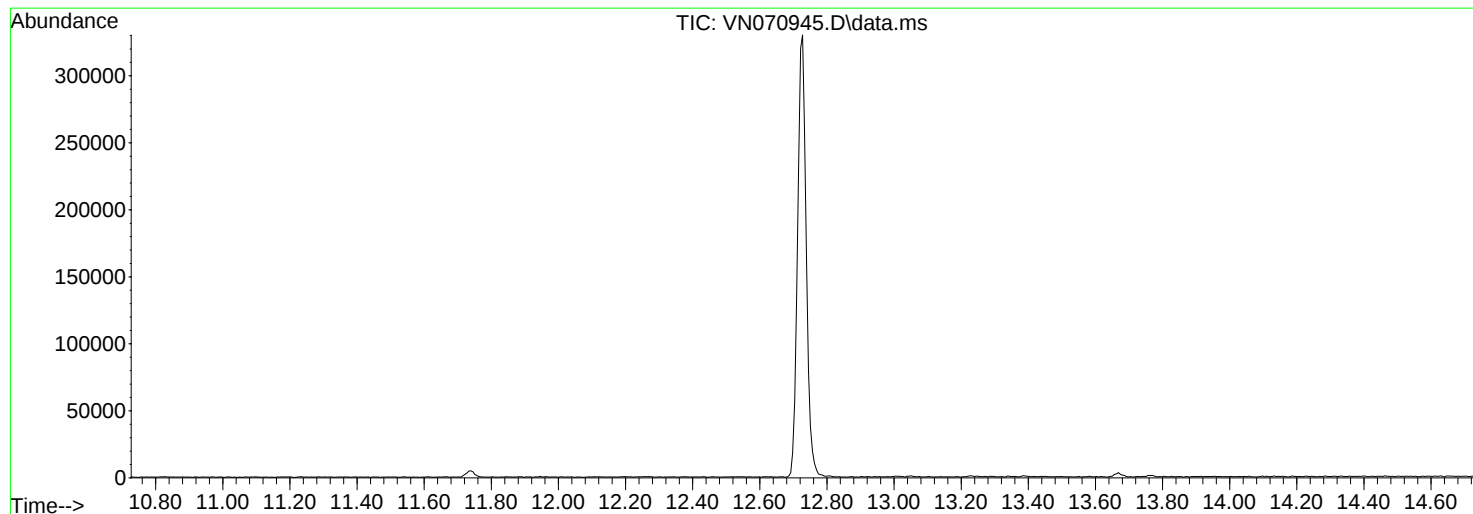

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	11186	PASS
75	95	30	60	50.4	31032	PASS
95	95	100	100	100.0	61544	PASS
96	95	5	9	7.3	4470	PASS
173	174	0.00	2	1.0	540	PASS
174	95	50	100	84.5	52011	PASS
175	174	5	9	7.5	3887	PASS
176	174	95	101	97.7	50811	PASS
177	176	5	9	6.8	3471	PASS