


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021523\
 Data File : VN076675.D
 Acq On : 15 Feb 2023 09:48
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N021523W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Feb 16 01:08:46 2023

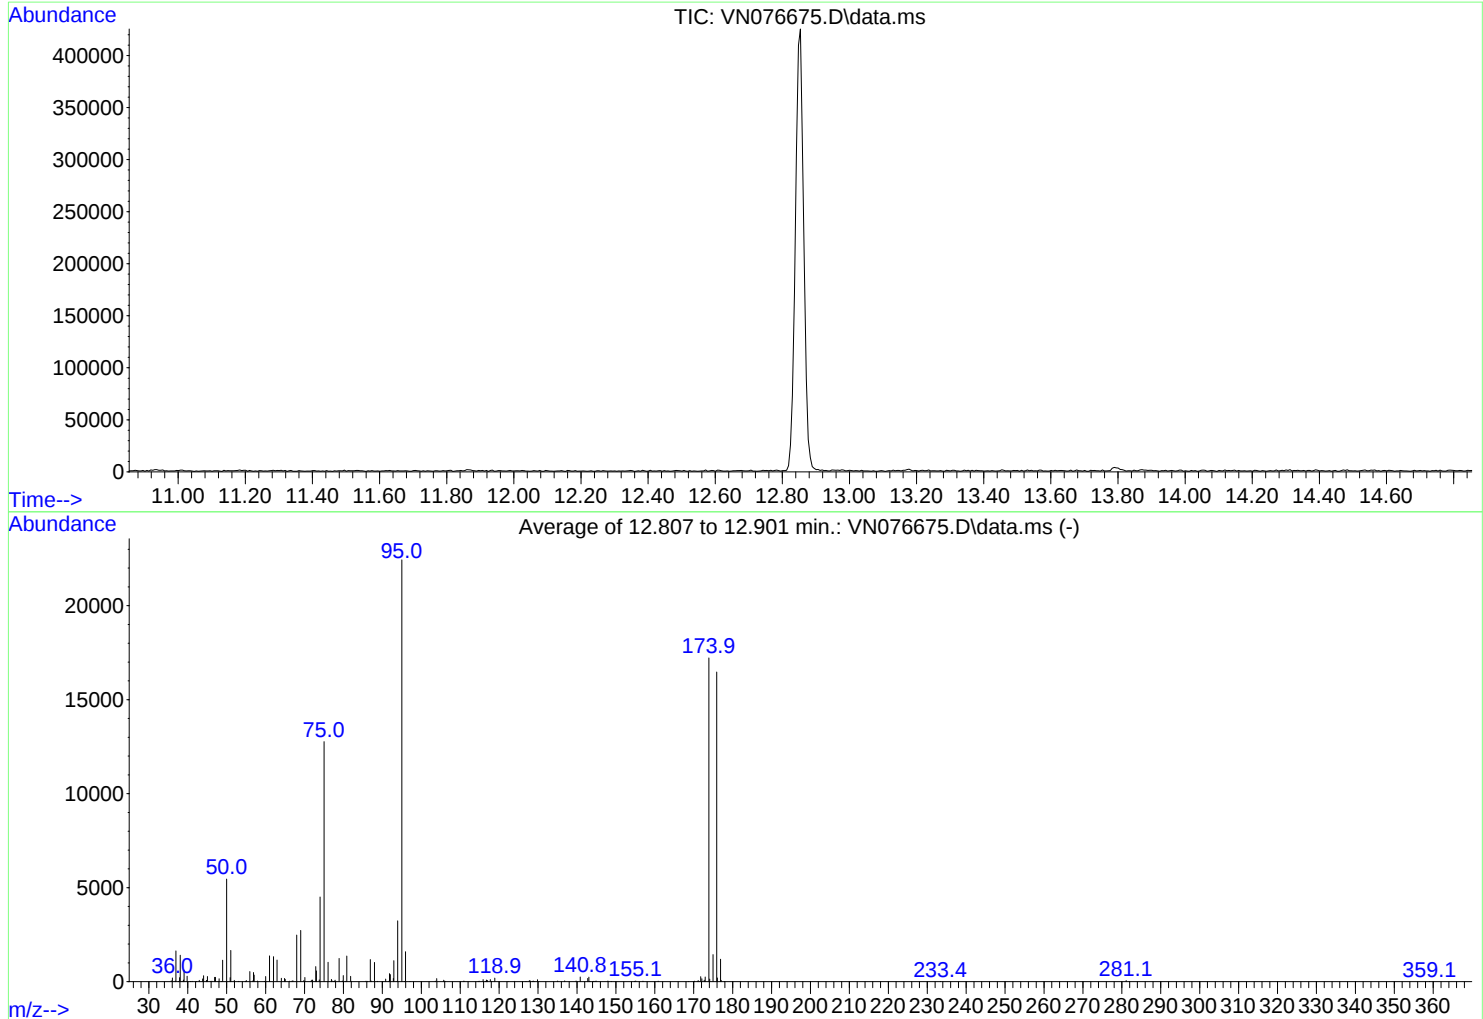

AutoFind: Averaged scan 1848 to 1864; Bkg corrected with scan 1847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.3	5454	PASS
75	95	30	60	56.9	12770	PASS
95	95	100	100	100.0	22436	PASS
96	95	5	9	7.1	1594	PASS
173	174	0.00	2	1.4	245	PASS
174	95	50	100	76.7	17217	PASS
175	174	5	9	8.4	1442	PASS
176	174	95	101	95.6	16466	PASS
177	176	5	9	7.3	1194	PASS