
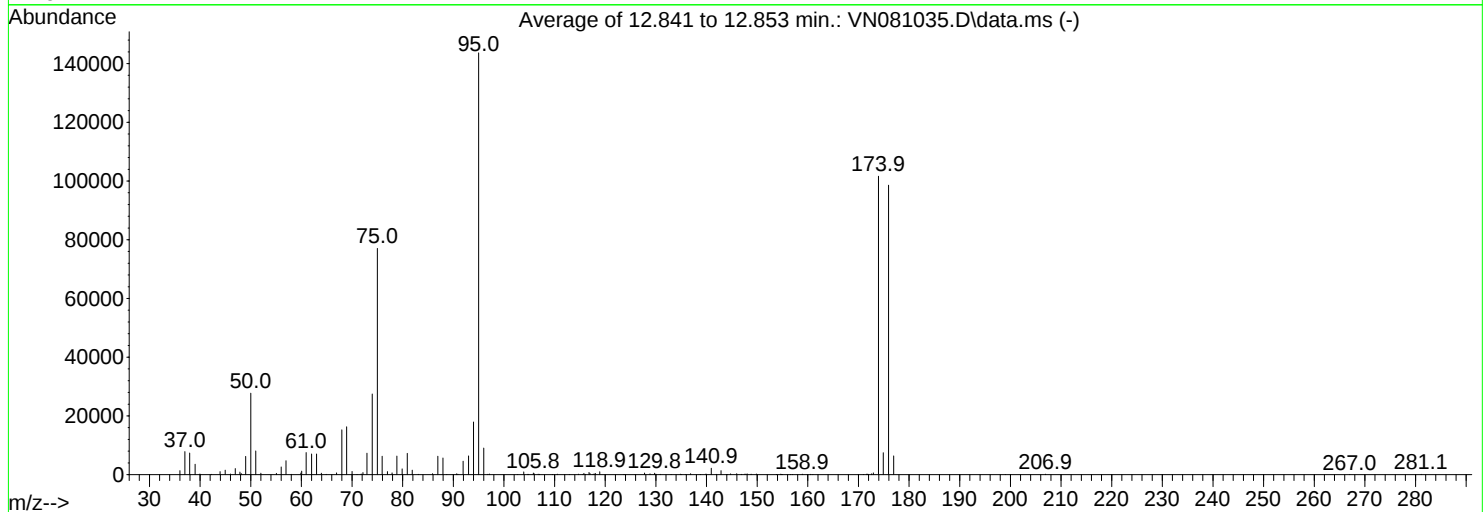


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021524\
Data File : VN081035.D
Acq On : 15 Feb 2024 08:34
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021424W.M
Title : SW846 8260
Last Update : Thu Feb 15 07:59:19 2024

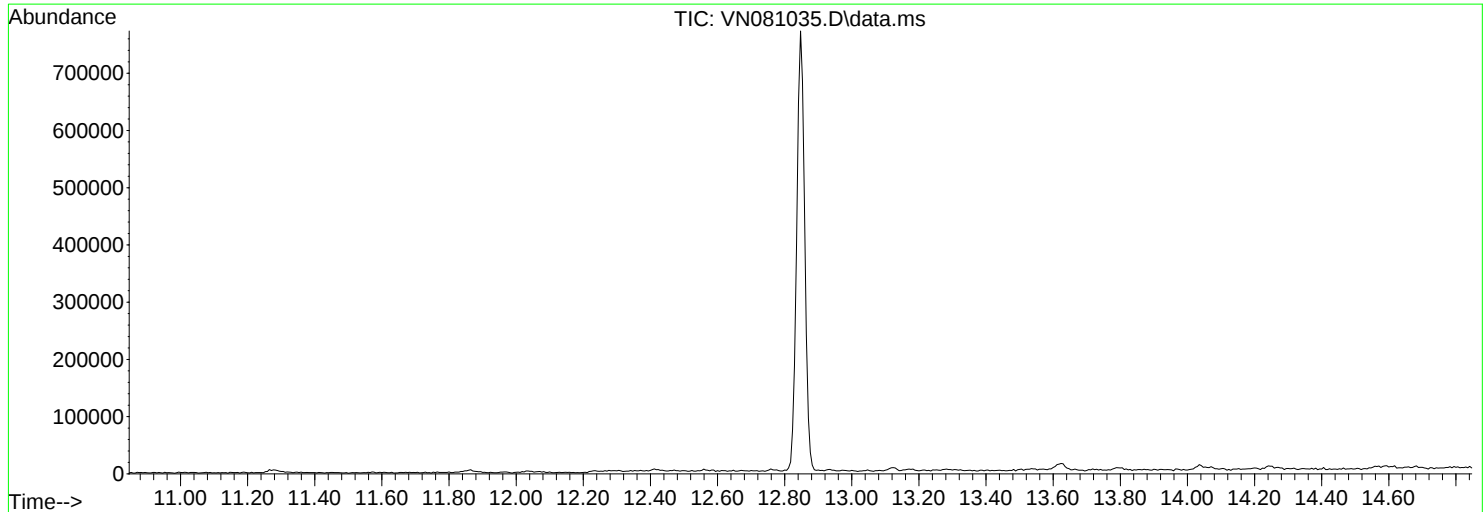

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	27725	PASS
75	95	30	60	53.6	77072	PASS
95	95	100	100	100.0	143659	PASS
96	95	5	9	6.3	9075	PASS
173	174	0.00	2	0.6	576	PASS
174	95	50	100	70.7	101627	PASS
175	174	5	9	7.4	7472	PASS
176	174	95	101	97.0	98597	PASS
177	176	5	9	6.5	6377	PASS

Average of 12.841 to 12.853 min.: VN081035.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	1361	48.10	401	60.95	7506	72.15	714
37.00	7877	49.00	6200	62.00	7056	72.95	730
37.95	7340	50.00	27725	63.00	7035	74.00	2748
39.00	3525	51.00	8085	63.95	505	75.00	7707
39.95	201	52.00	495	64.90	109	75.95	6278
42.20	142	55.05	436	66.95	619	77.00	1019
43.95	1030	56.00	2638	68.00	15251	77.90	577
44.95	1557	56.95	4741	68.95	16287	78.85	6319
46.00	209	58.00	137	70.00	1109	79.90	1964
46.95	2078	59.90	525	71.00	58	80.90	7238
47.85	901	60.05	1195	71.80	223	81.90	1511

Average of 12.841 to 12.853 min.: VN081035.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
83.10	125	96.00	9075	109.60	66	117.80	279
85.90	311	96.80	120	110.55	158	118.05	387
86.95	6261	97.10	213	112.00	82	118.90	965
87.95	5658	102.70	84	112.90	57	123.70	86
88.70	59	103.90	913	114.70	194	123.90	73
90.65	283	104.70	132	115.60	102	125.90	65
90.90	161	104.90	134	115.80	467	127.75	527
91.95	4607	105.80	525	116.10	132	128.85	270
93.00	6396	106.00	281	116.80	775	129.75	496
94.00	17918	106.75	185	117.00	373	130.00	184
95.00	143659	107.00	124	117.60	99	130.85	134

Average of 12.841 to 12.853 min.: VN081035.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
133.00	57	144.10	76	155.00	81	172.95	576
134.85	199	144.75	267	156.60	86	173.95	101627
135.10	80	145.95	343	157.00	67	174.90	7472
135.90	62	146.90	90	158.90	166	175.95	98597
136.85	333	147.60	206	160.55	123	176.95	6377
138.80	61	148.00	292	161.00	57	199.00	55
139.90	242	148.80	161	171.00	51	206.95	150
140.95	2187	149.85	206	171.60	148	267.00	53
141.90	130	153.80	57	171.80	167	281.10	113
142.85	1387	154.65	161	172.00	115		
143.90	75	154.80	123	172.60	292		