

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021621\
 Data File : VN065878.D
 Acq On : 16 Feb 2021 17:23
 Operator : JC/MD
 Sample : M1413-04
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 EB01-GW-021221

Quant Time: Feb 16 17:44:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 15 10:57:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.624	168	167758	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.547	114	282044	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	246767	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.315	152	87193	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.987	65	92609	41.96	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	83.92%
35) Dibromofluoromethane	7.547	113	80933	48.42	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	96.84%
50) Toluene-d8	10.058	98	347871	52.95	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	105.90%
62) 4-Bromofluorobenzene	12.373	95	110317	46.63	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	93.26%
Target Compounds						
16) Acetone	3.782	43	6338	7.38	ug/l	Qvalue # 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021621\
Data File : VN065878.D
Acq On : 16 Feb 2021 17:23
Operator : JC/MD
Sample : M1413-04
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
EB01-GW-021221

Quant Time: Feb 16 17:44:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
Quant Title : SW846 8260
QLast Update : Mon Feb 15 10:57:01 2021
Response via : Initial Calibration




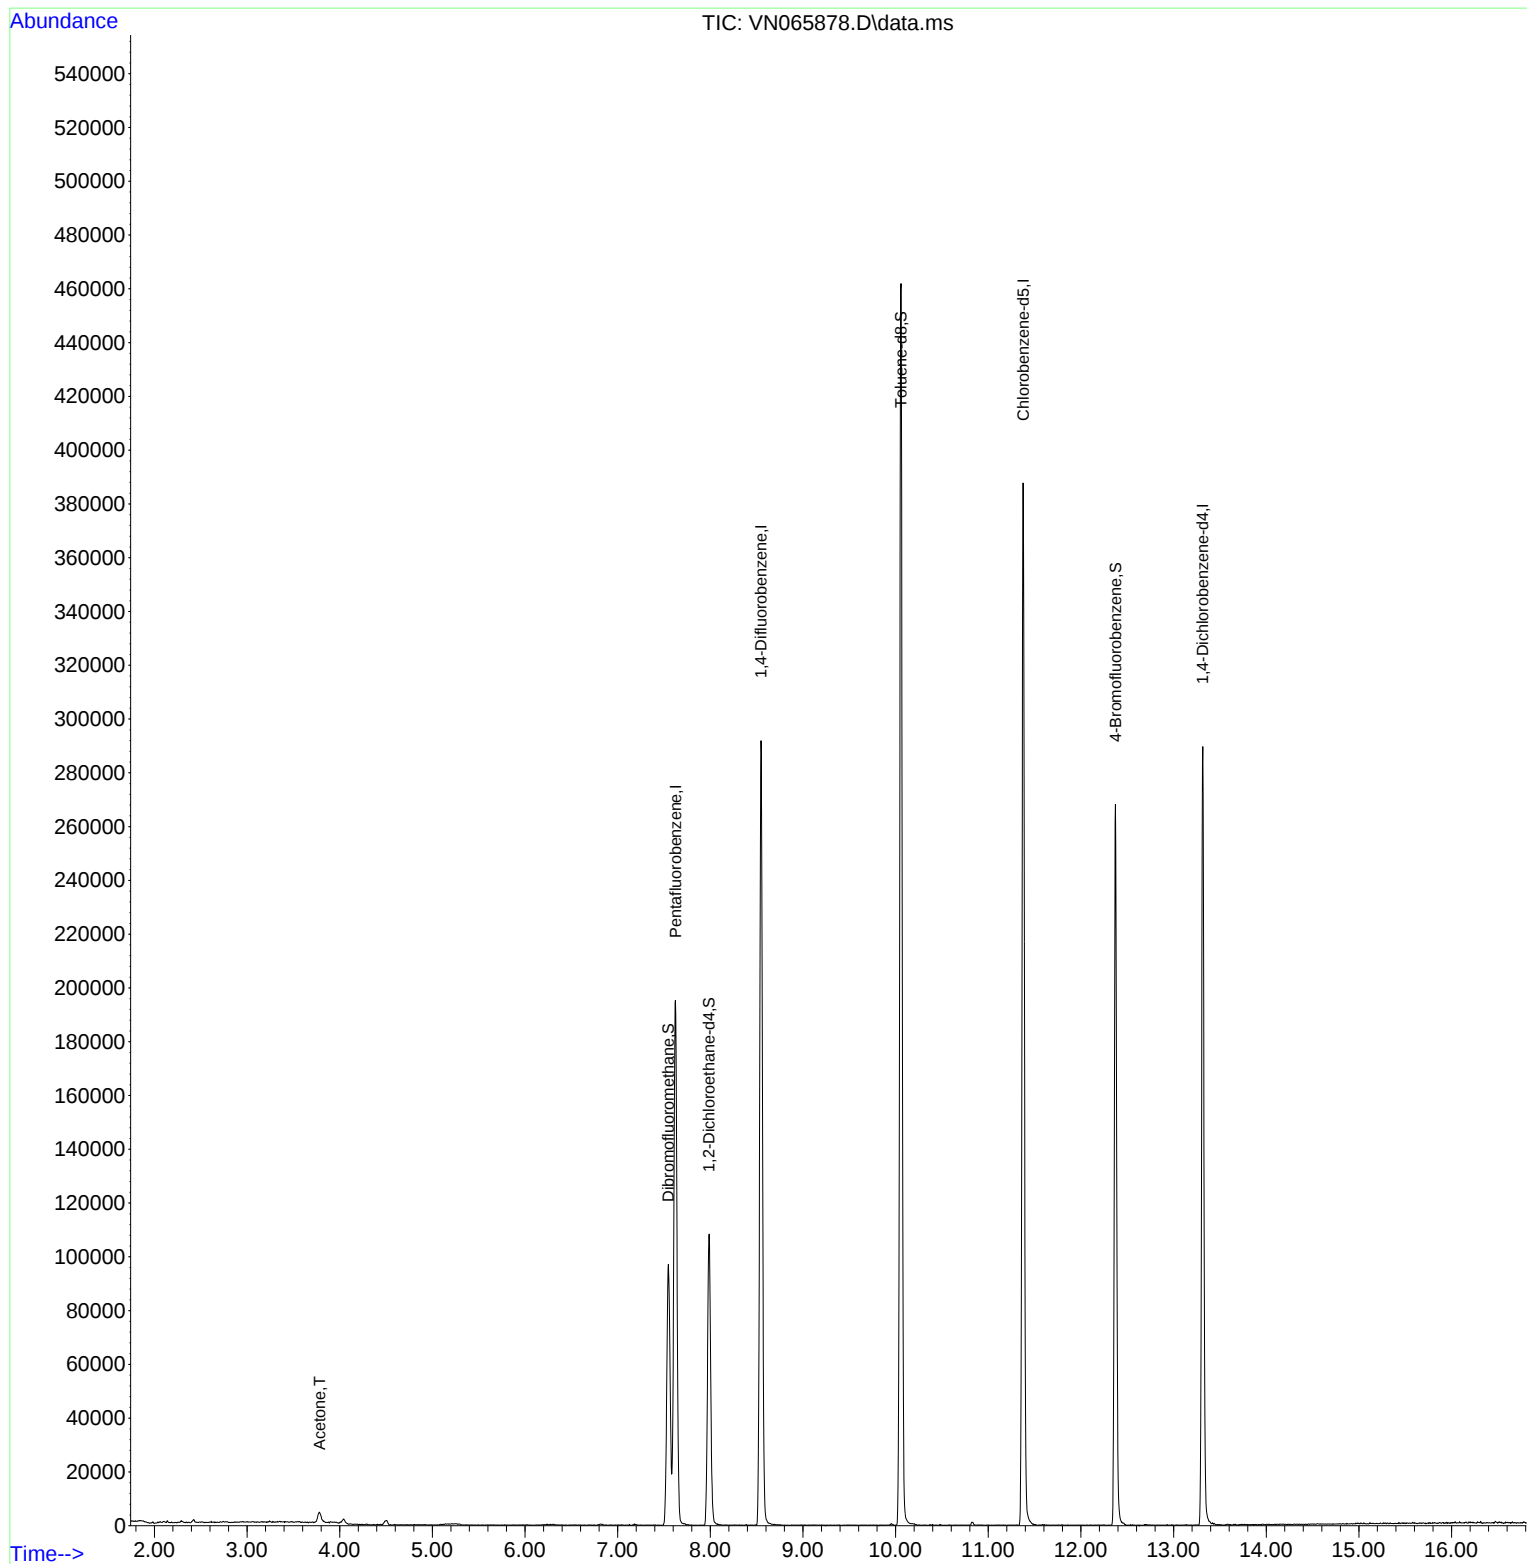


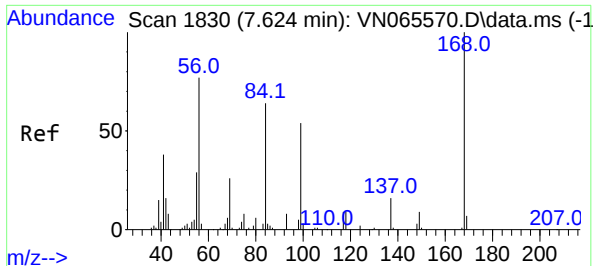

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.624 min Scan# 1830
Delta R.T. -0.000 min
Lab File: VN065878.D
Acq: 16 Feb 2021 17:23




Instrument :
MSVOA_N
ClientSampleId :
EB01-GW-021221


Tgt Ion:168 Resp: 167758
Ion Ratio Lower Upper
168 100
99 55.5 42.6 63.8

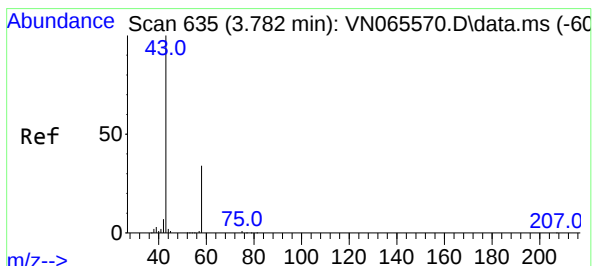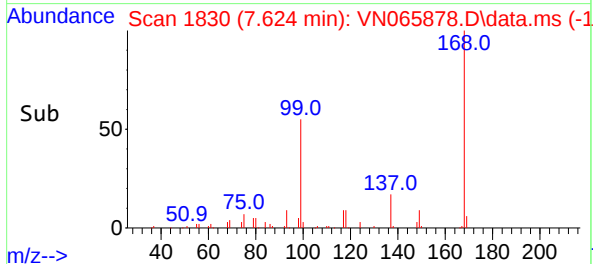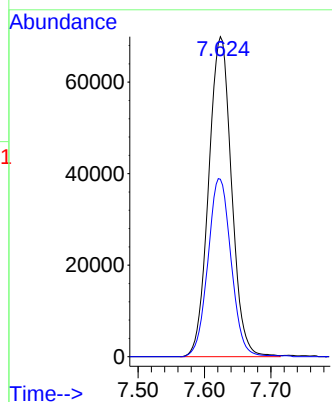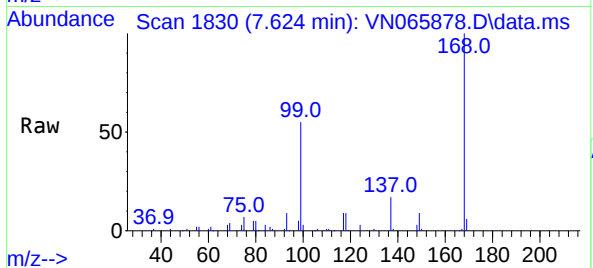

#16
Acetone
Concen: 7.38 ug/l
RT: 3.782 min Scan# 635
Delta R.T. -0.000 min
Lab File: VN065878.D
Acq: 16 Feb 2021 17:23

Tgt Ion: 43 Resp: 6338
Ion Ratio Lower Upper
43 100
58 41.6 27.0 40.6#


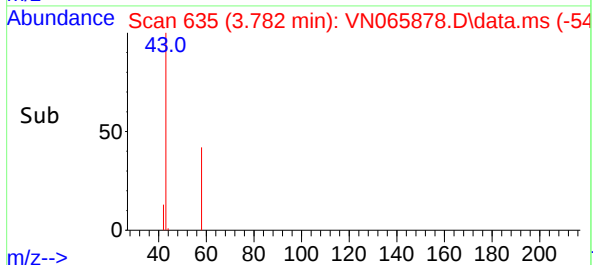
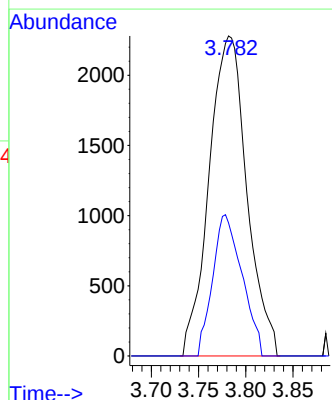
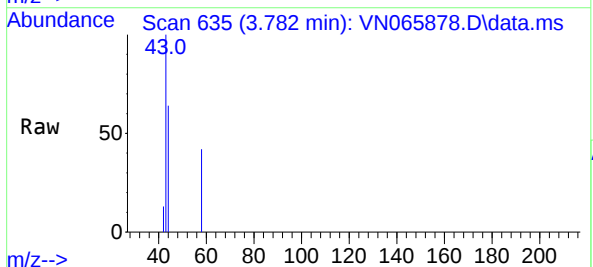


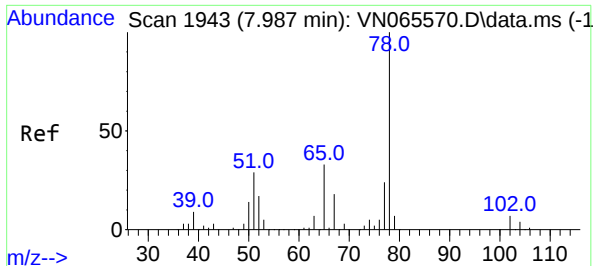

#33
1,2-Dichloroethane-d4
Concen: 41.96 ug/l
RT: 7.987 min Scan# 1943
Delta R.T. 0.000 min
Lab File: VN065878.D
Acq: 16 Feb 2021 17:23




Instrument :
MSVOA_N
ClientSampleId :
EB01-GW-021221


Tgt Ion: 65 Resp: 92609
Ion Ratio Lower Upper
65 100
67 55.7 0.0 107.2

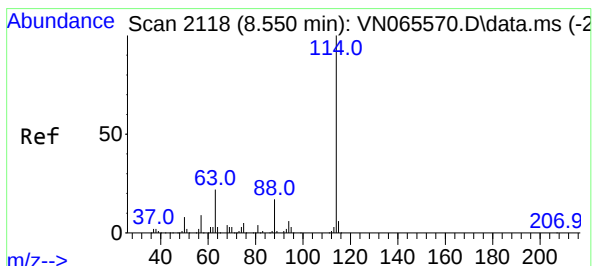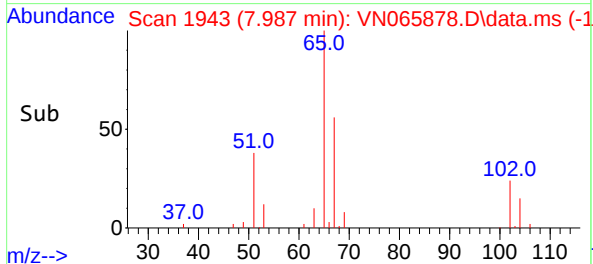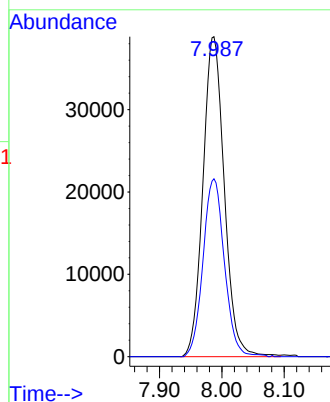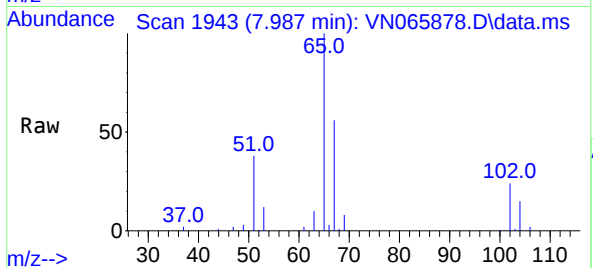

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.547 min Scan# 2117
Delta R.T. -0.003 min
Lab File: VN065878.D
Acq: 16 Feb 2021 17:23

Tgt Ion: 114 Resp: 282044
Ion Ratio Lower Upper
114 100
63 19.5 0.0 38.6
88 16.5 0.0 30.6


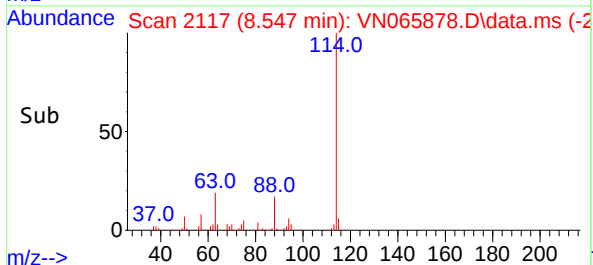
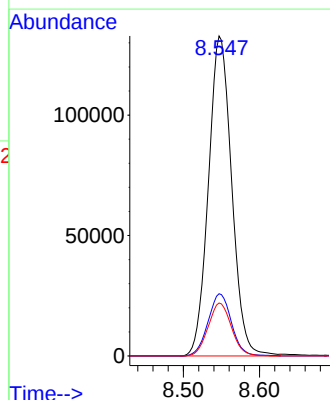
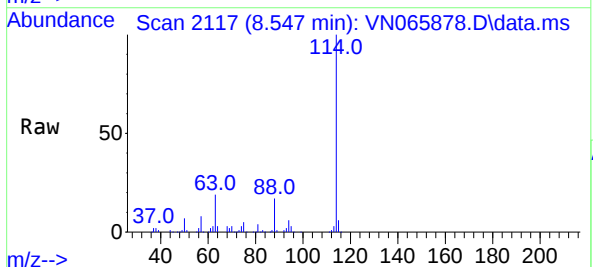


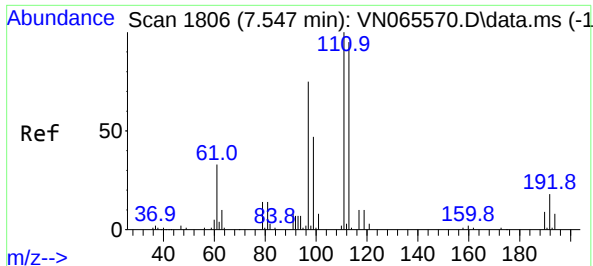

#35
Dibromofluoromethane
Concen: 48.42 ug/l
RT: 7.547 min Scan# 1806
Delta R.T. -0.000 min
Lab File: VN065878.D
Acq: 16 Feb 2021 17:23




Instrument :
MSVOA_N
ClientSampleId :
EB01-GW-021221


Tgt Ion:113 Resp: 80933
Ion Ratio Lower Upper
113 100
111 102.8 82.2 123.2
192 18.1 15.4 23.0

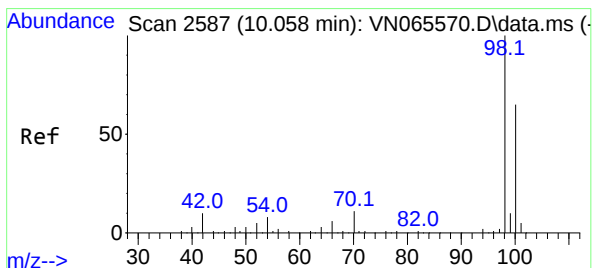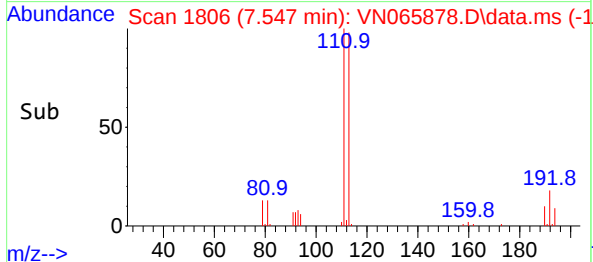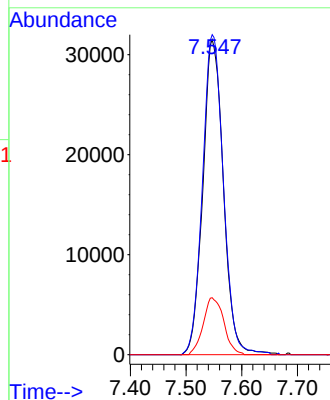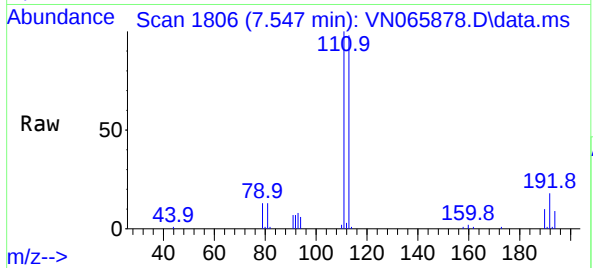

#50
Toluene-d8
Concen: 52.95 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. -0.000 min
Lab File: VN065878.D
Acq: 16 Feb 2021 17:23

Tgt Ion: 98 Resp: 347871
Ion Ratio Lower Upper
98 100
100 64.6 50.5 75.7


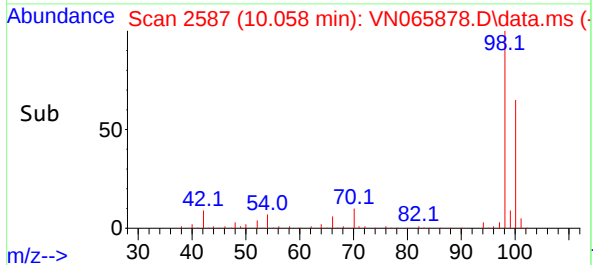
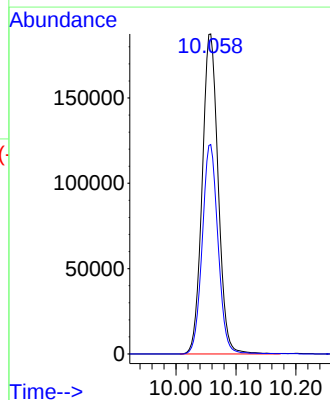
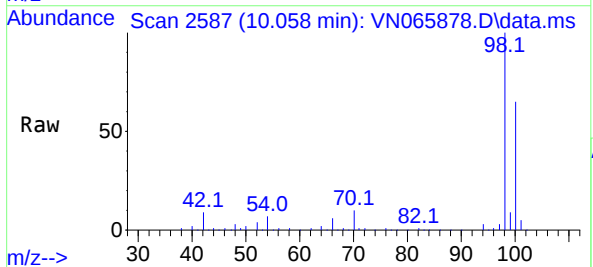


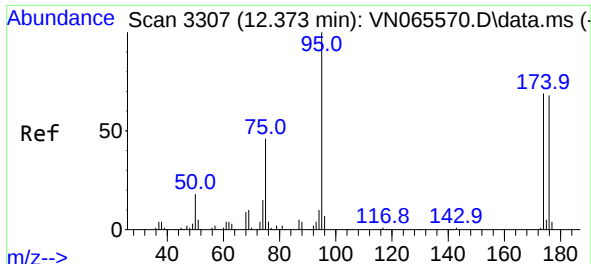

#62
4-Bromofluorobenzene
Concen: 46.63 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. -0.000 min
Lab File: VN065878.D
Acq: 16 Feb 2021 17:23




Instrument :
MSVOA_N
ClientSampleId :
EB01-GW-021221


Tgt Ion: 95 Resp: 110317
Ion Ratio Lower Upper
95 100
174 72.3 0.0 169.0
176 69.6 0.0 162.4

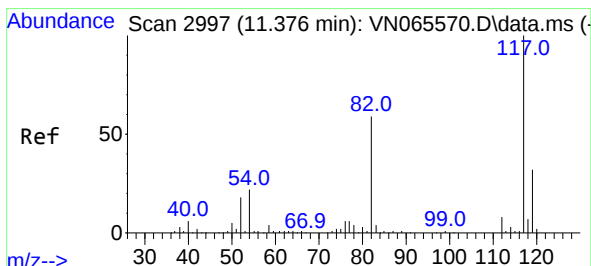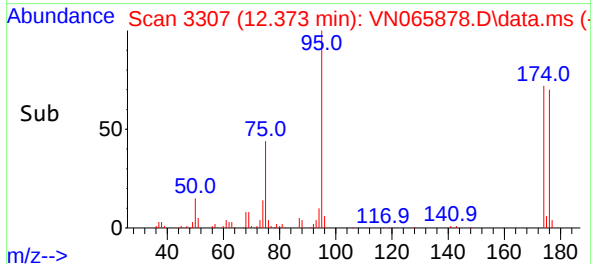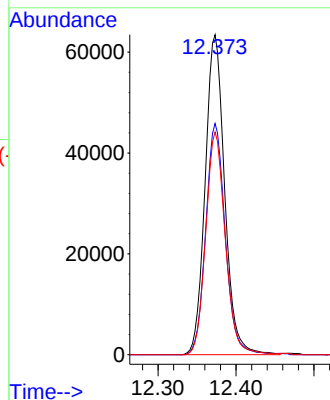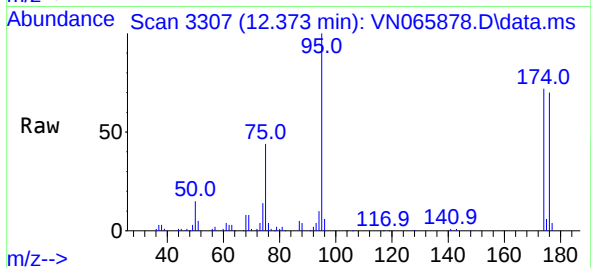

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN065878.D
Acq: 16 Feb 2021 17:23


Tgt Ion: 117 Resp: 246767
Ion Ratio Lower Upper
117 100
82 55.9 43.7 65.5
119 31.3 26.1 39.1

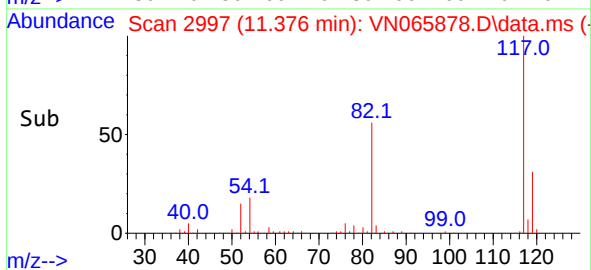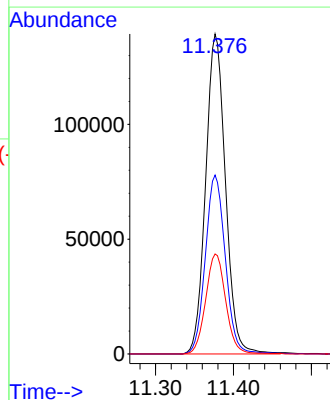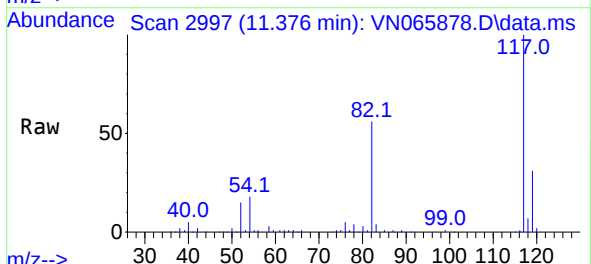

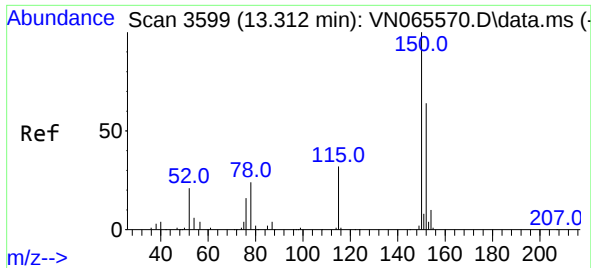

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 13.315 min Scan# 3600
 Delta R.T. 0.003 min
 Lab File: VN065878.D
 Acq: 16 Feb 2021 17:23

Instrument :
 MSVOA_N
 ClientSampleId :
 EB01-GW-021221

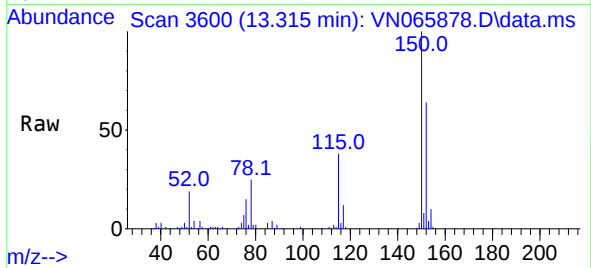

Tgt Ion:152 Resp: 87193

Ion	Ratio	Lower	Upper
152	100		
115	61.5	28.5	85.6
150	158.6	0.0	347.6

