

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021621\
 Data File : VN065884.D
 Acq On : 16 Feb 2021 19:46
 Operator : JC/MD
 Sample : M1417-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BP-TT-VPB-RW6-TB-20210211

Quant Time: Feb 17 00:14:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 15 10:57:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.621	168	148812	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.547	114	247878	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	220540	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.315	152	77246	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.987	65	80371	41.05	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	82.10%
35) Dibromofluoromethane	7.547	113	71513	48.68	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	97.36%
50) Toluene-d8	10.058	98	308574	53.44	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	106.88%
62) 4-Bromofluorobenzene	12.373	95	96608	46.46	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	92.92%


Target Compounds	Qvalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021621\
Data File : VN065884.D
Acq On : 16 Feb 2021 19:46
Operator : JC/MD
Sample : M1417-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BP-TT-VPB-RW6-TB-20210211

Quant Time: Feb 17 00:14:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
Quant Title : SW846 8260
QLast Update : Mon Feb 15 10:57:01 2021
Response via : Initial Calibration




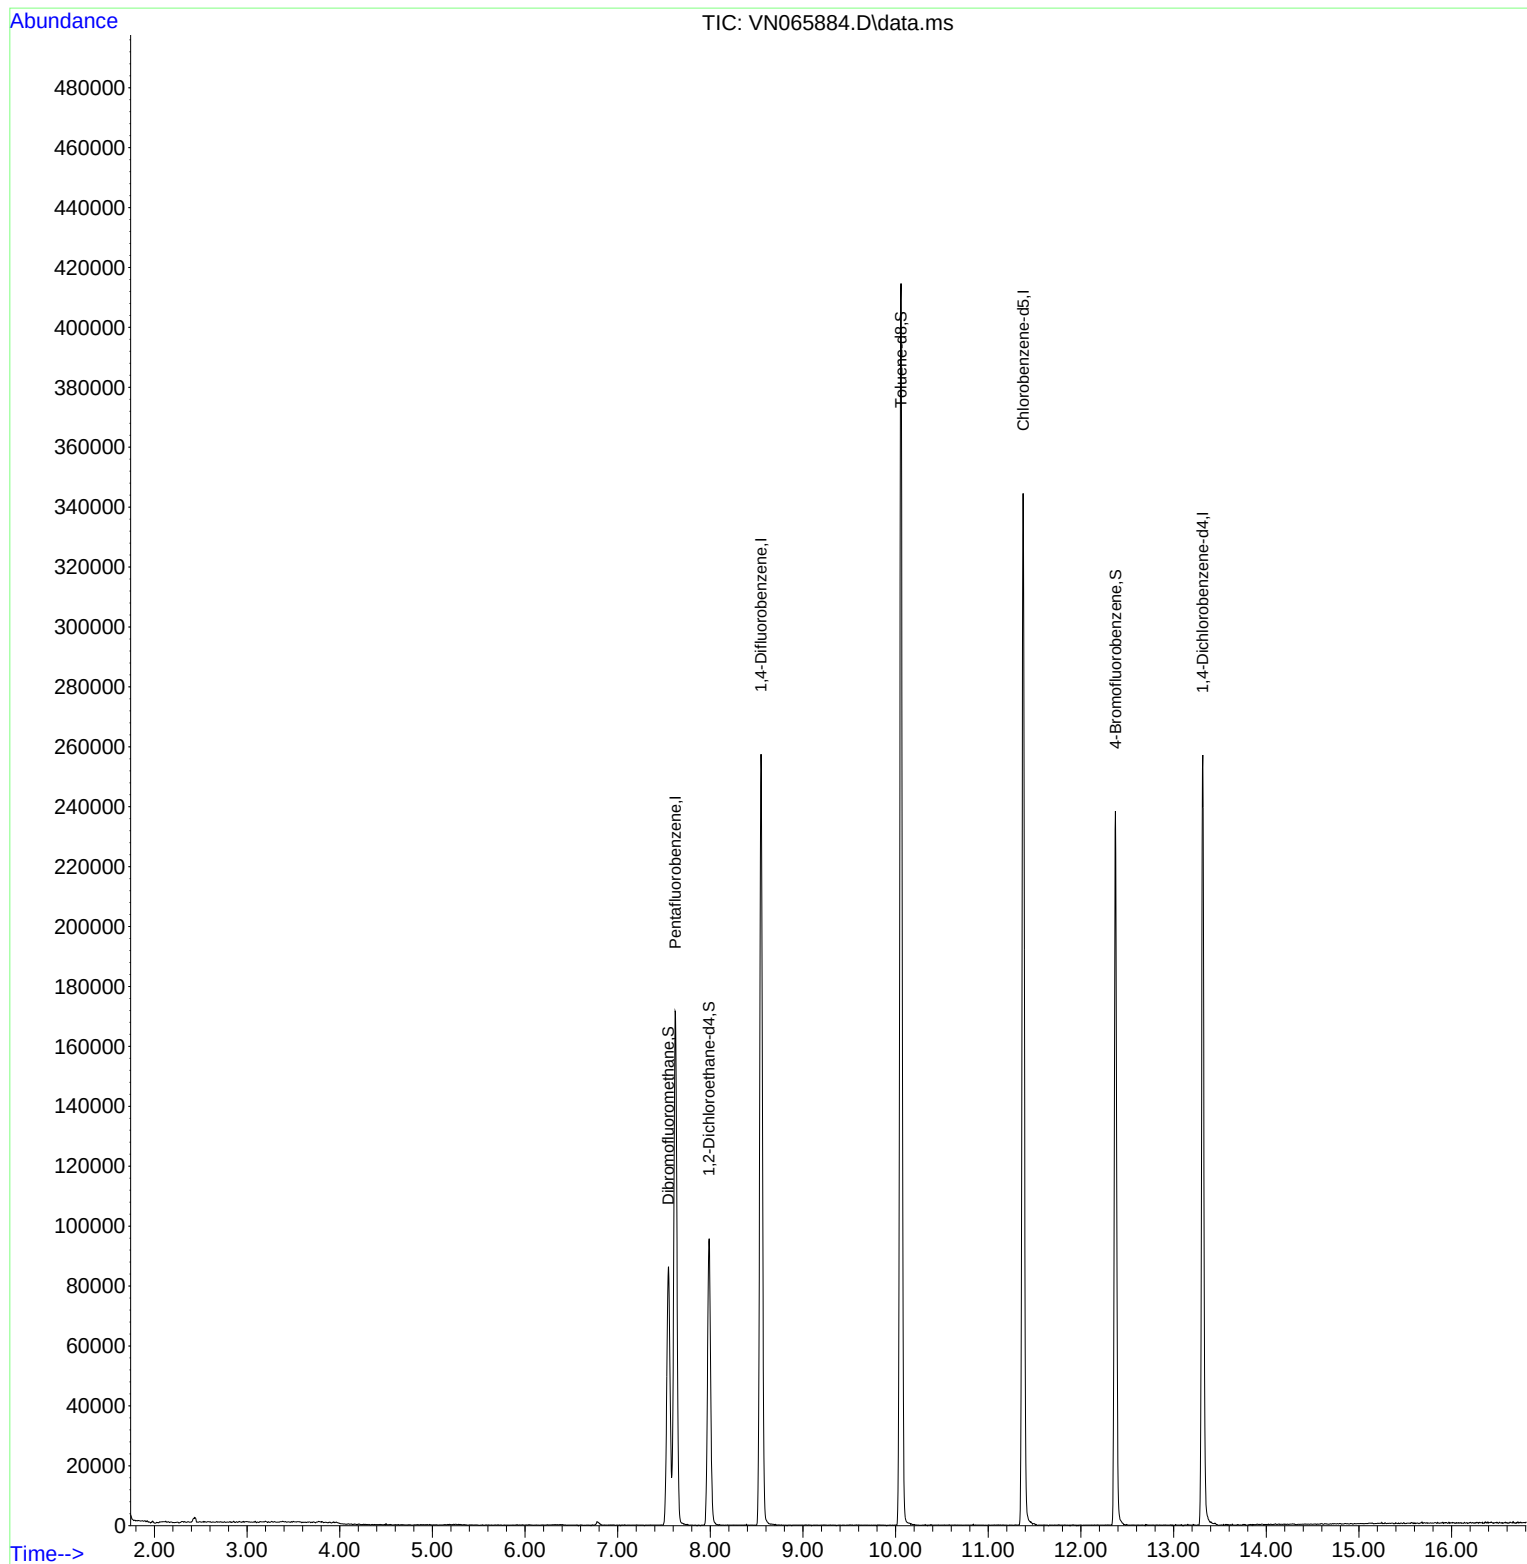


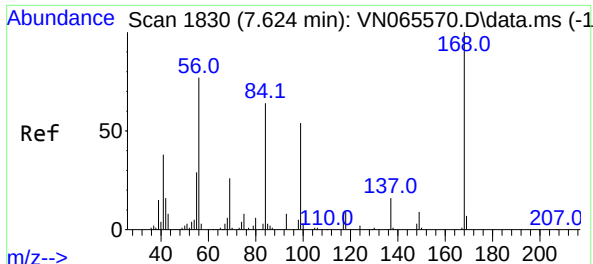

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.621 min Scan# 1829
Delta R.T. -0.003 min
Lab File: VN065884.D
Acq: 16 Feb 2021 19:46




Instrument :
MSVOA_N
ClientSampleId :
BP-TT-VPB-RW6-TB-20210211


Tgt Ion:168 Resp: 148812
Ion Ratio Lower Upper
168 100
99 53.6 42.6 63.8

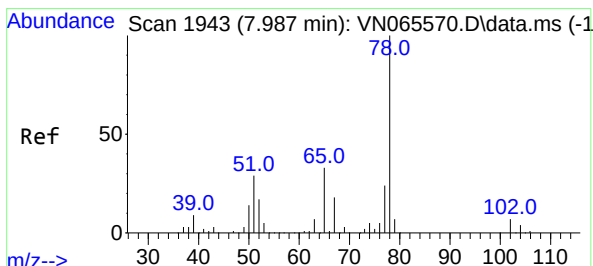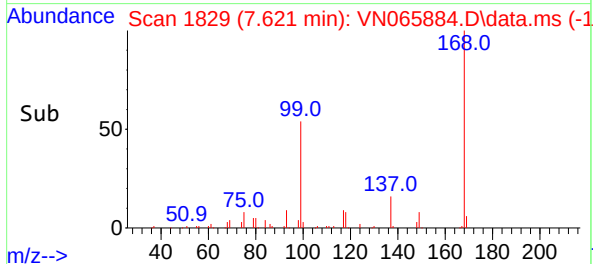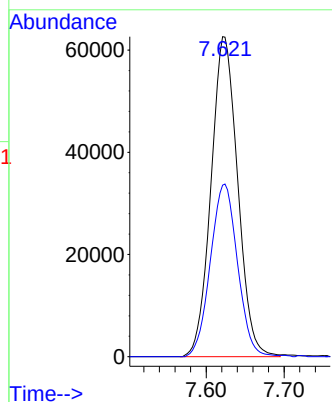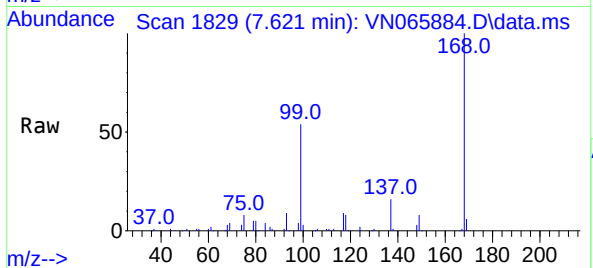

#33
1,2-Dichloroethane-d4
Concen: 41.05 ug/l
RT: 7.987 min Scan# 1943
Delta R.T. 0.000 min
Lab File: VN065884.D
Acq: 16 Feb 2021 19:46

Tgt Ion: 65 Resp: 80371
Ion Ratio Lower Upper
65 100
67 56.2 0.0 107.2

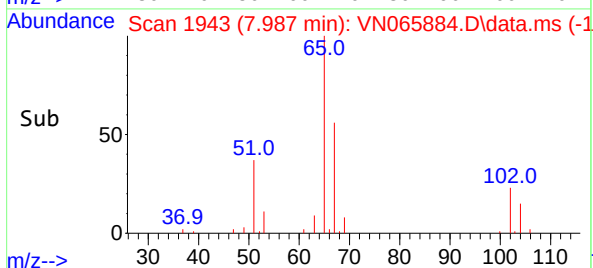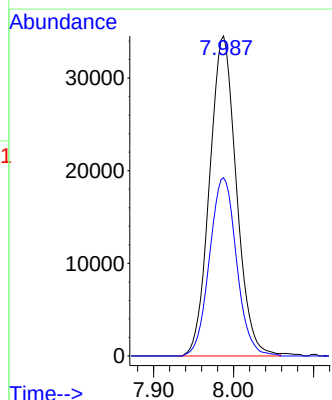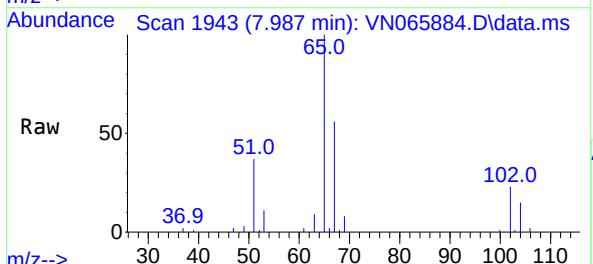




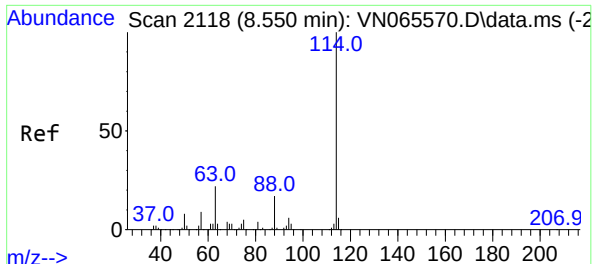


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.547 min Scan# 2117
Delta R.T. -0.003 min
Lab File: VN065884.D
Acq: 16 Feb 2021 19:46

Instrument :
MSVOA_N
ClientSampleId :
BP-TT-VPB-RW6-TB-20210211




Tgt Ion:114 Resp: 247878
Ion Ratio Lower Upper
114 100
63 19.1 0.0 38.6
88 16.2 0.0 30.6

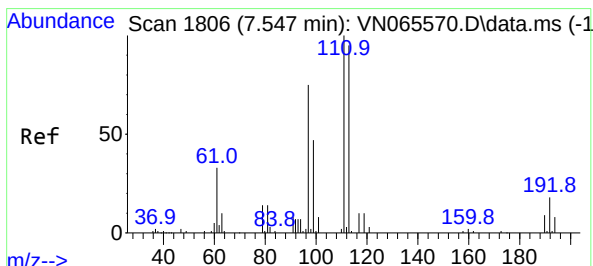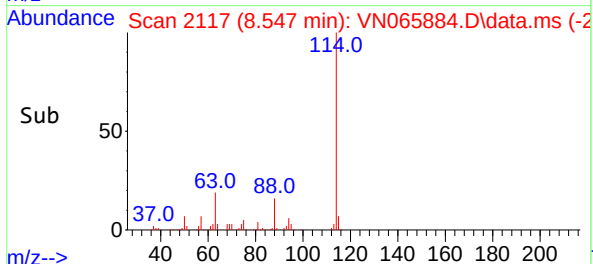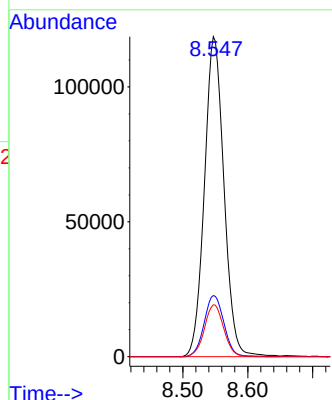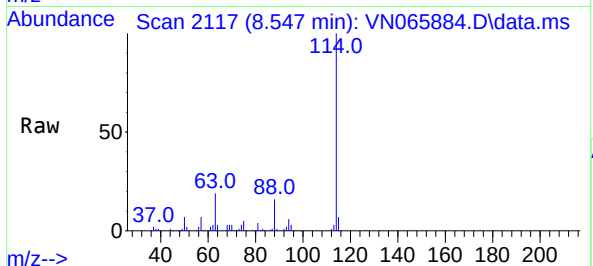


#35

Dibromofluoromethane
Concen: 48.68 ug/l
RT: 7.547 min Scan# 1806
Delta R.T. -0.000 min
Lab File: VN065884.D
Acq: 16 Feb 2021 19:46

Tgt Ion:113 Resp: 71513
Ion Ratio Lower Upper
113 100
111 100.0 82.2 123.2
192 18.1 15.4 23.0


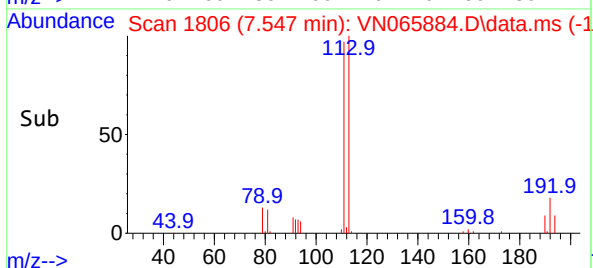
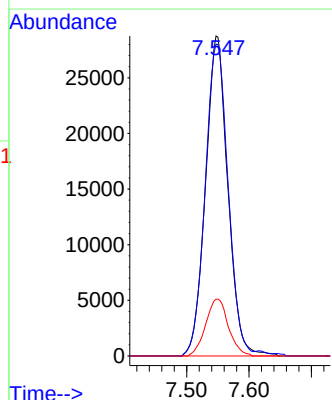
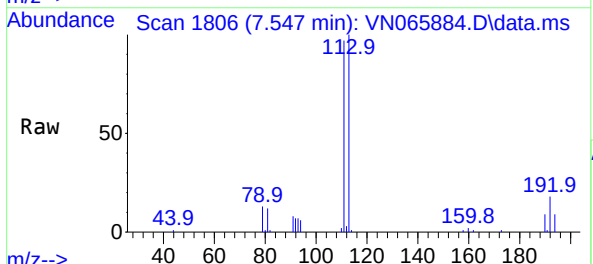


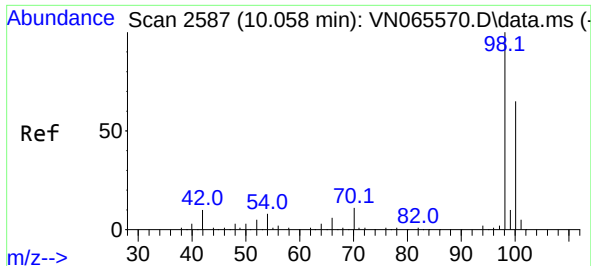

#50
Toluene-d8
Concen: 53.44 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. 0.000 min
Lab File: VN065884.D
Acq: 16 Feb 2021 19:46




Instrument :
MSVOA_N
ClientSampleId :
BP-TT-VPB-RW6-TB-20210211


Tgt Ion: 98 Resp: 308574
Ion Ratio Lower Upper
98 100
100 64.7 50.5 75.7

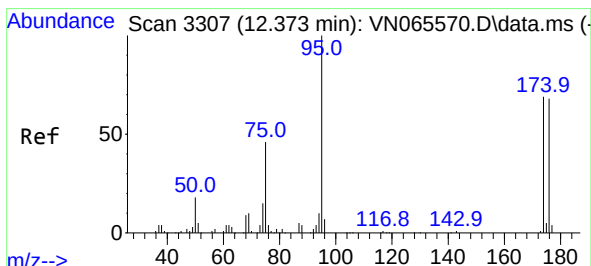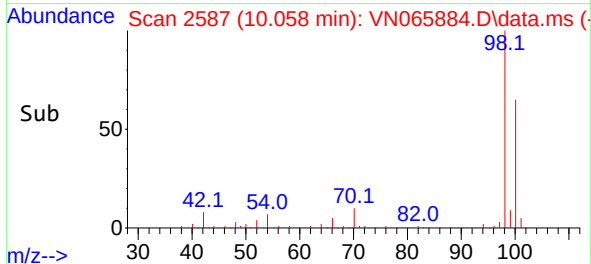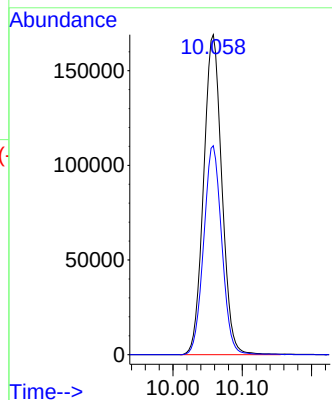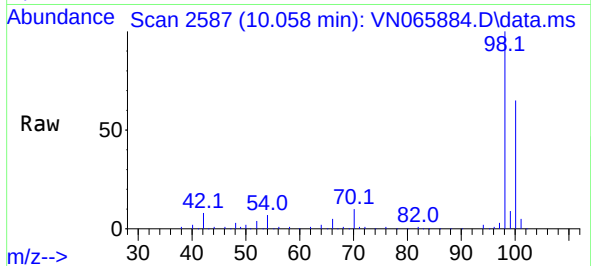

#62
4-Bromofluorobenzene
Concen: 46.46 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.000 min
Lab File: VN065884.D
Acq: 16 Feb 2021 19:46


Tgt Ion: 95 Resp: 96608
Ion Ratio Lower Upper
95 100
174 74.4 0.0 169.0
176 71.4 0.0 162.4

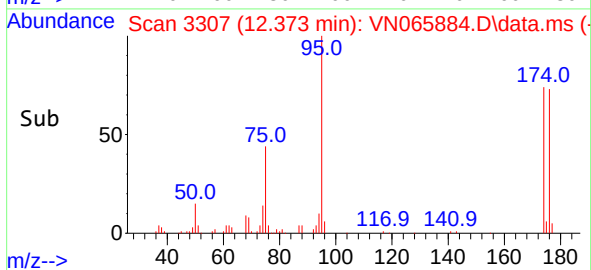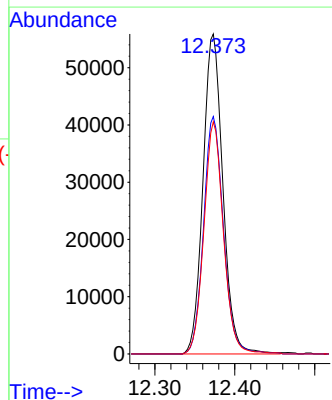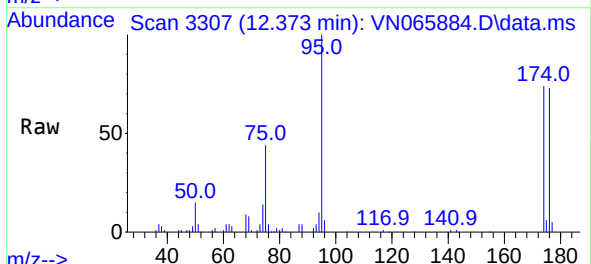



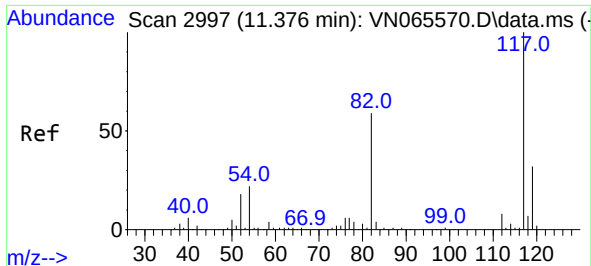


#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN065884.D
Acq: 16 Feb 2021 19:46


Instrument :
MSVOA_N
ClientSampleId :
BP-TT-VPB-RW6-TB-20210211

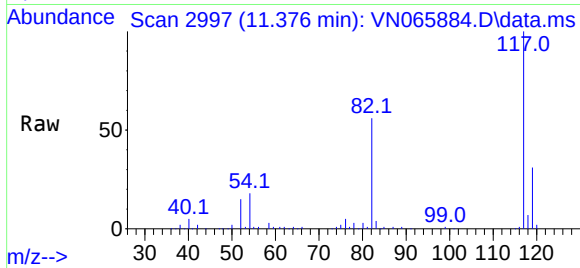

Tgt Ion:117 Resp: 220540
Ion Ratio Lower Upper
117 100
82 55.9 43.7 65.5
119 31.4 26.1 39.1

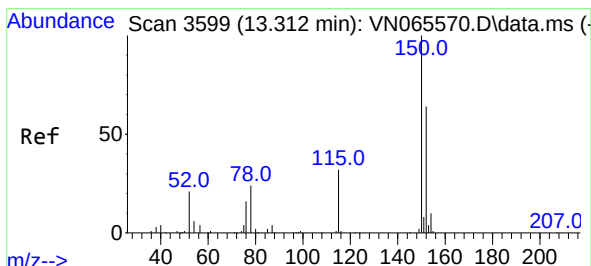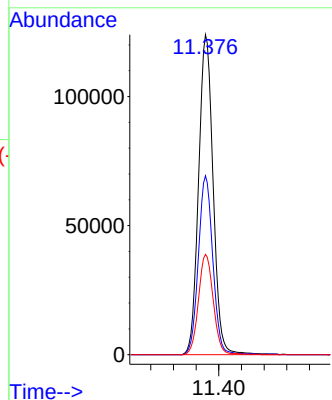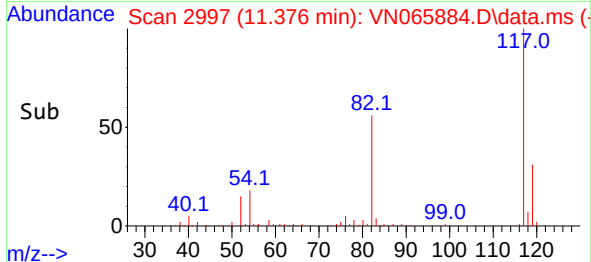

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.315 min Scan# 3600
Delta R.T. 0.003 min
Lab File: VN065884.D
Acq: 16 Feb 2021 19:46

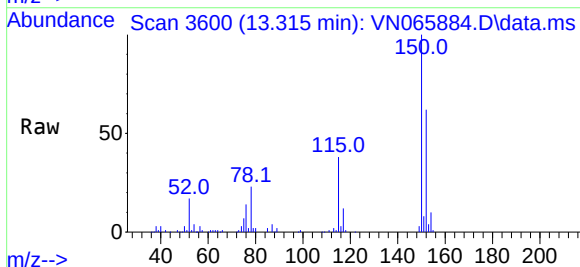

Tgt Ion:152 Resp: 77246
Ion Ratio Lower Upper
152 100
115 61.0 28.5 85.6
150 159.7 0.0 347.6

