


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021621\
Data File : VN065872.D
Acq On : 16 Feb 2021 13:44
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N012521W.M
Title : SW846 8260
Last Update : Mon Feb 15 10:57:01 2021

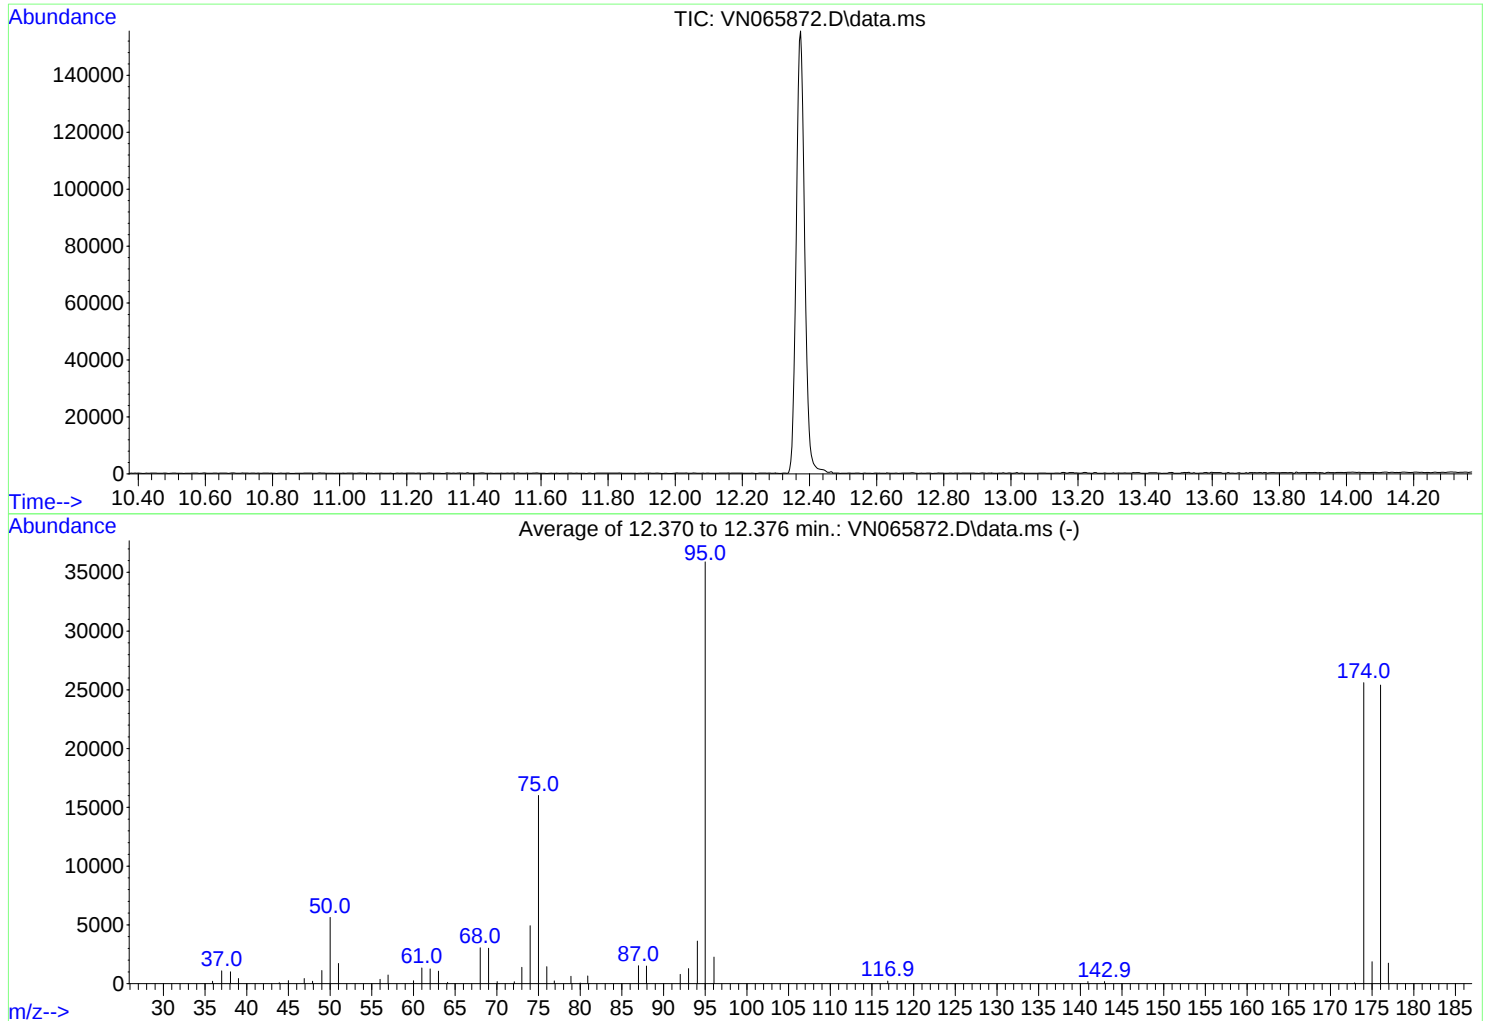

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.7	5636	PASS
75	95	30	60	44.6	16010	PASS
95	95	100	100	100.0	35893	PASS
96	95	5	9	6.3	2257	PASS
173	174	0.00	2	0.3	70	PASS
174	95	50	100	71.4	25611	PASS
175	174	5	9	7.3	1860	PASS
176	174	95	101	99.2	25411	PASS
177	176	5	9	6.9	1742	PASS