

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021622\
 Data File : VN070967.D
 Acq On : 16 Feb 2022 19:06
 Operator : JC\MD
 Sample : N1573-10
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-22R

Quant Time: Feb 17 04:14:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 16 07:52:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.081	168	963409	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1477923	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1321609	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	509602	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	542669	49.310	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	98.620%		
35) Dibromofluoromethane	8.016	113	438810	49.918	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	99.840%		
50) Toluene-d8	10.439	98	1757233	49.776	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	99.560%		
62) 4-Bromofluorobenzene	12.727	95	575335	45.594	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	91.180%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.299	50	3375	0.268	ug/l #	71
5) Bromomethane	2.869	94	1801	0.252	ug/l #	70
11) Tert butyl alcohol	5.381	59	1334	0.665	ug/l #	71
13) Acrolein	4.040	56	578	0.323	ug/l #	14
16) Acetone	4.293	43	86478	14.268	ug/l #	87
18) Methyl Acetate	4.851	43	7898	Below Cal		93
25) 2-Butanone	7.339	43	7350	0.912	ug/l #	81
29) Tetrahydrofuran	7.704	42	1425	0.273	ug/l #	77
31) Cyclohexane	8.081	56	22528	1.184	ug/l #	1
36) 1,1-Dichloropropene	8.081	75	70487	4.894	ug/l #	49
37) Ethyl Acetate	7.416	43	86175	5.579	ug/l	98
38) Carbon Tetrachloride	8.081	117	92293	6.504	ug/l #	16
40) Benzene	8.457	78	38073	0.894	ug/l	99
52) Toluene	10.498	92	161867	6.047	ug/l	95
59) 2-Hexanone	11.086	43	2725	0.267	ug/l	98
67) Ethyl Benzene	11.845	91	104955	2.106	ug/l	97
68) m/p-Xylenes	11.951	106	191199	9.931	ug/l	99
69) o-Xylene	12.274	106	118496	6.300	ug/l	99
70) Styrene	12.280	104	12314	0.412	ug/l #	1
73) Isopropylbenzene	12.568	105	9151	0.223	ug/l	95
74) N-amyl acetate	12.357	43	6705	0.511	ug/l #	50
76) 1,2,3-Trichloropropane	12.727	75	288219	24.021	ug/l #	1
78) n-propylbenzene	12.915	91	16283	0.353	ug/l	99
80) 1,3,5-Trimethylbenzene	13.057	105	40473	1.218	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.727	75	288219	77.839	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.363	105	71975	2.200	ug/l	100
85) sec-Butylbenzene	13.363	105	71975	1.733	ug/l #	56
90) Hexachloroethane	14.215	117	1945	0.319	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.257	180	976	2.099	ug/l #	52
95) Naphthalene	15.504	128	101254	8.990	ug/l	98
96) 1,2,3-Trichlorobenzene	15.698	180	584	2.580	ug/l #	24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021622\
Data File : VN070967.D
Acq On : 16 Feb 2022 19:06
Operator : JC\MD
Sample : N1573-10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-22R

Quant Time: Feb 17 04:14:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 16 07:52:42 2022
Response via : Initial Calibration




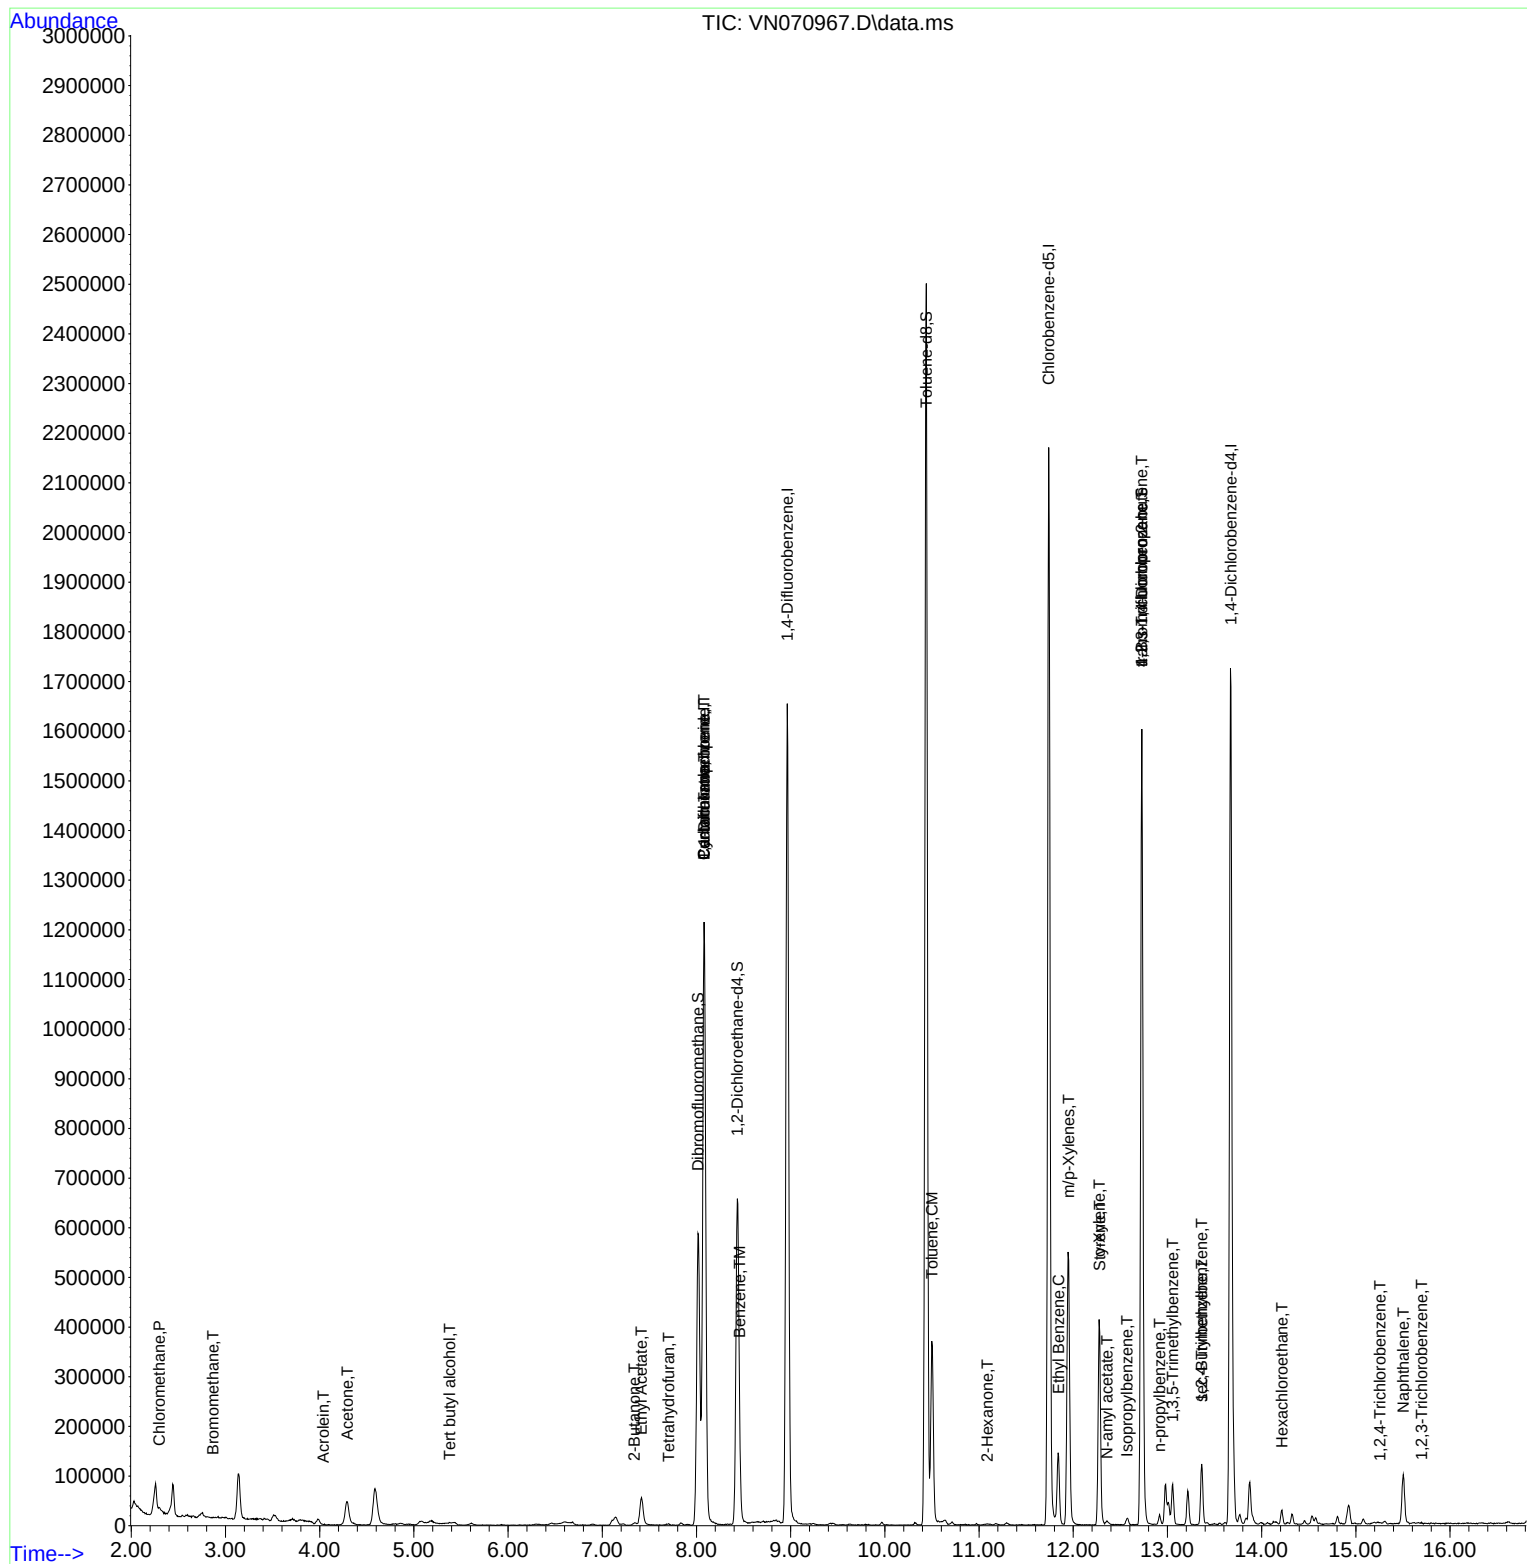




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion:168 Resp: 963409
Ion Ratio Lower Upper
168 100
99 55.7 41.3 61.9

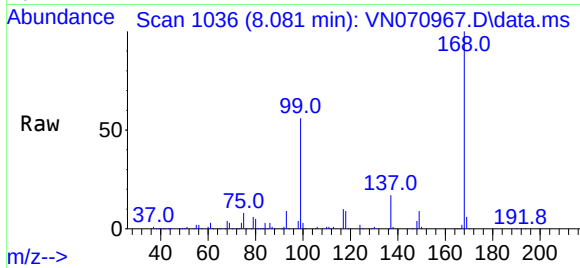

#3
Chloromethane
Concen: 0.268 ug/l
RT: 2.299 min Scan# 53
Delta R.T. -0.000 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion: 50 Resp: 3375
Ion Ratio Lower Upper
50 100
52 15.7 25.4 38.0#


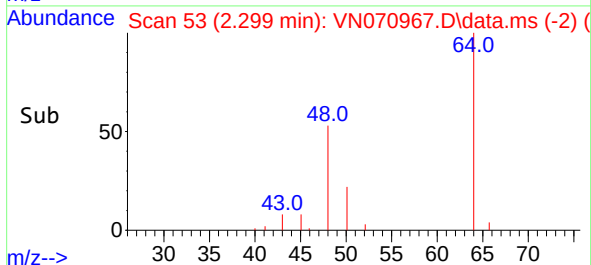
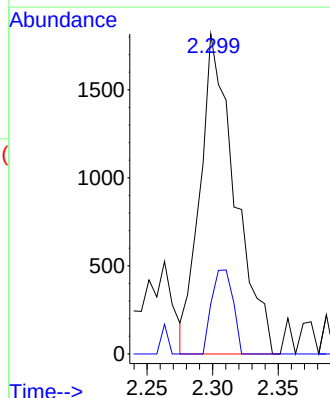
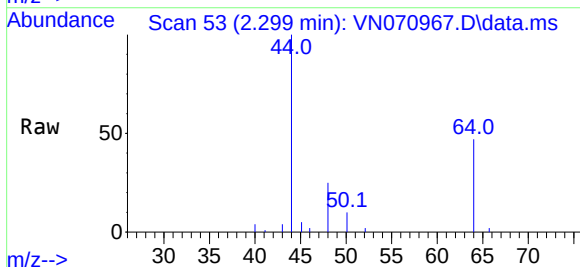




#5
Bromomethane
Concen: 0.252 ug/l
RT: 2.869 min Scan# 11
Delta R.T. 0.012 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion: 94 Resp: 1801
Ion Ratio Lower Upper
94 100
96 63.9 73.8 110.8#



#11
Tert butyl alcohol
Concen: 0.665 ug/l
RT: 5.381 min Scan# 577
Delta R.T. 0.012 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion: 59 Resp: 1334
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#


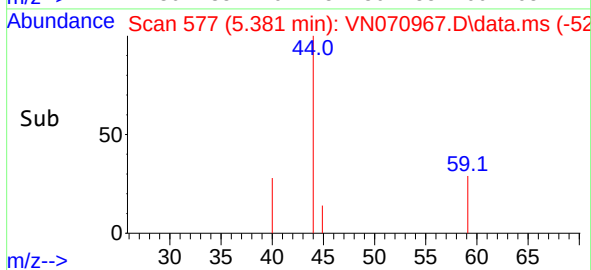






#13
Acrolein
Concen: 0.323 ug/l
RT: 4.040 min Scan# 348
Delta R.T. 0.006 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion: 56 Resp: 578
Ion Ratio Lower Upper
56 100
55 0.0 56.6 85.0#

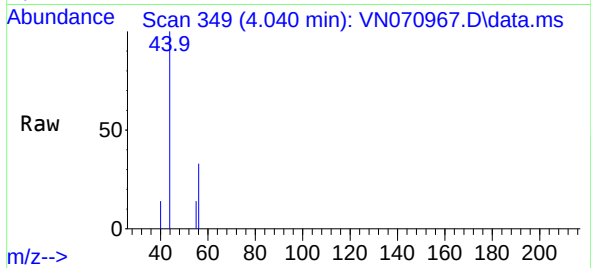

#16
Acetone
Concen: 14.268 ug/l
RT: 4.293 min Scan# 392
Delta R.T. 0.012 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion: 43 Resp: 86478
Ion Ratio Lower Upper
43 100
58 35.8 23.1 34.7#


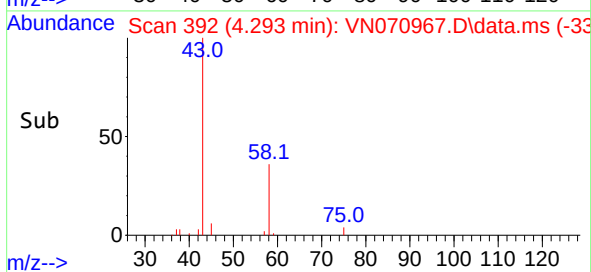






#25
2-Butanone
Concen: 0.912 ug/l
RT: 7.339 min Scan# 910
Delta R.T. 0.012 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion: 43 Resp: 7350
Ion Ratio Lower Upper
43 100
72 17.5 21.7 32.5#



#29
Tetrahydrofuran
Concen: 0.273 ug/l
RT: 7.704 min Scan# 972
Delta R.T. 0.023 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion: 42 Resp: 1425
Ion Ratio Lower Upper
42 100
72 49.1 36.3 54.5
71 17.2 34.7 52.1#


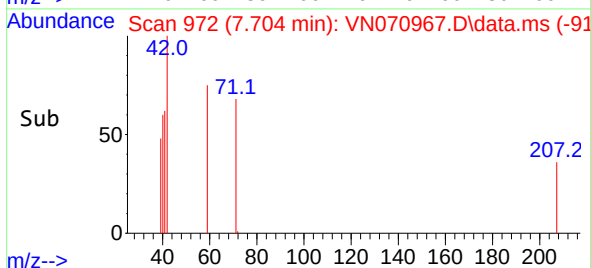
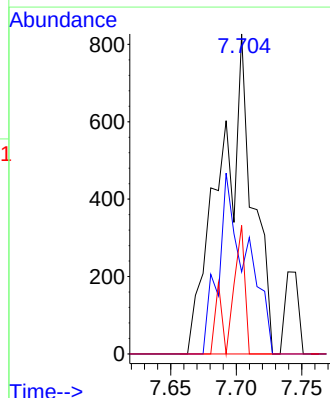



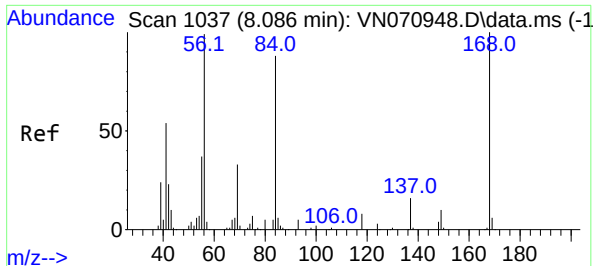

#31
Cyclohexane
Concen: 1.184 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.006 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion: 56 Resp: 22528
Ion Ratio Lower Upper
56 100
69 158.1 27.1 40.7#
84 149.5 73.4 110.0#

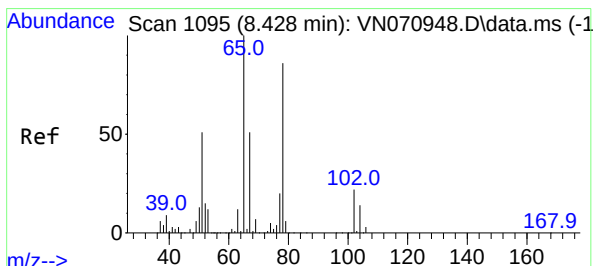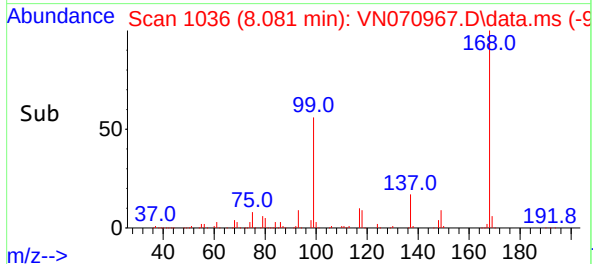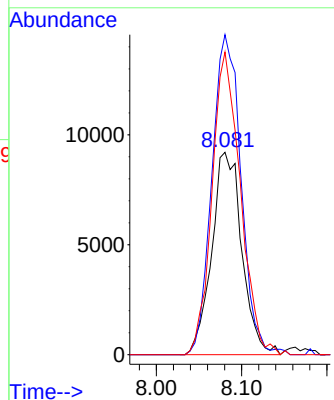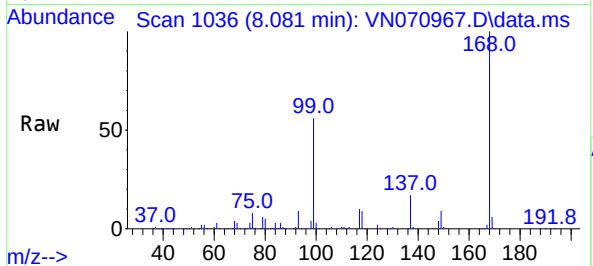

#33
1,2-Dichloroethane-d4
Concen: 49.310 ug/l
RT: 8.433 min Scan# 1096
Delta R.T. 0.006 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion: 65 Resp: 542669
Ion Ratio Lower Upper
65 100
67 52.1 0.0 103.0


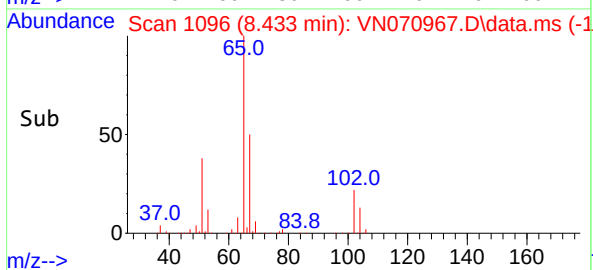
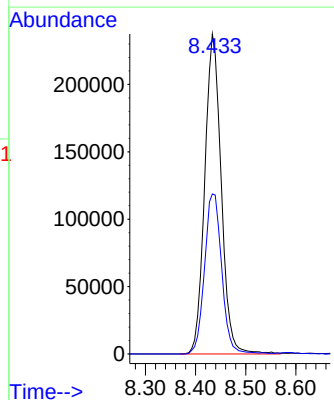
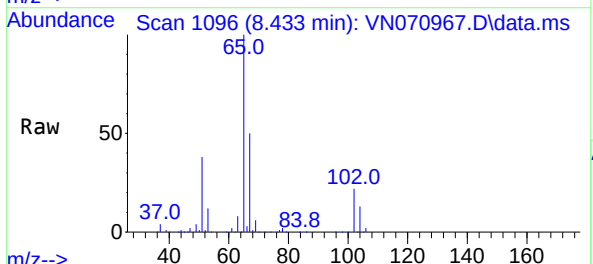


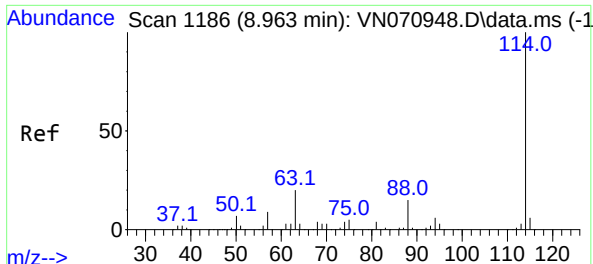

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. -0.000 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion:114 Resp: 1477923
Ion Ratio Lower Upper
114 100
63 21.2 0.0 37.8
88 16.1 0.0 27.4

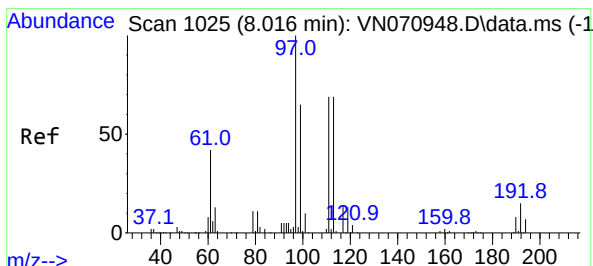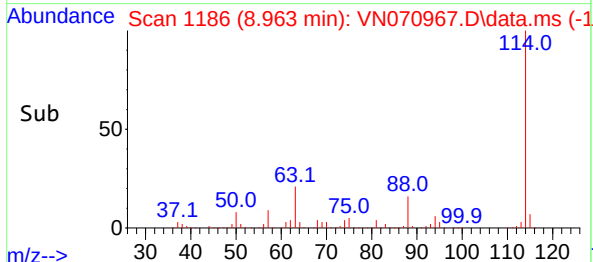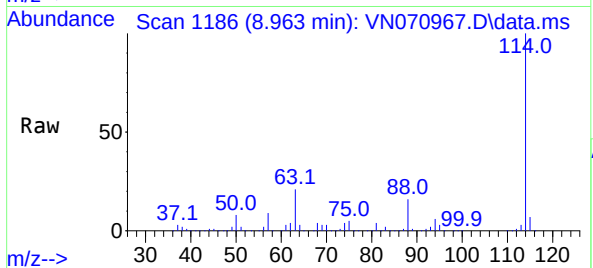

#35
Dibromofluoromethane
Concen: 49.918 ug/l
RT: 8.016 min Scan# 1025
Delta R.T. -0.000 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion:113 Resp: 438810
Ion Ratio Lower Upper
113 100
111 102.0 82.2 123.2
192 21.0 16.9 25.3


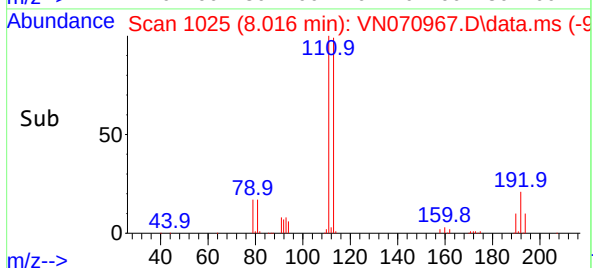

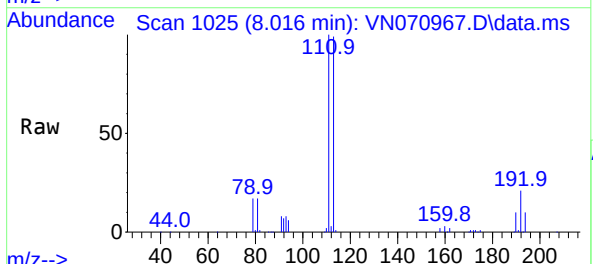


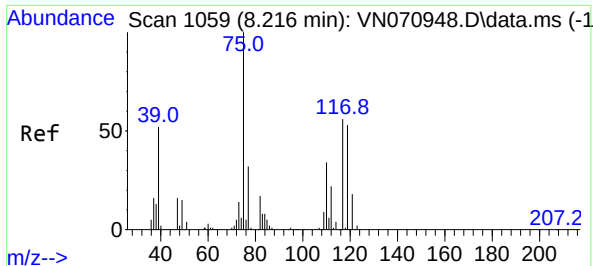

#36
1,1-Dichloropropene
Concen: 4.894 ug/l
RT: 8.081 min Scan# 1059
Delta R.T. -0.135 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion: 75 Resp: 70487
Ion Ratio Lower Upper
75 100
110 9.3 18.4 55.2#
77 0.0 24.4 36.6#

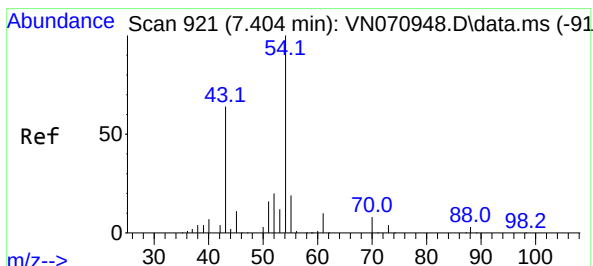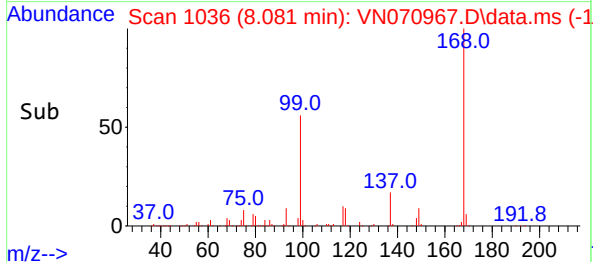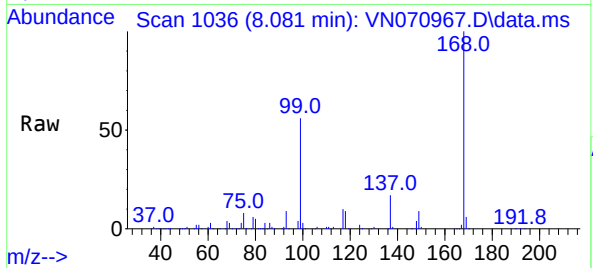

#37
Ethyl Acetate
Concen: 5.579 ug/l
RT: 7.416 min Scan# 923
Delta R.T. 0.012 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion: 43 Resp: 86175
Ion Ratio Lower Upper
43 100
61 14.7 11.5 17.3
70 11.2 7.9 11.9


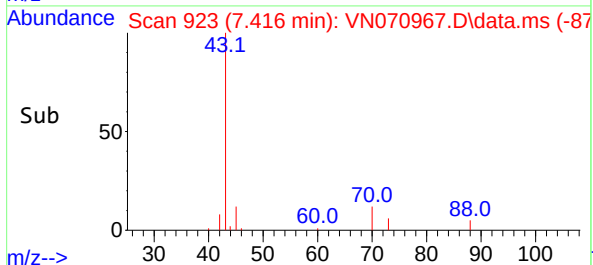
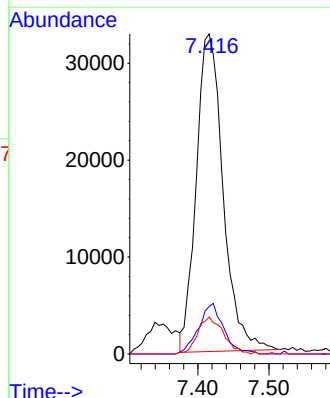
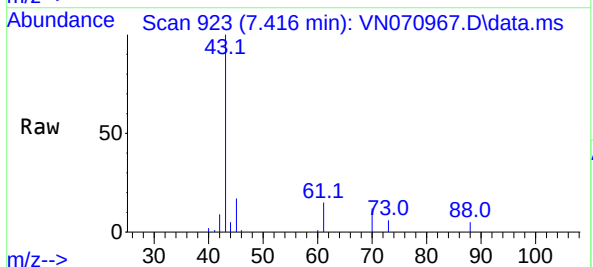


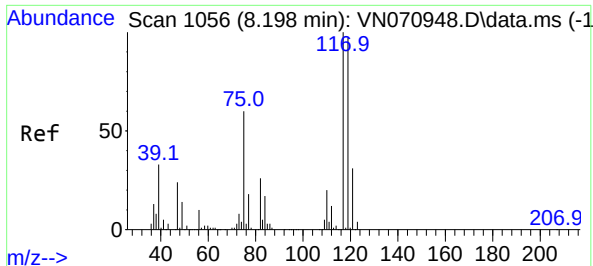

#38
Carbon Tetrachloride
Concen: 6.504 ug/l
RT: 8.081 min Scan# 1100
Delta R.T. -0.118 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion:117 Resp: 92293
Ion Ratio Lower Upper
117 100
119 4.6 76.1 114.1#
121 0.0 24.2 36.2#

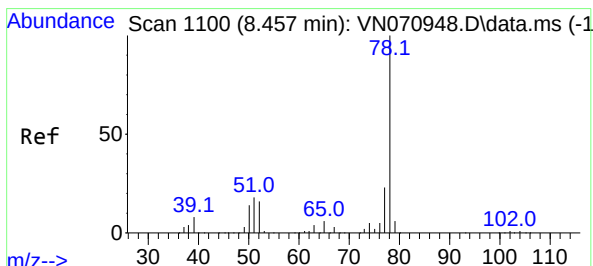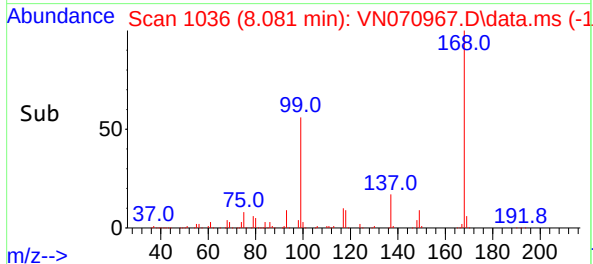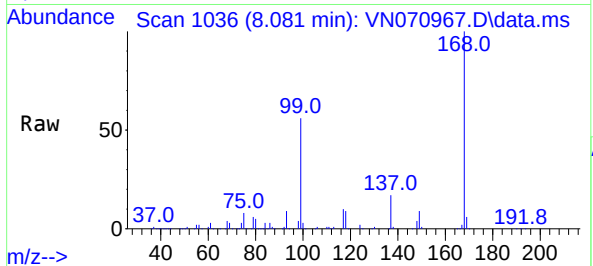

#40
Benzene
Concen: 0.894 ug/l
RT: 8.457 min Scan# 1100
Delta R.T. -0.000 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion: 78 Resp: 38073
Ion Ratio Lower Upper
78 100
77 23.7 18.6 27.8


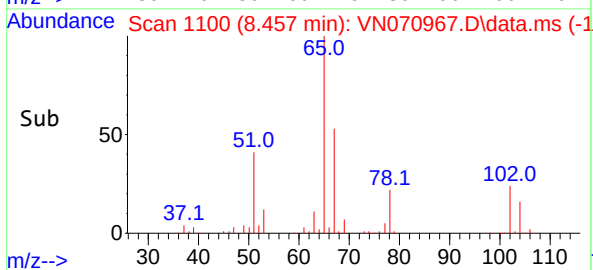

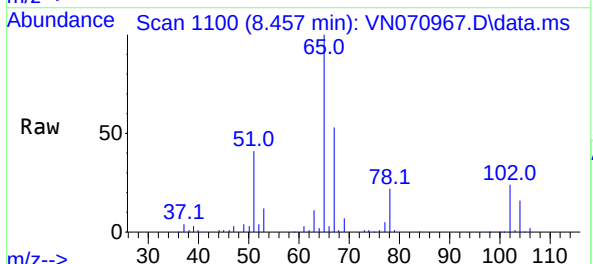




#50
Toluene-d8
Concen: 49.776 ug/l
RT: 10.439 min Scan# 1436
Delta R.T. 0.006 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion: 98 Resp: 1757233
Ion Ratio Lower Upper
98 100
100 65.2 50.4 75.6

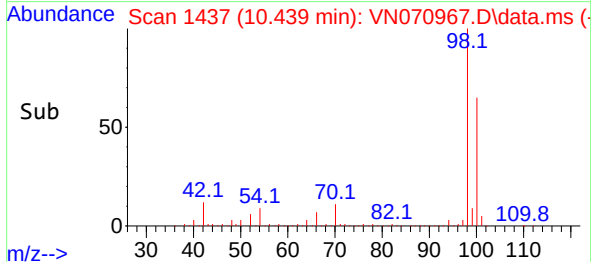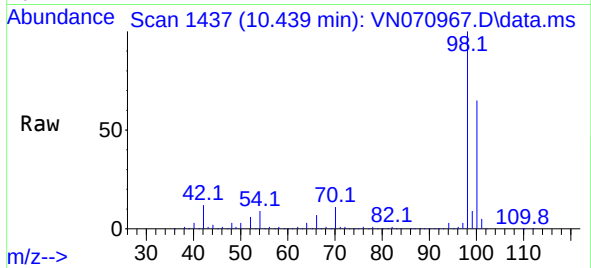

#52
Toluene
Concen: 6.047 ug/l
RT: 10.498 min Scan# 1447
Delta R.T. -0.000 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion: 92 Resp: 161867
Ion Ratio Lower Upper
92 100
91 170.2 142.0 213.0


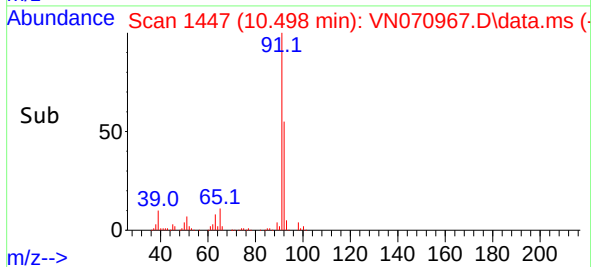

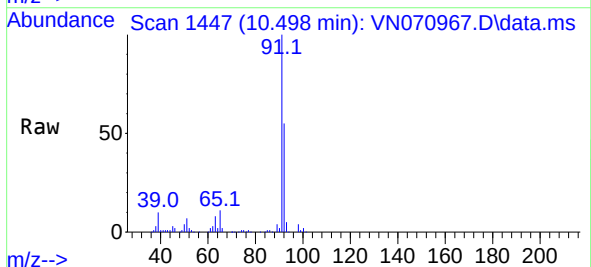




#59
2-Hexanone
Concen: 0.267 ug/l
RT: 11.086 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion: 43 Resp: 2725
Ion Ratio Lower Upper
43 100
58 52.2 26.9 80.7



#62
4-Bromofluorobenzene
Concen: 45.594 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.006 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion: 95 Resp: 575335
Ion Ratio Lower Upper
95 100
174 81.5 0.0 187.2
176 78.8 0.0 181.4


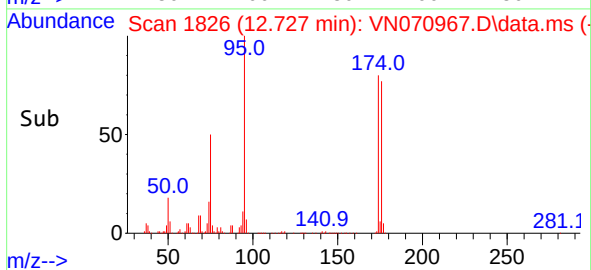






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion:117 Resp: 1321609
Ion Ratio Lower Upper
117 100
82 55.0 42.4 63.6
119 32.2 25.4 38.2

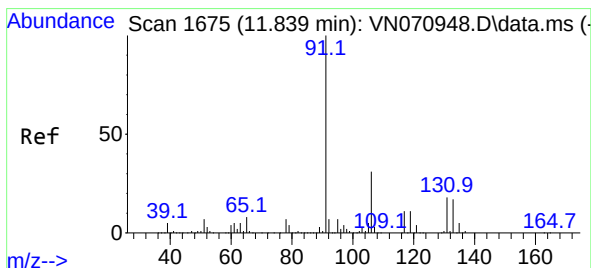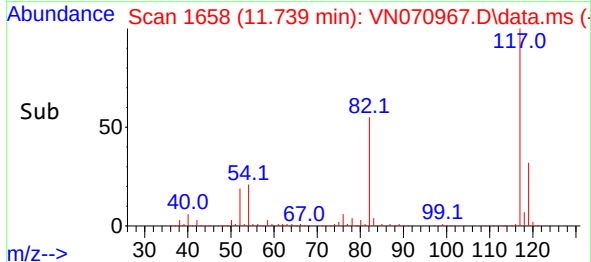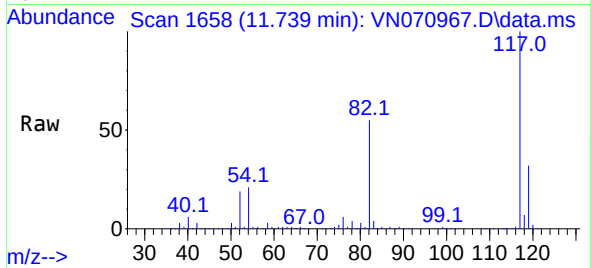

#67
Ethyl Benzene
Concen: 2.106 ug/l
RT: 11.845 min Scan# 1676
Delta R.T. 0.006 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion: 91 Resp: 104955
Ion Ratio Lower Upper
91 100
106 30.6 25.7 38.5


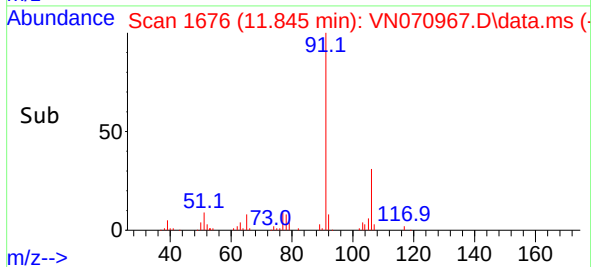

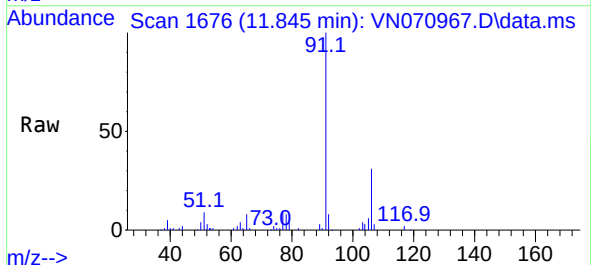




#68
m/p-Xylenes
Concen: 9.931 ug/l
RT: 11.951 min Scan# 1694
Delta R.T. 0.006 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion:106 Resp: 191199
Ion Ratio Lower Upper
106 100
91 202.4 160.6 240.8

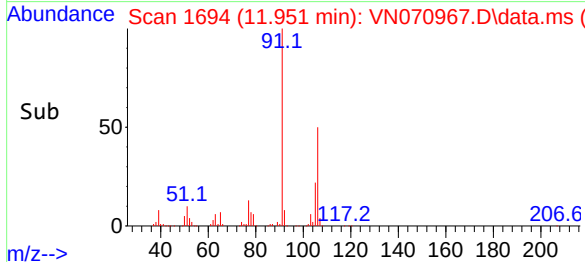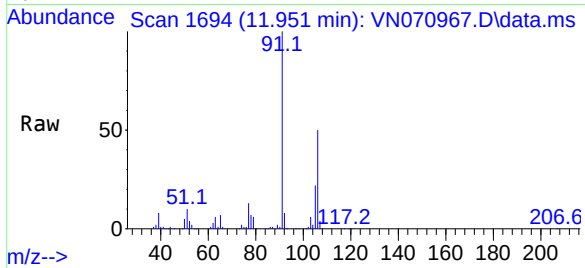

#69
o-Xylene
Concen: 6.300 ug/l
RT: 12.274 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion:106 Resp: 118496
Ion Ratio Lower Upper
106 100
91 210.6 105.8 317.3


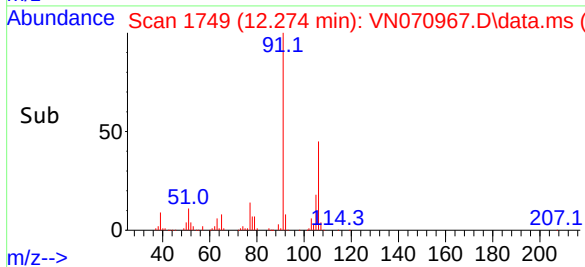

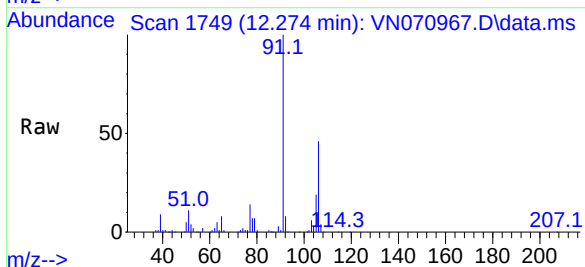




#70
Styrene
Concen: 0.412 ug/l
RT: 12.280 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion:104 Resp: 12314
Ion Ratio Lower Upper
104 100
78 150.4 38.7 58.1#
103 155.4 45.0 67.6#

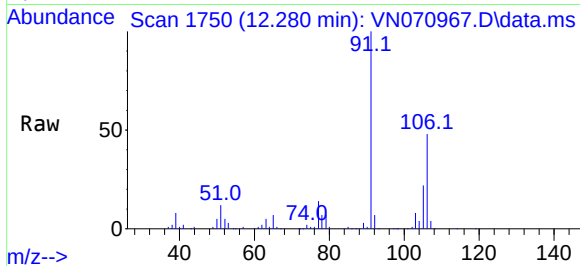

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1987
Delta R.T. 0.006 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion:152 Resp: 509602
Ion Ratio Lower Upper
152 100
115 58.6 27.5 82.5
150 155.6 0.0 344.4


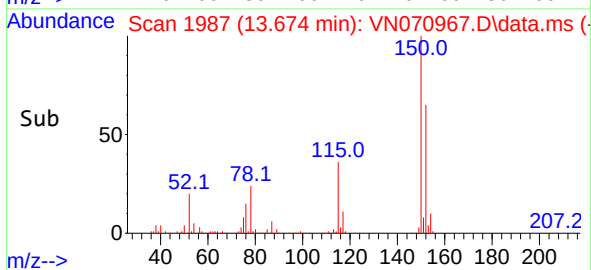

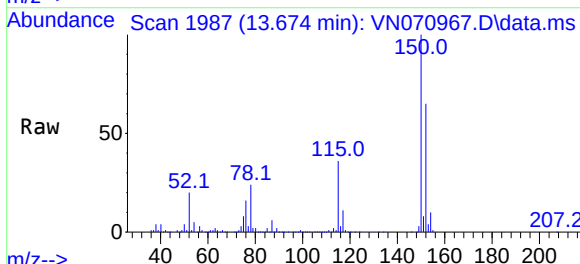




#73
Isopropylbenzene
Concen: 0.223 ug/l
RT: 12.568 min Scan# 1799
Delta R.T. -0.000 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion:105 Resp: 9151
Ion Ratio Lower Upper
105 100
120 29.0 13.4 40.1

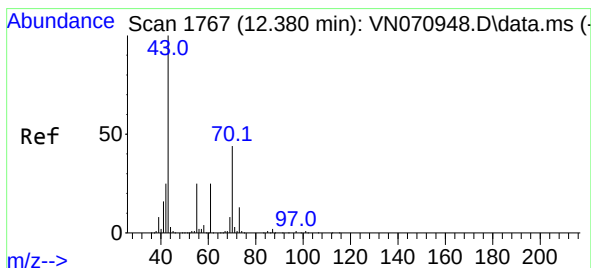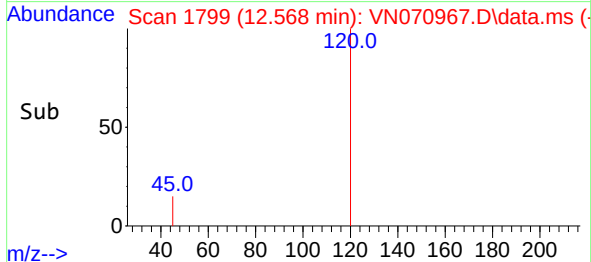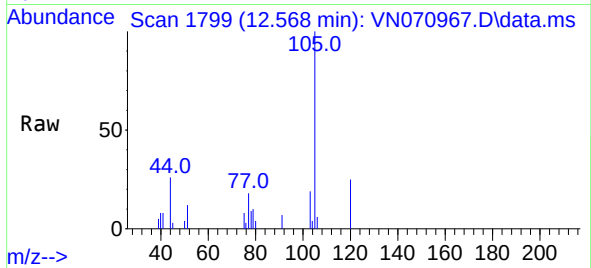

#74
N-ethyl acetate
Concen: 0.511 ug/l
RT: 12.357 min Scan# 1763
Delta R.T. -0.024 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion: 43 Resp: 6705
Ion Ratio Lower Upper
43 100
70 0.9 33.4 50.0#
55 10.2 19.3 28.9#
61 0.0 18.5 27.7#


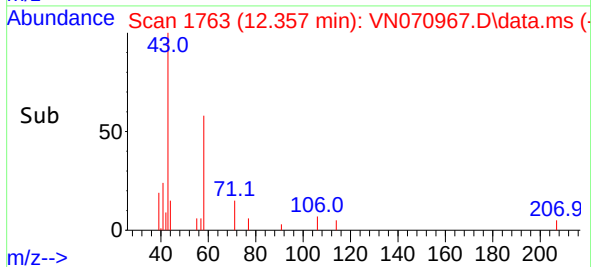

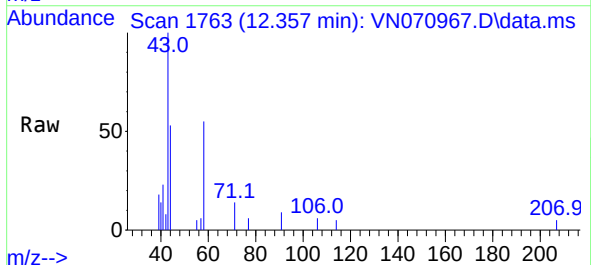




#76
1,2,3-Trichloropropane
Concen: 24.021 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.141 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion: 75 Resp: 288219
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#

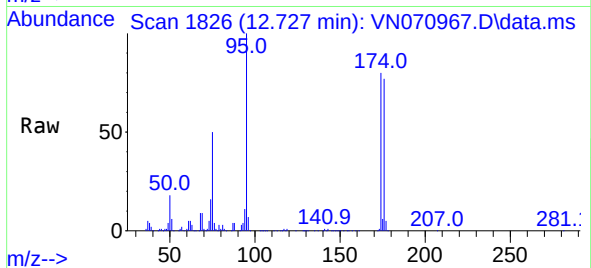

#78
n-propylbenzene
Concen: 0.353 ug/l
RT: 12.915 min Scan# 1858
Delta R.T. -0.000 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion: 91 Resp: 16283
Ion Ratio Lower Upper
91 100
120 24.5 11.9 35.9


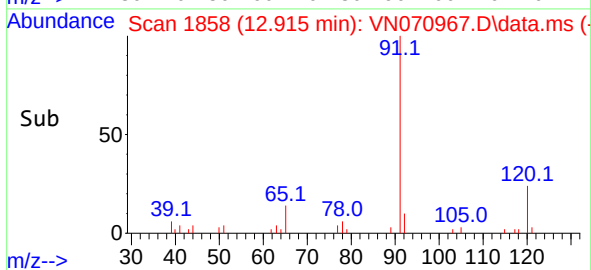






#80
1,3,5-Trimethylbenzene
Concen: 1.218 ug/l
RT: 13.057 min Scan# 1881
Delta R.T. 0.006 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion:105 Resp: 40473
Ion Ratio Lower Upper
105 100
120 52.0 24.6 73.6

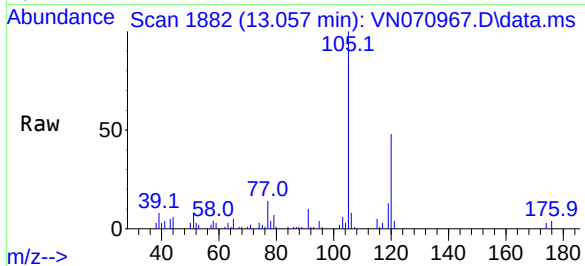

#81
trans-1,4-Dichloro-2-butene
Concen: 77.839 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion: 75 Resp: 288219
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#


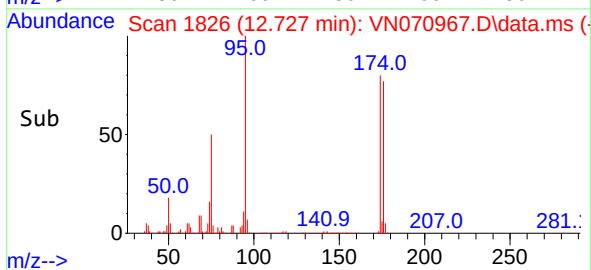

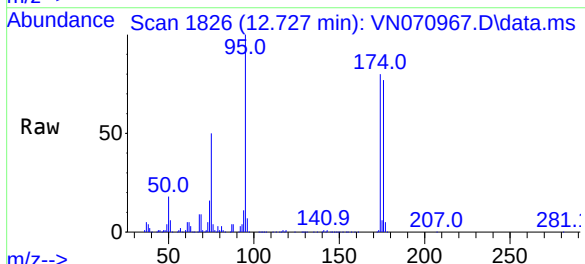




#84
1,2,4-Trimethylbenzene
Concen: 2.200 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. -0.000 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument : MSVOA_N
ClientSampleId : MW-22R


Tgt Ion:105 Resp: 71975
Ion Ratio Lower Upper
105 100
120 45.8 22.8 68.4

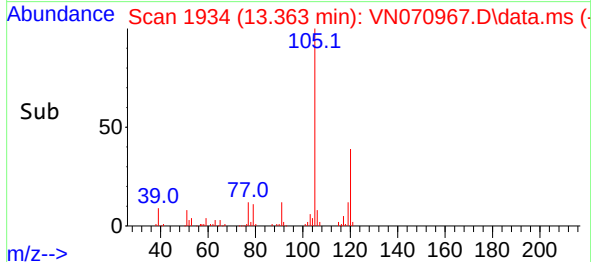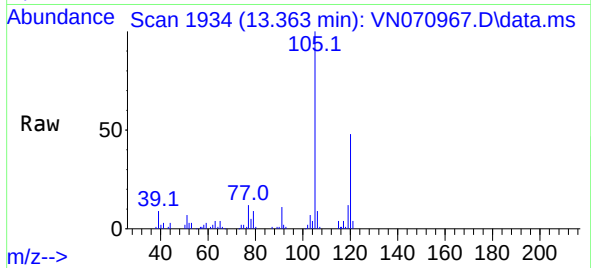

#85
sec-Butylbenzene
Concen: 1.733 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. -0.129 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion:105 Resp: 71975
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#


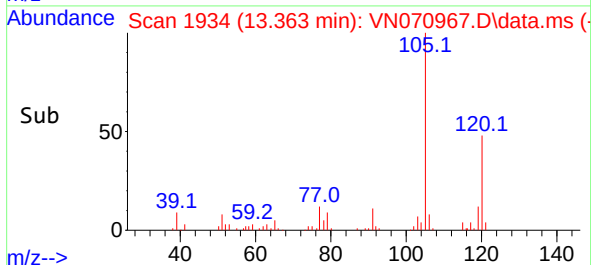
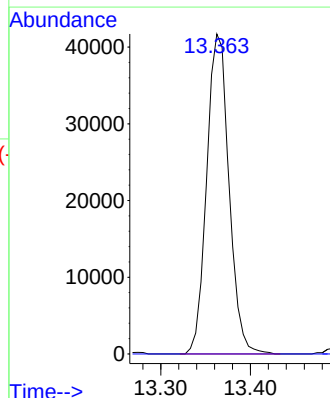
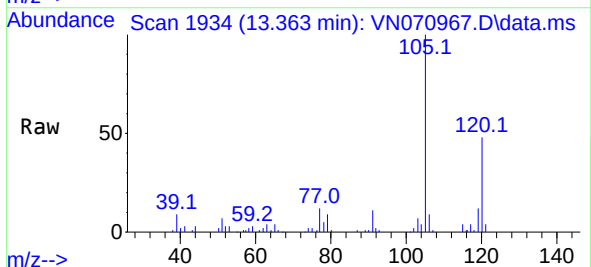




#90
Hexachloroethane
Concen: 0.319 ug/l
RT: 14.215 min Scan# 2077
Delta R.T. 0.012 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
MW-22R


Tgt Ion:117 Resp: 1945
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#

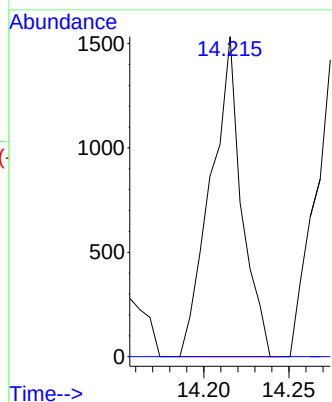

#93
1,2,4-Trichlorobenzene
Concen: 2.099 ug/l
RT: 15.257 min Scan# 2256
Delta R.T. -0.000 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion:180 Resp: 976
Ion Ratio Lower Upper
180 100
182 42.9 48.3 144.9#
145 43.2 14.5 43.5


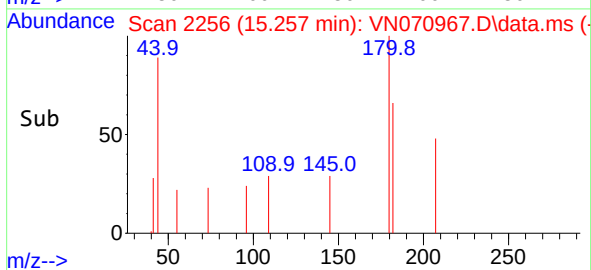






#95
Naphthalene
Concen: 8.990 ug/l
RT: 15.504 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Instrument :
MSVOA_N
ClientSampleId :
MW-22R

Tgt Ion:128 Resp: 101254
Ion Ratio Lower Upper
128 100
127 12.0 10.5 15.7
129 10.3 8.7 13.1



#96
1,2,3-Trichlorobenzene
Concen: 2.580 ug/l
RT: 15.698 min Scan# 2331
Delta R.T. 0.006 min
Lab File: VN070967.D
Acq: 16 Feb 2022 19:06

Tgt Ion:180 Resp: 584
Ion Ratio Lower Upper
180 100
182 0.0 47.4 142.2#
145 35.3 15.0 45.1

