
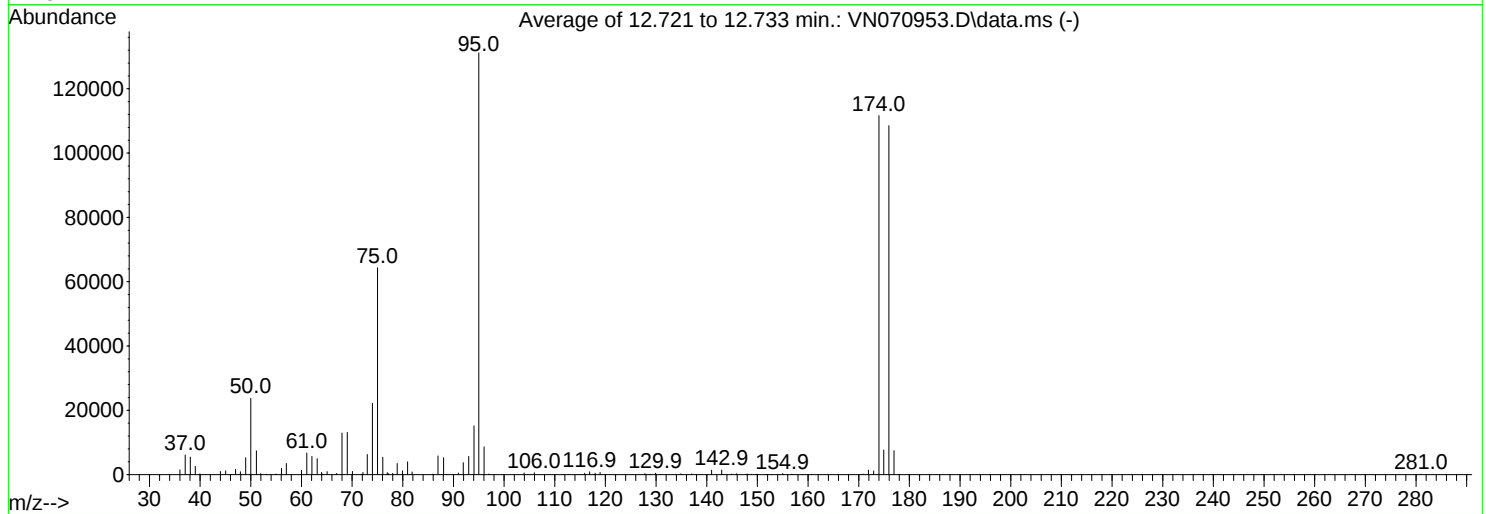


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021622\
 Data File : VN070953.D
 Acq On : 16 Feb 2022 10:41
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
 Title : SW846 8260
 Last Update : Mon Feb 21 07:57:15 2022

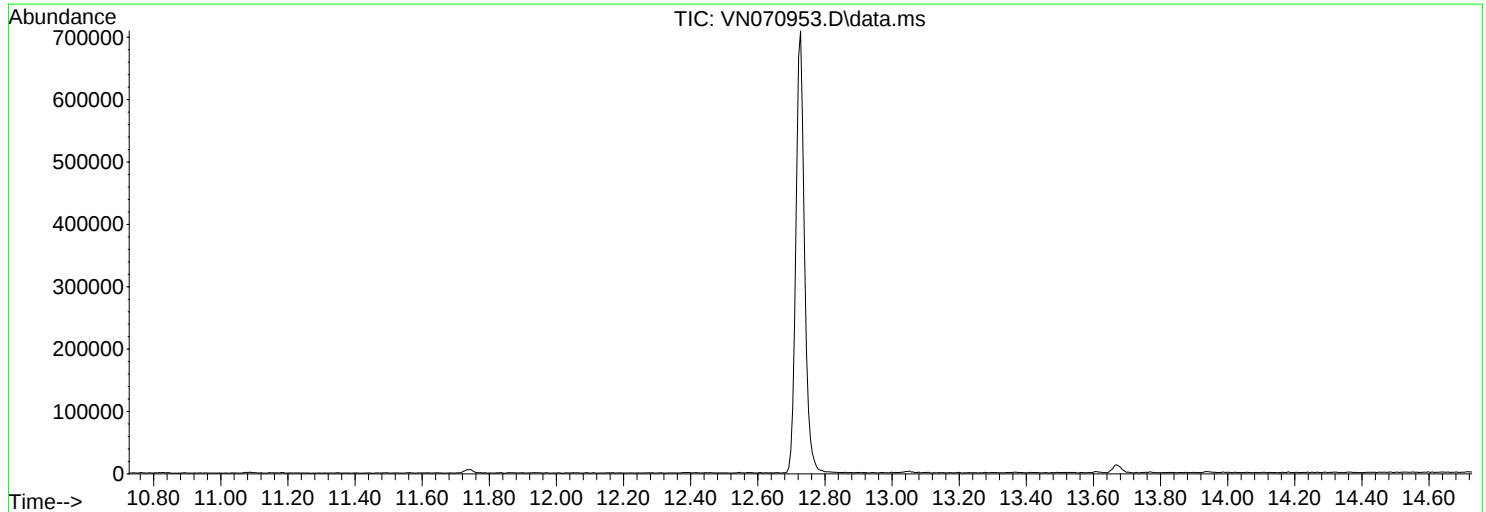

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	23747	PASS
75	95	30	60	49.0	64339	PASS
95	95	100	100	100.0	131184	PASS
96	95	5	9	6.6	8605	PASS
173	174	0.00	2	1.0	1136	PASS
174	95	50	100	85.1	111640	PASS
175	174	5	9	6.9	7648	PASS
176	174	95	101	97.2	108547	PASS
177	176	5	9	6.9	7456	PASS