
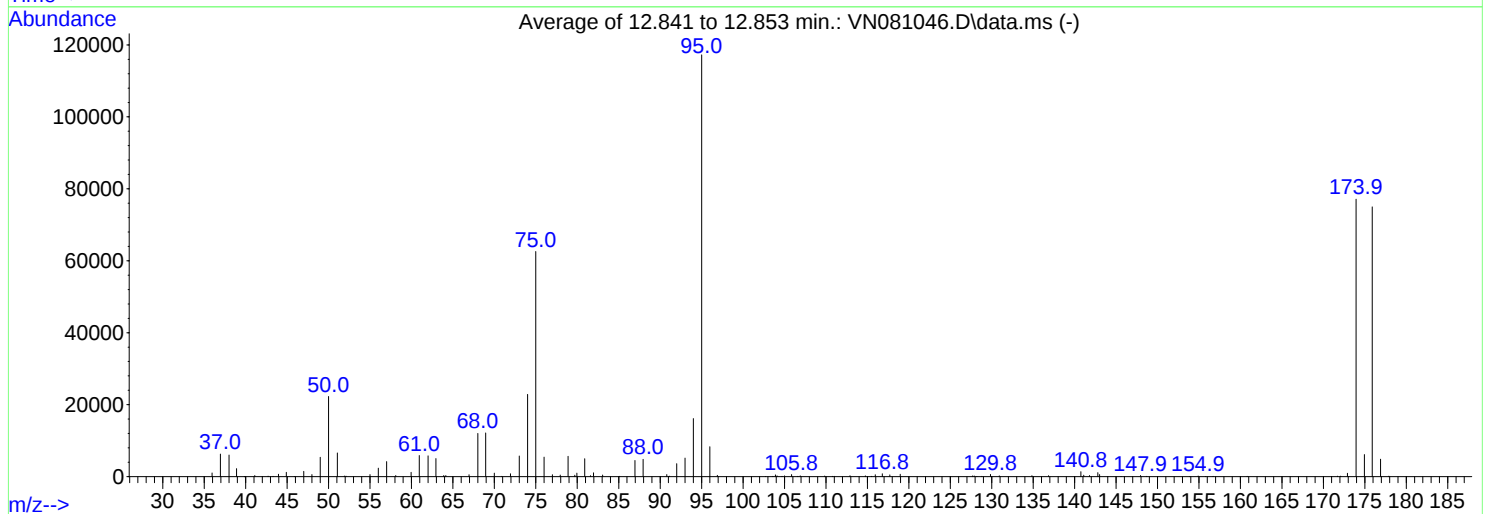


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021624\
Data File : VN081046.D
Acq On : 16 Feb 2024 09:12
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
Title : SW846 8260
Last Update : Fri Feb 16 23:45:20 2024

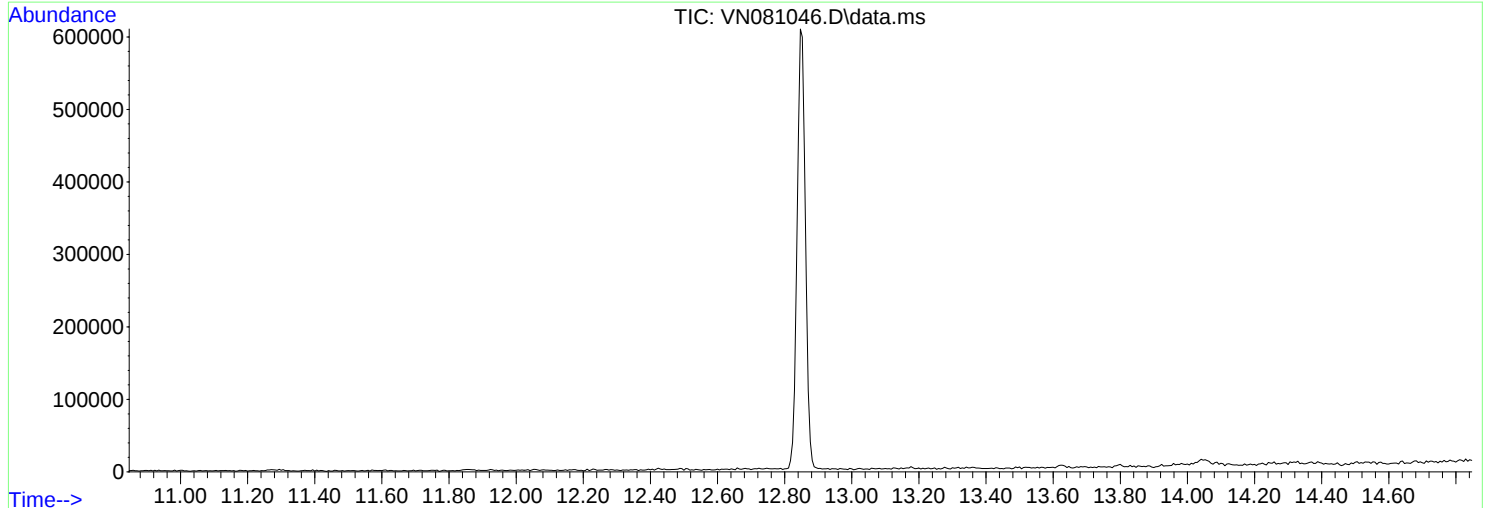

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	22307	PASS
75	95	30	60	53.4	62595	PASS
95	95	100	100	100.0	117240	PASS
96	95	5	9	7.1	8313	PASS
173	174	0.00	2	1.2	922	PASS
174	95	50	100	65.8	77128	PASS
175	174	5	9	8.0	6143	PASS
176	174	95	101	97.2	74992	PASS
177	176	5	9	6.5	4837	PASS

Average of 12.841 to 12.853 min.: VN081046.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	1013	45.90	52	58.10	318	70.90	71
36.95	6291	47.00	1475	59.95	1195	71.95	79
38.00	6019	48.00	574	60.95	5888	73.00	575
38.90	2231	49.00	5380	62.00	5793	74.00	2284
39.85	17	50.00	22307	62.95	5020	75.00	62595
41.10	302	51.05	6584	63.90	306	76.00	5431
42.00	53	51.90	202	64.15	310	77.00	517
42.70	148	52.10	129	66.95	528	77.95	466
43.30	95	55.00	599	68.00	12030	78.90	5665
43.95	664	56.00	2371	68.95	12160	79.70	387
44.90	1200	57.00	4164	70.00	971	79.95	966

Average of 12.841 to 12.853 min.: VN081046.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.90	4983	94.00	16135	106.60	78	118.95	654
81.60	259	95.00	117240	106.90	247	127.70	230
81.95	1088	96.00	8313	109.85	196	127.90	194
83.05	453	96.90	375	110.80	104	128.20	51
85.10	75	102.70	70	111.00	73	128.80	95
86.95	4504	103.60	98	112.90	258	129.85	607
87.95	4824	103.90	514	114.75	237	130.90	229
90.80	591	104.10	230	115.50	86	134.85	278
91.10	121	104.70	111	115.95	558	136.85	286
92.00	3594	105.00	216	116.80	789	140.00	64
93.00	5140	105.85	568	117.70	515	140.75	1384

Average of 12.841 to 12.853 min.: VN081046.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
141.10	391	153.90	60	175.90	74992		
141.80	329	154.90	186	176.90	4837		
142.80	1111	155.80	70	177.90	155		
143.00	589	156.70	101				
144.00	63	160.80	76				
145.60	67	171.00	60				
146.00	52	171.70	158				
147.00	62	172.10	120				
147.95	304	172.90	922				
148.70	73	173.95	77128				
150.00	59	174.95	6143				

Instrument :

MSVOA_N

ClientSampleId :

BFB