


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN021720\
 Data File : VN060109.D
 Acq On : 17 Feb 2020 10:16
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N021220W.M
 Title : SW846 8260
 Last Update : Wed Feb 12 14:12:21 2020

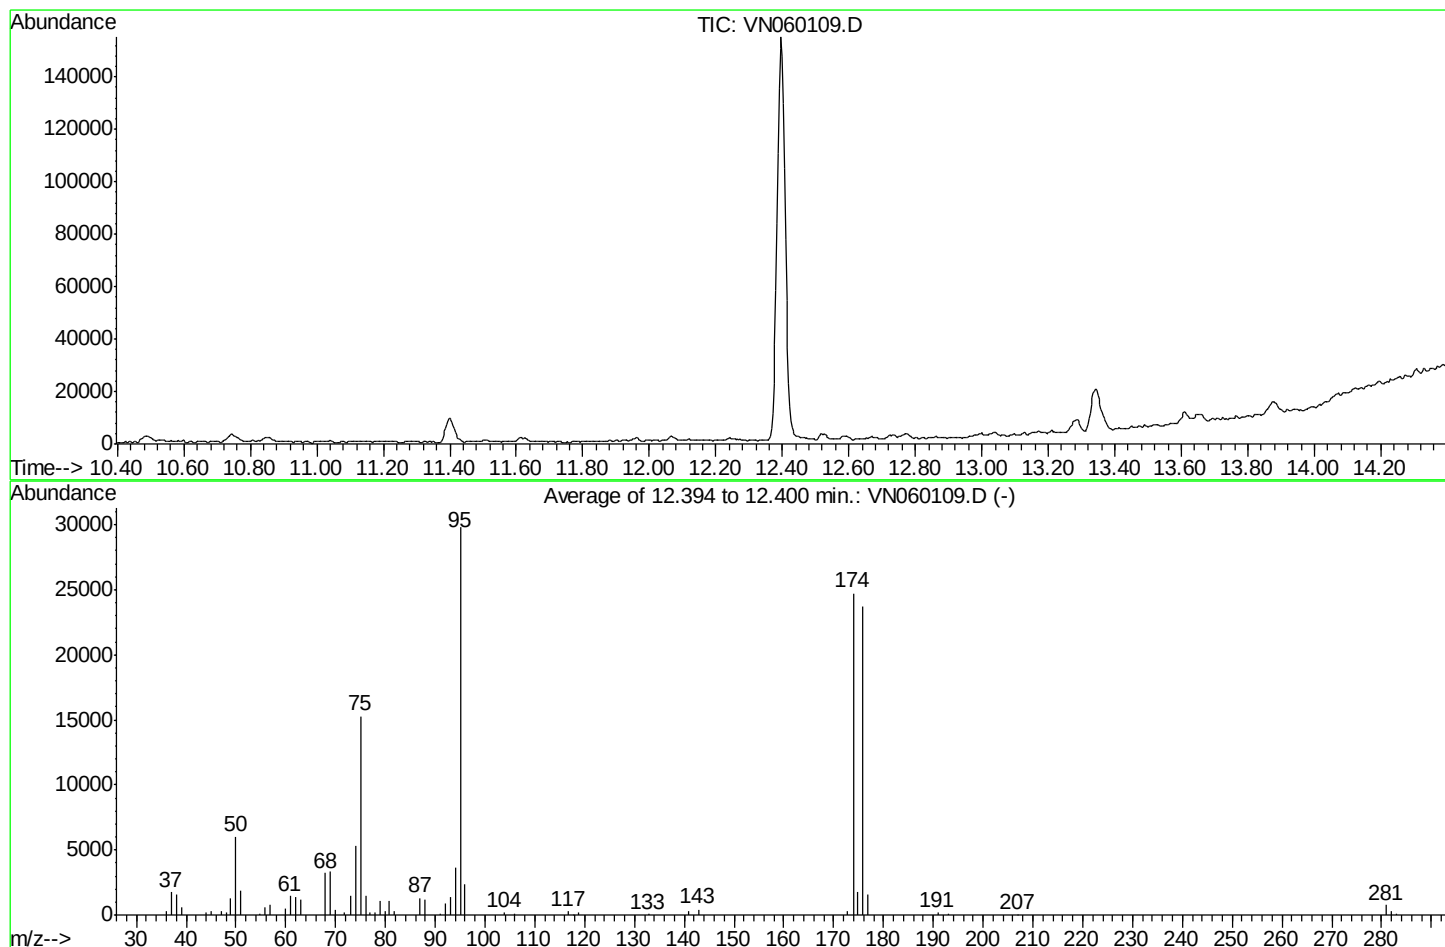

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	6049	PASS
75	95	30	60	51.3	15297	PASS
95	95	100	100	100.0	29792	PASS
96	95	5	9	7.8	2329	PASS
173	174	0.00	2	1.2	304	PASS
174	95	50	100	83.0	24738	PASS
175	174	5	9	7.1	1751	PASS
176	174	95	101	95.8	23693	PASS
177	176	5	9	6.7	1584	PASS