

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021721\
 Data File : VN065910.D
 Acq On : 17 Feb 2021 22:27
 Operator : JC/MD
 Sample : M1382-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BP-TT-VPB-RW6-TB-20210210

Quant Time: Feb 18 01:48:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 17 15:48:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.627	168	193777	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.550	114	325690	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	294027	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.312	152	102954	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.987	65	126590	46.72	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	93.44%
35) Dibromofluoromethane	7.553	113	95297	47.28	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	94.56%
50) Toluene-d8	10.058	98	401430	48.52	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	97.04%
62) 4-Bromofluorobenzene	12.373	95	134270	43.23	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	86.46%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021721\
Data File : VN065910.D
Acq On : 17 Feb 2021 22:27
Operator : JC/MD
Sample : M1382-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BP-TT-VPB-RW6-TB-20210210

Quant Time: Feb 18 01:48:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 17 15:48:13 2021
Response via : Initial Calibration




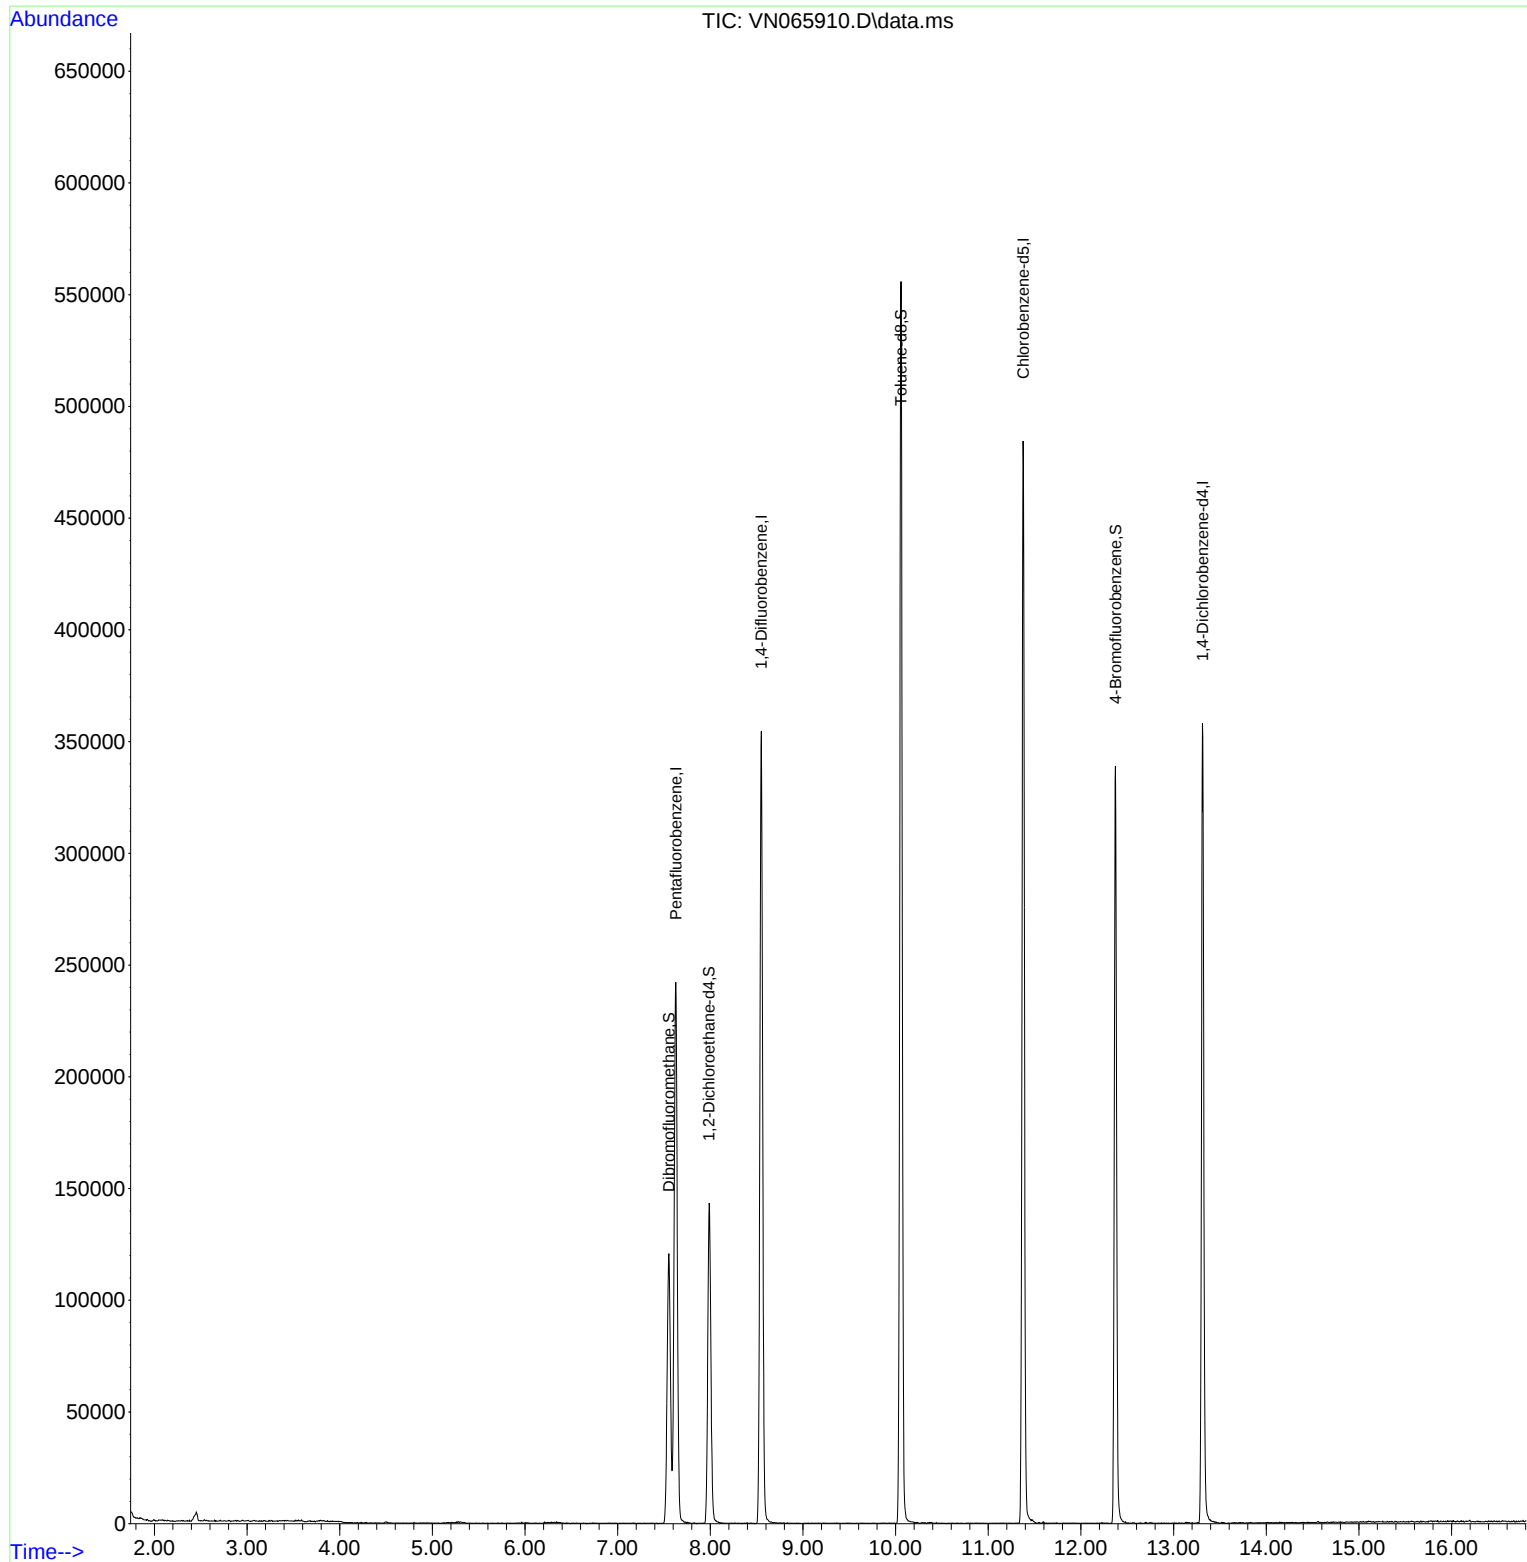


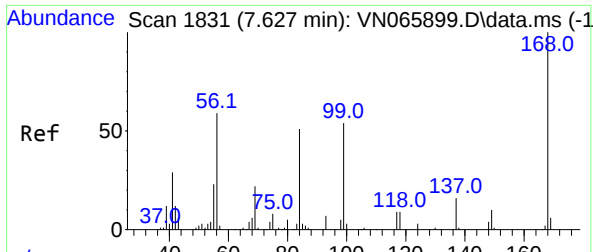

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.627 min Scan# 1831
Delta R.T. 0.000 min
Lab File: VN065910.D
Acq: 17 Feb 2021 22:27




Instrument :
MSVOA_N
ClientSampleId :
BP-TT-VPB-RW6-TB-20210210


Tgt Ion:168 Resp: 193777
Ion Ratio Lower Upper
168 100
99 60.0 42.6 63.8

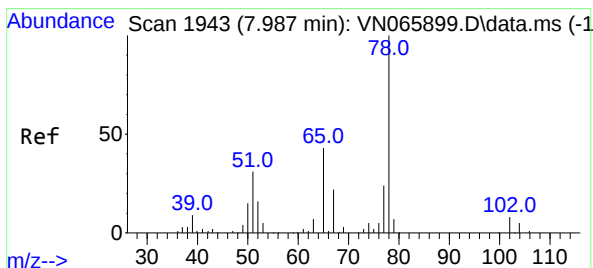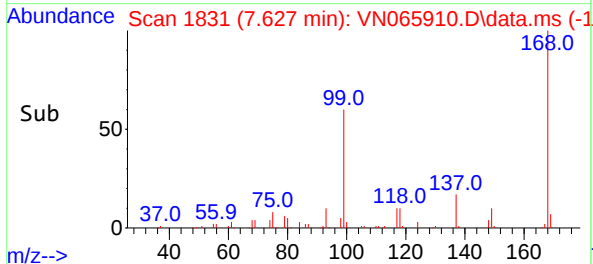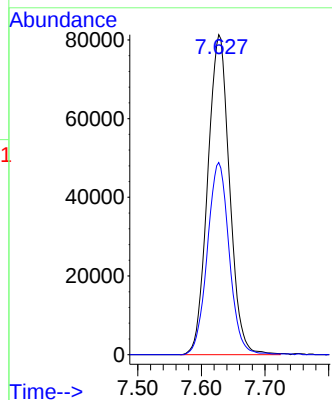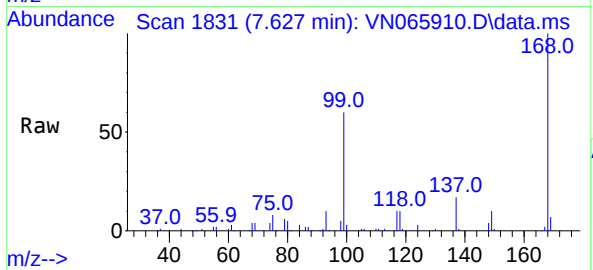

#33
1,2-Dichloroethane-d4
Concen: 46.72 ug/l
RT: 7.987 min Scan# 1943
Delta R.T. 0.000 min
Lab File: VN065910.D
Acq: 17 Feb 2021 22:27

Tgt Ion: 65 Resp: 126590
Ion Ratio Lower Upper
65 100
67 53.1 0.0 107.2

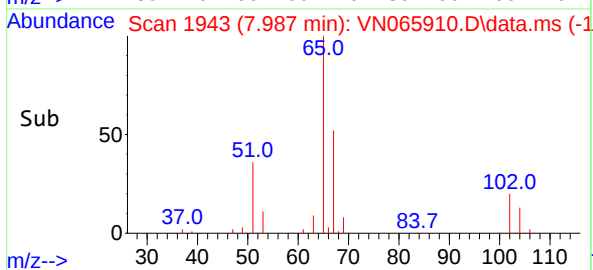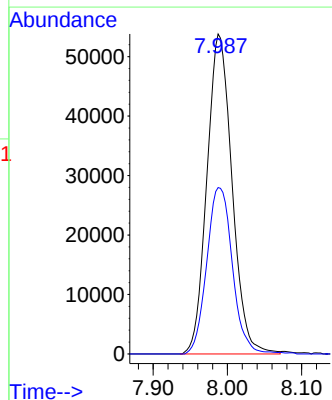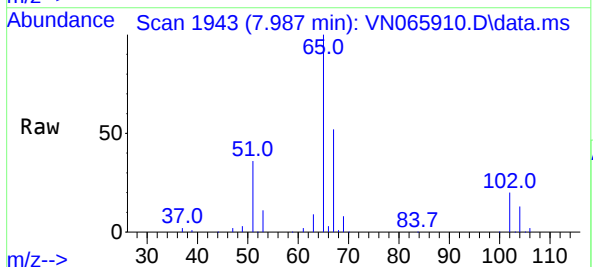




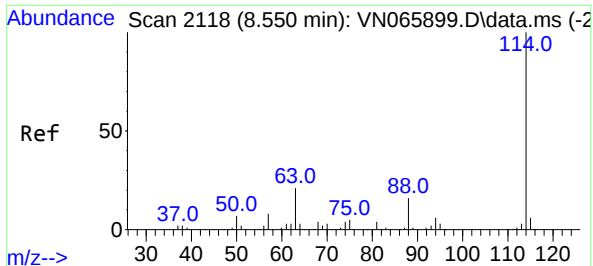


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.550 min Scan# 2118
Delta R.T. 0.000 min
Lab File: VN065910.D
Acq: 17 Feb 2021 22:27

Instrument :
MSVOA_N
ClientSampleId :
BP-TT-VPB-RW6-TB-20210210




Tgt Ion:114 Resp: 325690
Ion Ratio Lower Upper
114 100
63 21.2 0.0 38.6
88 16.7 0.0 30.6

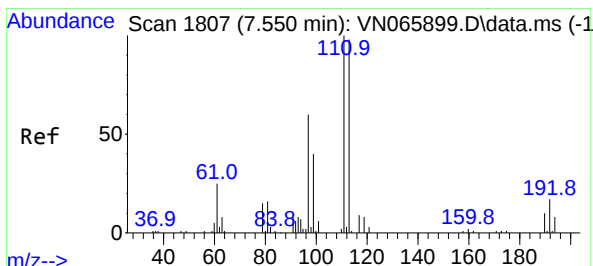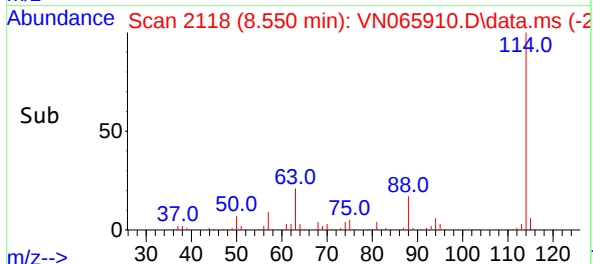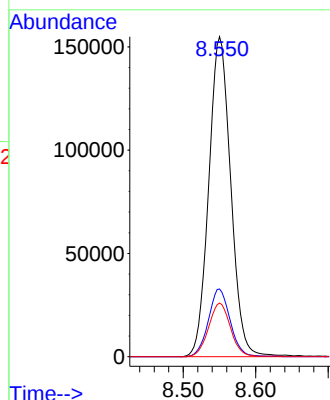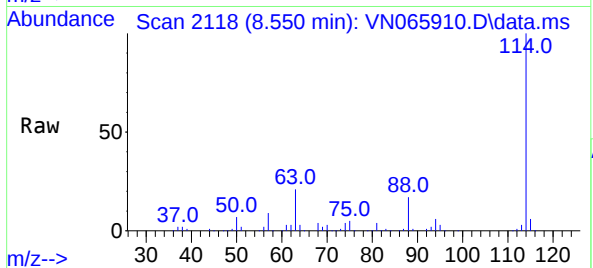


#35

Dibromofluoromethane
Concen: 47.28 ug/l
RT: 7.553 min Scan# 1808
Delta R.T. 0.003 min
Lab File: VN065910.D
Acq: 17 Feb 2021 22:27

Tgt Ion:113 Resp: 95297
Ion Ratio Lower Upper
113 100
111 103.7 82.2 123.2
192 17.9 15.4 23.0


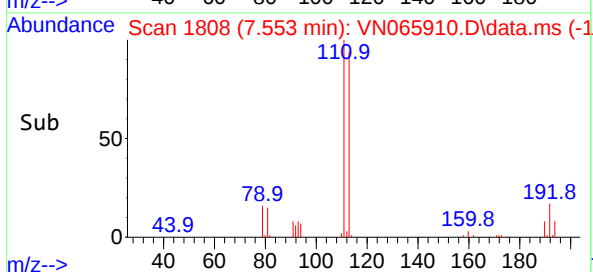
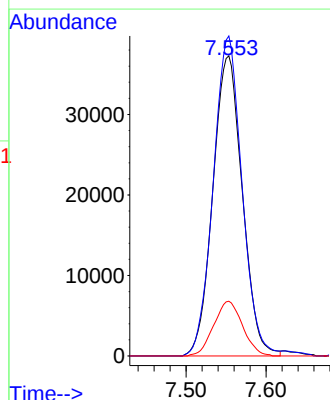
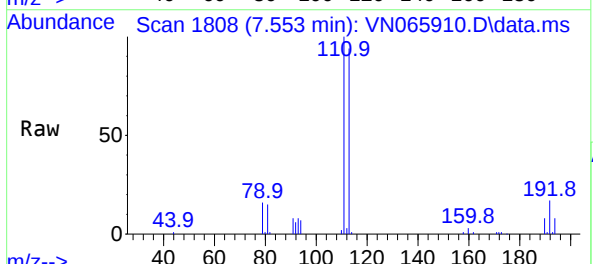


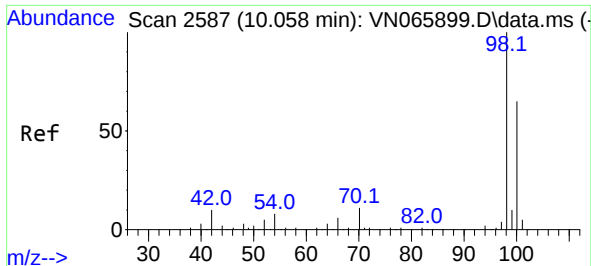

#50
Toluene-d8
Concen: 48.52 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. 0.000 min
Lab File: VN065910.D
Acq: 17 Feb 2021 22:27




Instrument :
MSVOA_N
ClientSampleId :
BP-TT-VPB-RW6-TB-20210210


Tgt Ion: 98 Resp: 401430
Ion Ratio Lower Upper
98 100
100 64.3 50.5 75.7

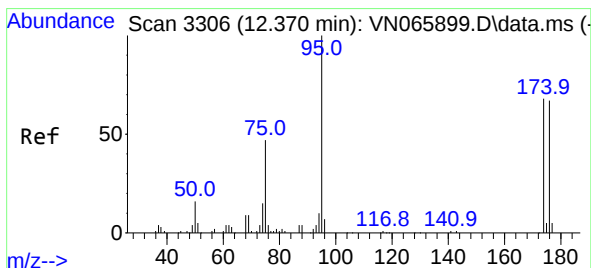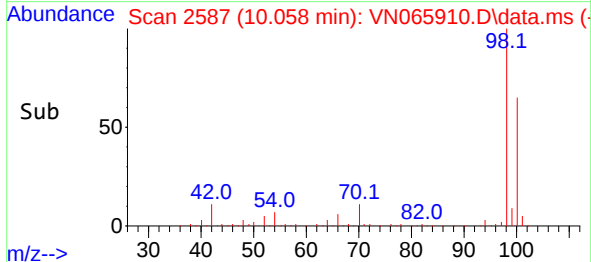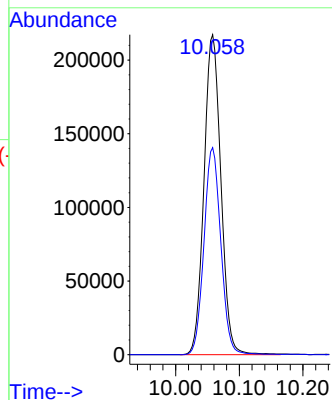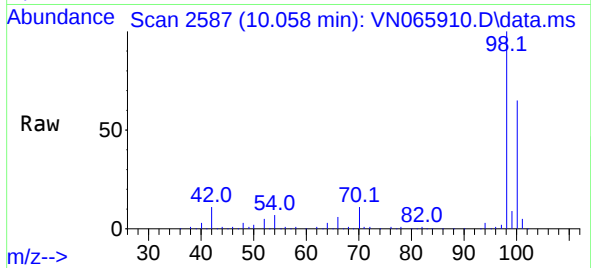

#62
4-Bromofluorobenzene
Concen: 43.23 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.003 min
Lab File: VN065910.D
Acq: 17 Feb 2021 22:27

Tgt Ion: 95 Resp: 134270
Ion Ratio Lower Upper
95 100
174 70.5 0.0 169.0
176 68.0 0.0 162.4


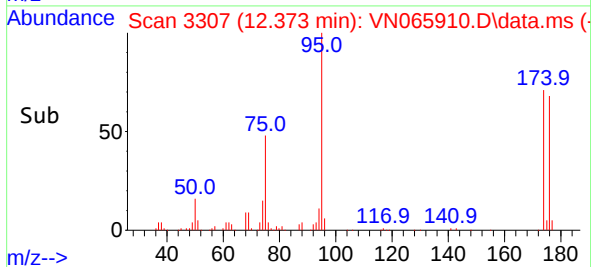
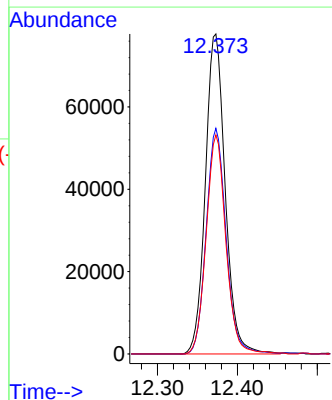
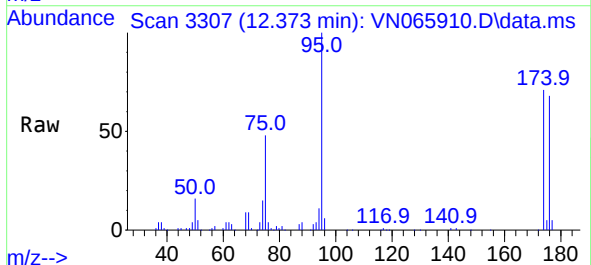


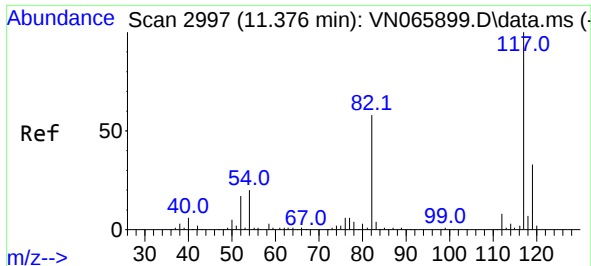

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN065910.D
Acq: 17 Feb 2021 22:27

Instrument :
MSVOA_N
ClientSampleId :
BP-TT-VPB-RW6-TB-20210210

Tgt Ion:	117	Resp:	294027
Ion Ratio	Lower	Upper	
117	100		
82	57.2	43.7	65.5
119	31.7	26.1	39.1

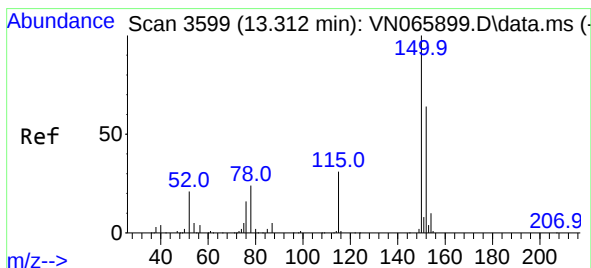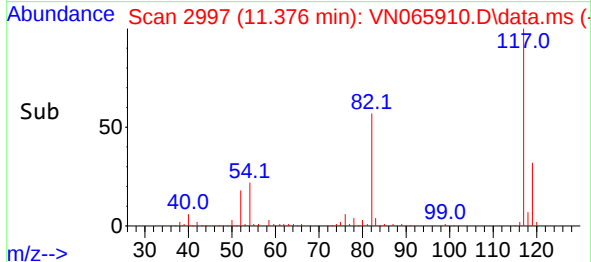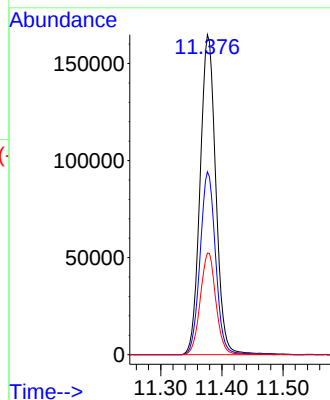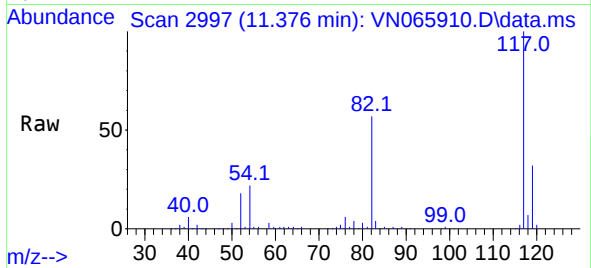

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.312 min Scan# 3599
Delta R.T. -0.000 min
Lab File: VN065910.D
Acq: 17 Feb 2021 22:27

Tgt Ion:	152	Resp:	102954
Ion Ratio	Lower	Upper	
152	100		
115	62.2	28.5	85.6
150	158.7	0.0	347.6

