

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021722\
Data File : VN070976.D
Acq On : 17 Feb 2022 13:49
Operator : JC\MD
Sample : N1581-24 40X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DUP01-20220215

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M

Title : SW846 8260

Signal : TIC: VN070976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	8.022	1014	1026	1030	rBV	517738	1212175	30.30%	6.086%
2	8.081	1030	1036	1056	rVB	1051370	2398034	59.95%	12.040%
3	8.433	1086	1096	1111	rBV	573469	1336197	33.40%	6.709%
4	8.963	1177	1186	1202	rVB	1430149	2929413	73.23%	14.708%
5	10.439	1428	1437	1455	rBV	2171240	4000042	100.00%	20.084%
6	11.739	1650	1658	1680	rBV	1844246	3348838	83.72%	16.814%
7	12.727	1818	1826	1839	rBV	1263283	2211766	55.29%	11.105%
8	13.674	1980	1987	2000	rVB	1367132	2387643	59.69%	11.988%
9	15.504	2291	2298	2304	rBV2	25807	52254	1.31%	0.262%
10	15.704	2325	2332	2338	rBV3	21441	40368	1.01%	0.203%




Sum of corrected areas: 19916730

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021722\
Data File : VN070976.D
Acq On : 17 Feb 2022 13:49
Operator : JC\MD
Sample : N1581-24 40X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DUP01-20220215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

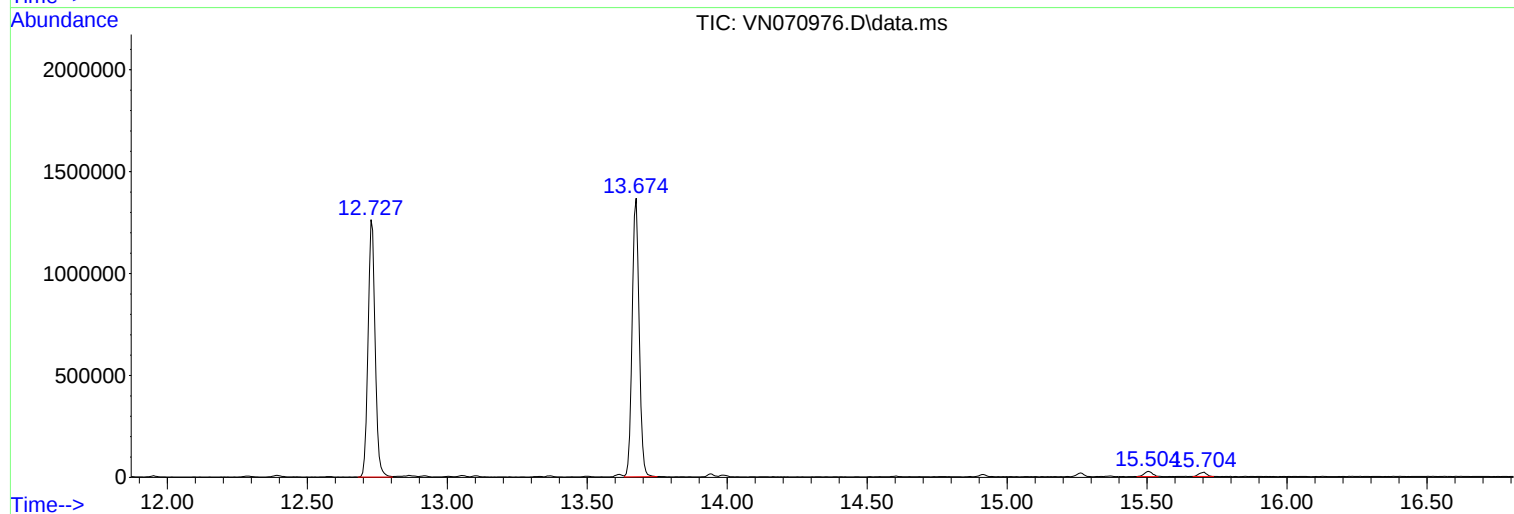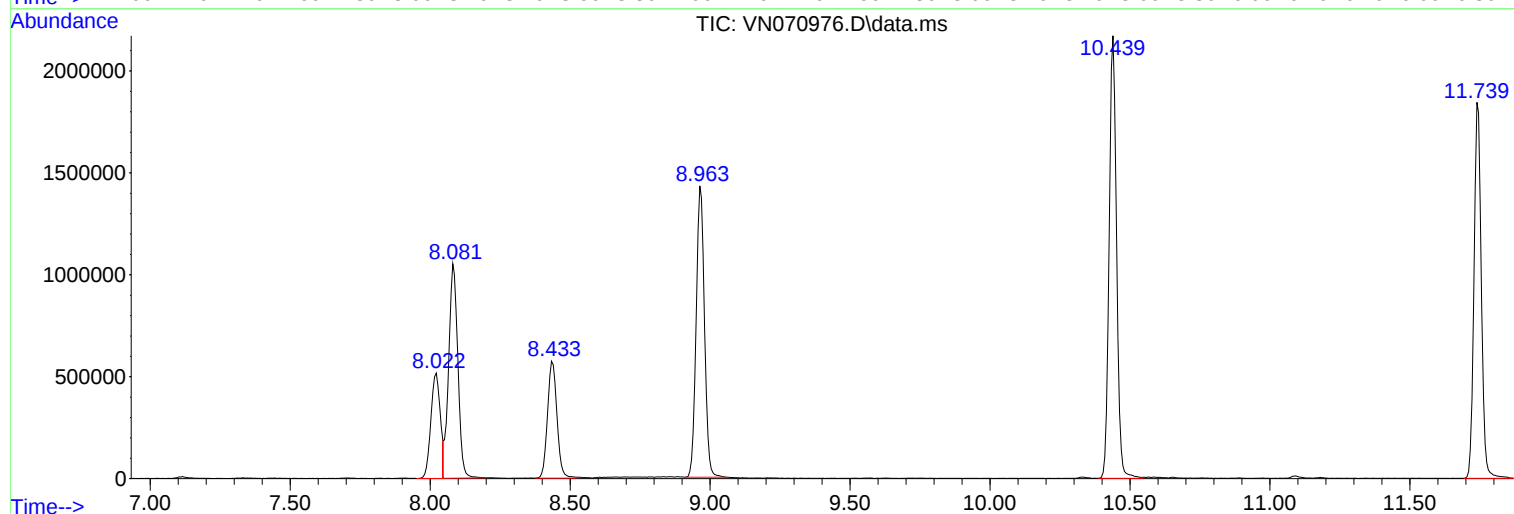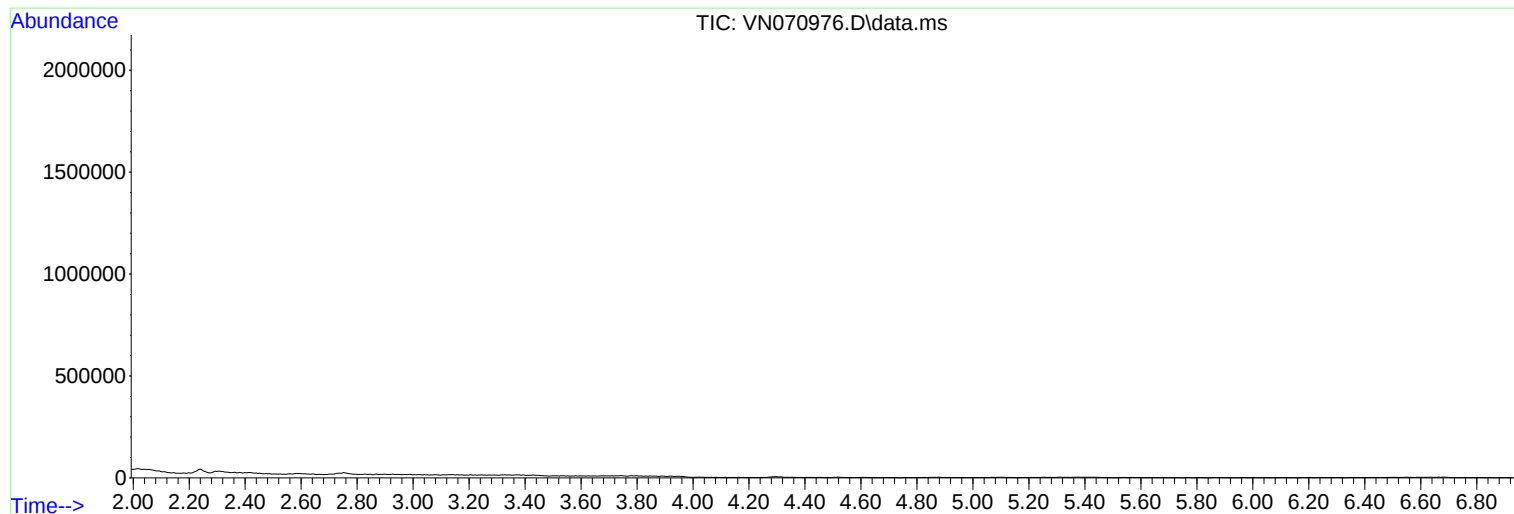

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021722\
Data File : VN070976.D
Acq On : 17 Feb 2022 13:49
Operator : JC\MD
Sample : N1581-24 40X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DUP01-20220215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021722\
Data File : VN070976.D
Acq On : 17 Feb 2022 13:49
Operator : JC\MD
Sample : N1581-24 40X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DUP01-20220215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc