


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021723\
Data File : VN076728.D
Acq On : 17 Feb 2023 11:17
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N021523W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Feb 16 01:08:46 2023

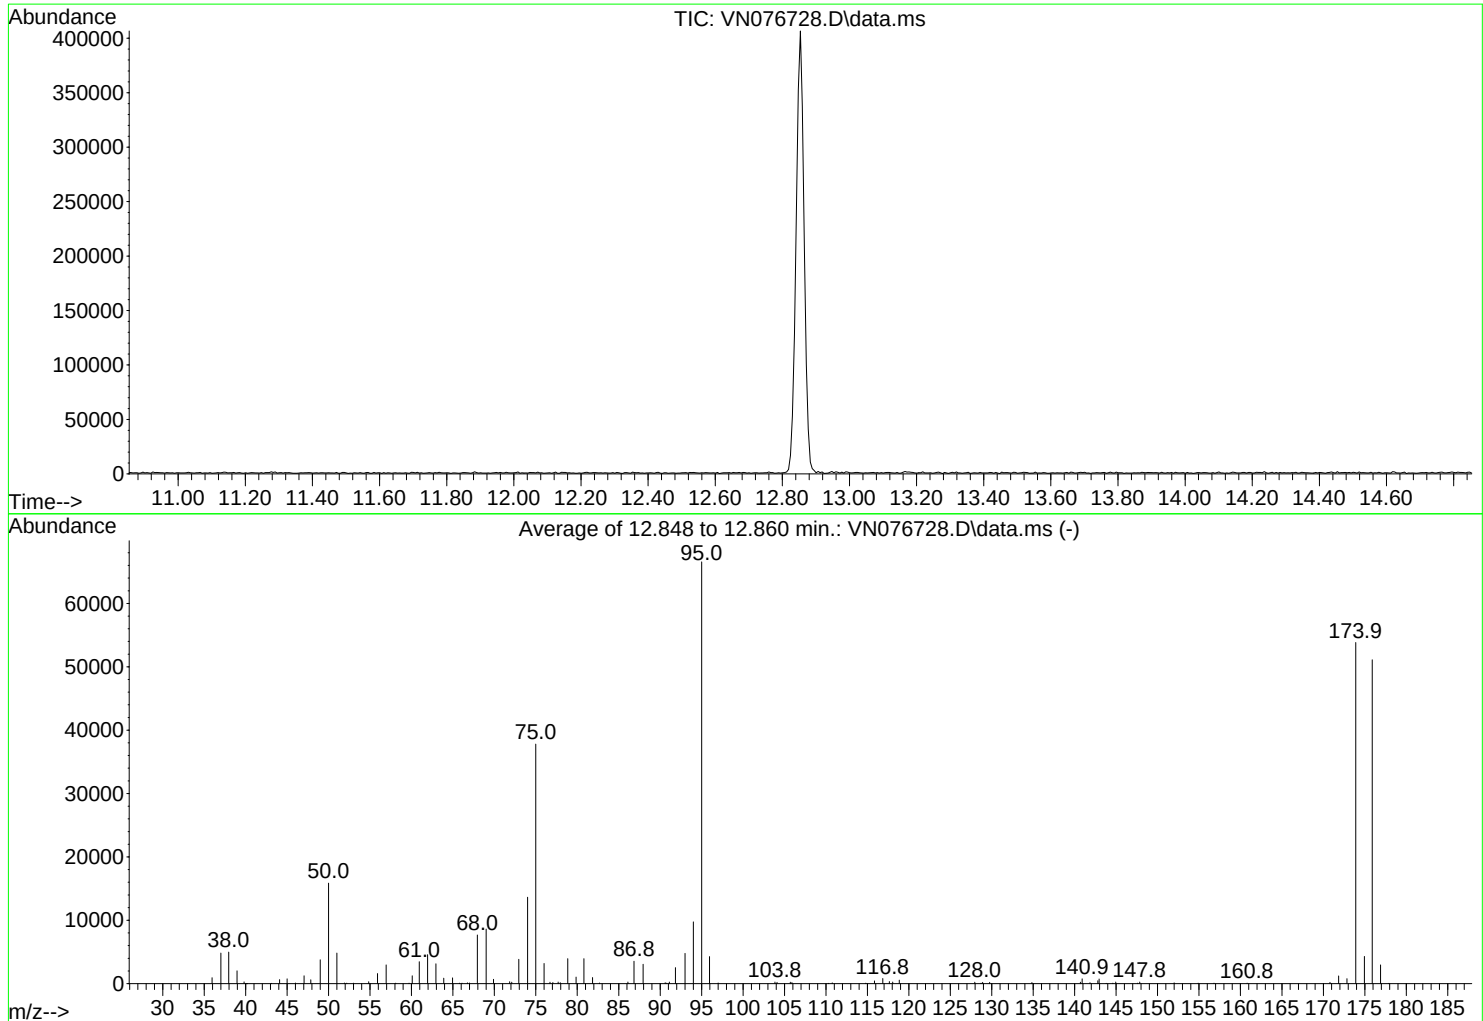

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1847

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.8	15858	PASS
75	95	30	60	56.8	37811	PASS
95	95	100	100	100.0	66565	PASS
96	95	5	9	6.4	4281	PASS
173	174	0.00	2	1.4	780	PASS
174	95	50	100	80.9	53843	PASS
175	174	5	9	8.0	4286	PASS
176	174	95	101	94.9	51115	FAIL*
177	176	5	9	5.8	2953	PASS