

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN021822\  
Data File : VN071005.D  
Acq On : 18 Feb 2022 17:03  
Operator : JC\MD  
Sample : N1581-21  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
ROOF-DRAIN-20220215

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N021522W.M

Title : SW846 8260

Signal : TIC: VN071006.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 8.022       | 1013          | 1026        | 1030         | rBV      | 542616         | 1282034       | 29.34%          | 5.951%        |
| 2         | 8.087       | 1030          | 1037        | 1052         | rVB      | 1107874        | 2557570       | 58.53%          | 11.871%       |
| 3         | 8.434       | 1086          | 1096        | 1107         | rBV      | 612856         | 1416035       | 32.41%          | 6.573%        |
| 4         | 8.963       | 1177          | 1186        | 1207         | rBV      | 1571537        | 3191774       | 73.05%          | 14.815%       |
| 5         | 9.216       | 1222          | 1229        | 1237         | rVB      | 46733          | 96393         | 2.21%           | 0.447%        |
| 6         | 10.439      | 1427          | 1437        | 1456         | rBV      | 2440436        | 4369369       | 100.00%         | 20.281%       |
| 7         | 11.739      | 1647          | 1658        | 1673         | rBV      | 2040200        | 3632922       | 83.15%          | 16.863%       |
| 8         | 12.727      | 1816          | 1826        | 1839         | rBV      | 1519305        | 2590760       | 59.29%          | 12.026%       |
| 9         | 13.669      | 1979          | 1986        | 2000         | rBV      | 1378944        | 2407023       | 55.09%          | 11.173%       |




Sum of corrected areas: 21543880

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN021822\  
Data File : VN071005.D  
Acq On : 18 Feb 2022 17:03  
Operator : JC\MD  
Sample : N1581-21  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
ROOF-DRAIN-20220215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N021522W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

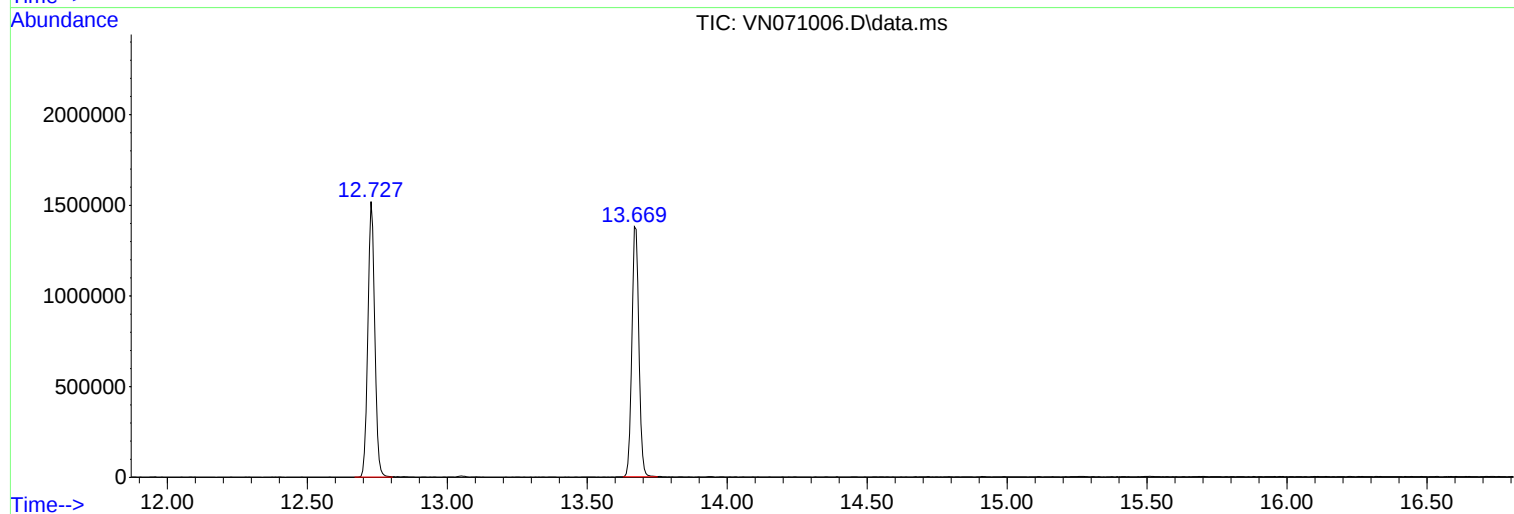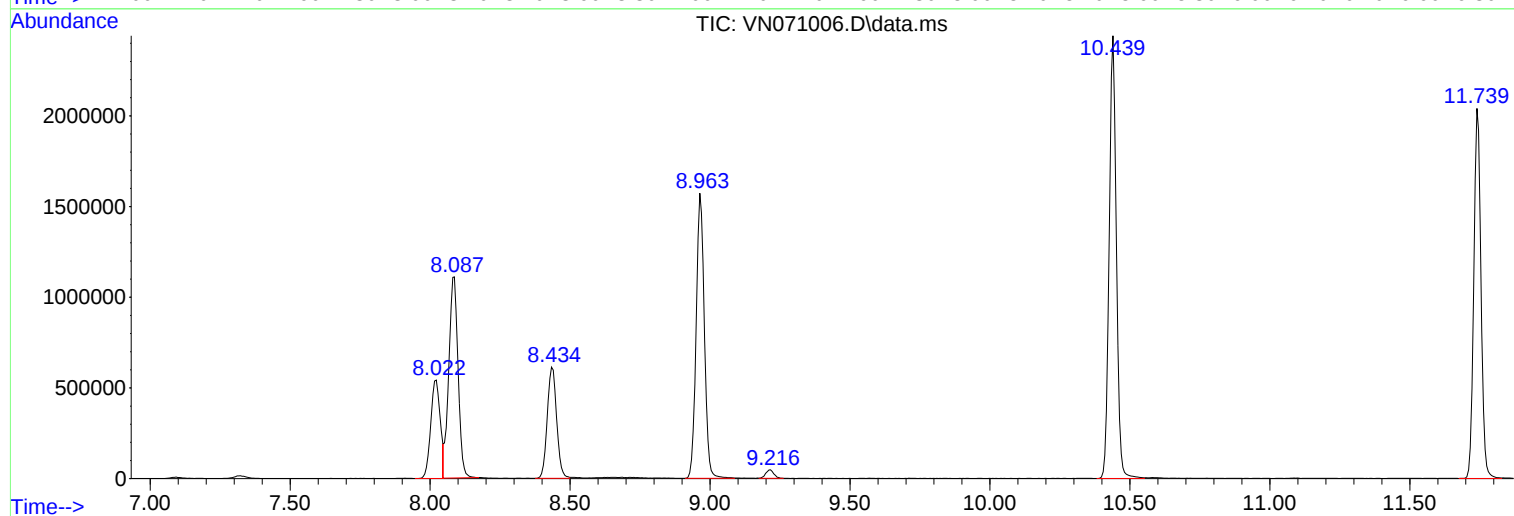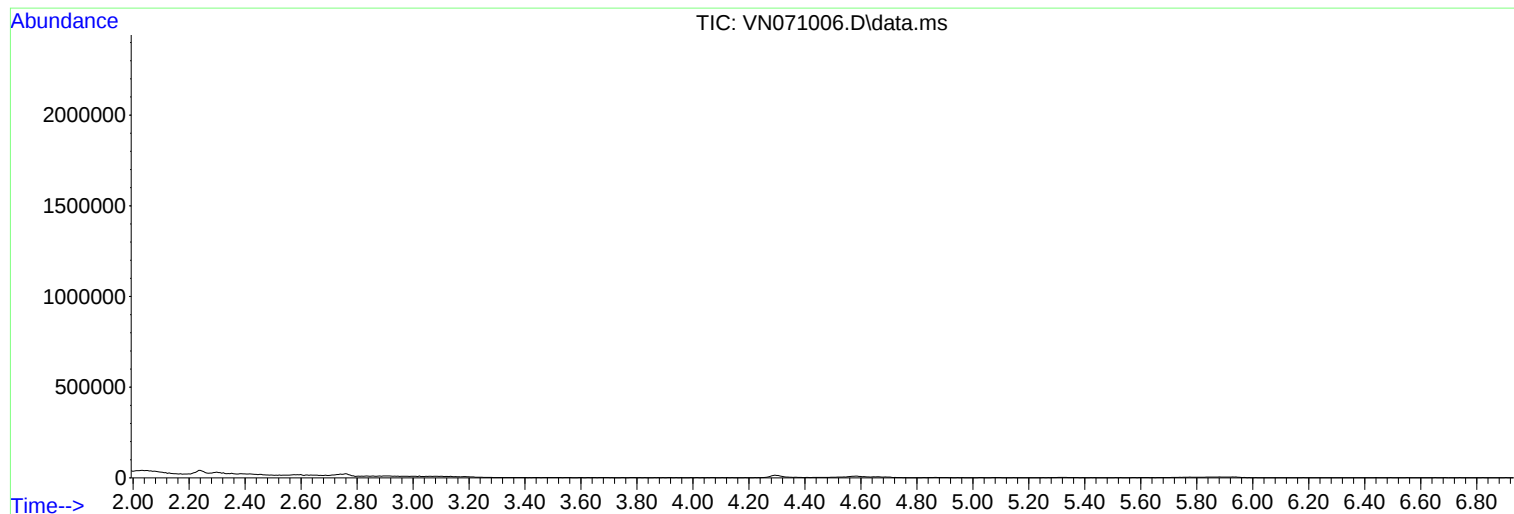

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN021822\  
Data File : VN071005.D  
Acq On : 18 Feb 2022 17:03  
Operator : JC\MD  
Sample : N1581-21  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
ROOF-DRAIN-20220215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N021522W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN021822\  
Data File : VN071005.D  
Acq On : 18 Feb 2022 17:03  
Operator : JC\MD  
Sample : N1581-21  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
ROOF-DRAIN-20220215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N021522W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |