


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN021919\
 Data File : VN053855.D
 Acq On : 19 Feb 2019 8:32
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N013019W.M
 Title : SW846 8260
 Last Update : Fri Feb 01 09:11:52 2019

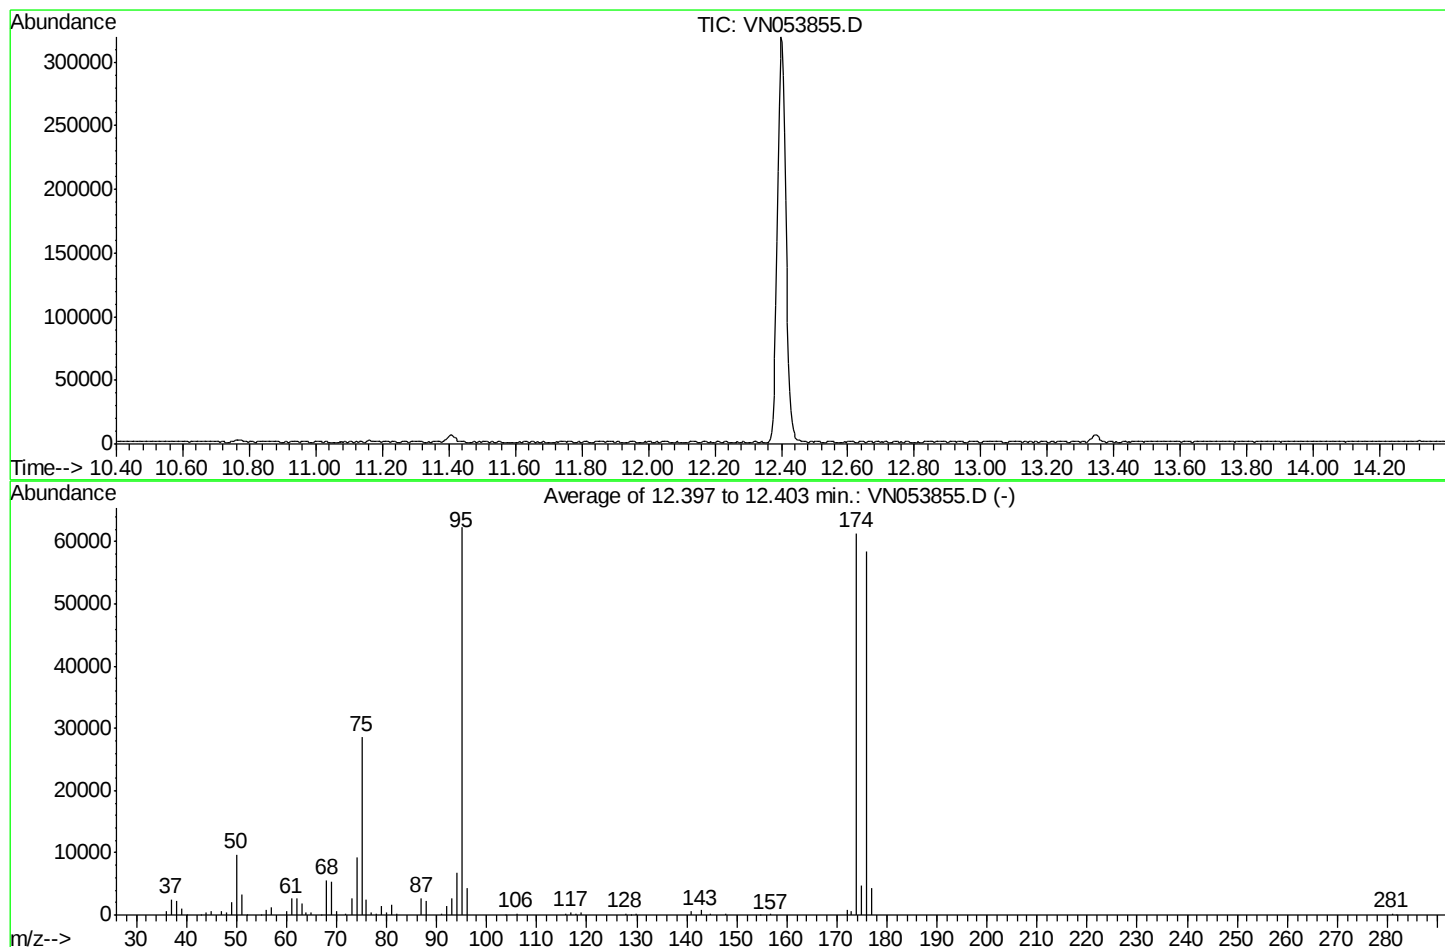

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	9689	PASS
75	95	30	60	46.0	28658	PASS
95	95	100	100	100.0	62328	PASS
96	95	5	9	7.0	4373	PASS
173	174	0.00	2	1.0	616	PASS
174	95	50	100	98.5	61400	PASS
175	174	5	9	7.6	4667	PASS
176	174	95	101	95.2	58472	PASS
177	176	5	9	7.3	4249	PASS