

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN021920\
 Data File : VN060153.D
 Acq On : 19 Feb 2020 14:09
 Operator : JC/MD
 Sample : L1362-03
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BU-03-021820

Quant Time: Feb 20 03:05:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N021220W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 12 14:12:21 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	185908	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.57	114	296221	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	275230	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	124919	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.00	65	108192	47.83	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.66%	
35) Dibromofluoromethane	7.57	113	89168	48.97	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.94%	
50) Toluene-d8	10.08	98	356102	49.66	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.32%	
62) 4-Bromofluorobenzene	12.40	95	128098	48.62	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.24%	
Target Compounds						
16) Acetone	3.79	43	7801	7.906	ug/l	99
20) Methylene Chloride	4.53	84	8187	4.159	ug/l	97
43) Isopropyl Acetate	8.14	43	21693	5.118	ug/l #	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN021920\
Data File : VN060153.D
Acq On : 19 Feb 2020 14:09
Operator : JC/MD
Sample : L1362-03
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BU-03-021820

Quant Time: Feb 20 03:05:55 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N021220W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 12 14:12:21 2020
Response via : Initial Calibration

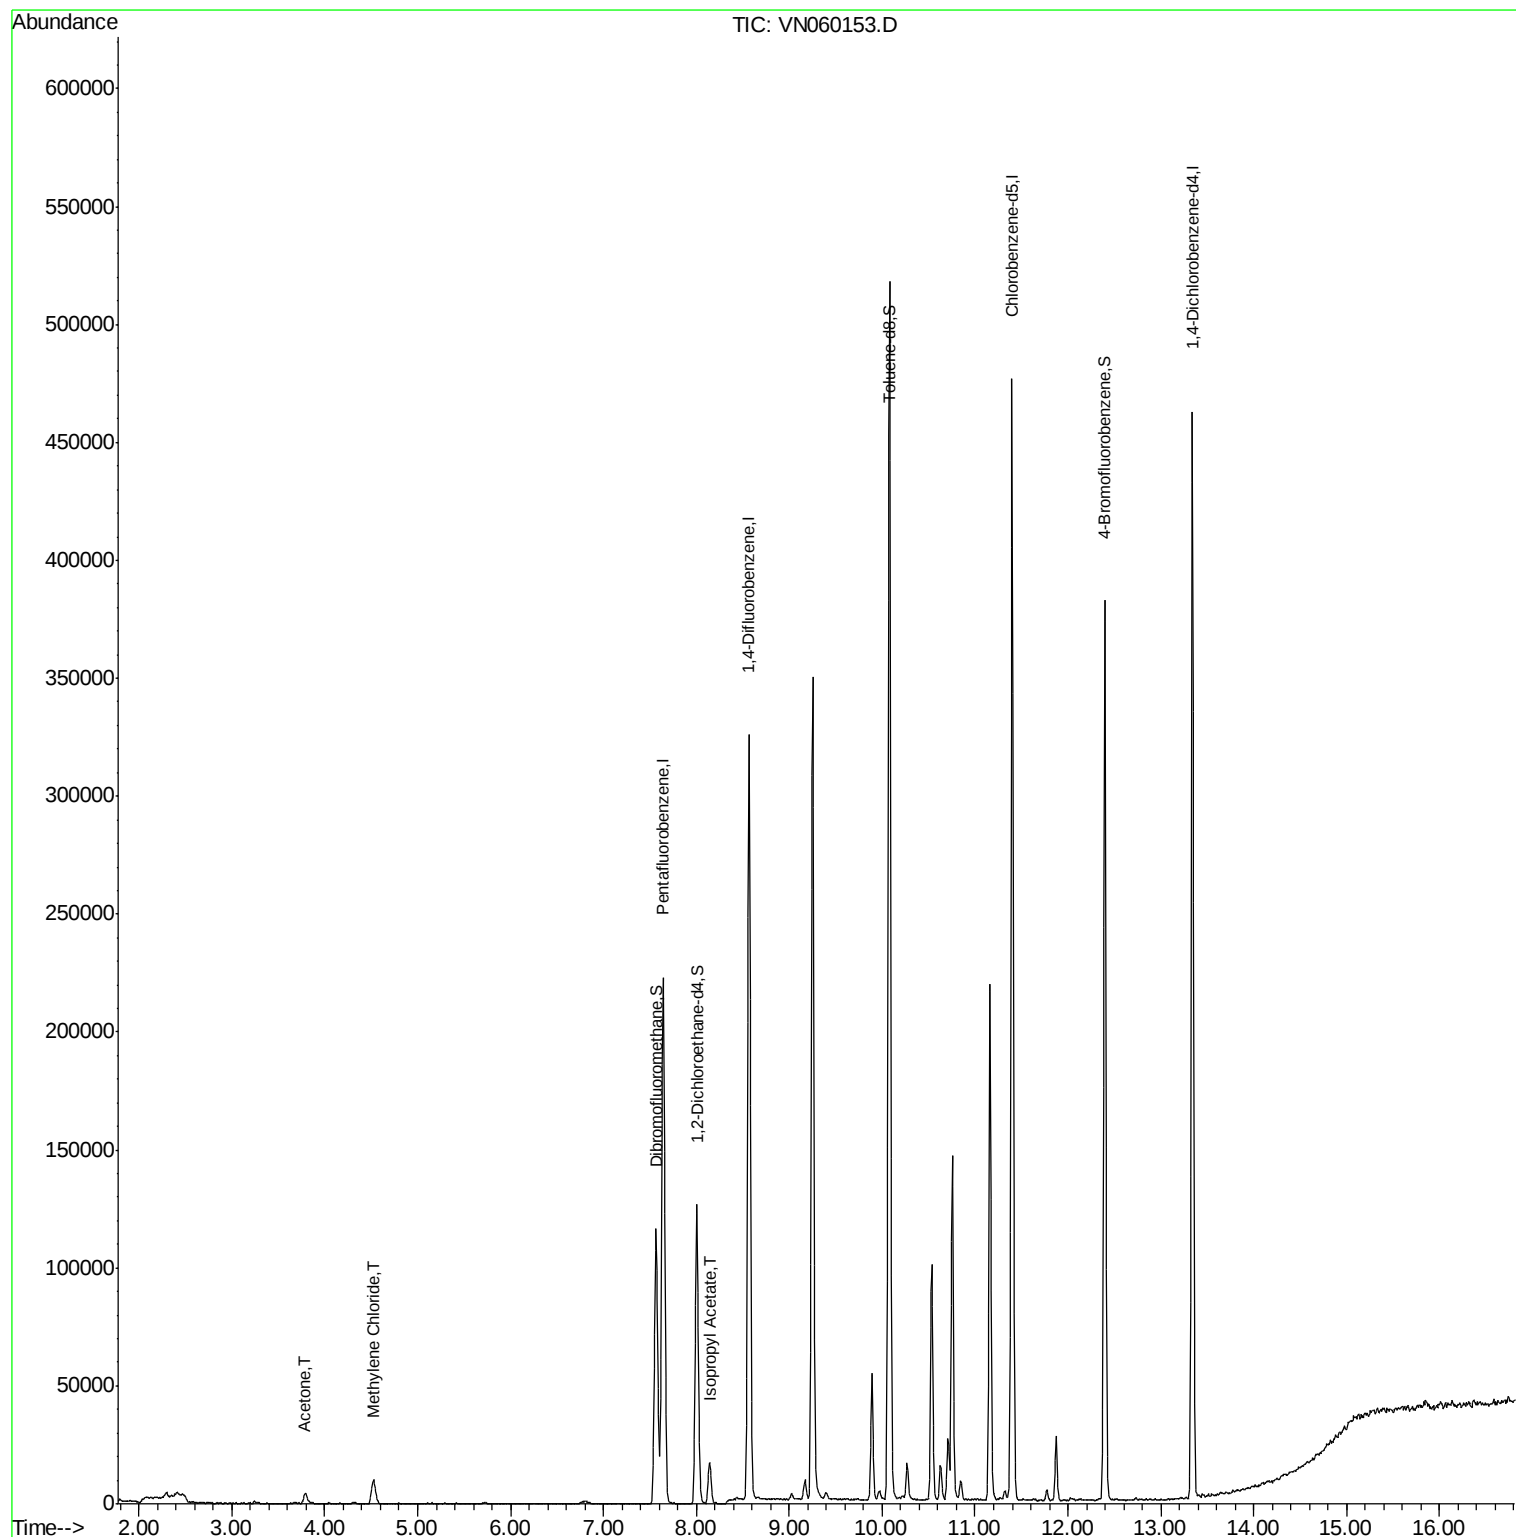



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1826

Delta R.T. -0.00 min

Lab File: VN060153.D

Acq: 19 Feb 2020 14:09

Instrument :

MSVOA_N

ClientSampleId :


BU-03-021820

Tot Ion:168 Resp: 185908

Ion Ratio Lower Upper




168 100

99 52.0 42.7 64.1

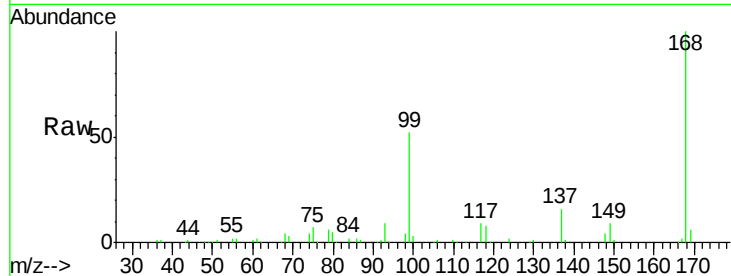

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

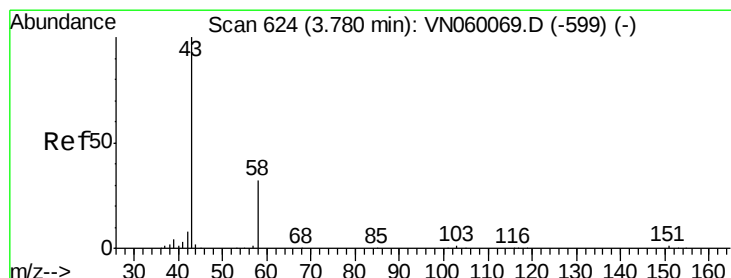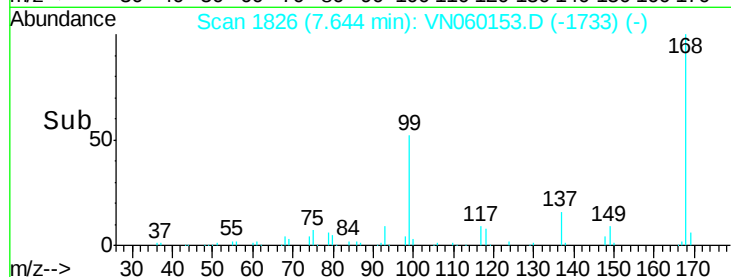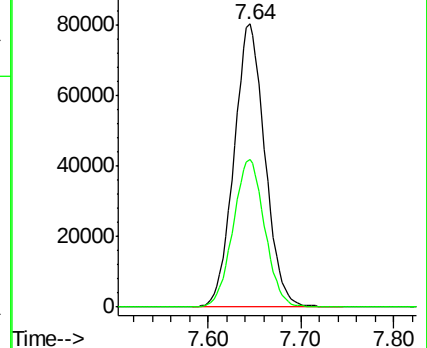

#16

Acetone

Concen: 7.906 ug/l

RT: 3.79 min Scan# 627

Delta R.T. 0.01 min

Lab File: VN060153.D


Acq: 19 Feb 2020 14:09

Tgt Ion: 43 Resp: 7801

Ion Ratio Lower Upper



43 100


58 32.3 25.2 37.8

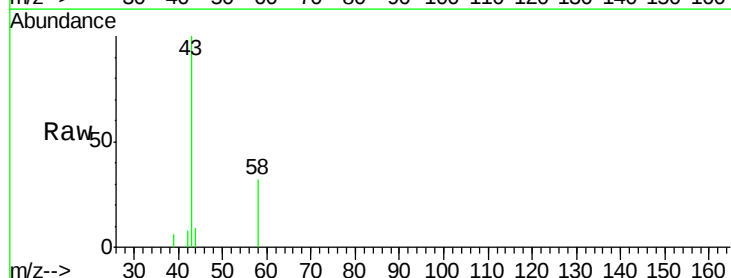

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

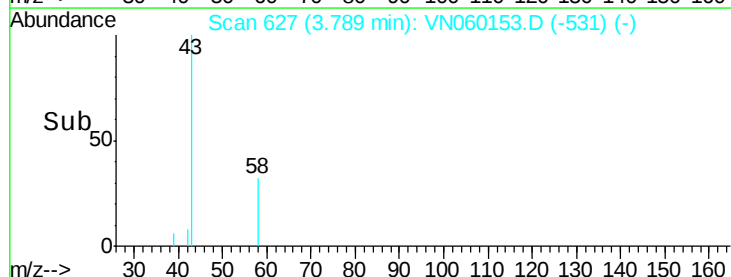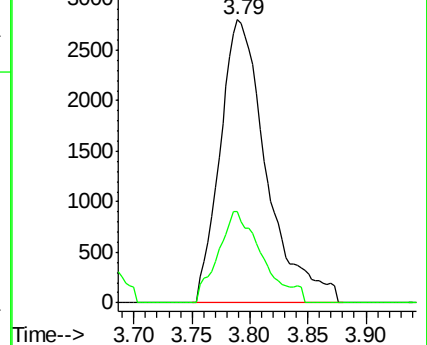

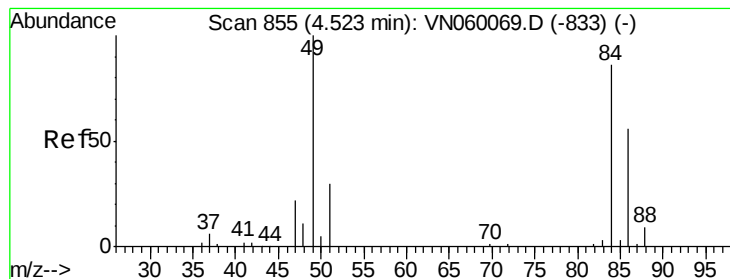

#20

Methylene Chloride

Concen: 4.159 ug/l

RT: 4.53 min Scan# 856

Delta R.T. 0.00 min

Lab File: VN060153.D

Acq: 19 Feb 2020 14:09

Instrument :

MSVOA_N

ClientSampled :

BU-03-021820

Tot Ion: 84 Resp: 8187


Ion Ratio Lower Upper

84 100

49 120.9 93.4 140.0

51 34.8 28.4 42.6

86 62.6 52.5 78.7



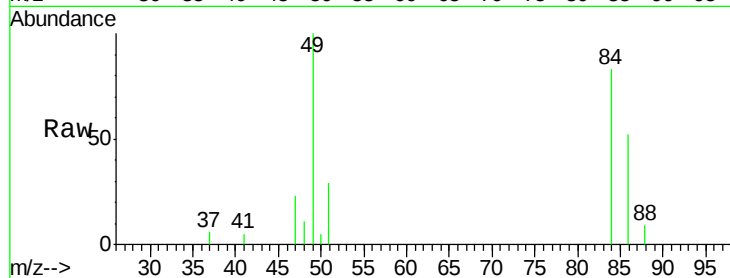


Abundance Ion 83.90 (83.60 to 84.60): VN0

Ion 48.90 (48.60 to 49.60): VN0

Ion 50.90 (50.60 to 51.60): VN0

Ion 85.90 (85.60 to 86.60): VN0

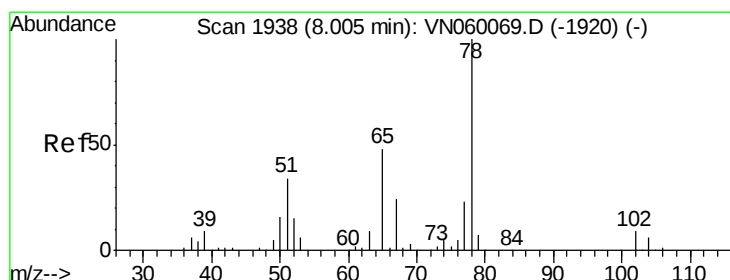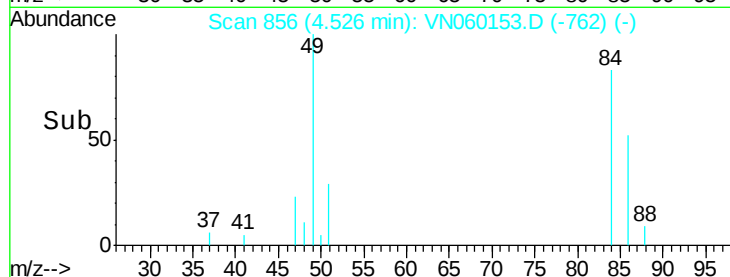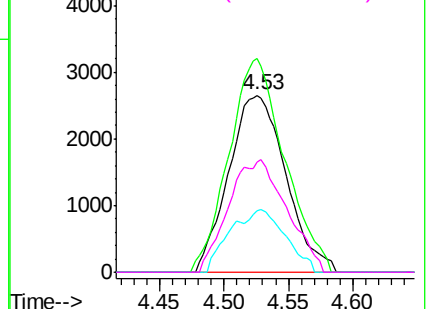

#33

1,2-Dichloroethane-d4

Concen: 47.826 ug/l

RT: 8.00 min Scan# 1938

Delta R.T. -0.00 min

Lab File: VN060153.D


Acq: 19 Feb 2020 14:09

Tgt Ion: 65 Resp: 108192

Ion Ratio Lower Upper



65 100


67 52.0 0.0 104.0

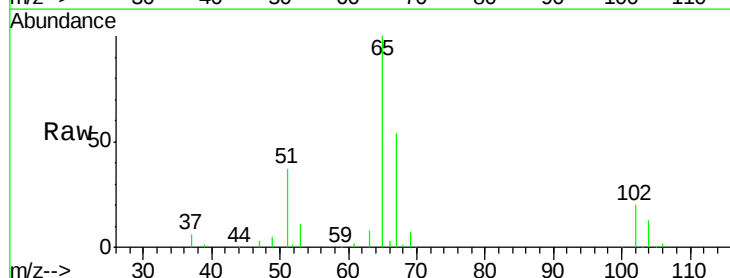

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

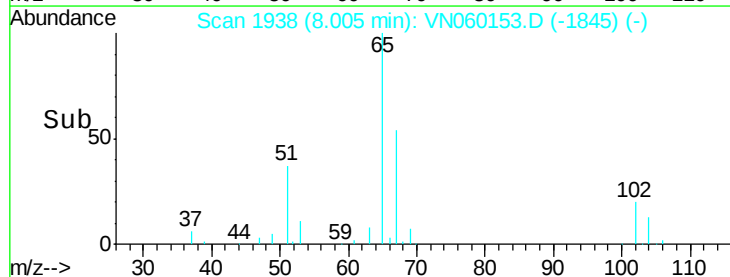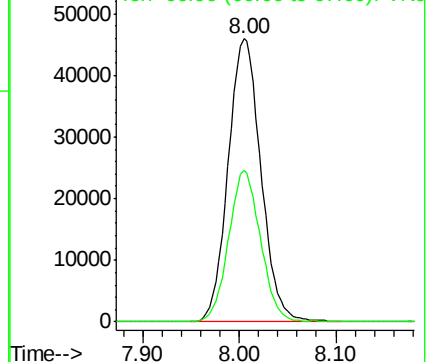


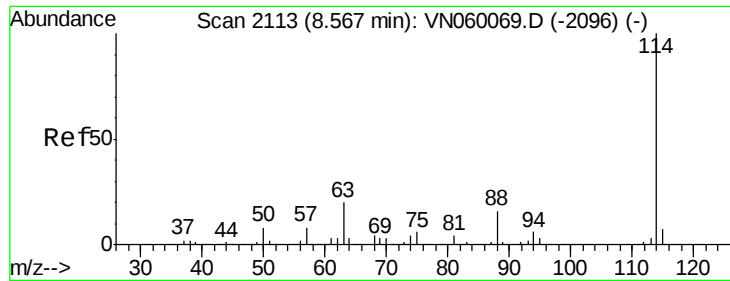




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.57 min Scan# 2113
 Delta R.T. -0.00 min
 Lab File: VN060153.D
 Acq: 19 Feb 2020 14:09

Instrument :
 MSVOA_N
 ClientSampleId :
 BU-03-021820

Tot Ion:114 Resp: 296221
 Ion Ratio Lower Upper
 114 100
 63 19.5 0.0 40.0
 88 14.8 0.0 31.6

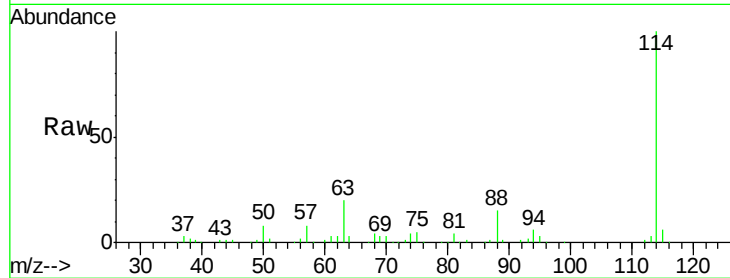


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

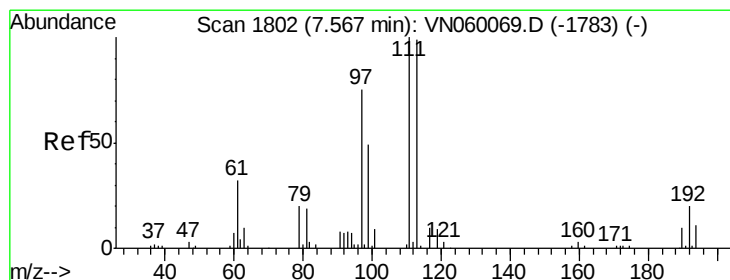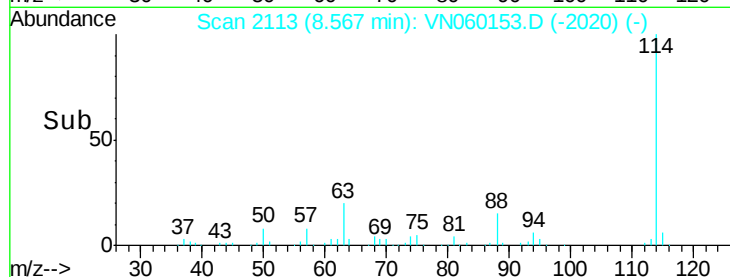
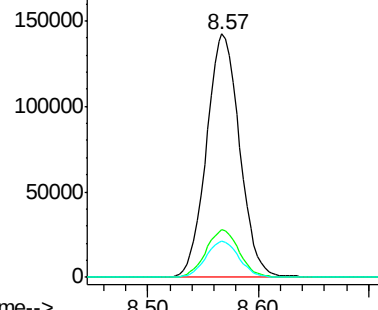



#35
 Dibromofluoromethane
 Concen: 48.970 ug/l
 RT: 7.57 min Scan# 1803
 Delta R.T. 0.00 min
 Lab File: VN060153.D
 Acq: 19 Feb 2020 14:09

Tgt Ion:113 Resp: 89168
 Ion Ratio Lower Upper
 113 100
 111 102.0 81.4 122.2
 192 20.6 16.2 24.2

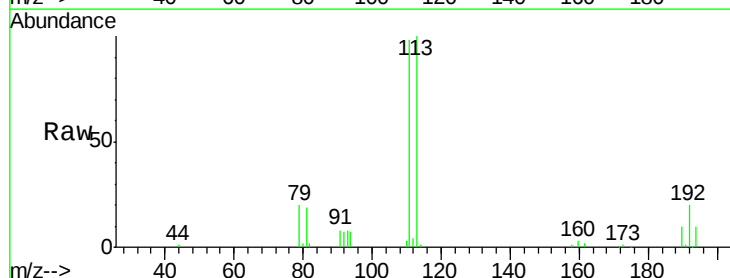

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

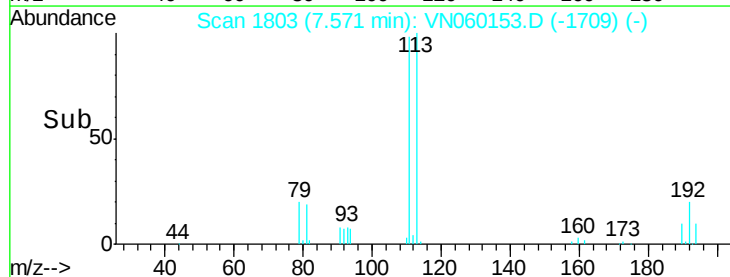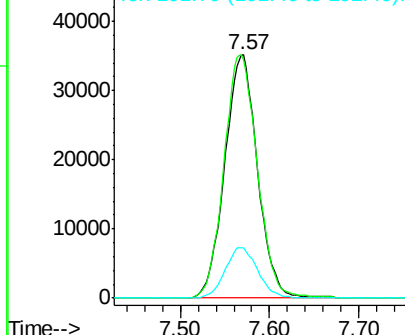

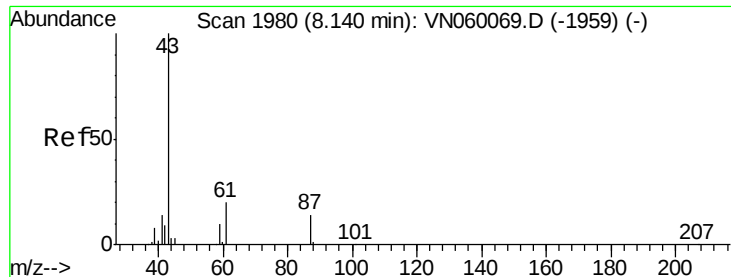

#43

Isopropyl Acetate

Concen: 5.118 ug/l

RT: 8.14 min Scan# 1981

Delta R.T. 0.00 min

Lab File: VN060153.D

Acq: 19 Feb 2020 14:09

Instrument :

MSVOA_N

ClientSampleId :

BU-03-021820


Tot Ion: 43 Resp: 21693

Ion Ratio Lower Upper

43 100

61 17.8 21.8 32.6#

87 13.2 11.4 17.2

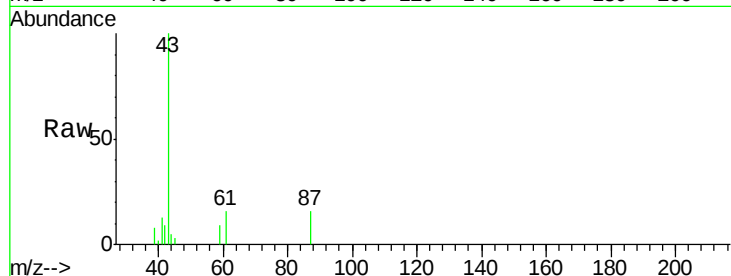



Abundance Ion 43.00 (42.70 to 43.70): VN060069.D (-1959) (-)

Ion 61.00 (60.70 to 61.70): VN060069.D (-1959) (-)

Ion 87.00 (86.70 to 87.70): VN060069.D (-1959) (-)

8.14

Time-->

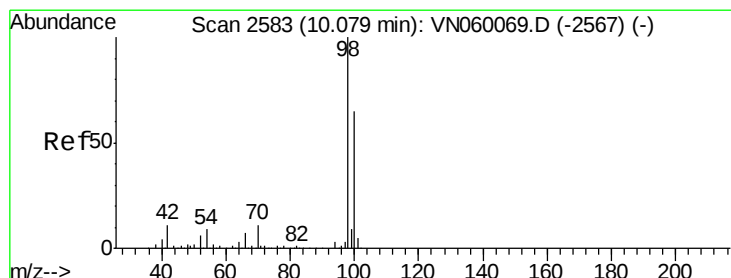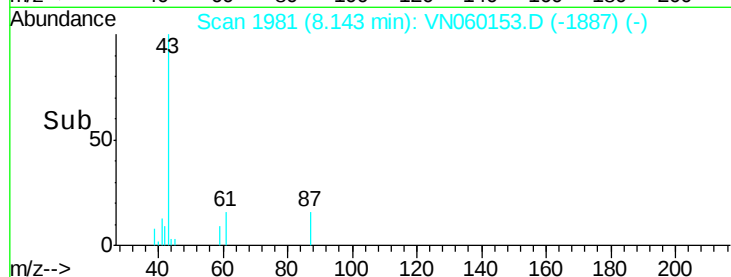

#50

Toluene-d8

Concen: 49.662 ug/l

RT: 10.08 min Scan# 2583

Delta R.T. -0.00 min

Lab File: VN060153.D


Acq: 19 Feb 2020 14:09

Tgt Ion: 98 Resp: 356102

Ion Ratio Lower Upper

98 100

100 64.8 51.7 77.5

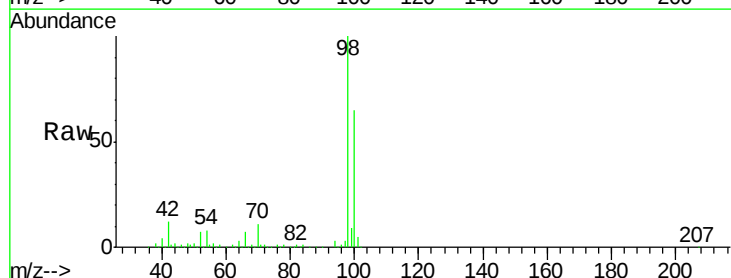



Abundance Ion 98.00 (97.70 to 98.70): VN060069.D (-2567) (-)

Ion 100.00 (99.70 to 100.70): VN060069.D (-2567) (-)

10.08

Time-->

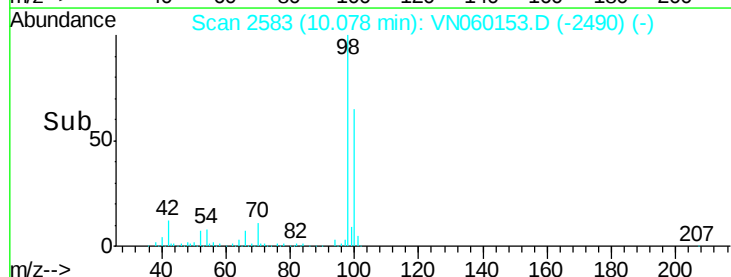

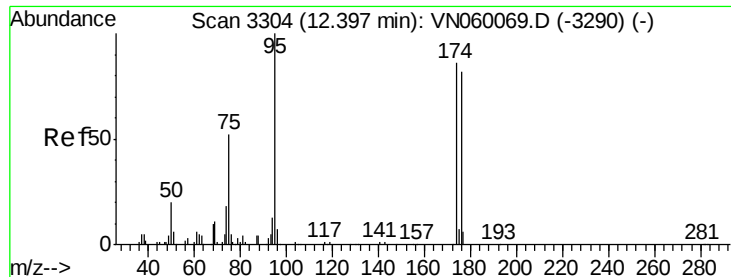

#62

4-Bromofluorobenzene

Concen: 48.617 ug/l

RT: 12.40 min Scan# 3304

Delta R.T. -0.00 min

Lab File: VN060153.D

Acq: 19 Feb 2020 14:09

Instrument :

MSVOA_N

ClientSampled :

BU-03-021820


Tot Ion: 95 Resp: 128098

Ion Ratio Lower Upper

95 100

174 85.2 0.0 169.8




176 82.3 0.0 164.8

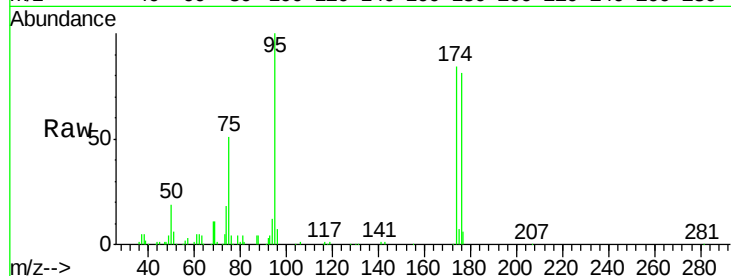

Abundance Ion 94.90 (94.60 to 95.60): VN060153.D (-3211) (-)

Ion 173.80 (173.50 to 174.50): VN060153.D (-3211) (-)

Ion 175.80 (175.50 to 176.50): VN060153.D (-3211) (-)

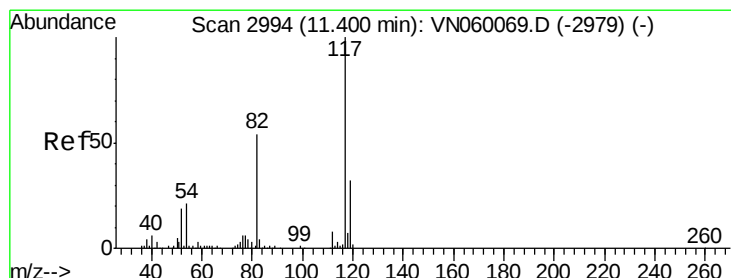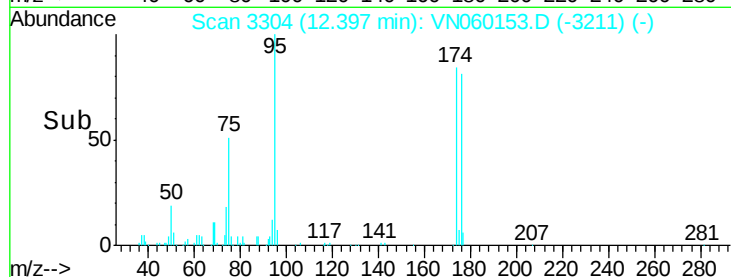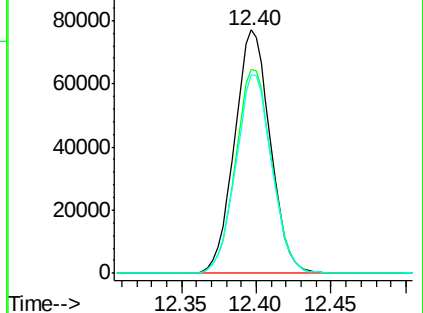

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.40 min Scan# 2994

Delta R.T. -0.00 min

Lab File: VN060153.D

Acq: 19 Feb 2020 14:09


Tgt Ion: 117 Resp: 275230

Ion Ratio Lower Upper

117 100

82 54.7 43.4 65.0



119 32.2 25.8 38.6

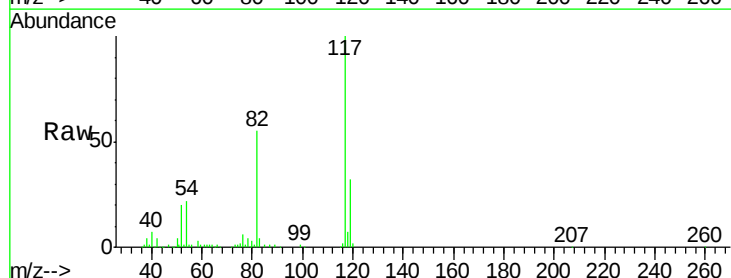


Abundance Ion 116.90 (116.60 to 117.60): VN060153.D (-2901) (-)

Ion 82.00 (81.70 to 82.70): VN060153.D (-2901) (-)

Ion 118.90 (118.60 to 119.60): VN060153.D (-2901) (-)

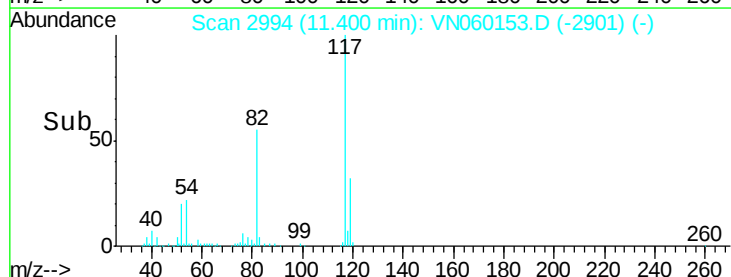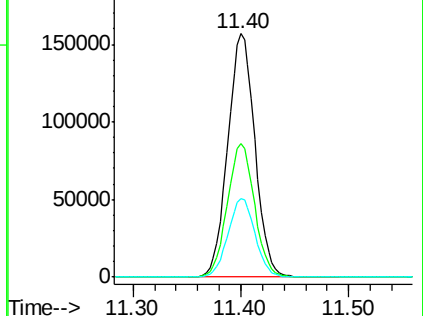

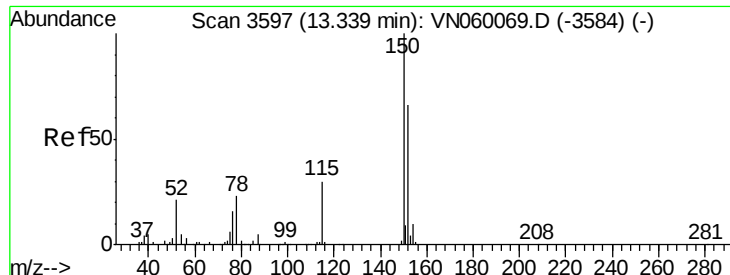

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3597

Delta R.T. -0.00 min

Lab File: VN060153.D

Acq: 19 Feb 2020 14:09

Instrument :

MSVOA_N

ClientSampleId :

BU-03-021820


Tot Ion:152 Resp: 124919

Ion Ratio Lower Upper

152 100

115 57.7 28.9 86.8

150 156.5 0.0 342.4

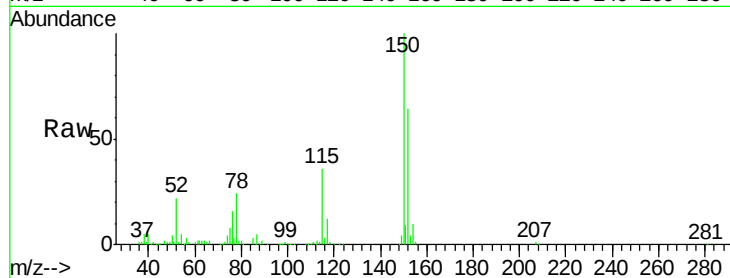

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

