
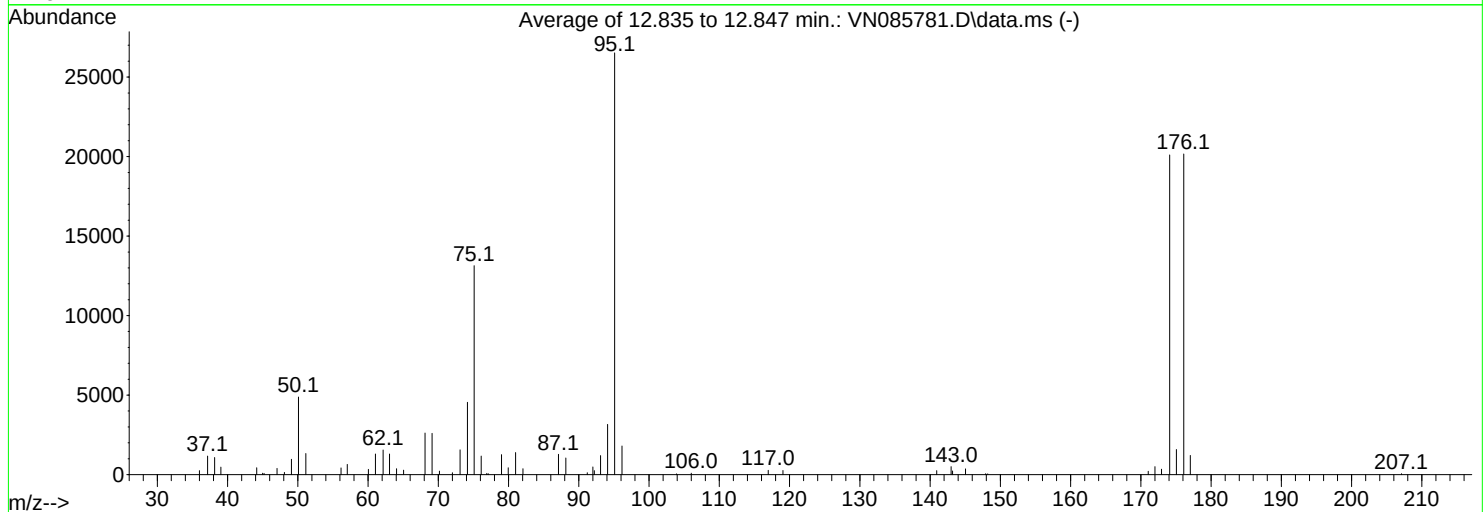


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN021925\
Data File : VN085781.D
Acq On : 19 Feb 2025 10:14
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Title : SW846 8260
Last Update : Wed Feb 19 03:43:32 2025

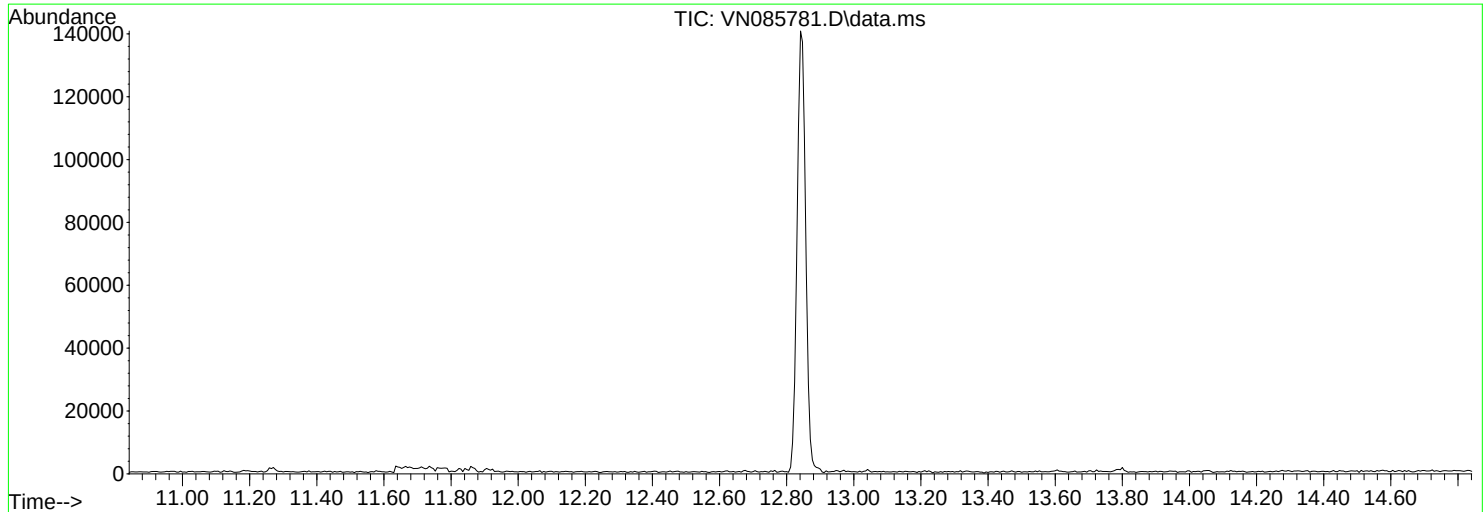

AutoFind: Scans 1850, 1851, 1852; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	4884	PASS
75	95	30	60	49.6	13144	PASS
95	95	100	100	100.0	26523	PASS
96	95	5	9	6.8	1797	PASS
173	174	0.00	2	1.7	338	PASS
174	95	50	100	75.8	20107	PASS
175	174	5	9	7.9	1580	PASS
176	174	95	101	100.3	20159	PASS
177	176	5	9	6.0	1207	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	255	51.15	1328	70.15	217	82.05	361
37.15	1163	56.15	420	72.00	117	87.10	127
38.15	1074	57.05	649	73.10	1561	88.15	105
39.05	472	60.05	337	74.15	4549	91.20	11
44.15	436	61.05	1300	75.10	13144	92.00	480
45.00	86	62.15	1545	76.10	1169	92.20	248
45.20	83	63.05	1297	76.90	78	93.10	1200
47.05	389	64.05	372	77.10	65	94.10	3158
48.10	140	65.05	281	79.00	1260	95.10	26523
49.10	965	68.10	2615	79.95	429	96.15	1797
50.10	4884	69.10	2598	81.00	1390	103.90	55

Average of 12.835 to 12.847 min.: VN085781.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
106.00	92	172.95	338				
116.95	274	174.10	20107				
119.05	260	175.05	1580				
140.95	253	176.10	20159				
143.00	502	177.05	1207				
143.20	229	207.10	58				
145.05	362						
147.90	60						
148.20	54						
171.05	210						
172.00	502						

Instrument :

MSVOA_N

ClientSampleId :

BFB