




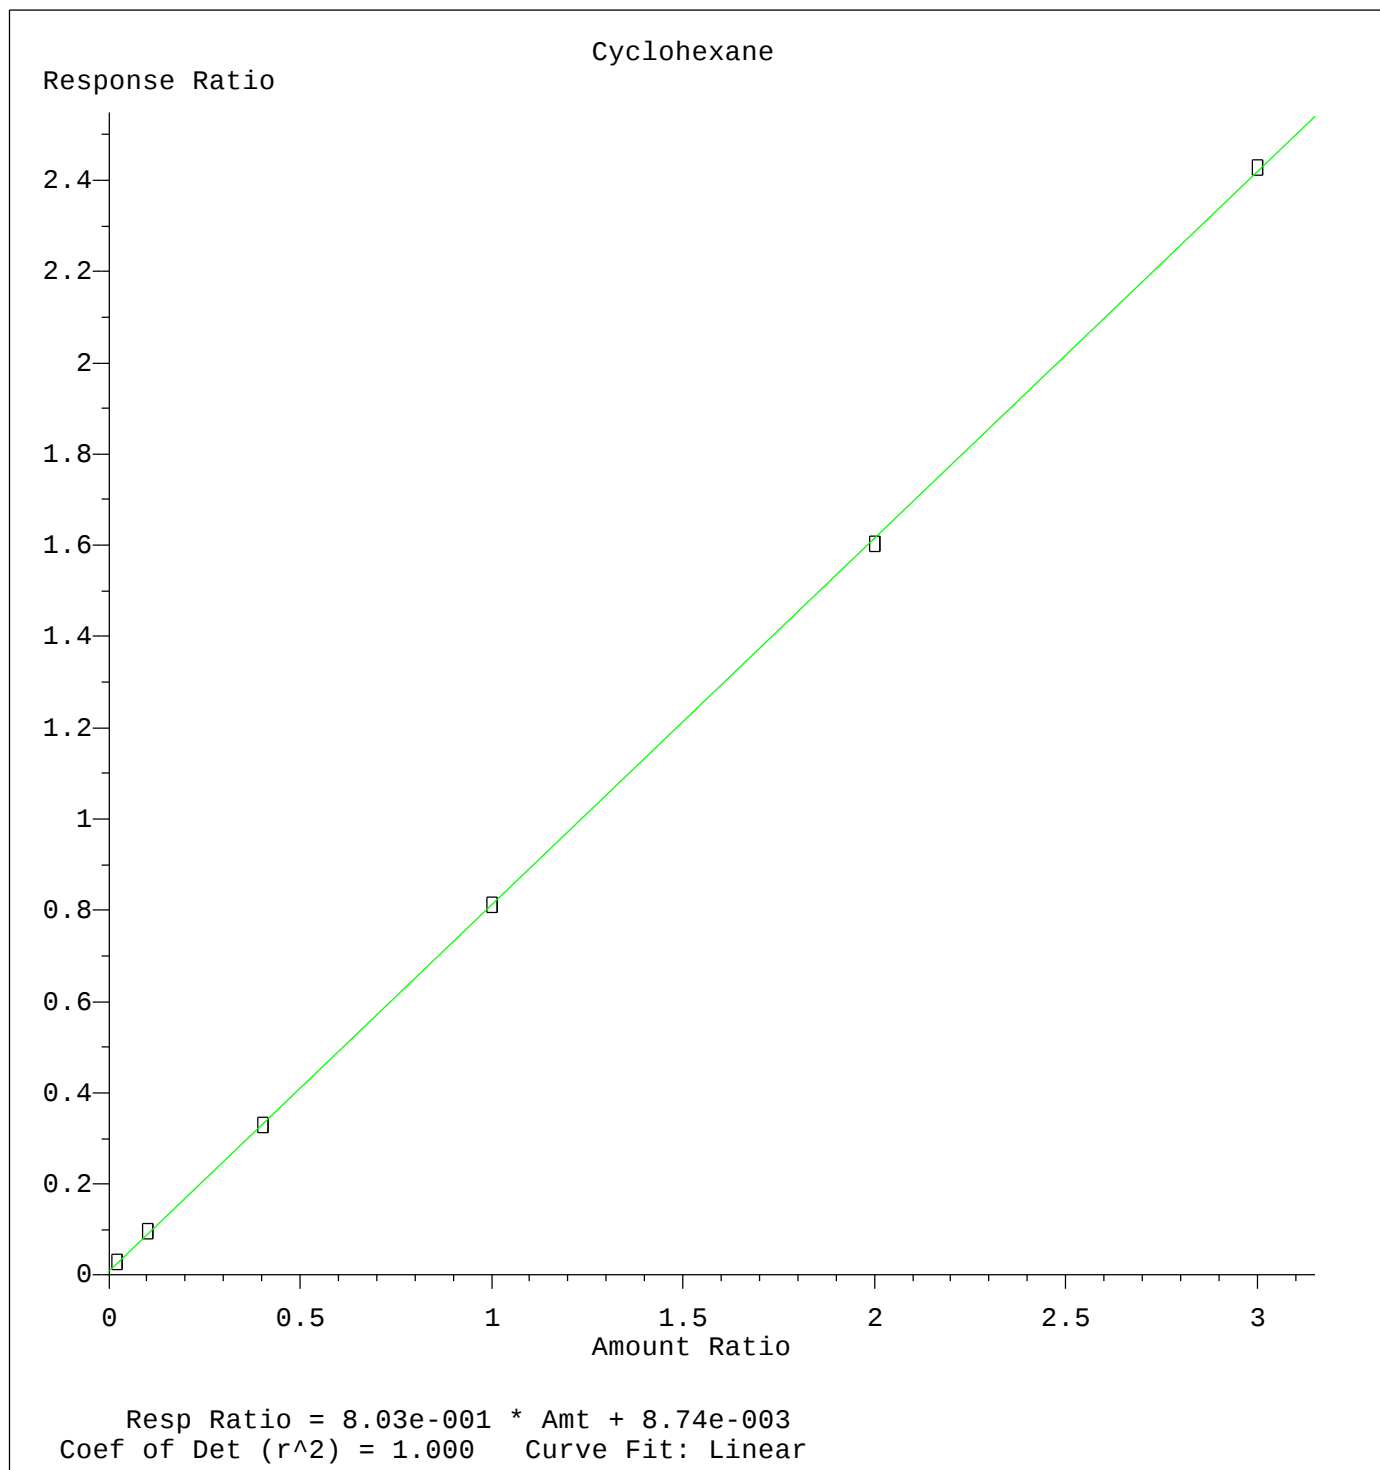


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022019W.M
Calibration Table Last Updated: Thu Feb 21 03:36:07 2019

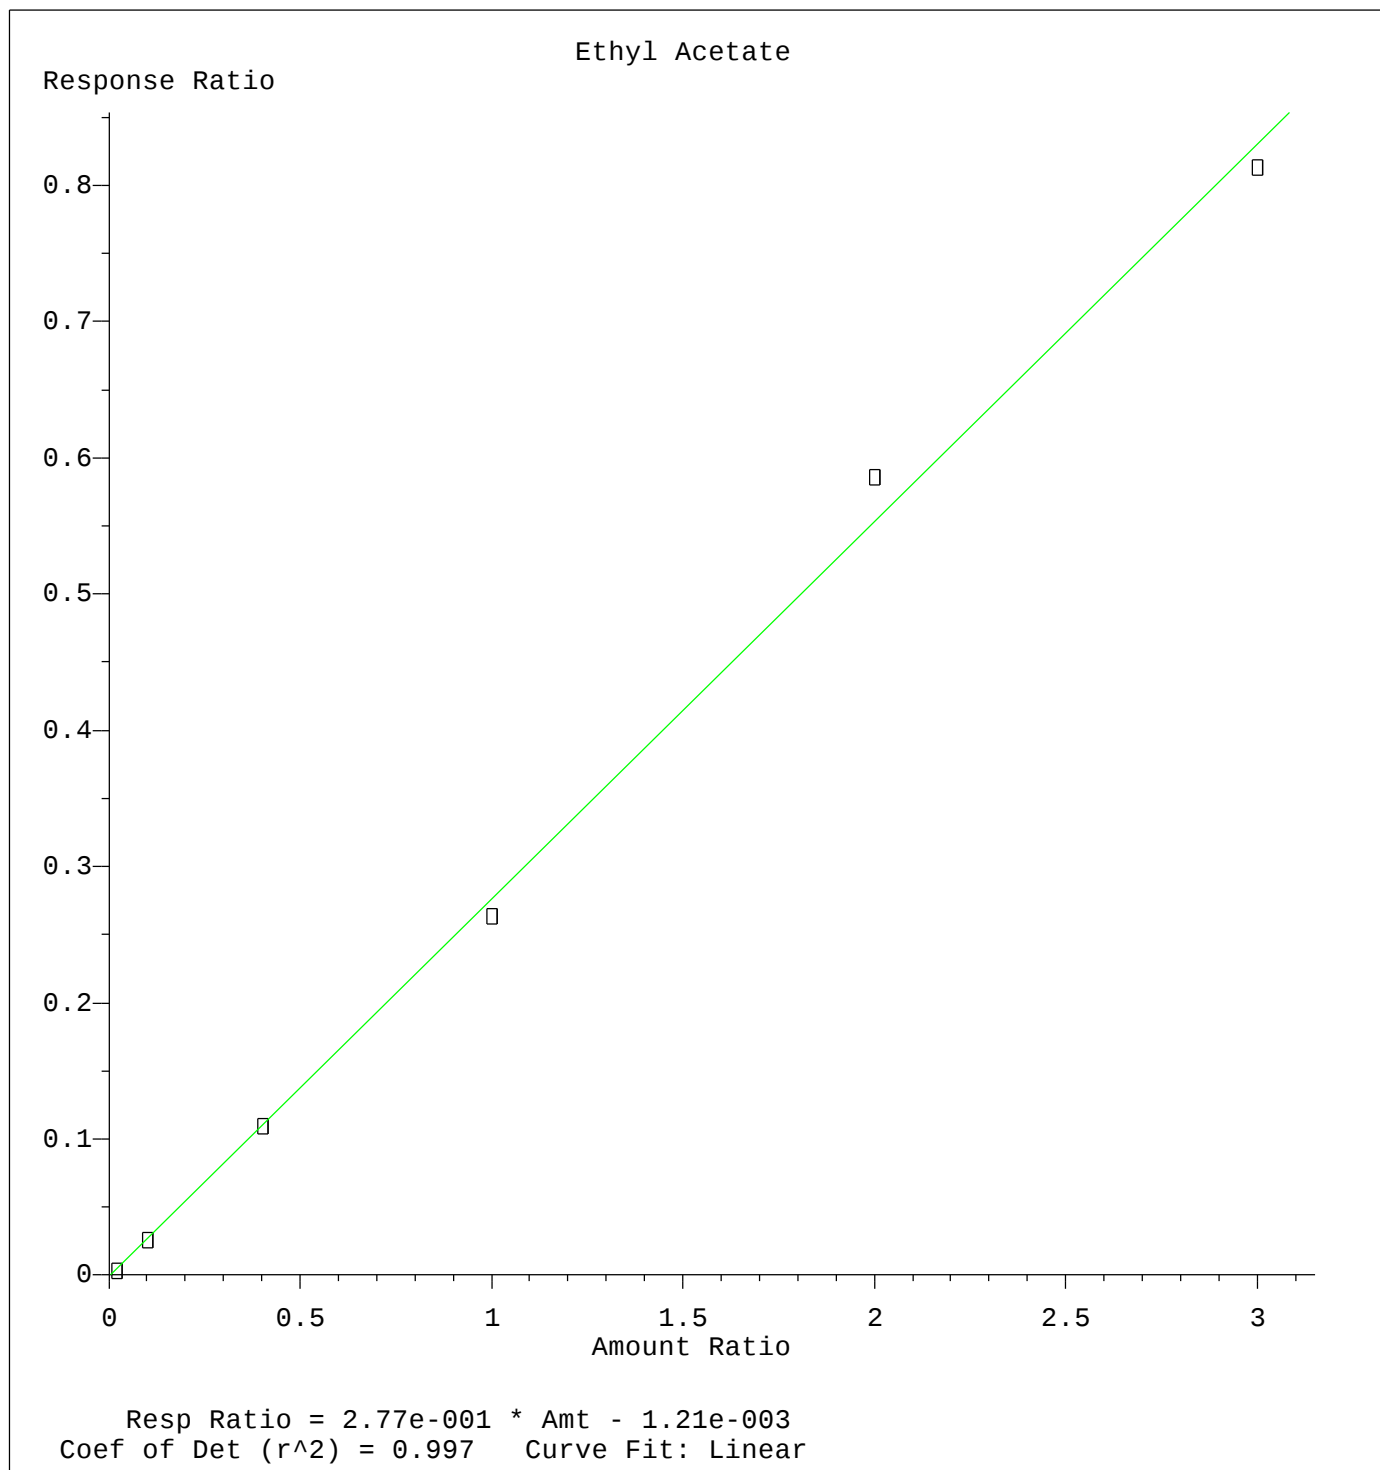


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022019W.M
Calibration Table Last Updated: Thu Feb 21 03:36:07 2019

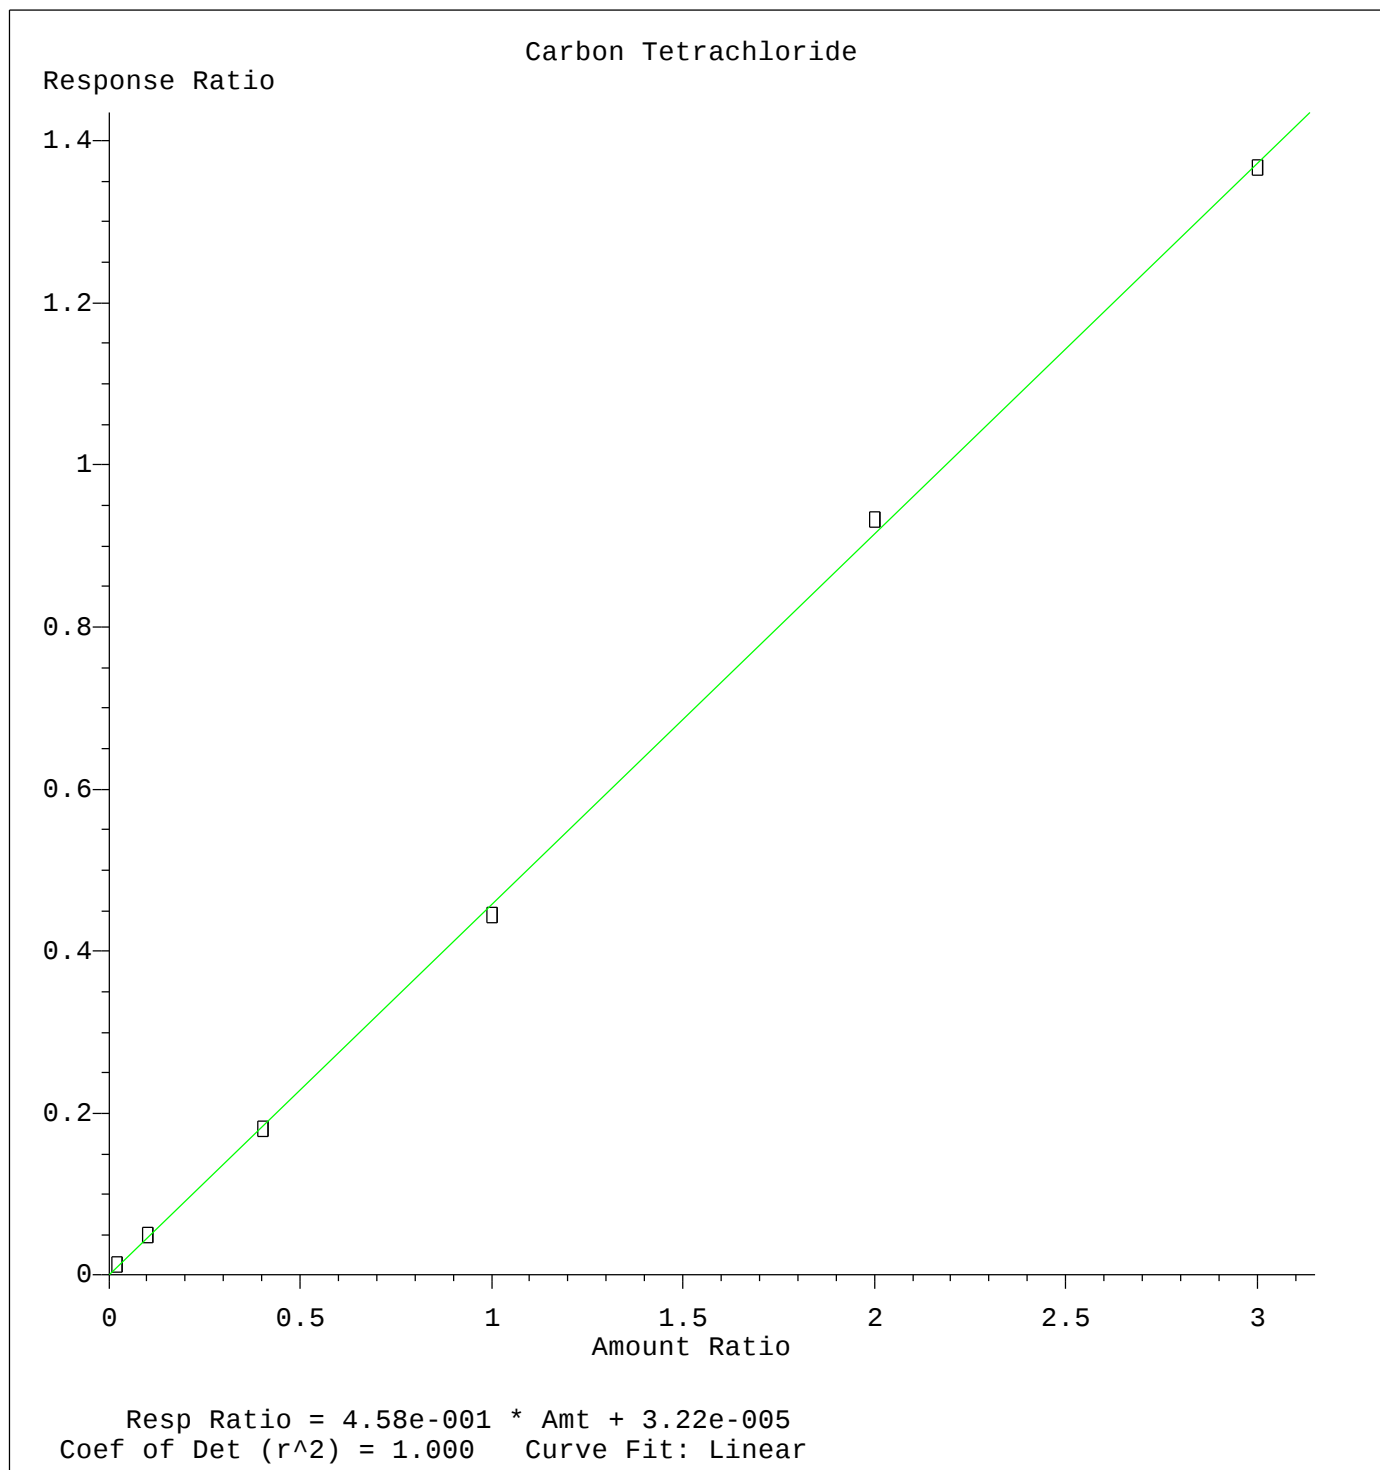

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022019W.M
Calibration Table Last Updated: Thu Feb 21 03:36:07 2019

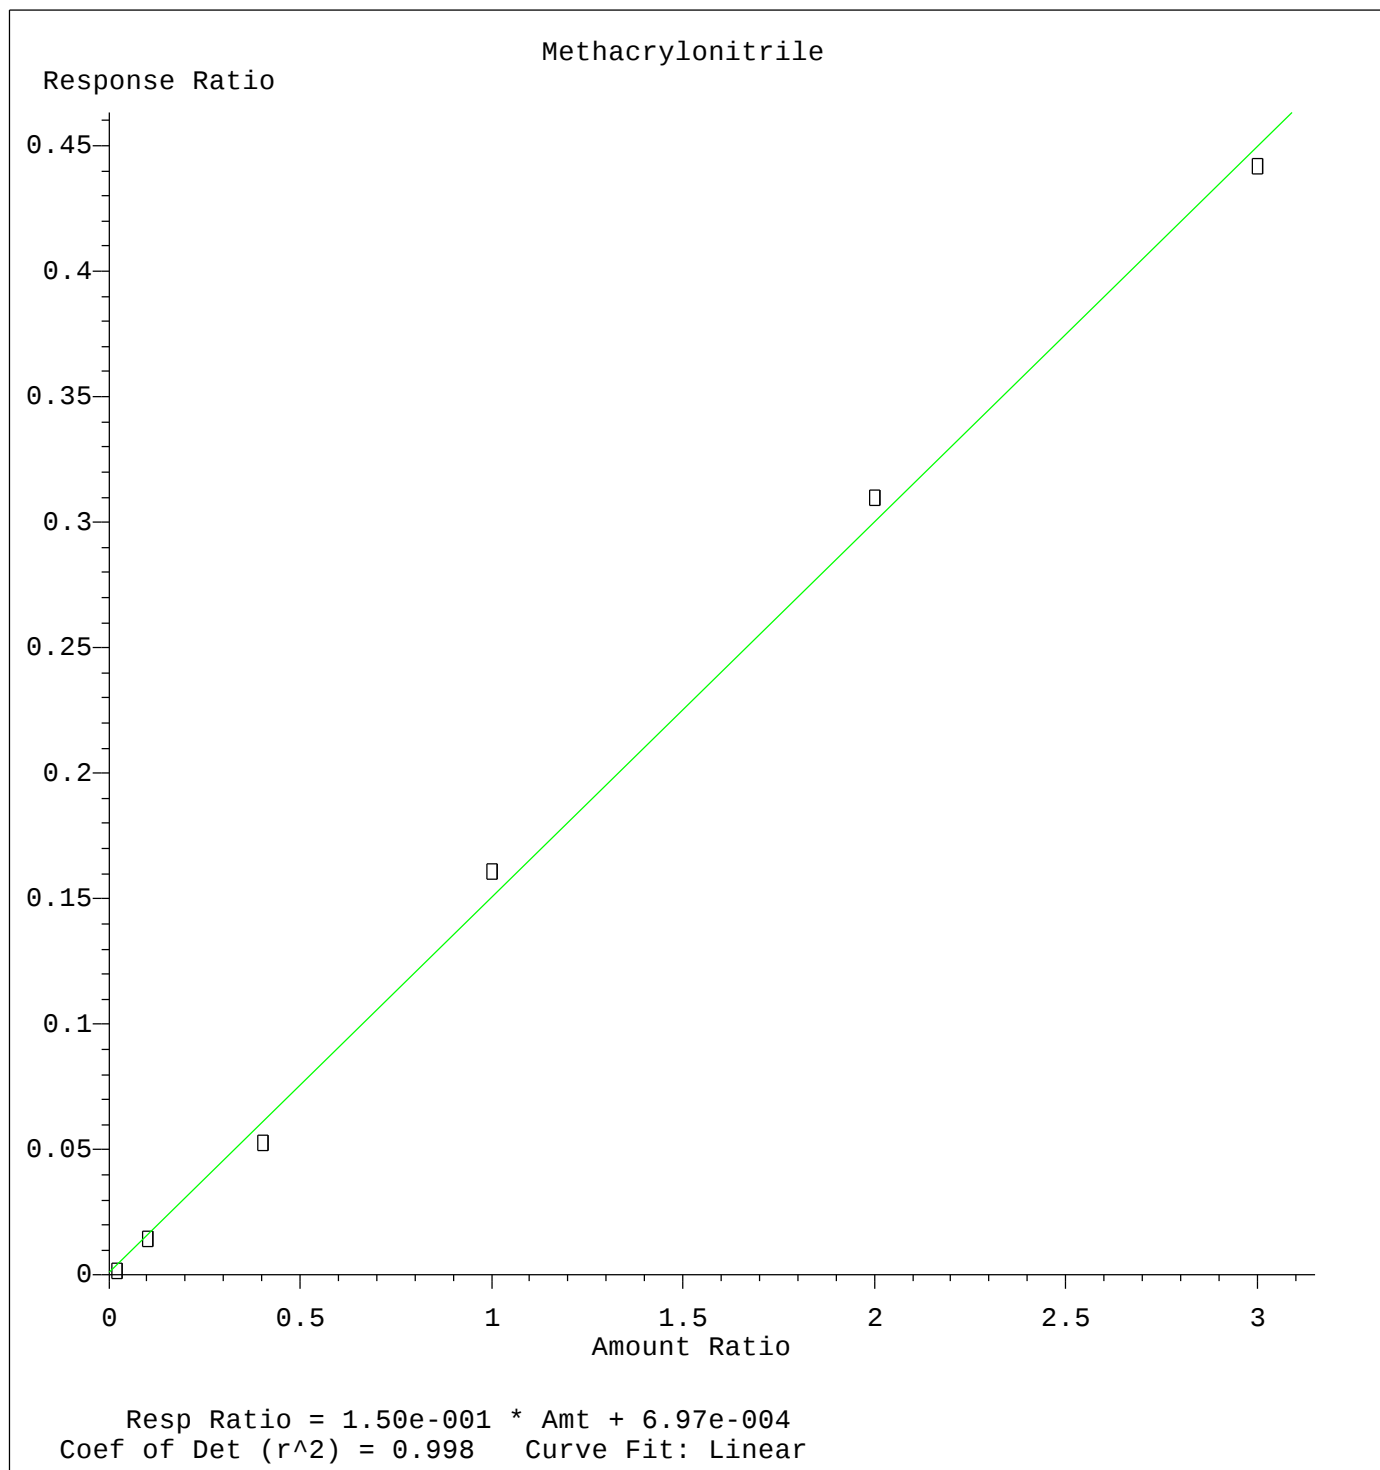


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022019W.M
Calibration Table Last Updated: Thu Feb 21 03:36:07 2019

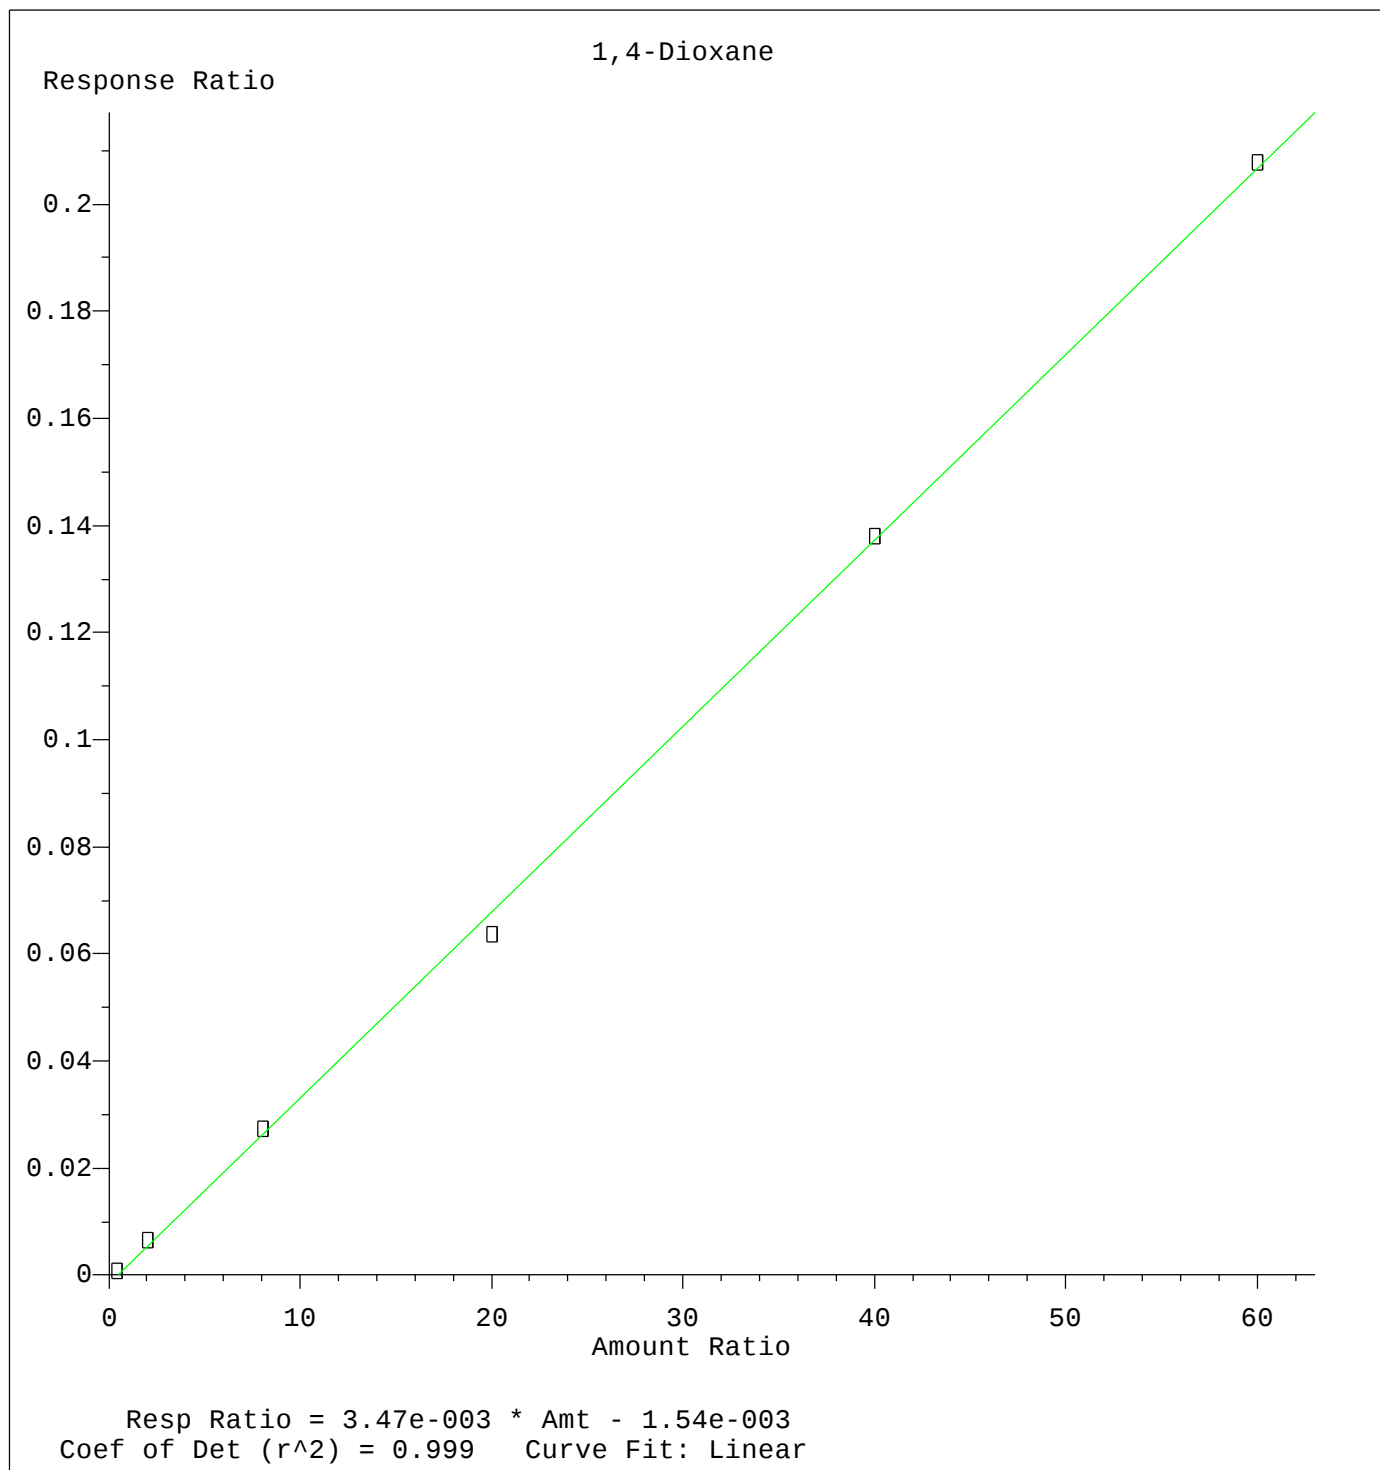

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022019W.M
Calibration Table Last Updated: Thu Feb 21 03:36:07 2019


4-Methyl-2-Pentanone

Response Ratio

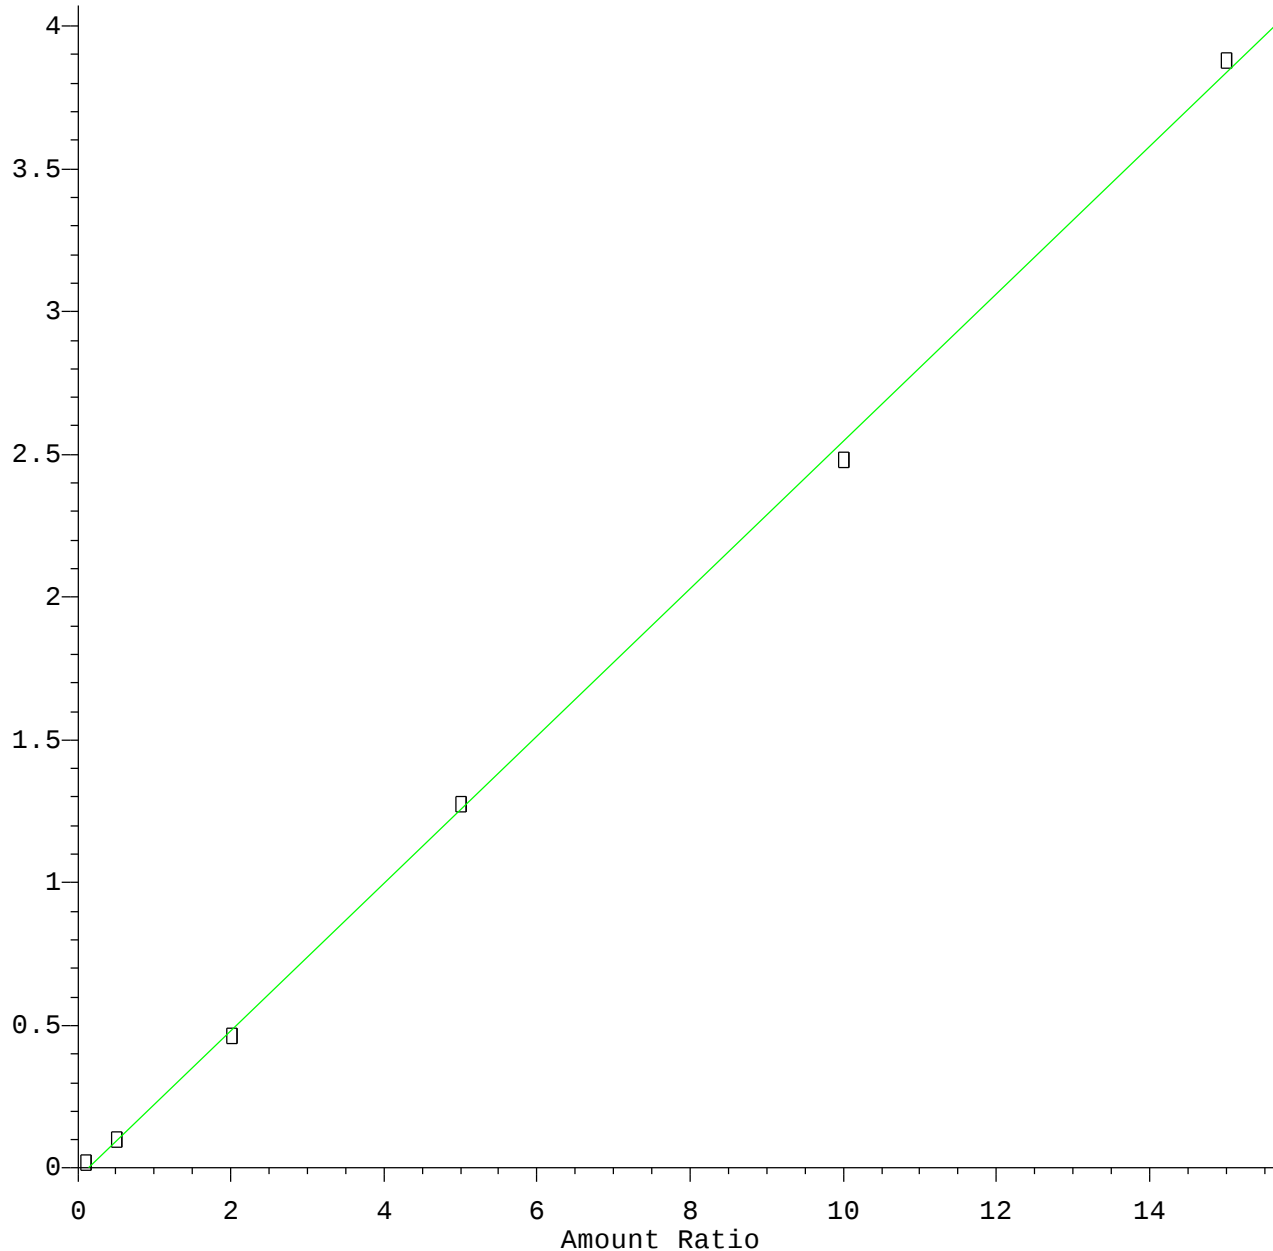

Resp Ratio = 2.58×10^{-1} * Amt - 3.36×10^{-2}
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022019W.M
Calibration Table Last Updated: Thu Feb 21 03:36:07 2019

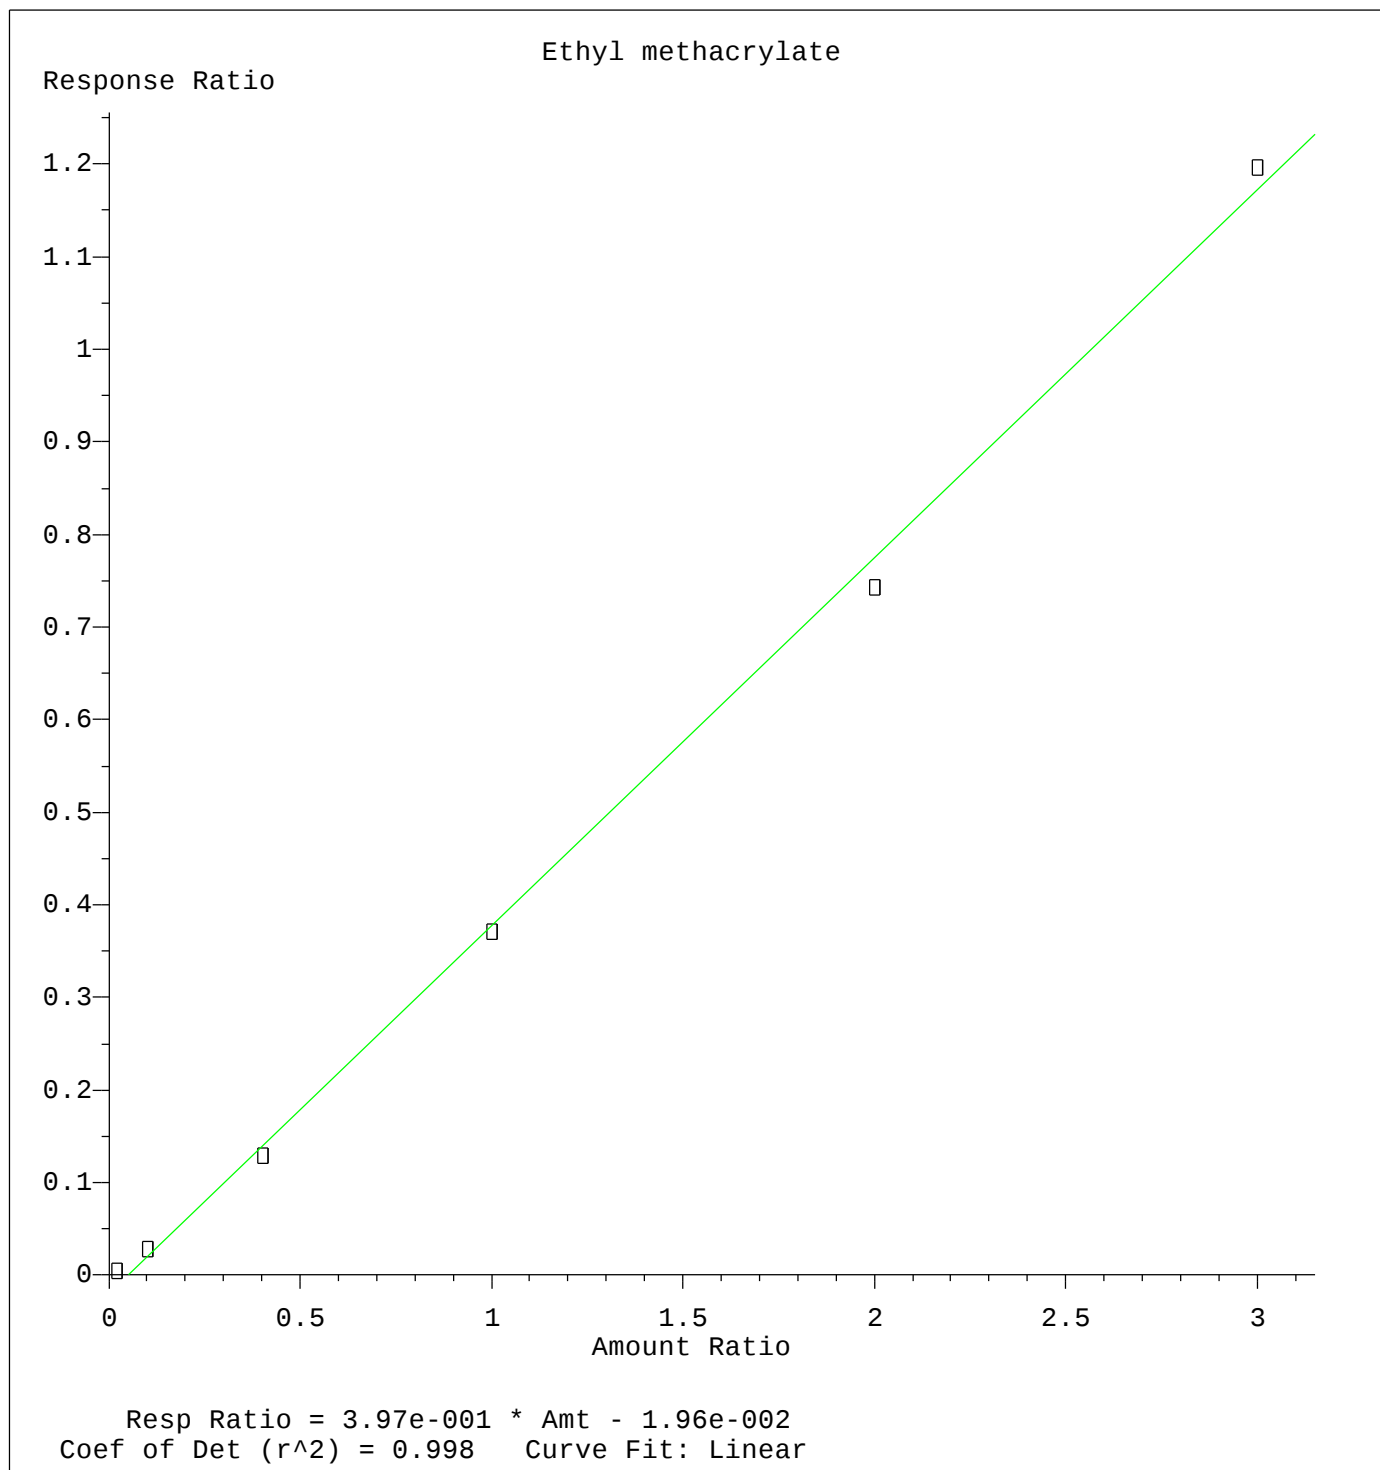

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022019W.M
Calibration Table Last Updated: Thu Feb 21 03:36:07 2019

2-Chloroethyl Vinyl ether

Response Ratio

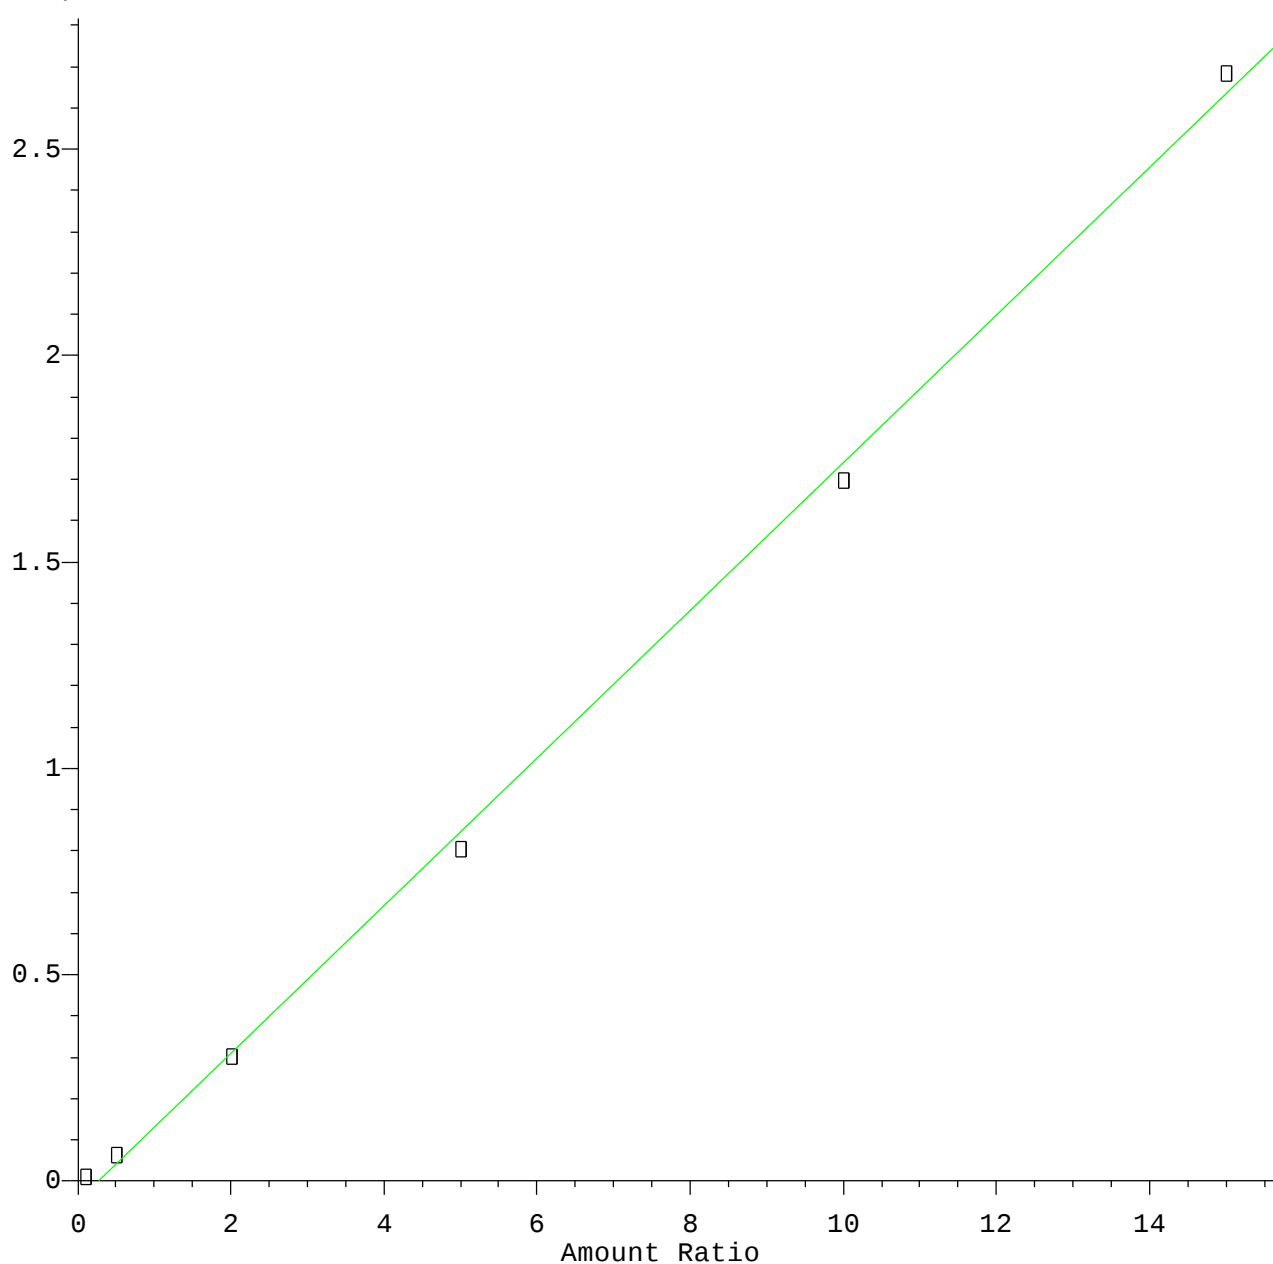


Resp Ratio = $1.79 \times 10^{-1} \times \text{Amt} - 4.64 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022019W.M
Calibration Table Last Updated: Thu Feb 21 03:36:07 2019

1,2,4-Trichlorobenzene

Response Ratio

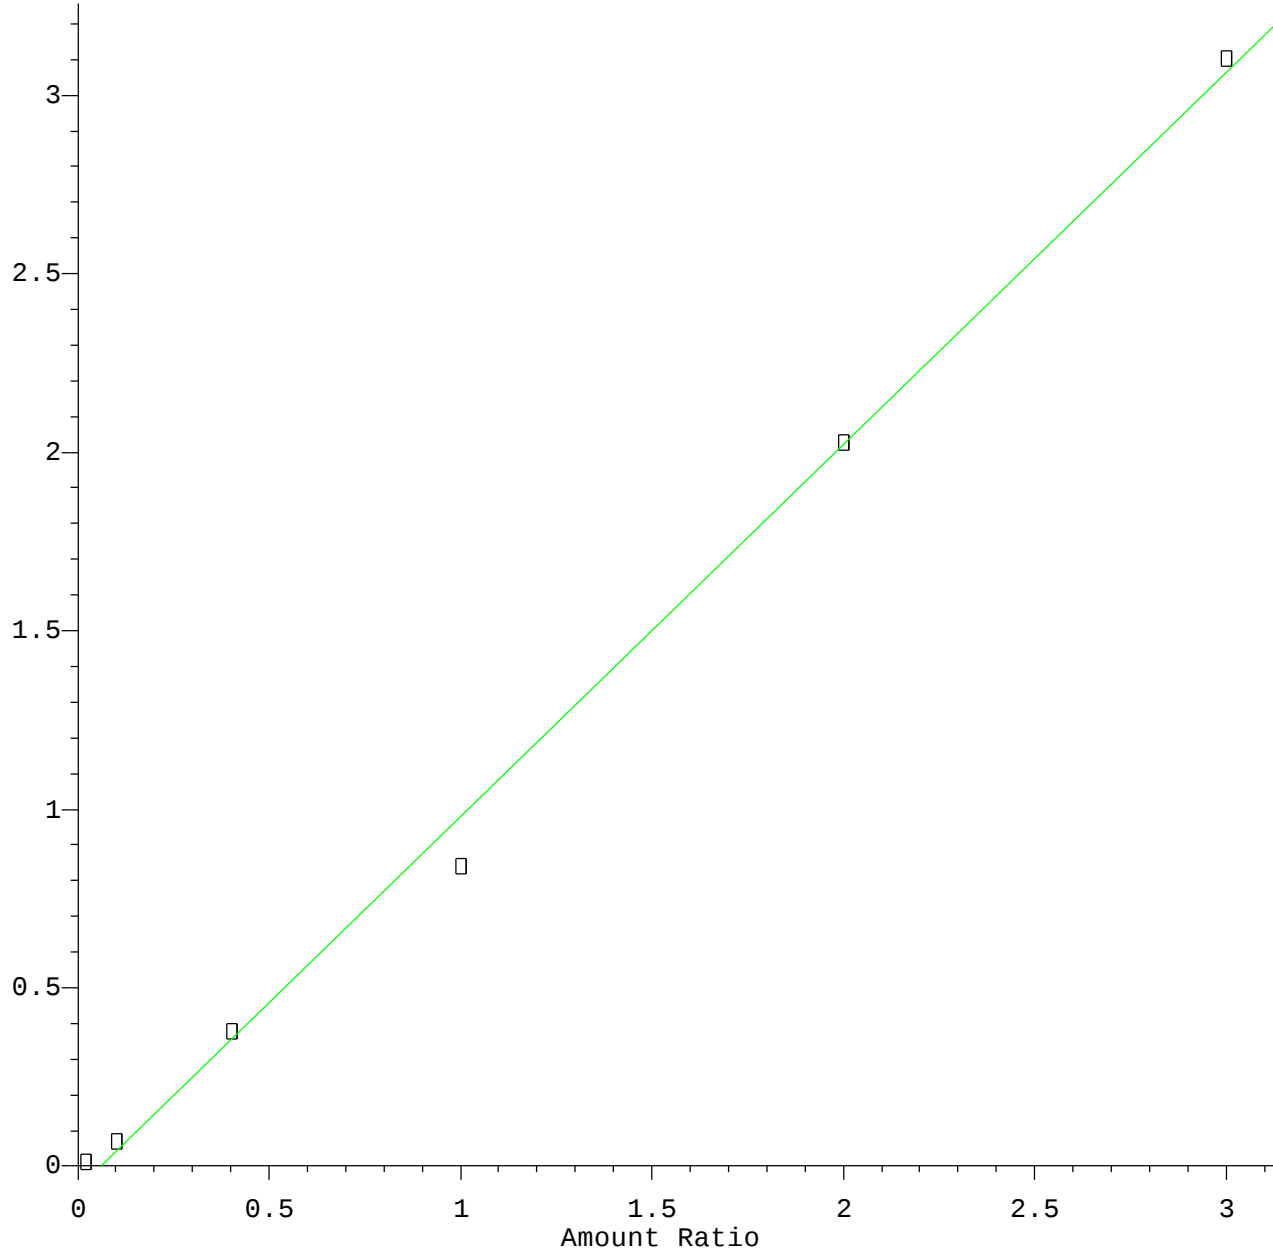


Resp Ratio = 1.04×10^0 * Amt - 6.09×10^{-2}
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022019W.M
Calibration Table Last Updated: Thu Feb 21 03:36:07 2019

Naphthalene

Response Ratio

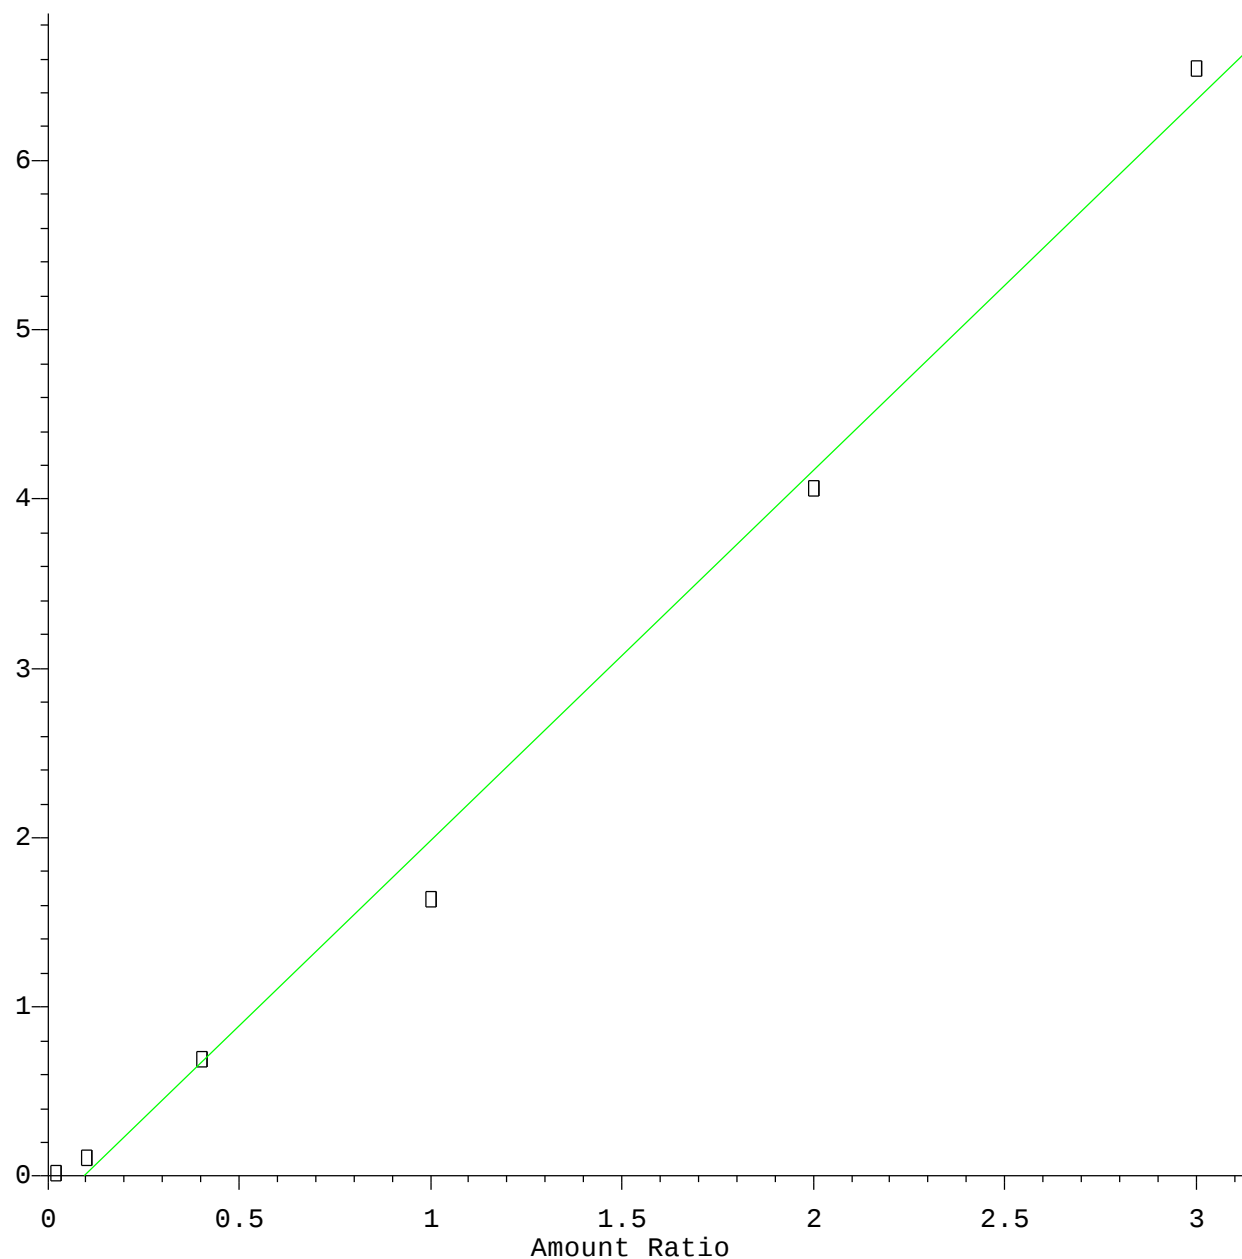


Resp Ratio = 2.19e+000 * Amt - 2.02e-001
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022019W.M
Calibration Table Last Updated: Thu Feb 21 03:36:07 2019

1,2,3-Trichlorobenzene

Response Ratio

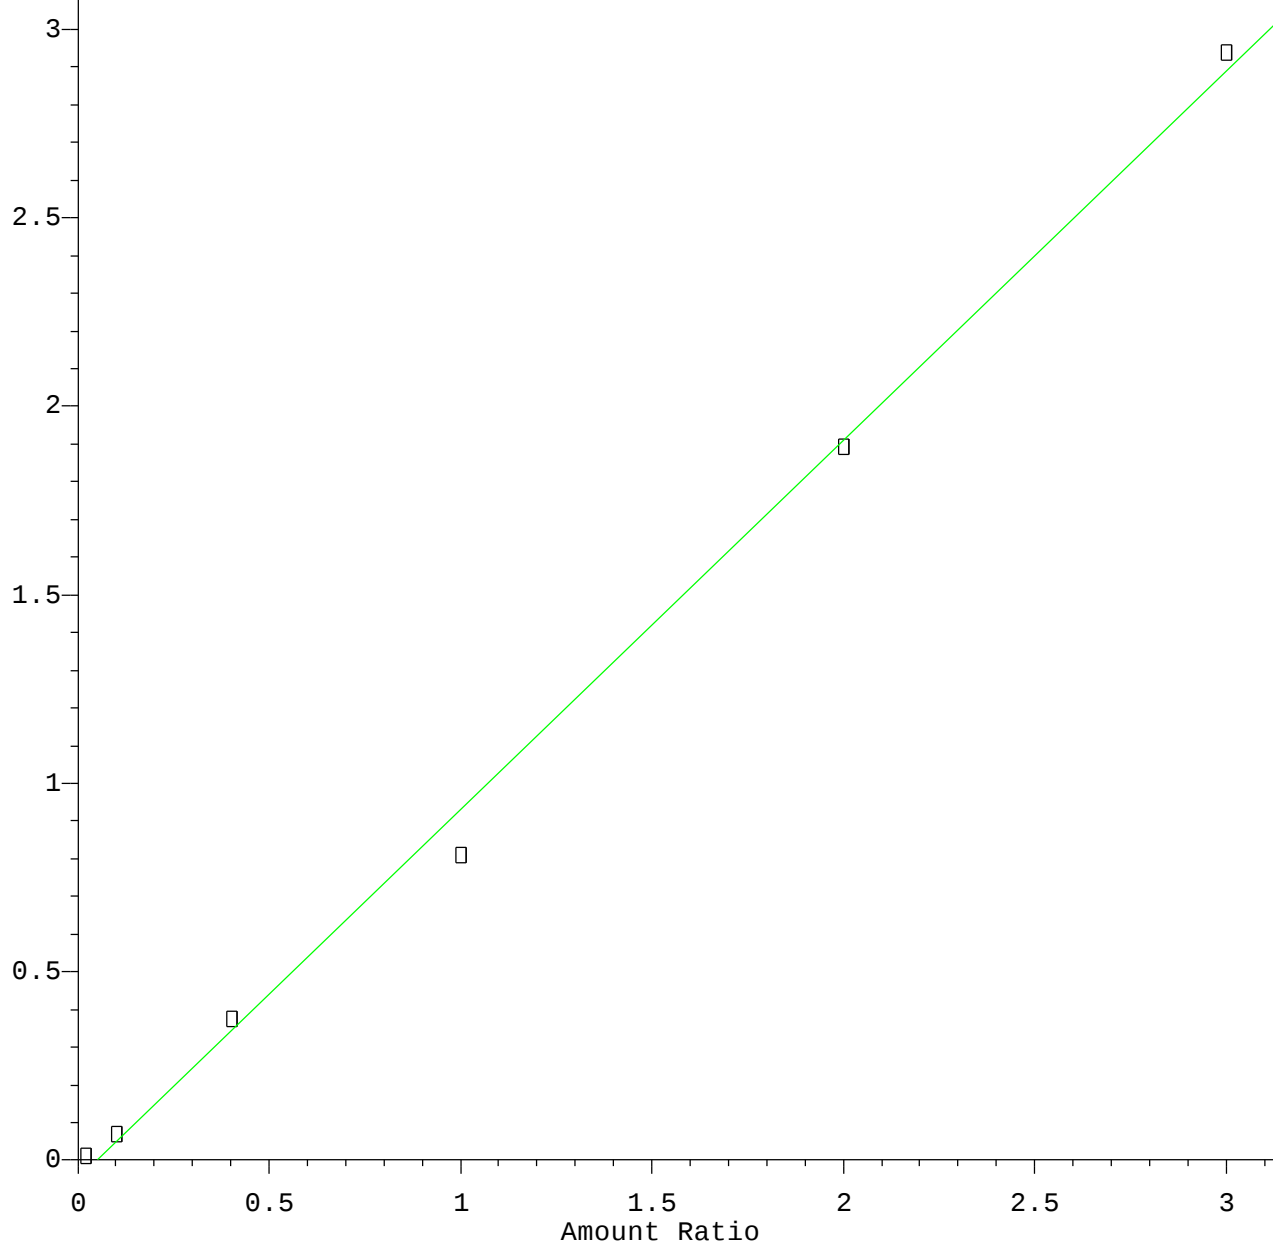

Resp Ratio = $9.80 \times 10^{-1} \times \text{Amt} - 5.03 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022019W.M
Calibration Table Last Updated: Thu Feb 21 03:36:07 2019