


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN022019\
 Data File : VN053869.D
 Acq On : 20 Feb 2019 7:56
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022019W.M
 Title : SW846 8260
 Last Update : Thu Feb 21 03:36:07 2019

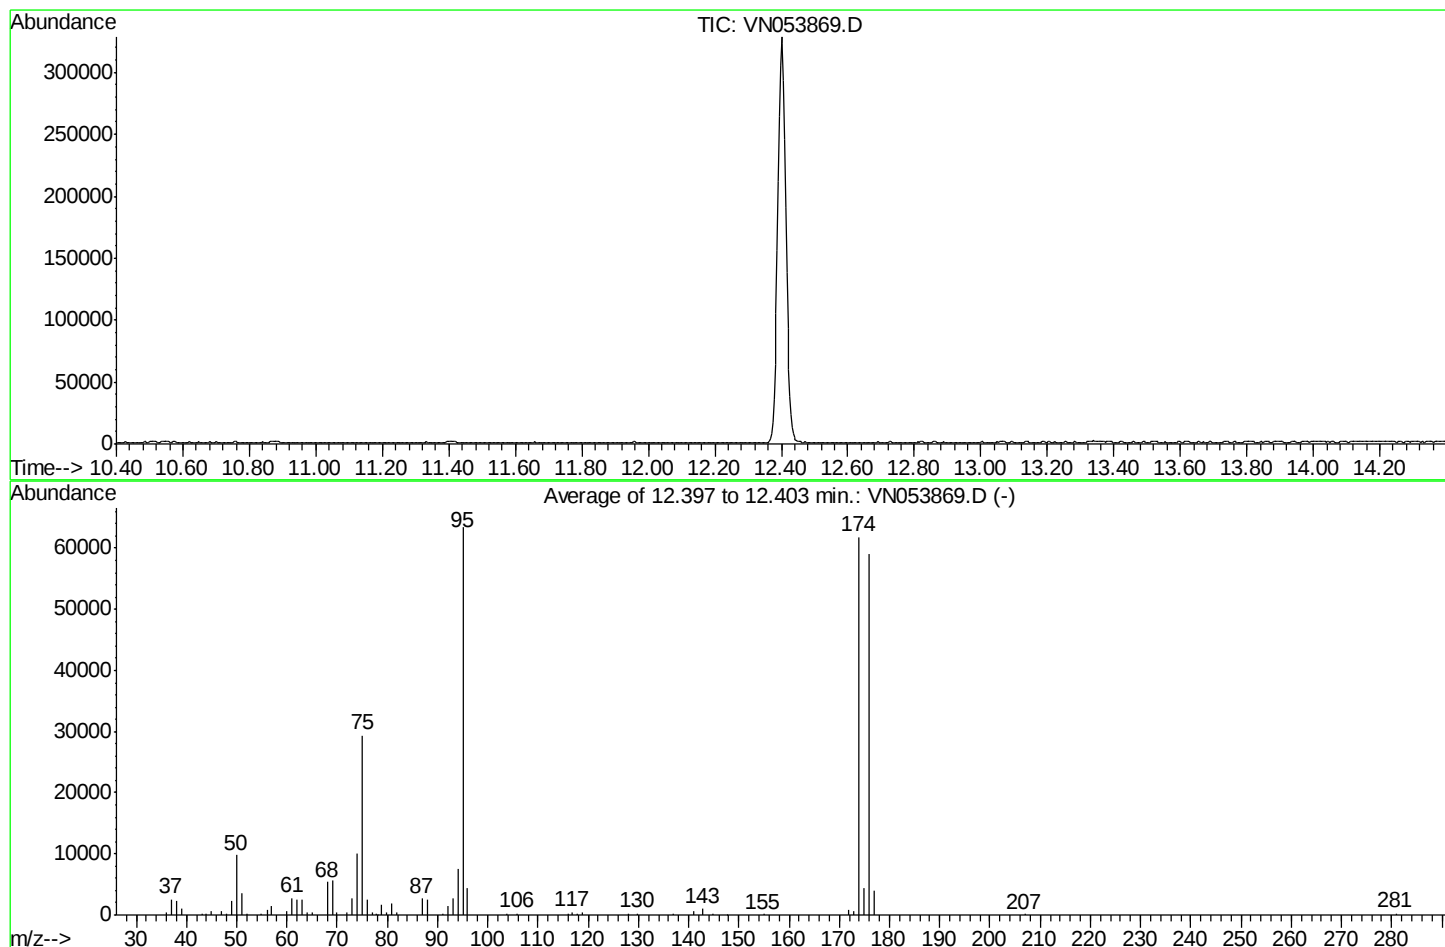

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	9818	PASS
75	95	30	60	46.3	29352	PASS
95	95	100	100	100.0	63400	PASS
96	95	5	9	6.9	4372	PASS
173	174	0.00	2	1.0	623	PASS
174	95	50	100	97.5	61802	PASS
175	174	5	9	7.2	4432	PASS
176	174	95	101	95.6	59088	PASS
177	176	5	9	6.6	3927	PASS