


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN022020\
Data File : VN060160.D
Acq On : 20 Feb 2020 9:25
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N021220W.M
Title : SW846 8260
Last Update : Wed Feb 12 14:12:21 2020

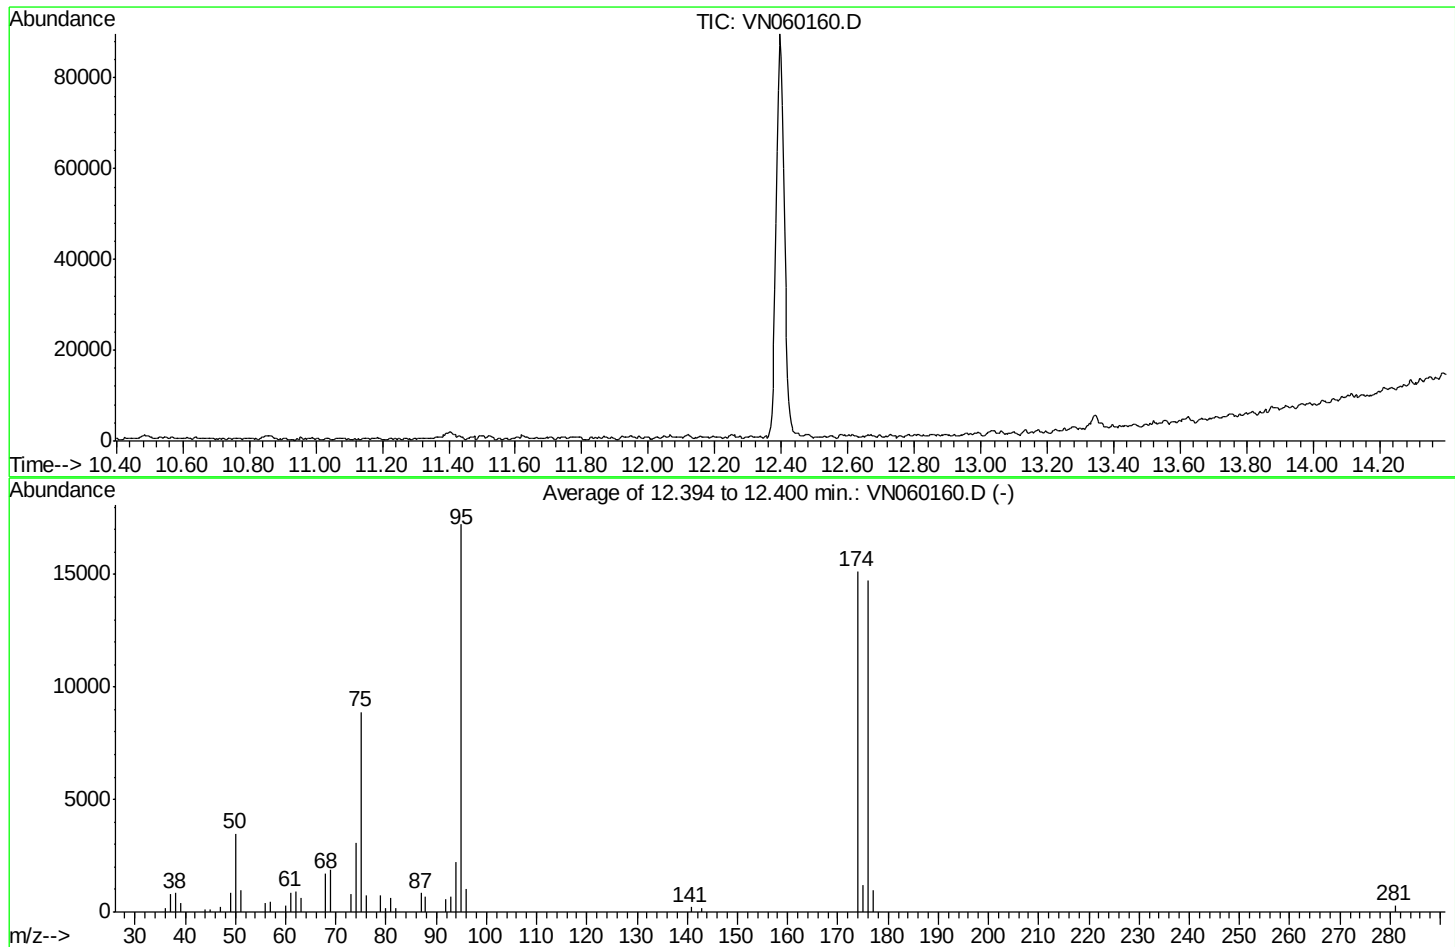

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	3490	PASS
75	95	30	60	51.7	8901	PASS
95	95	100	100	100.0	17232	PASS
96	95	5	9	6.0	1040	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.7	15110	PASS
175	174	5	9	7.8	1184	PASS
176	174	95	101	97.6	14748	PASS
177	176	5	9	6.6	975	PASS