
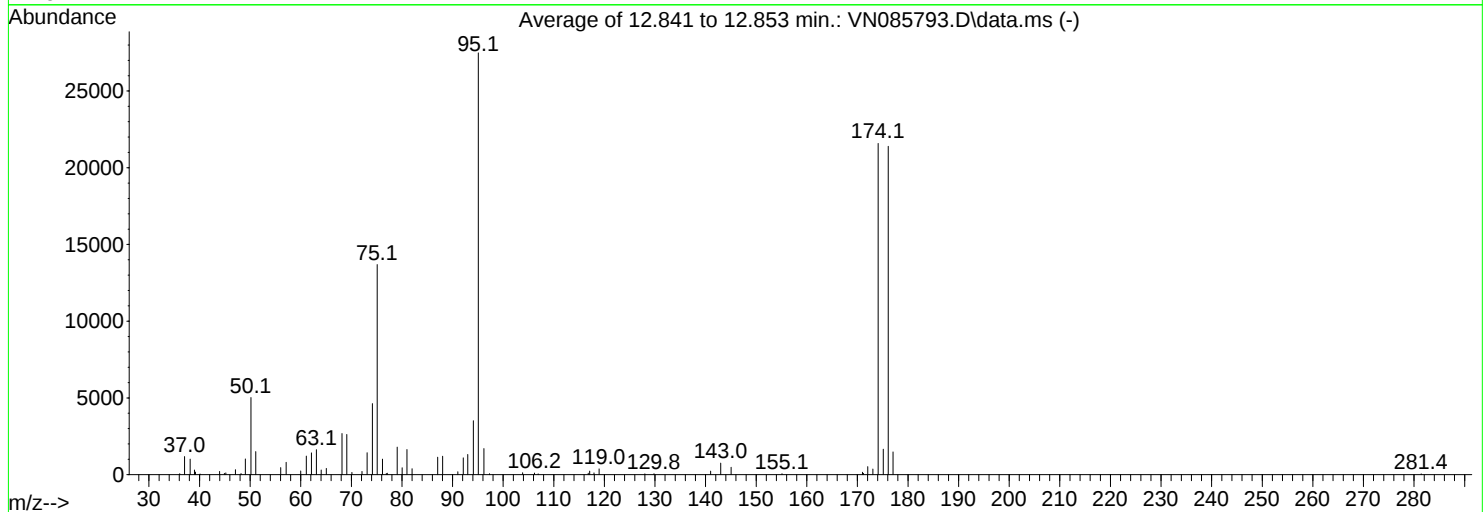


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022025\
Data File : VN085793.D
Acq On : 20 Feb 2025 10:09
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Title : SW846 8260
Last Update : Wed Feb 19 03:43:32 2025

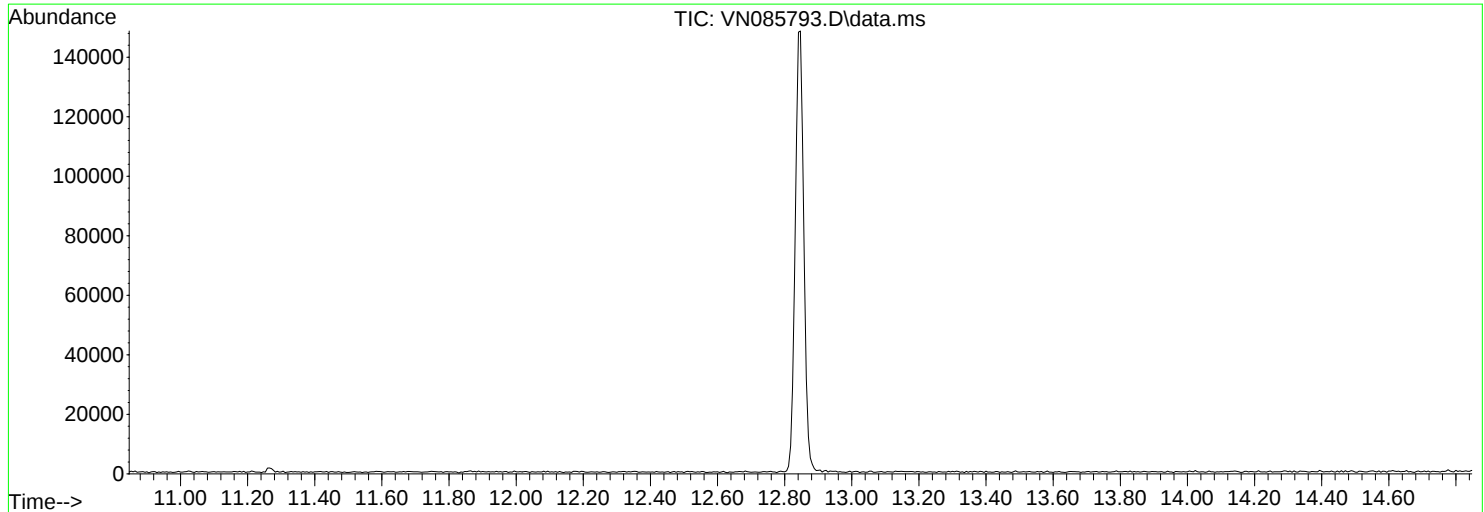

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.3	5026	PASS
75	95	30	60	49.8	13688	PASS
95	95	100	100	100.0	27488	PASS
96	95	5	9	6.2	1703	PASS
173	174	0.00	2	1.7	370	PASS
174	95	50	100	78.5	21584	PASS
175	174	5	9	7.7	1663	PASS
176	174	95	101	99.1	21395	PASS
177	176	5	9	6.9	1482	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	62	49.05	1024	68.15	2680	80.05	451
37.05	1183	50.15	5026	69.10	2614	81.00	164
38.15	1014	51.10	1506	70.10	147	82.00	39
39.00	302	56.05	463	72.10	209	87.05	114
39.20	167	57.10	807	73.10	1426	88.05	1197
40.10	47	60.00	238	74.15	4635	91.05	193
43.95	207	61.10	1212	75.10	13688	92.10	1094
44.90	82	62.10	1415	76.15	1011	93.00	1311
45.20	115	63.10	1622	76.90	73	94.10	3515
47.10	320	64.05	305	77.10	95	95.10	27488
48.20	76	65.05	409	79.05	1797	96.20	1703

Average of 12.841 to 12.853 min.: VN085793.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
97.30	59	143.00	753	281.40	55		
103.85	130	145.05	479				
106.20	102	155.10	63				
106.90	51	171.00	161				
116.80	97	171.20	81				
117.10	227	172.05	522				
117.95	113	173.05	370				
118.95	377	174.10	21584				
128.00	50	175.10	1663				
129.80	64	176.10	21395				
141.00	230	177.05	1482				

Instrument :

MSVOA_N

ClientSampleId :

BFB