


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN022119\
Data File : VN053877.D
Acq On : 21 Feb 2019 7:59
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022019W.M
Title : SW846 8260
Last Update : Thu Feb 21 03:36:07 2019

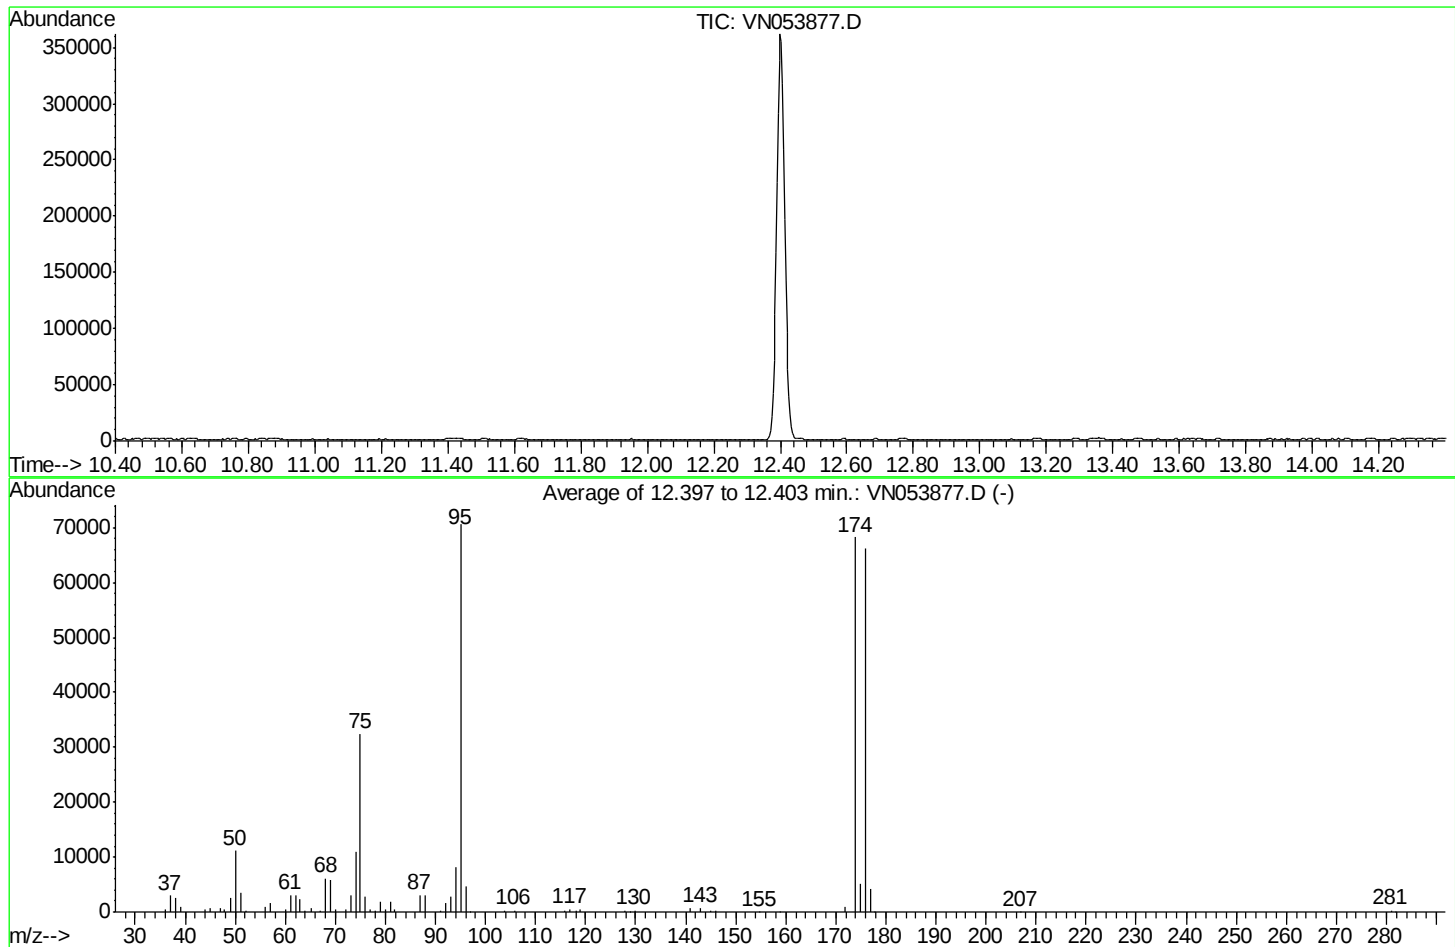

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	11170	PASS
75	95	30	60	45.9	32424	PASS
95	95	100	100	100.0	70605	PASS
96	95	5	9	6.5	4616	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	96.7	68256	PASS
175	174	5	9	7.4	5026	PASS
176	174	95	101	96.9	66160	PASS
177	176	5	9	6.3	4160	PASS