

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN022120\
 Data File : VN060180.D
 Acq On : 21 Feb 2020 11:01
 Operator : JC/MD
 Sample : VN0221MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0221MBL01

Quant Time: Feb 21 22:36:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N021220W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 12 14:12:21 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	171820	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.56	114	269717	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	241743	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	95131	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.00	65	98362	47.05	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.10%	
35) Dibromofluoromethane	7.56	113	81095	48.91	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.82%	
50) Toluene-d8	10.08	98	323582	49.56	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.12%	
62) 4-Bromofluorobenzene	12.40	95	107017	44.61	ug/l	0.00
Spiked Amount	50.000		Recovery	=	89.22%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN022120\
Data File : VN060180.D
Acq On : 21 Feb 2020 11:01
Operator : JC/MD
Sample : VN0221MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0221MBL01

Quant Time: Feb 21 22:36:07 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N021220W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 12 14:12:21 2020
Response via : Initial Calibration

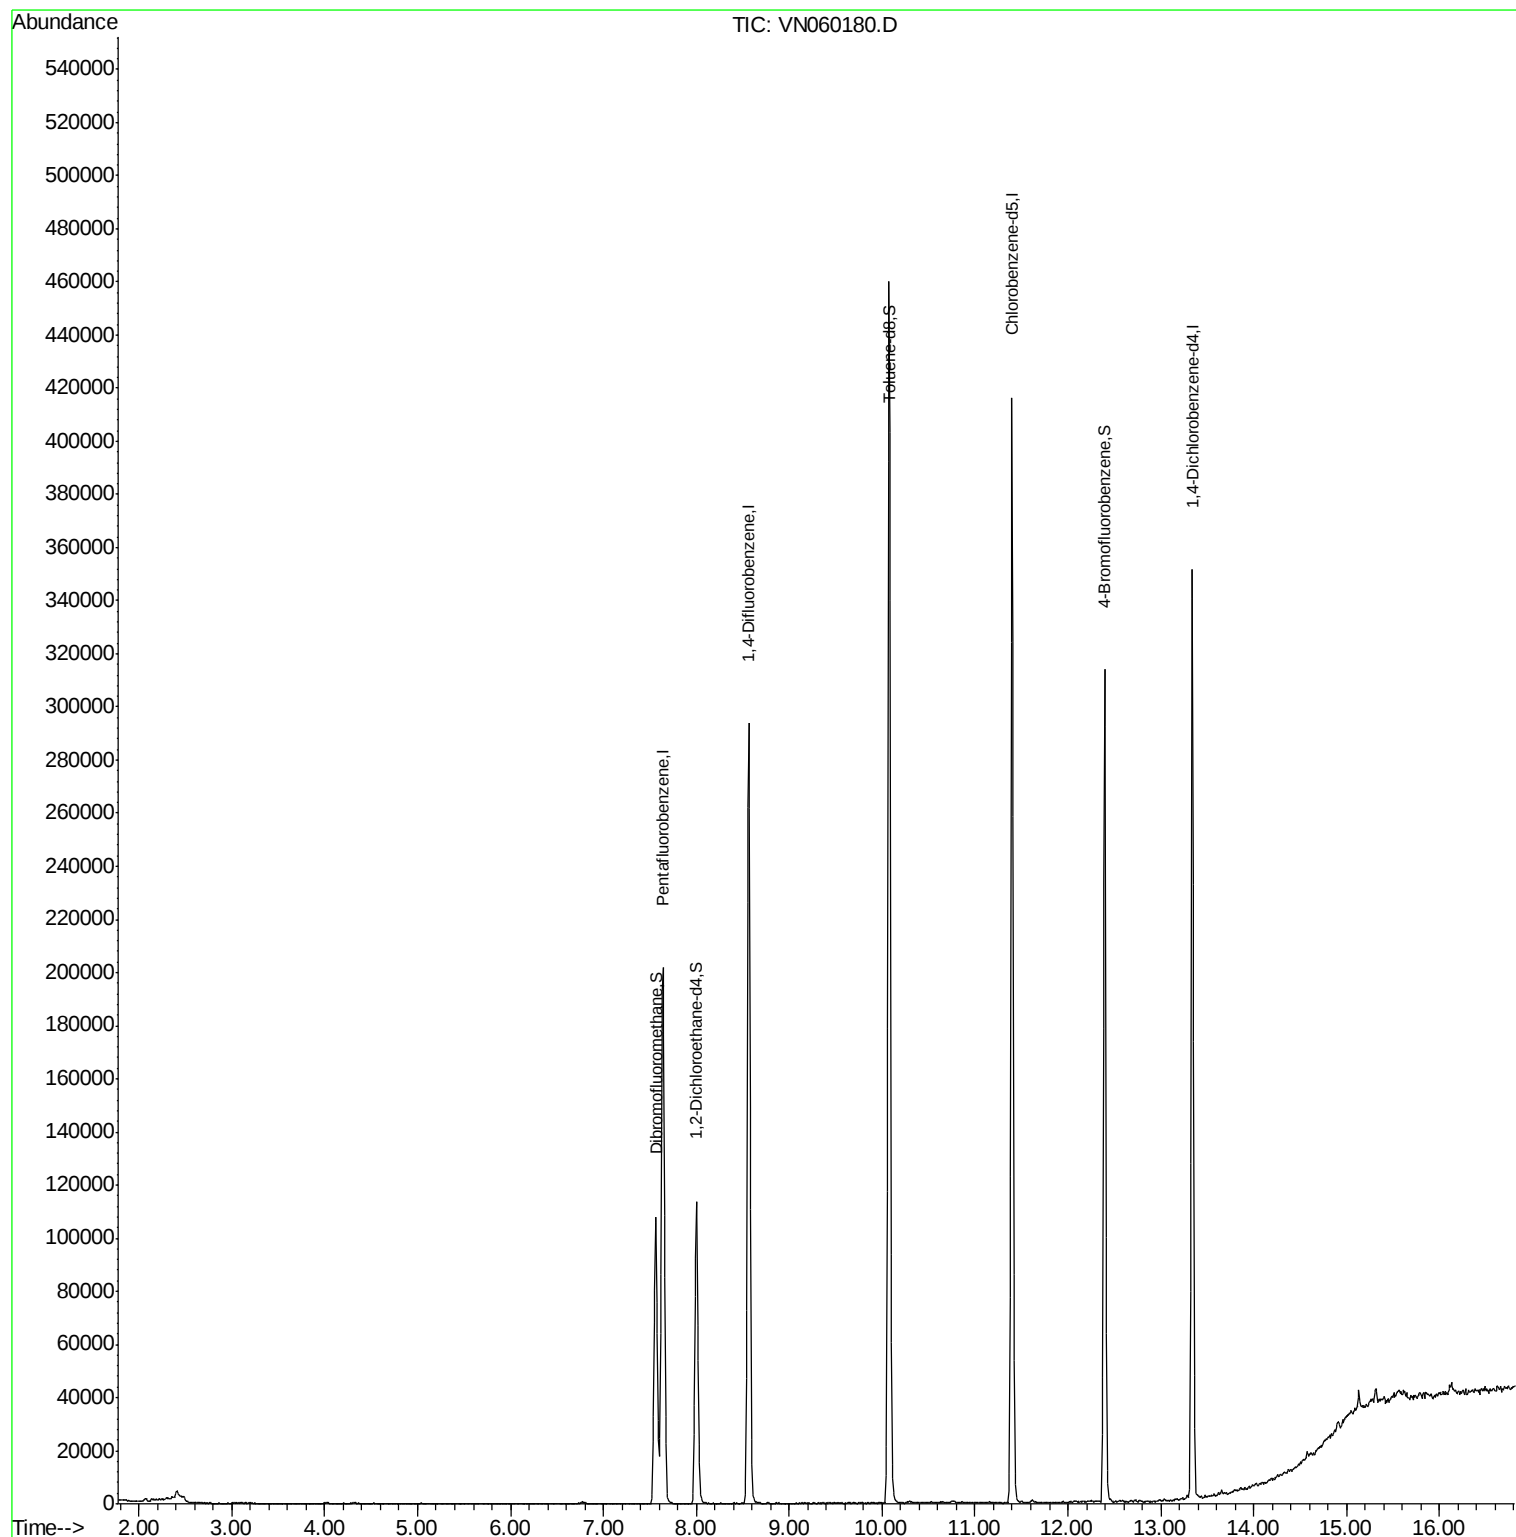

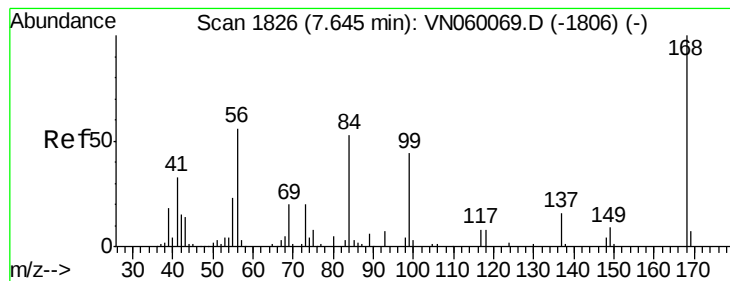

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1825

Delta R.T. -0.00 min

Lab File: VN060180.D

Acq: 21 Feb 2020 11:01

Instrument :

MSVOA_N

ClientSampleId :


VN0221MBL01

Tot Ion:168 Resp: 171820

Ion Ratio Lower Upper

168 100

99 54.1 42.7 64.1

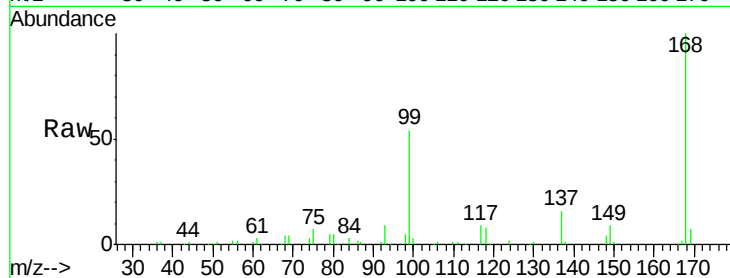

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.64

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70 7.80

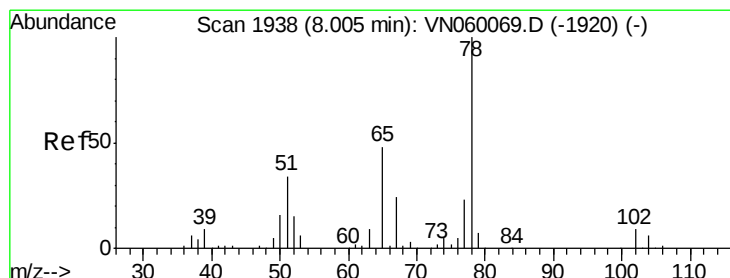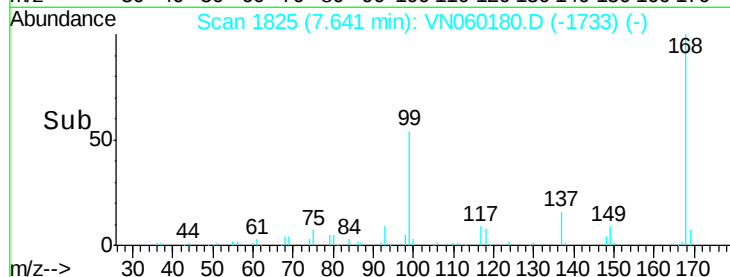

#33

1,2-Dichloroethane-d4

Concen: 47.046 ug/l

RT: 8.00 min Scan# 1937

Delta R.T. -0.00 min

Lab File: VN060180.D


Acq: 21 Feb 2020 11:01

Tgt Ion: 65 Resp: 98362

Ion Ratio Lower Upper

65 100

67 52.1 0.0 104.0

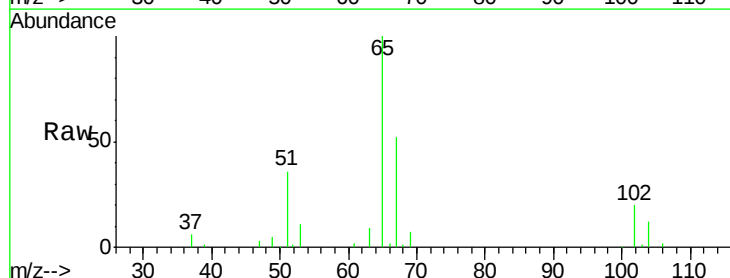

Abundance Ion 64.90 (64.60 to 65.60): V

Ion 66.90 (66.60 to 67.60): VN

8.00

50000

40000


30000


20000

10000

0

Time--> 7.90 8.00 8.10

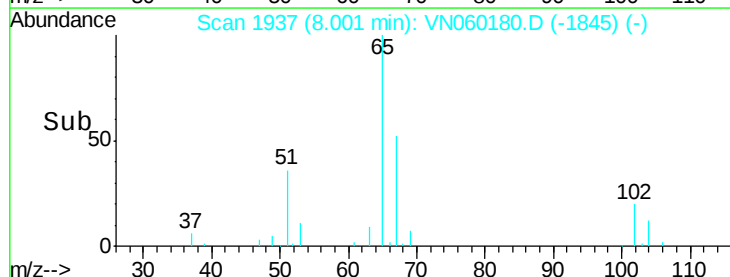


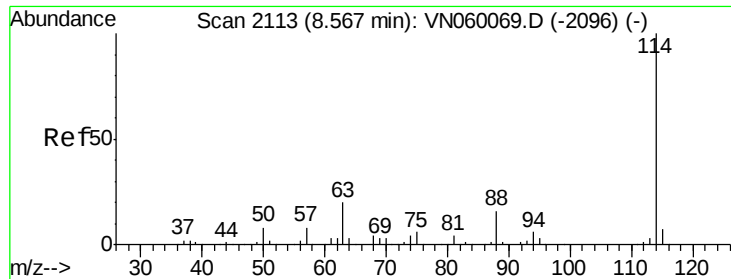




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.56 min Scan# 2112
Delta R.T. -0.00 min
Lab File: VN060180.D
Acq: 21 Feb 2020 11:01

Instrument :
MSVOA_N
ClientSampleId :
VN0221MBL01

Tot Ion:114 Resp: 269717
Ion Ratio Lower Upper
114 100
63 19.9 0.0 40.0
88 15.8 0.0 31.6

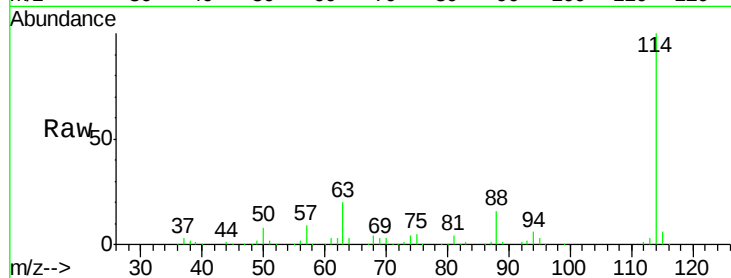


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VN
Ion 87.90 (87.60 to 88.60): VN

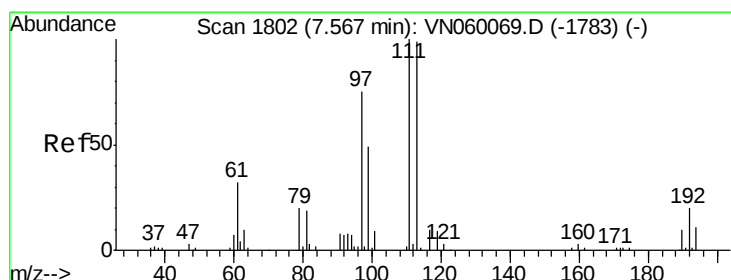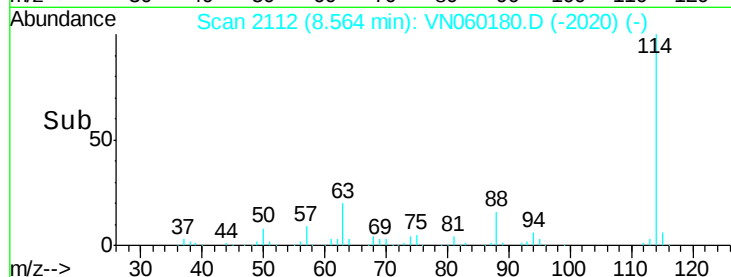
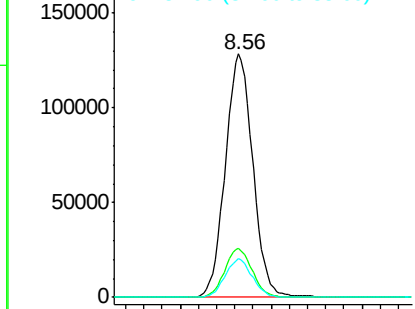



#35
Dibromofluoromethane
Concen: 48.913 ug/l
RT: 7.56 min Scan# 1801
Delta R.T. -0.00 min
Lab File: VN060180.D
Acq: 21 Feb 2020 11:01

Tgt Ion:113 Resp: 81095
Ion Ratio Lower Upper
113 100
111 102.3 81.4 122.2
192 20.7 16.2 24.2

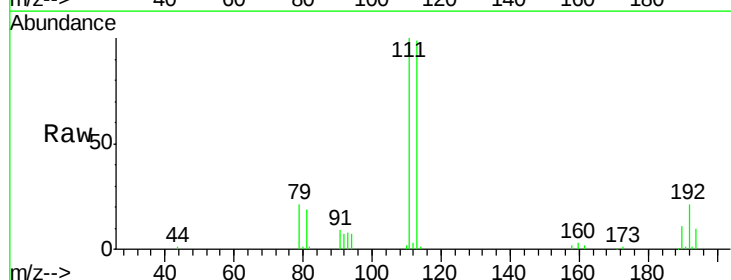

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V



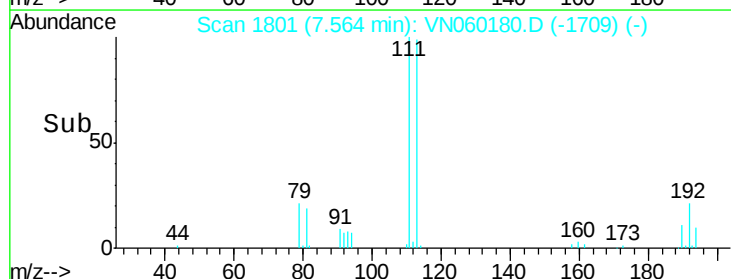
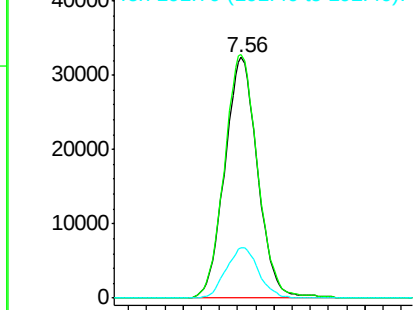


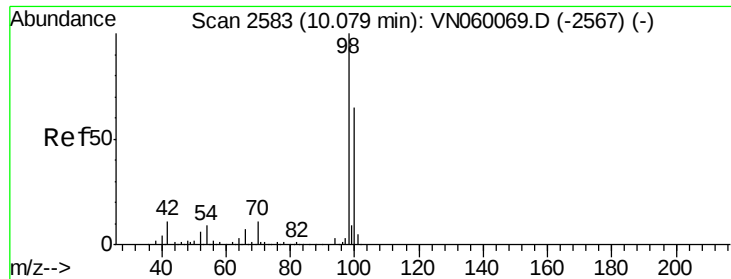

#50
Toluene-d8
Concen: 49.561 ug/l
RT: 10.08 min Scan# 2582
Delta R.T. -0.00 min
Lab File: VN060180.D
Acq: 21 Feb 2020 11:01




Instrument :
MSVOA_N
ClientSampled :
VN0221MBL01


Tot Ion: 98 Resp: 323582
Ion Ratio Lower Upper
98 100
100 64.2 51.7 77.5

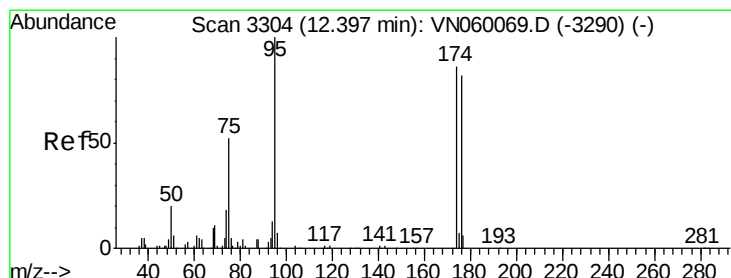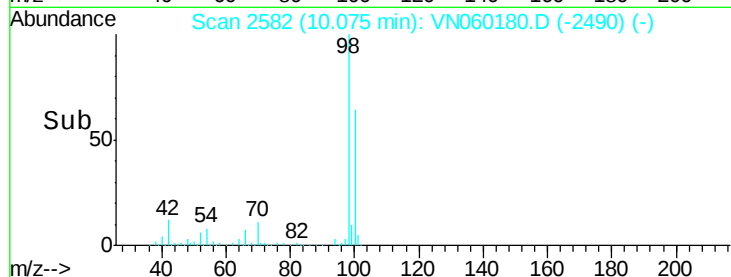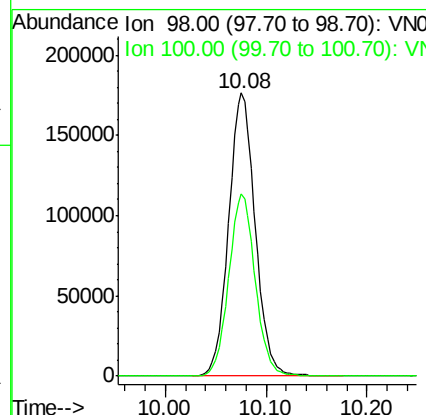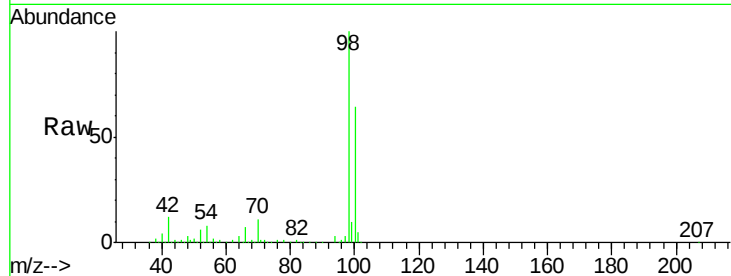

#62
4-Bromofluorobenzene
Concen: 44.608 ug/l
RT: 12.40 min Scan# 3304
Delta R.T. -0.00 min
Lab File: VN060180.D
Acq: 21 Feb 2020 11:01

Tgt Ion: 95 Resp: 107017
Ion Ratio Lower Upper
95 100
174 84.7 0.0 169.8
176 82.3 0.0 164.8

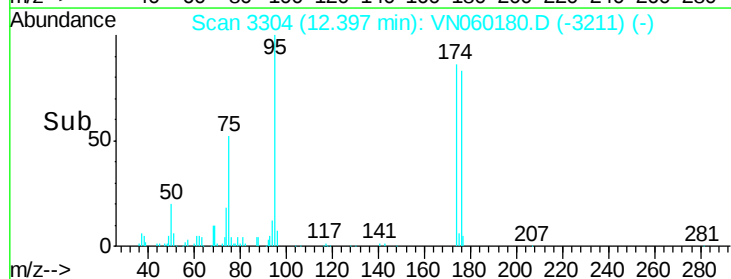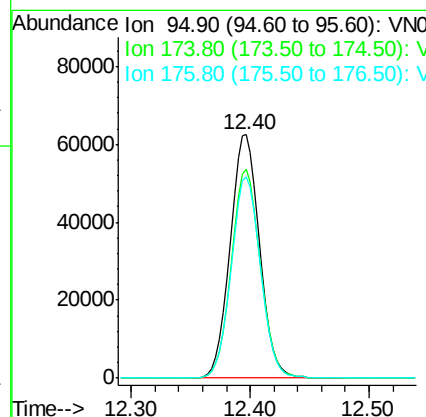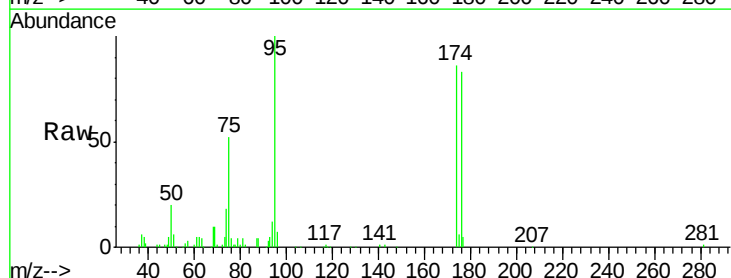


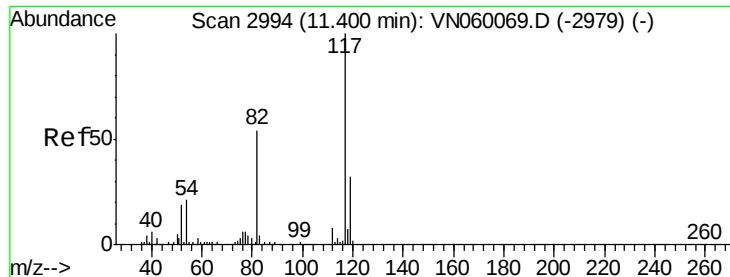




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.40 min Scan# 2994
Delta R.T. -0.00 min
Lab File: VN060180.D
Acq: 21 Feb 2020 11:01

Instrument :
MSVOA_N
ClientSampleId :
VN0221MBL01

Tot Ion:117 Resp: 241743
Ion Ratio Lower Upper
117 100
82 54.0 43.4 65.0
119 32.4 25.8 38.6

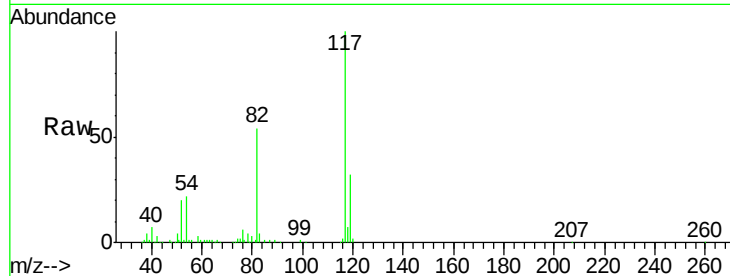


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

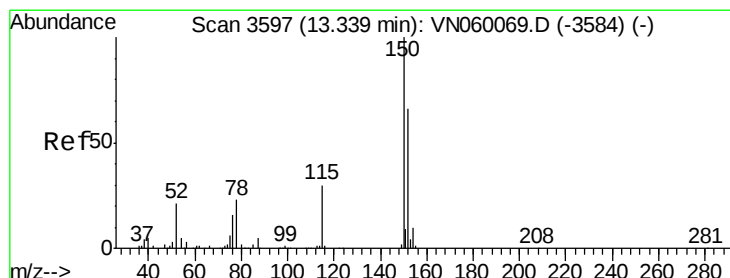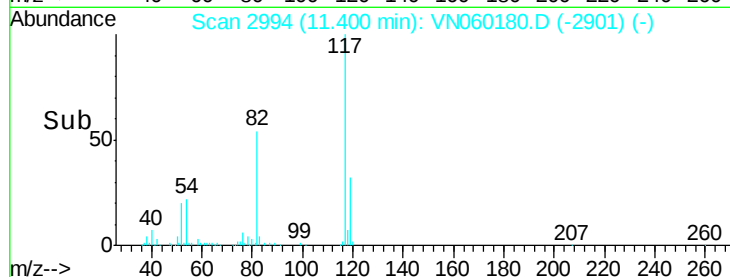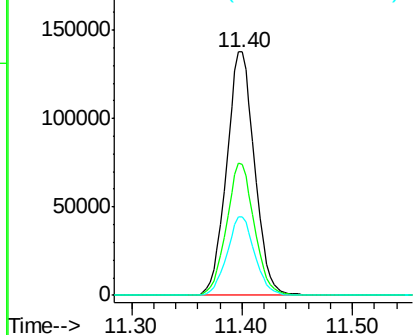

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3597
Delta R.T. -0.00 min
Lab File: VN060180.D
Acq: 21 Feb 2020 11:01

Tgt Ion:152 Resp: 95131
Ion Ratio Lower Upper
152 100
115 58.2 28.9 86.8
150 157.8 0.0 342.4

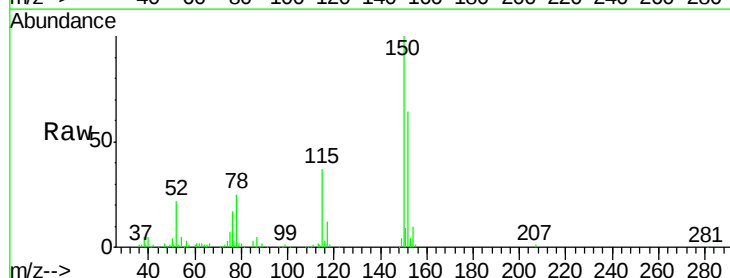

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

