
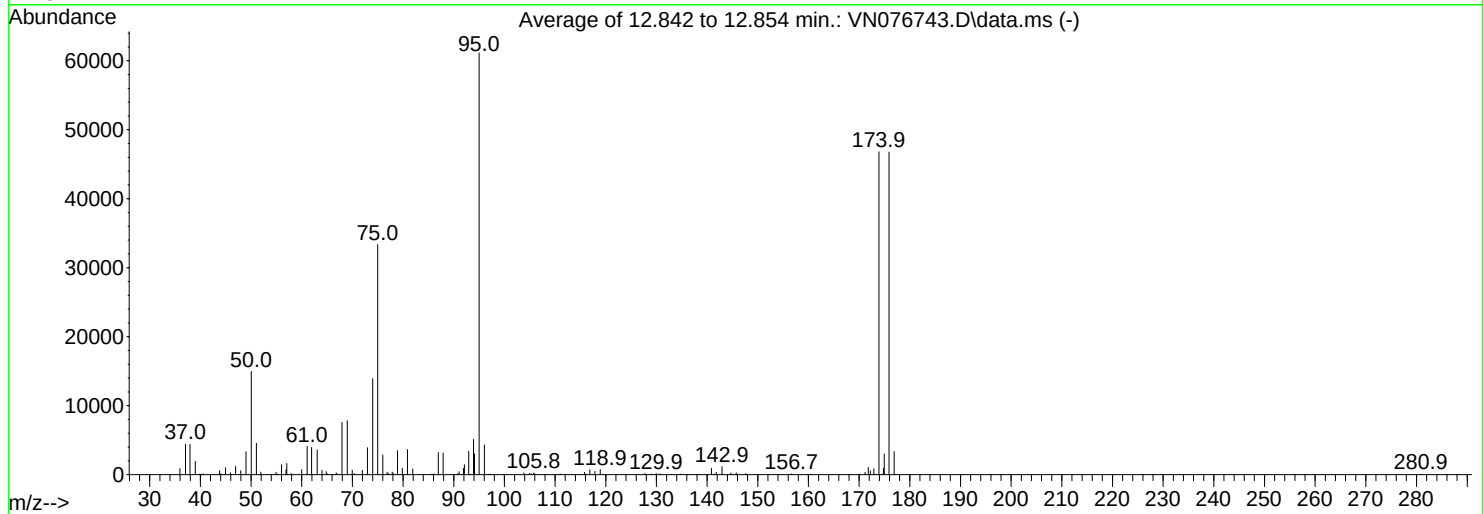


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022123\
Data File : VN076743.D
Acq On : 21 Feb 2023 09:23
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
Title : SW846 8260
Last Update : Tue Feb 14 01:44:47 2023

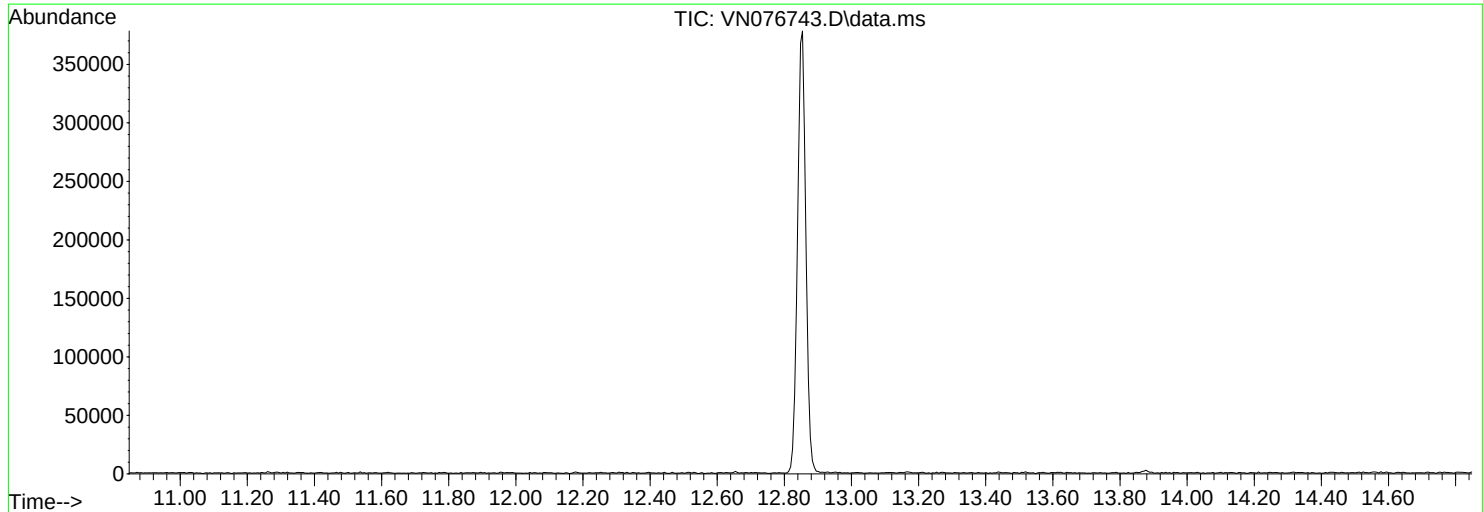

AutoFind: Scans 1854, 1855, 1856; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.5	14956	PASS
75	95	30	60	54.5	33349	PASS
95	95	100	100	100.0	61149	PASS
96	95	5	9	7.1	4324	PASS
173	174	0.00	2	1.8	850	PASS
174	95	50	100	76.6	46819	PASS
175	174	5	9	6.4	2986	PASS
176	174	95	101	99.9	46765	PASS
177	176	5	9	7.2	3350	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	877	46.95	1203	57.90	153	67.95	757
37.05	4437	47.95	559	58.30	55	69.00	782
37.95	4375	49.00	3310	60.00	720	69.95	65
39.00	1928	50.05	14956	61.05	4073	70.30	17
39.85	64	51.05	4540	61.95	3947	70.80	52
40.20	100	51.95	383	63.05	3562	71.95	632
40.60	102	54.95	342	64.00	623	72.95	3892
43.80	580	55.20	88	64.85	415	74.00	13927
44.05	115	56.00	1439	65.10	128	75.00	33349
44.95	989	56.90	675	66.80	248	76.00	2848
45.95	255	57.05	1633	67.10	86	76.85	377

Average of 12.842 to 12.854 min.: VN076743.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.10	138	90.70	137	103.85	249	118.90	752
77.85	379	91.05	426	104.95	189	124.00	62
78.10	172	91.90	901	105.30	85	127.75	164
78.90	3470	92.10	1430	105.80	236	129.00	64
79.85	915	92.95	3386	106.00	134	129.95	160
80.85	3645	93.90	5104	111.00	93	130.70	112
81.90	840	94.10	3009	114.80	54	133.00	56
85.70	68	95.00	61149	115.80	321	134.70	103
86.10	106	96.05	4324	116.10	99	136.80	56
86.95	3200	96.80	50	116.85	708	140.85	912
87.90	3132	97.20	83	117.85	468	141.40	75

Average of 12.842 to 12.854 min.: VN076743.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
141.80	356	172.90	850				
142.95	1158	173.90	46819				
144.70	237	174.80	902				
145.75	251	174.95	2986				
147.65	159	175.90	46765				
156.70	126	176.90	3350				
160.50	59	280.90	66				
170.10	100						
171.15	349						
171.80	1064						
172.20	566						

Instrument :

MSVOA_N

ClientSampleId :

BFB