

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022124\
 Data File : VN081115.D
 Acq On : 21 Feb 2024 13:11
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Feb 22 04:45:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 16 23:45:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	315022	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	615188	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	523168	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	212341	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	201477	52.179	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 104.360%	
35) Dibromofluoromethane	8.171	113	166323	47.812	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 95.620%	
50) Toluene-d8	10.565	98	531311	43.002	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 86.000%	
62) 4-Bromofluorobenzene	12.847	95	191819	41.317	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 82.640%#	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022124\
Data File : VN081115.D
Acq On : 21 Feb 2024 13:11
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Feb 22 04:45:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 16 23:45:20 2024
Response via : Initial Calibration




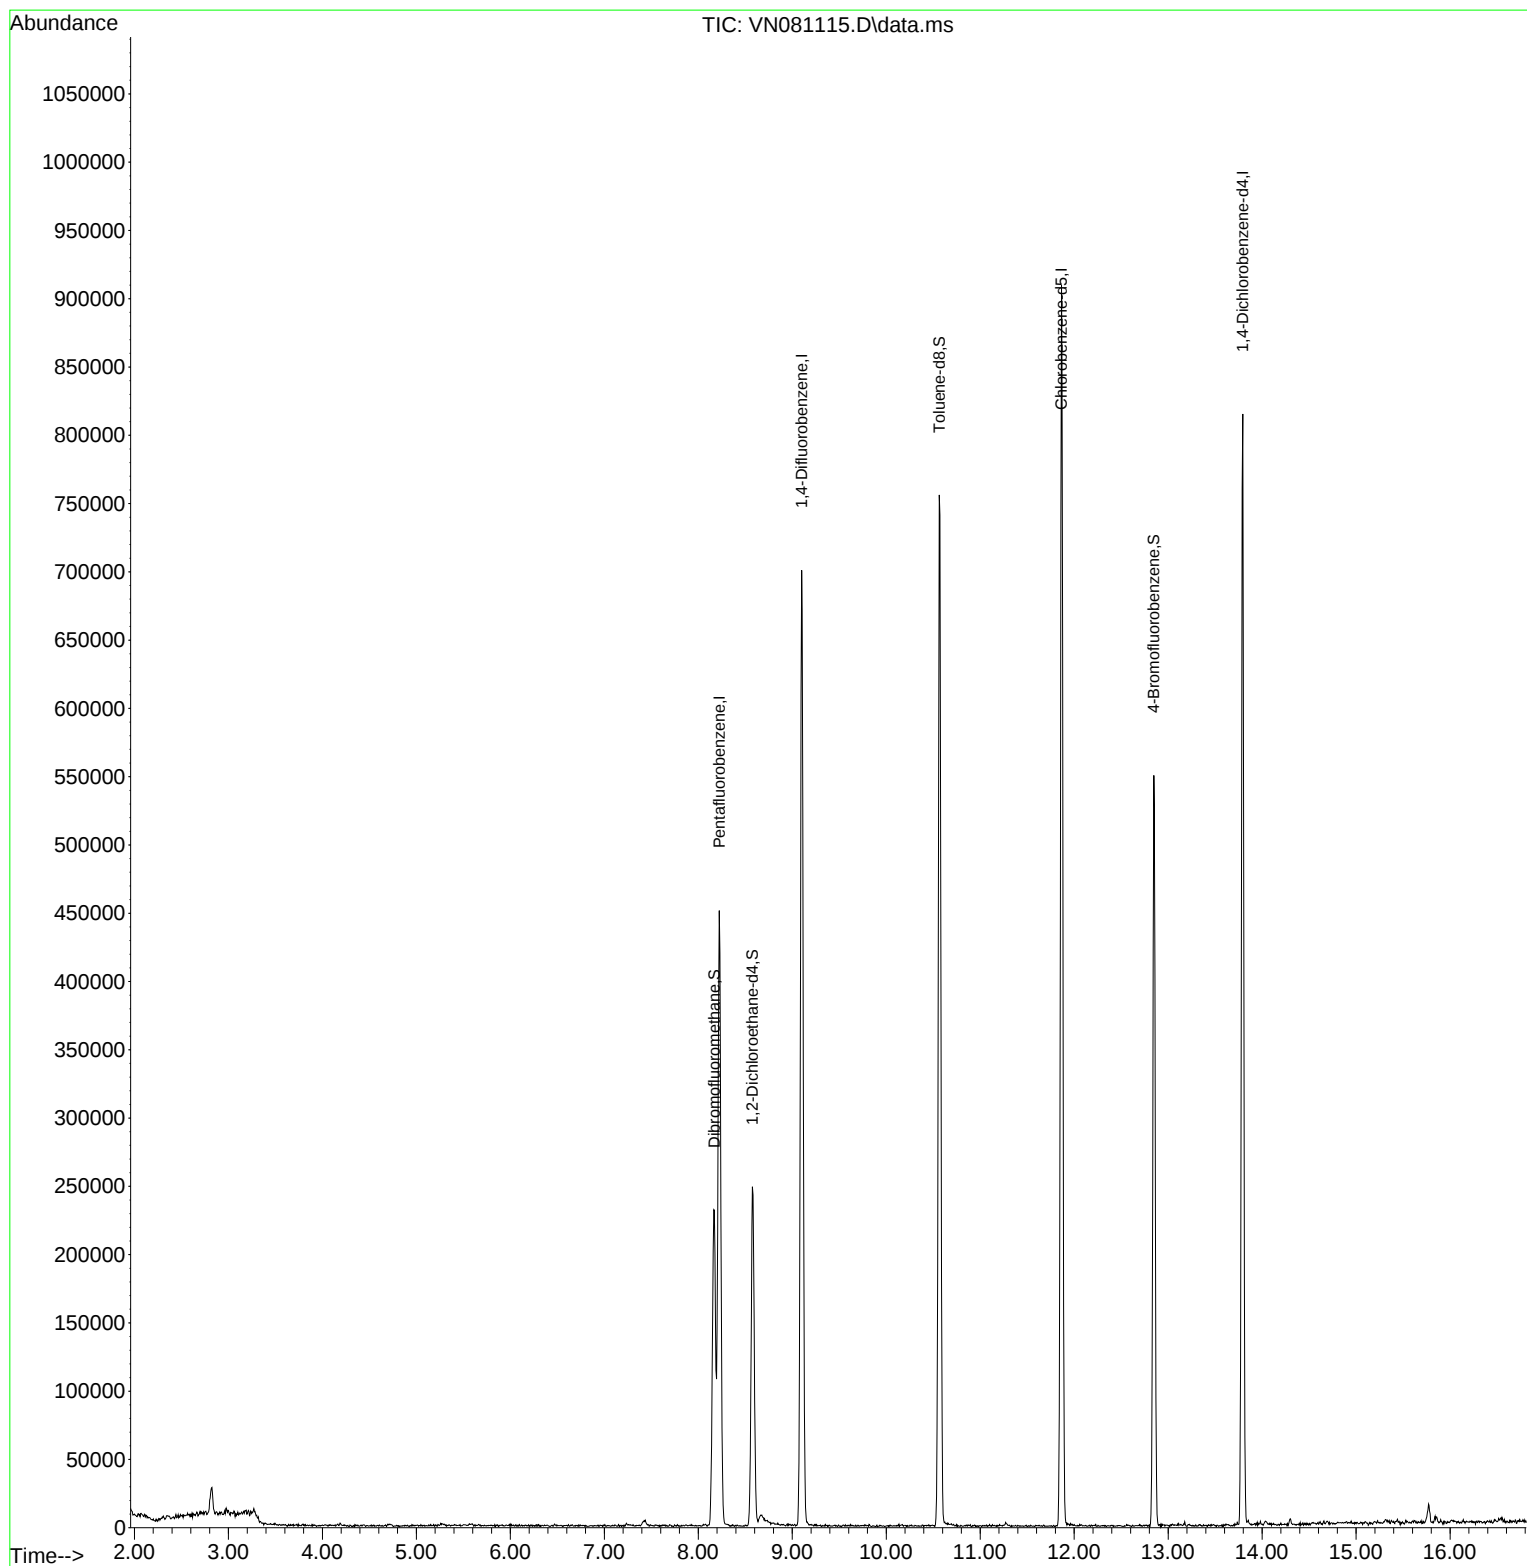


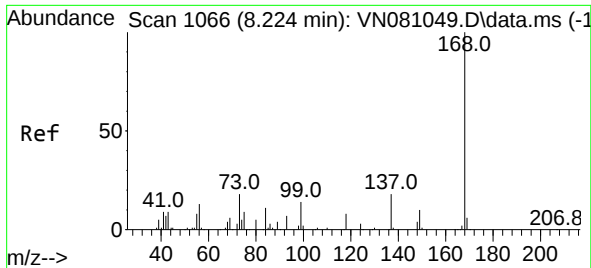

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN081115.D
Acq: 21 Feb 2024 13:11




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 315022
Ion Ratio Lower Upper
168 100
99 66.8 59.9 89.9

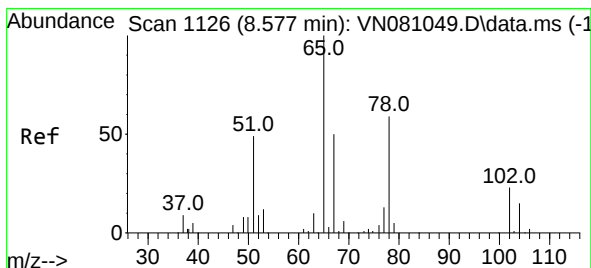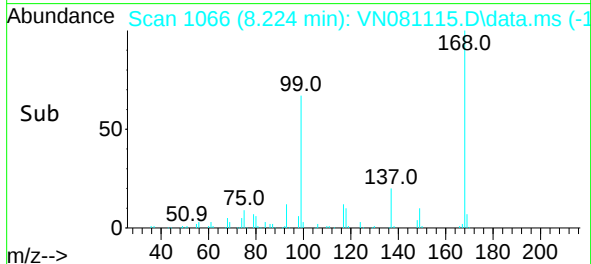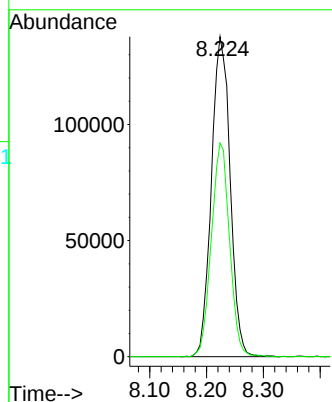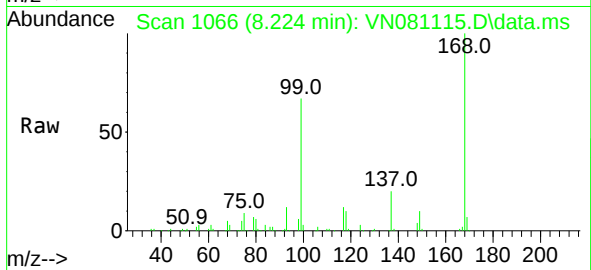

#33
1,2-Dichloroethane-d4
Concen: 52.179 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN081115.D
Acq: 21 Feb 2024 13:11

Tgt Ion: 65 Resp: 201477
Ion Ratio Lower Upper
65 100
67 51.7 0.0 102.4

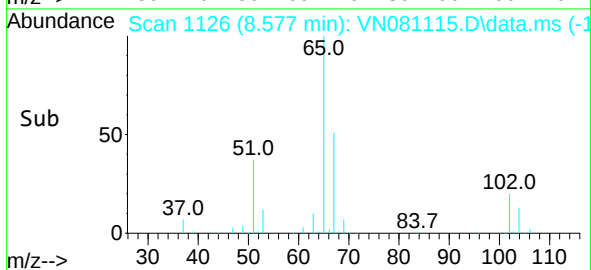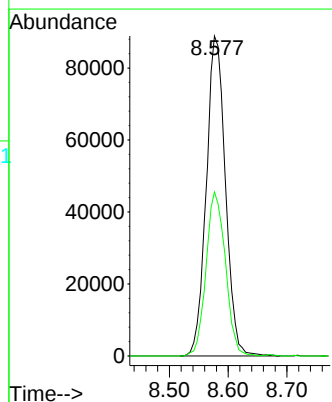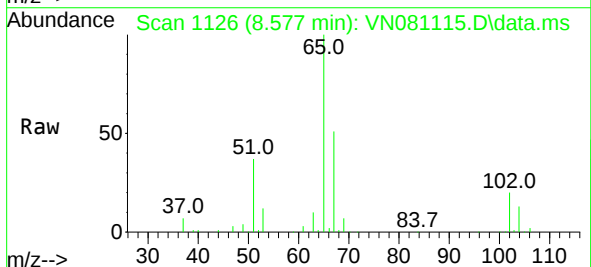

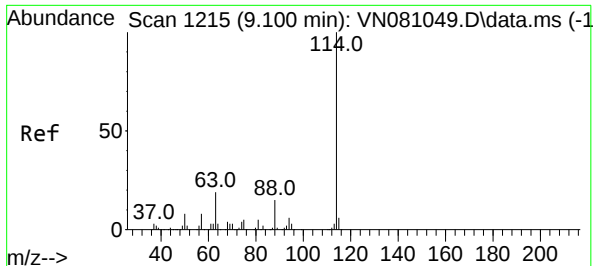

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN081115.D

Acq: 21 Feb 2024 13:11

Instrument :

MSVOA_N

ClientSampleId :

IBLK





Tgt Ion:114 Resp: 615188

Ion Ratio Lower Upper

114 100

63 18.6 0.0 48.0

88 15.4 0.0 34.8

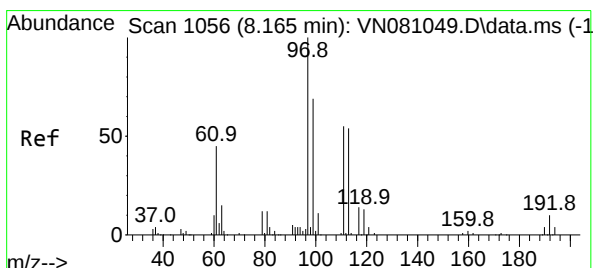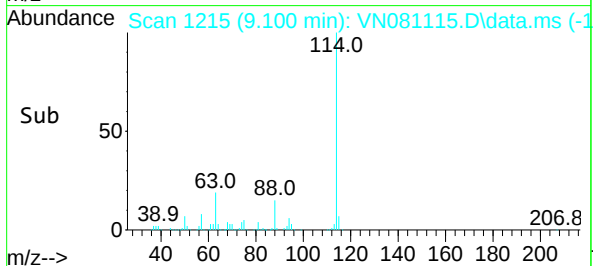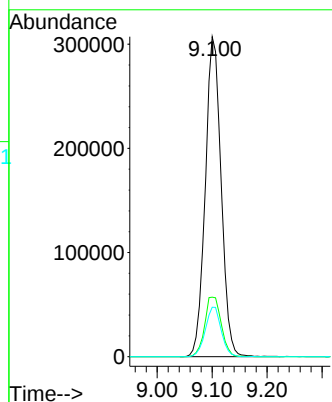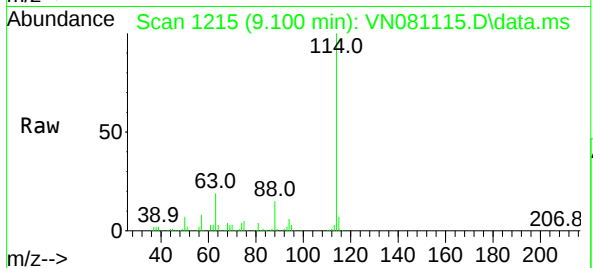

#35

Dibromofluoromethane

Concen: 47.812 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VN081115.D

Acq: 21 Feb 2024 13:11




Tgt Ion:113 Resp: 166323


Ion Ratio Lower Upper

113 100

111 105.2 82.2 123.4

192 15.7 12.5 18.7


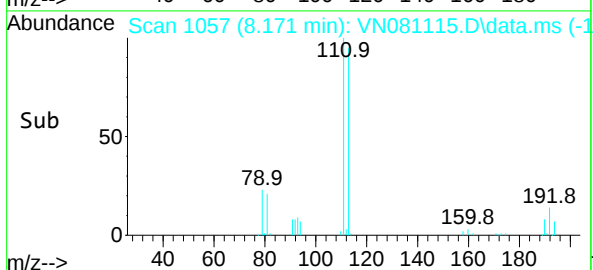
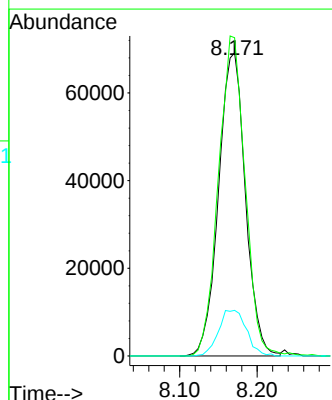
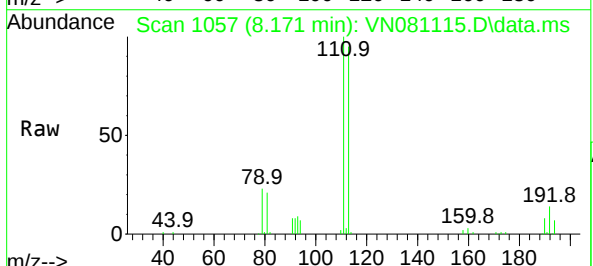


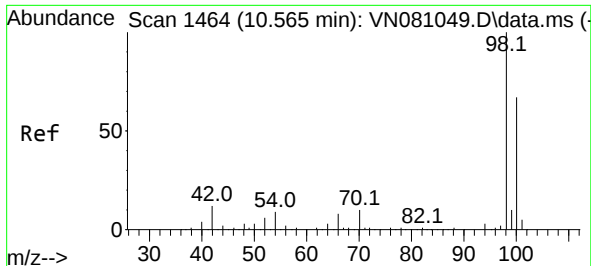

#50
Toluene-d8
Concen: 43.002 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN081115.D
Acq: 21 Feb 2024 13:11




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 531311
Ion Ratio Lower Upper
98 100
100 65.0 51.4 77.0

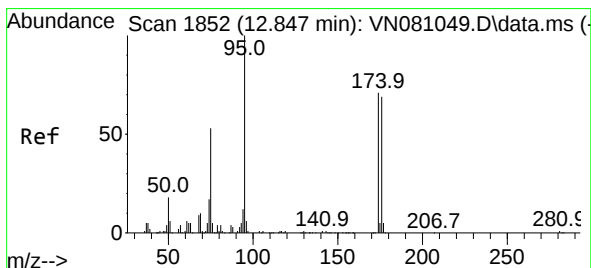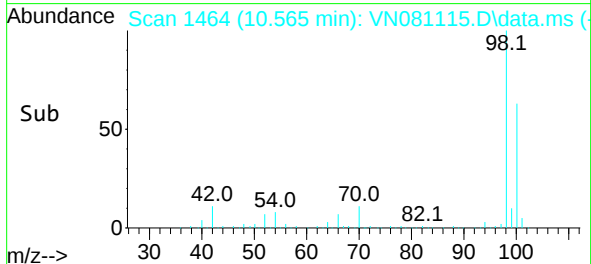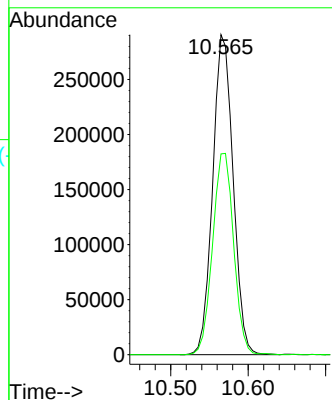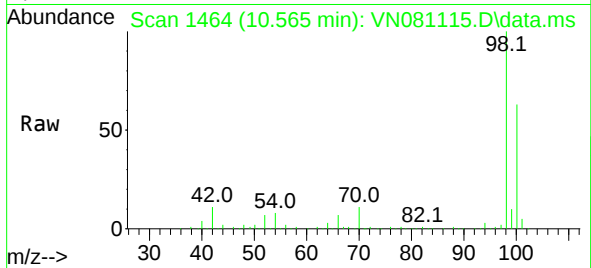

#62
4-Bromofluorobenzene
Concen: 41.317 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN081115.D
Acq: 21 Feb 2024 13:11

Tgt Ion: 95 Resp: 191819
Ion Ratio Lower Upper
95 100
174 71.7 0.0 120.4
176 69.4 0.0 121.0


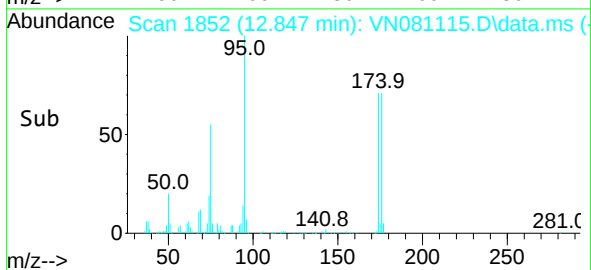
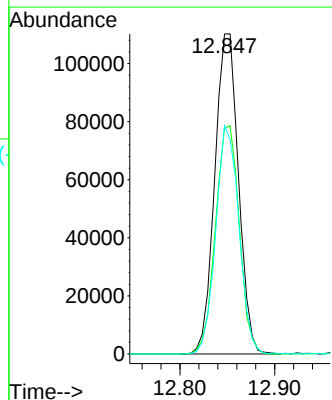
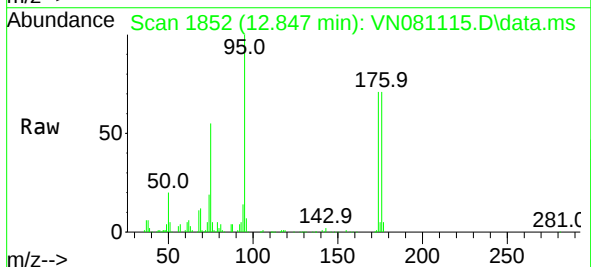


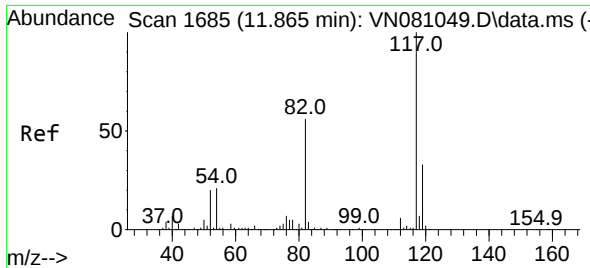

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1170
Delta R.T. -0.000 min
Lab File: VN081115.D
Acq: 21 Feb 2024 13:11

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 523168
Ion Ratio Lower Upper
117 100
82 53.0 52.7 79.1
119 31.7 25.3 37.9

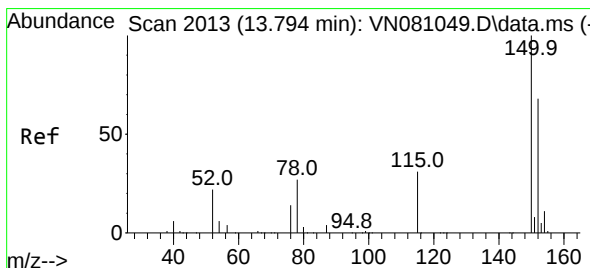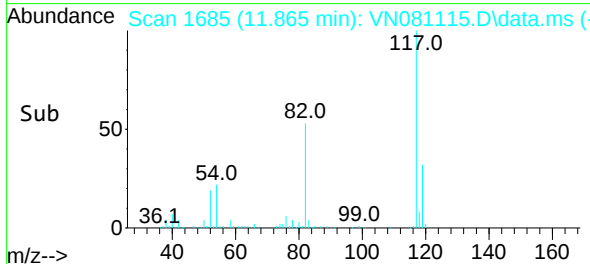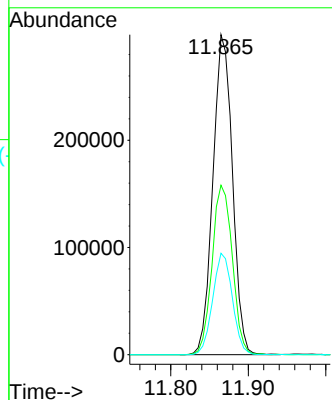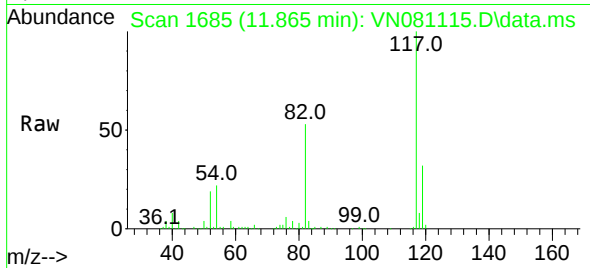

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN081115.D
Acq: 21 Feb 2024 13:11

Tgt Ion:152 Resp: 212341
Ion Ratio Lower Upper
152 100
115 63.1 32.3 96.8
150 159.8 0.0 339.8

