
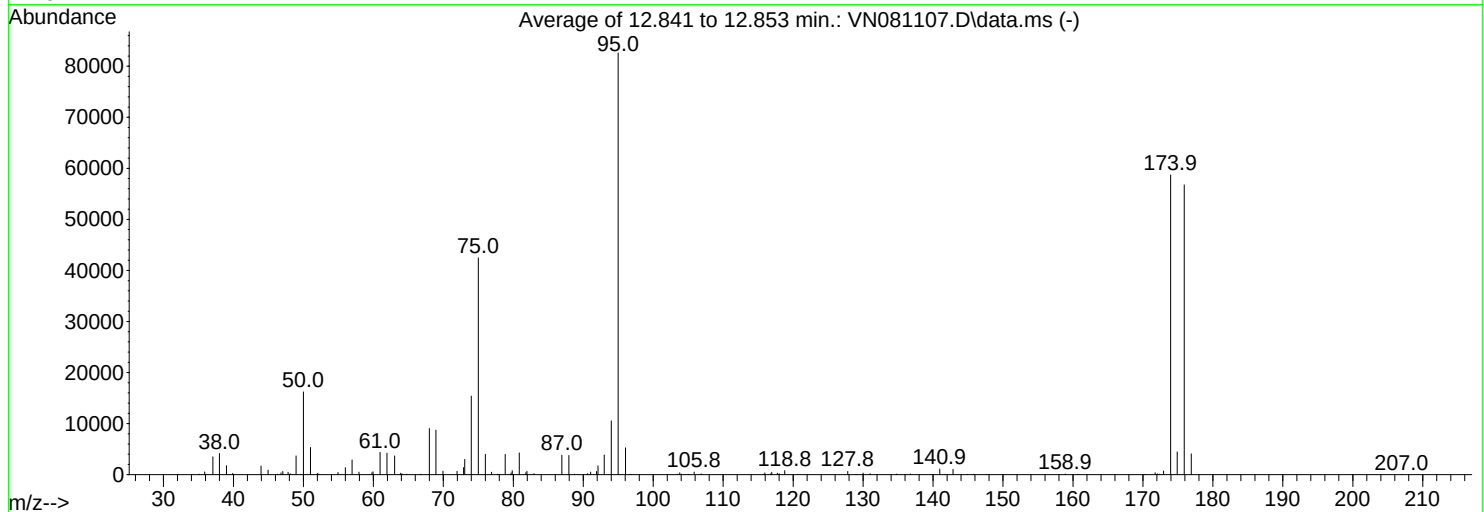


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022124\
Data File : VN081107.D
Acq On : 21 Feb 2024 08:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
Title : SW846 8260
Last Update : Fri Feb 16 23:45:20 2024

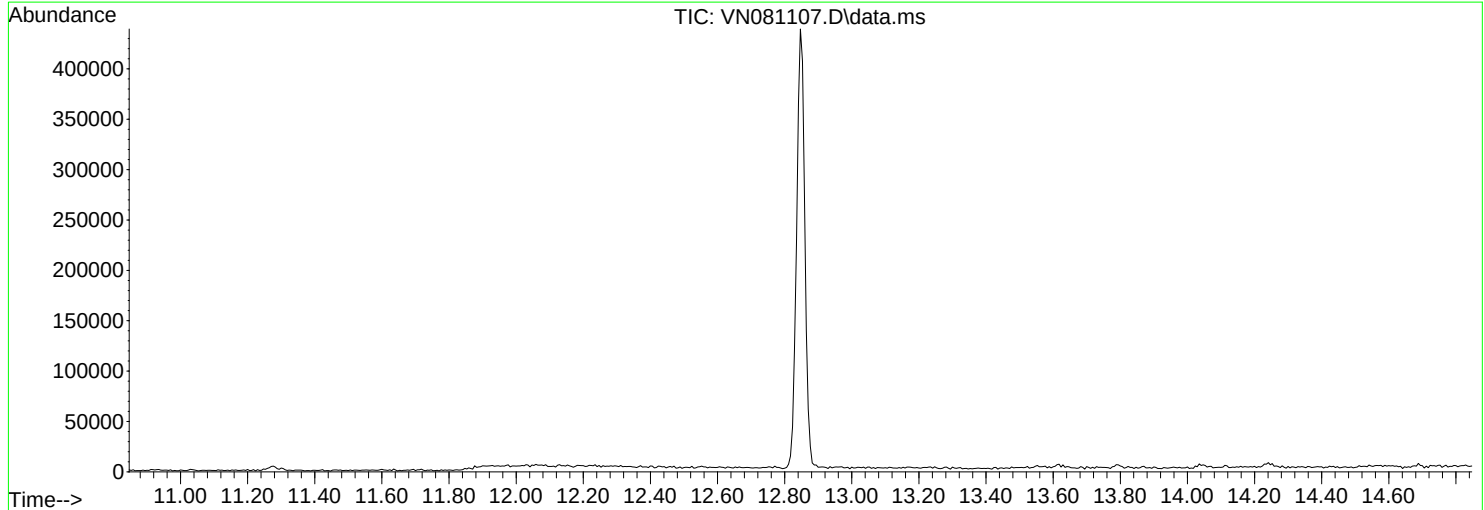

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	16194	PASS
75	95	30	60	51.4	42461	PASS
95	95	100	100	100.0	82619	PASS
96	95	5	9	6.4	5266	PASS
173	174	0.00	2	1.2	716	PASS
174	95	50	100	71.0	58699	PASS
175	174	5	9	7.6	4467	PASS
176	174	95	101	96.7	56773	PASS
177	176	5	9	7.2	4071	PASS

Average of 12.841 to 12.853 min.: VN081107.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.10	92	47.80	480	59.80	375	69.95	681
35.90	525	48.10	179	59.95	562	71.95	653
37.05	3484	48.95	3673	60.95	4352	72.90	1381
38.00	4126	50.00	16194	61.95	4214	73.05	2981
39.00	1757	51.00	5336	63.05	3676	74.00	15407
39.90	240	52.00	263	63.90	293	75.00	42461
43.95	1707	52.20	141	64.10	164	76.00	3999
44.95	866	54.95	450	64.80	81	76.90	481
46.30	105	56.00	1380	66.80	96	77.80	90
46.80	349	56.95	2893	68.00	9030	78.85	3996
47.05	620	57.95	498	68.95	8701	79.70	359

Average of 12.841 to 12.853 min.: VN081107.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.85	781	92.10	1719	106.85	161	131.00	199
80.85	4273	93.00	3869	115.80	97	134.80	135
81.80	371	94.00	10522	115.95	356	135.90	51
81.95	652	95.00	82619	116.80	195	136.75	147
82.95	178	96.05	5266	116.95	461	140.95	1113
86.95	3837	96.80	55	117.75	298	141.60	72
87.95	3762	103.50	99	118.00	183	142.85	1041
88.80	109	103.80	344	118.80	785	144.90	55
90.65	208	104.00	135	127.80	635	145.80	89
91.05	502	105.00	60	129.00	59	147.60	77
91.90	640	105.85	518	130.00	324	147.90	52

Average of 12.841 to 12.853 min.: VN081107.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
158.90	142	207.00	54				
160.75	104						
170.30	51						
171.75	366						
172.05	156						
172.40	110						
172.95	716						
173.95	58699						
174.90	4467						
175.90	56773						
176.90	4071						

Instrument :

MSVOA_N

ClientSampleId :

BFB