

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022125\
 Data File : VN085822.D
 Acq On : 21 Feb 2025 23:01
 Operator : JC\MD
 Sample : Q1405-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-04-021325

Quant Time: Feb 22 02:44:55 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 19 03:43:32 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	285100	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	501960	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	442801	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	183668	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	192280	52.021	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 104.040%			
35) Dibromofluoromethane	8.159	113	172034	52.376	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 104.760%			
50) Toluene-d8	10.565	98	597693	50.015	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 100.020%			
62) 4-Bromofluorobenzene	12.847	95	180373	45.811	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 91.620%			
Target Compounds						
						Qvalue
3) Chloromethane	2.359	50	1586	0.408	ug/l	90
4) Vinyl Chloride	2.518	62	4855	1.178	ug/l	96
11) Tert butyl alcohol	5.777	59	1121	2.466	ug/l #	72
12) 1,1-Dichloroethene	4.342	96	188256	60.213	ug/l	94
16) Acetone	4.436	43	1946	1.664	ug/l	92
18) Methyl Acetate	5.030	43	2240	0.557	ug/l #	47
21) trans-1,2-Dichloroethene	5.789	96	44630	13.257	ug/l	86
24) 1,1-Dichloroethane	6.565	63	48248	7.652	ug/l	99
27) cis-1,2-Dichloroethene	7.483	96	6819018	1746.917	ug/l	91
29) Tetrahydrofuran	7.835	42	930	0.837	ug/l #	38
30) Chloroform	7.953	83	6184	0.938	ug/l	97
31) Cyclohexane	8.224	56	5761	1.091	ug/l #	1
32) 1,1,1-Trichloroethane	8.165	97	79594	13.581	ug/l	95
36) 1,1-Dichloropropene	8.377	75	2044	0.440	ug/l #	65
38) Carbon Tetrachloride	8.224	117	30012	5.434	ug/l #	17
39) Methylcyclohexane	9.353	83	373664	81.823	ug/l #	1
40) Benzene	8.606	78	11646	0.782	ug/l	96
43) Isopropyl Acetate	8.665	43	10412	1.016	ug/l #	54
44) Trichloroethene	9.341	130	22713356	6208.955	ug/l	99
45) 1,2-Dichloropropane	9.347	63	78340	21.783	ug/l #	1
49) 1,4-Dioxane	9.700	88	1332	24.655	ug/l #	74
55) 1,1,2-Trichloroethane	11.012	97	1198	0.345	ug/l #	77
60) Dibromochloromethane	11.100	129	12647	3.128	ug/l #	10
64) Tetrachloroethene	11.100	164	13909	4.055	ug/l	98
65) Chlorobenzene	11.882	112	3536	0.349	ug/l	93
76) 1,2,3-Trichloropropane	12.847	75	88605	21.717	ug/l #	1
78) n-propylbenzene	13.123	91	72514	5.032	ug/l #	53
79) 2-Chlorotoluene	13.123	91	72514	7.531	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.847	75	88605	63.366	ug/l #	12
82) 4-Chlorotoluene	13.123	91	72514	7.597	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022125\
Data File : VN085822.D
Acq On : 21 Feb 2025 23:01
Operator : JC\MD
Sample : Q1405-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-04-021325

Quant Time: Feb 22 02:44:55 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 19 03:43:32 2025
Response via : Initial Calibration




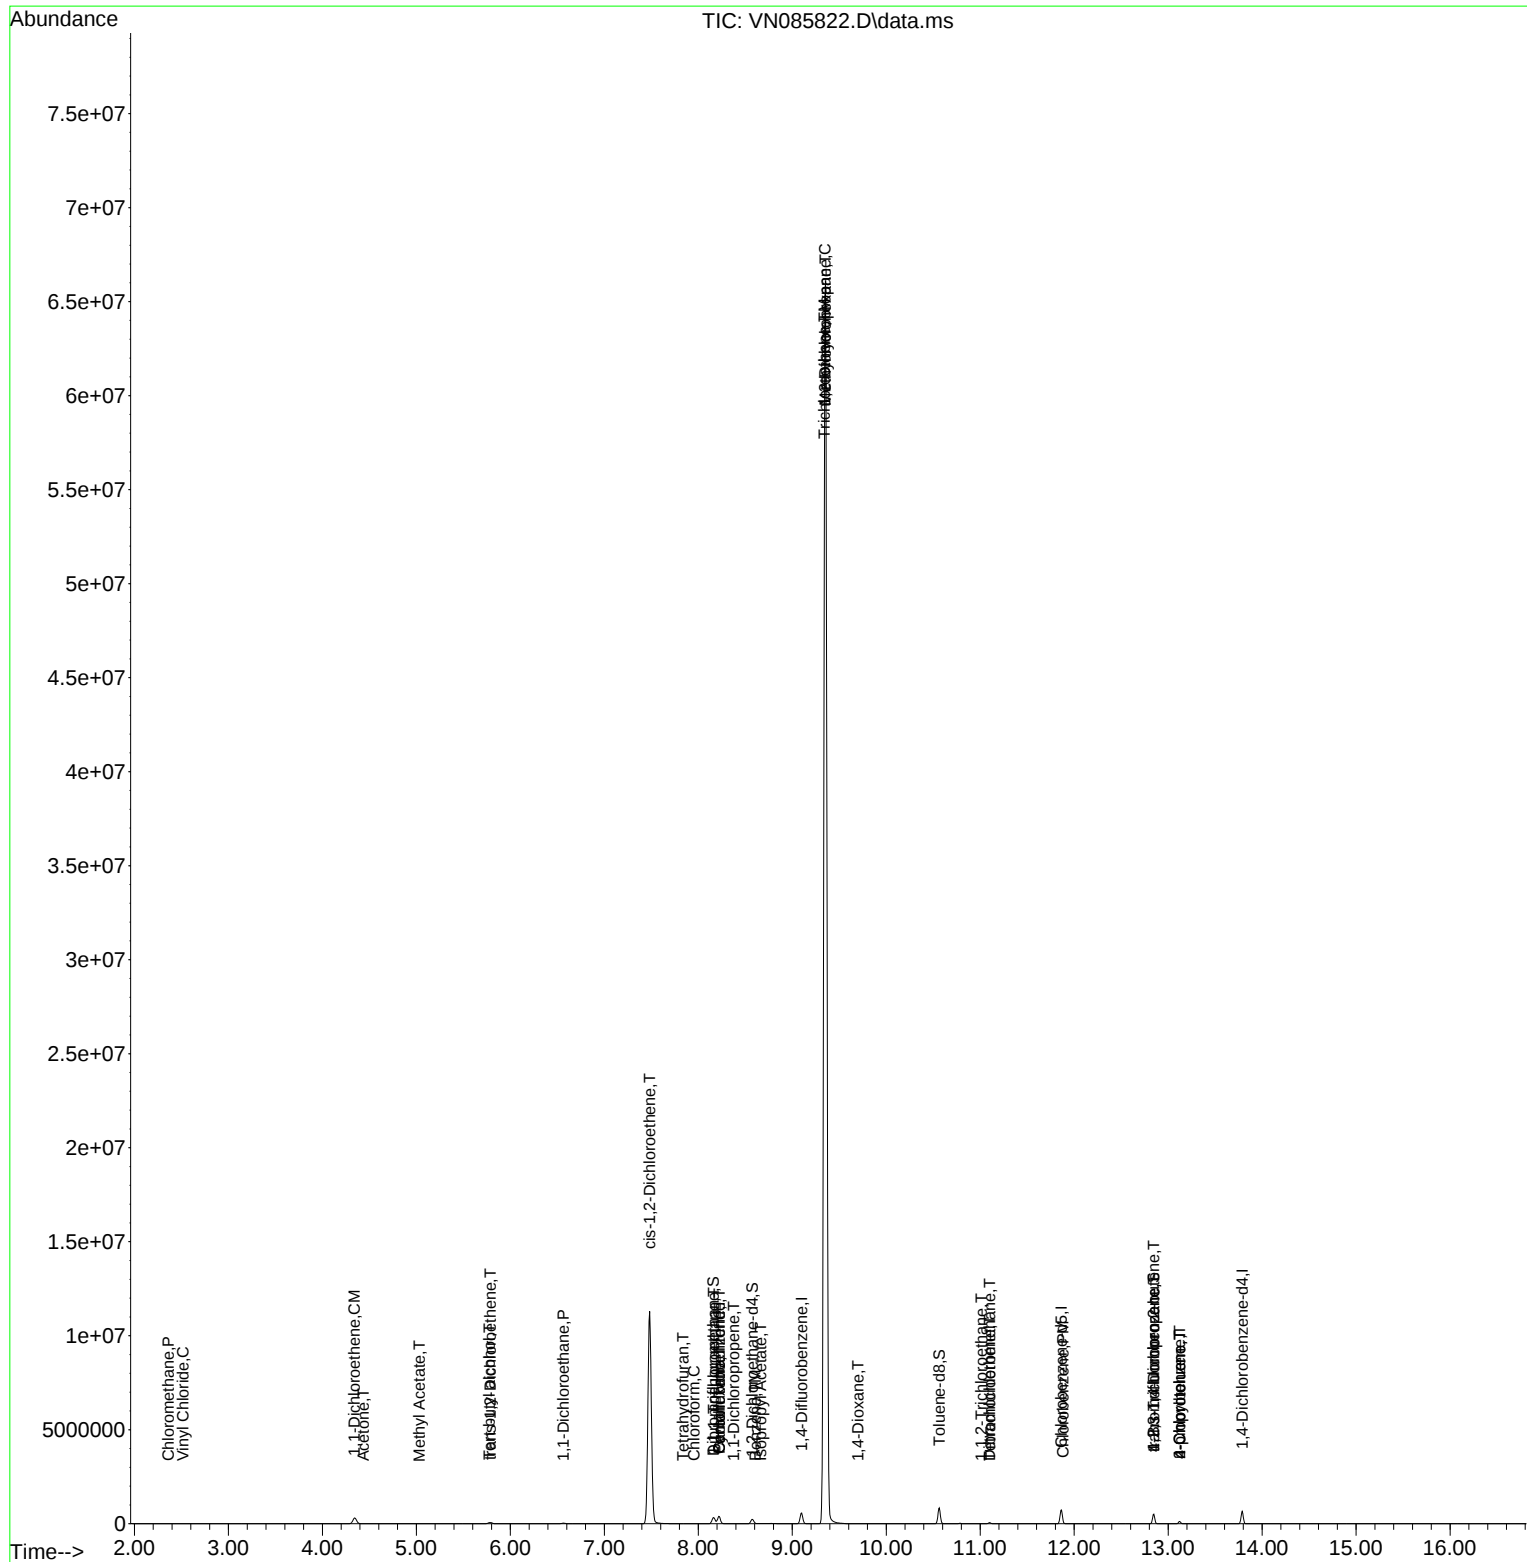




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1
Delta R.T. 0.006 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01




Instrument :
MSVOA_N
ClientSampleId :
MW-04-021325


Tgt Ion:168 Resp: 285100
Ion Ratio Lower Upper
168 100
99 59.7 47.9 71.9

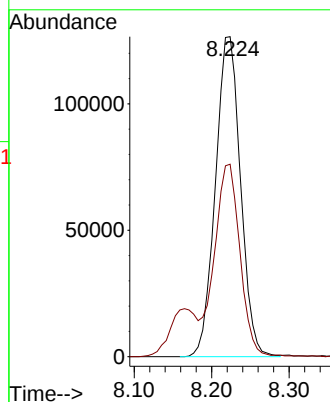

#3
Chloromethane
Concen: 0.408 ug/l
RT: 2.359 min Scan# 69
Delta R.T. -0.000 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01

Tgt Ion: 50 Resp: 1586
Ion Ratio Lower Upper
50 100
52 27.9 26.7 40.1


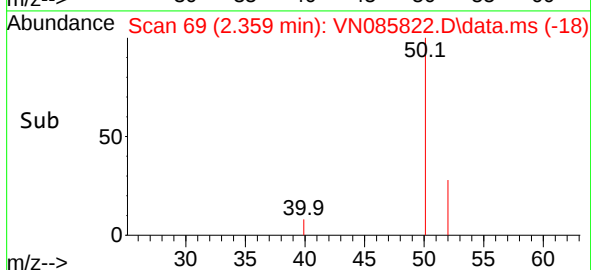

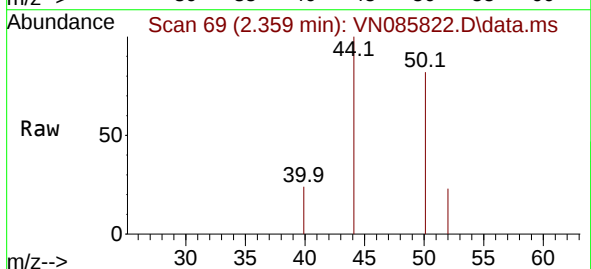


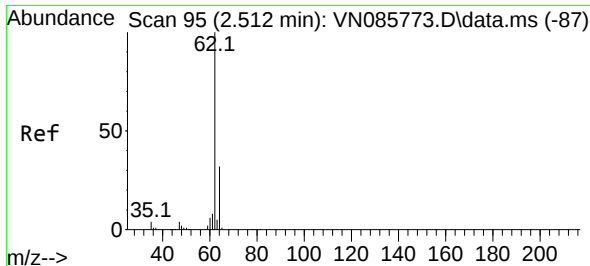

#4
 Vinyl Chloride
 Concen: 1.178 ug/l
 RT: 2.518 min Scan# 90
 Delta R.T. 0.006 min
 Lab File: VN085822.D
 Acq: 21 Feb 2025 23:01




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-04-021325


Tgt Ion: 62 Resp: 4855
 Ion Ratio Lower Upper
 62 100
 64 30.0 25.9 38.9

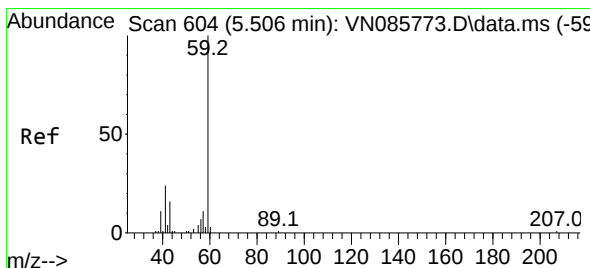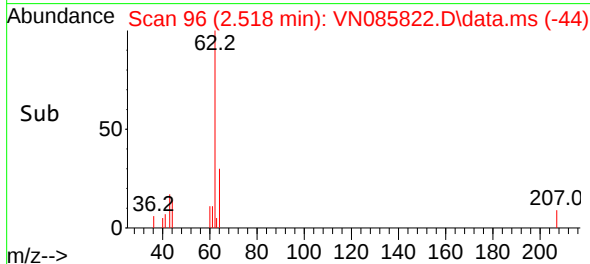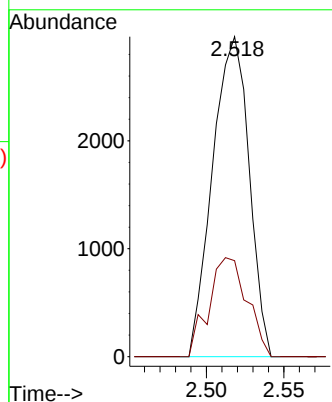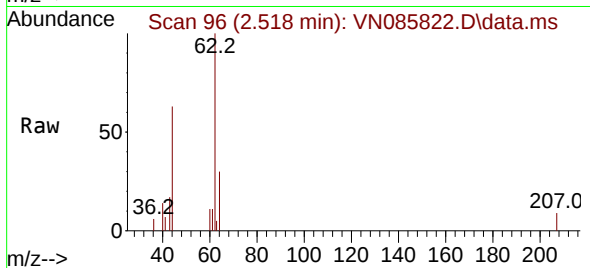

#11
 Tert butyl alcohol
 Concen: 2.466 ug/l
 RT: 5.777 min Scan# 650
 Delta R.T. 0.271 min
 Lab File: VN085822.D
 Acq: 21 Feb 2025 23:01

Tgt Ion: 59 Resp: 1121
 Ion Ratio Lower Upper
 59 100
 57 0.0 8.3 12.5#


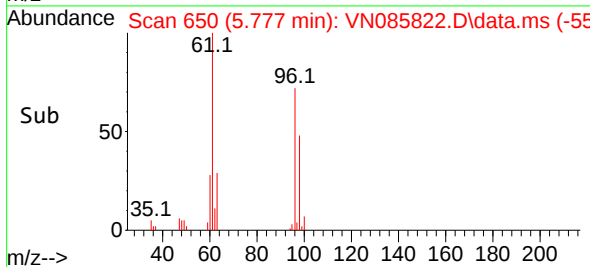
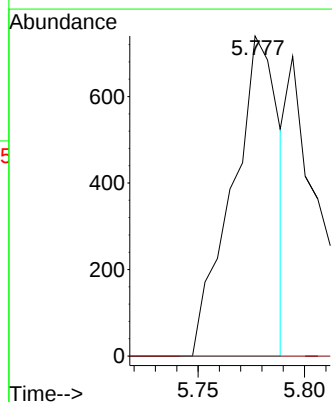
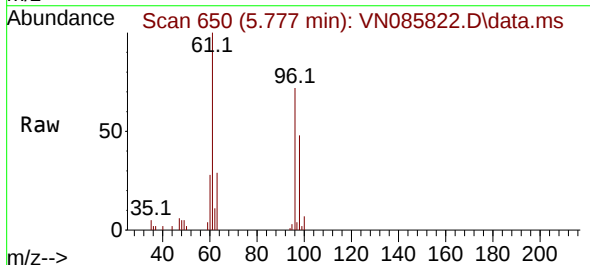




#12
 1,1-Dichloroethene
 Concen: 60.213 ug/l
 RT: 4.342 min Scan# 406
 Delta R.T. 0.006 min
 Lab File: VN085822.D
 Acq: 21 Feb 2025 23:01




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-04-021325


Tgt Ion: 96 Resp: 188256
 Ion Ratio Lower Upper
 96 100
 61 162.6 123.3 184.9
 98 65.3 48.6 72.8

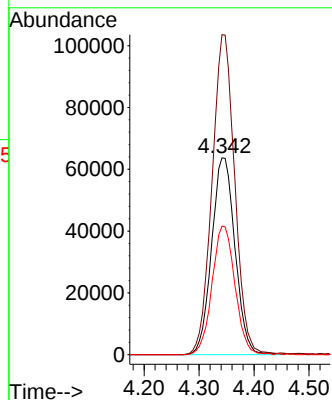

#16
 Acetone
 Concen: 1.664 ug/l
 RT: 4.436 min Scan# 422
 Delta R.T. 0.018 min
 Lab File: VN085822.D
 Acq: 21 Feb 2025 23:01


Tgt Ion: 43 Resp: 1946
 Ion Ratio Lower Upper
 43 100
 58 29.8 27.5 41.3

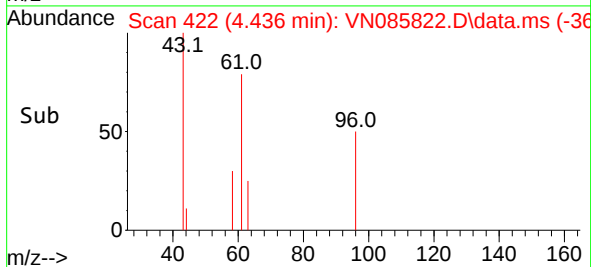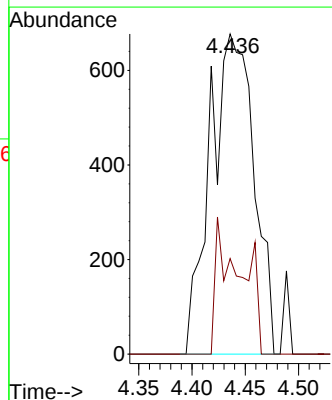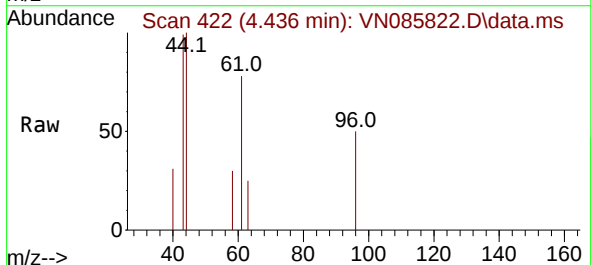






#18
Methyl Acetate
Concen: 0.557 ug/l
RT: 5.030 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01

Instrument :
MSVOA_N
ClientSampleId :
MW-04-021325







Tgt Ion: 43 Resp: 2240
Ion Ratio Lower Upper
43 100
74 0.0 22.2 33.4#

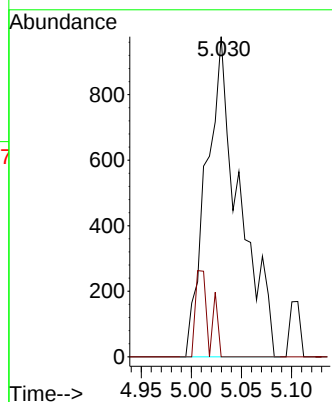

#21
trans-1,2-Dichloroethene
Concen: 13.257 ug/l
RT: 5.789 min Scan# 652
Delta R.T. 0.006 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01

Tgt Ion: 96 Resp: 44630
Ion Ratio Lower Upper
96 100
61 117.1 112.6 168.8
98 64.3 53.3 79.9


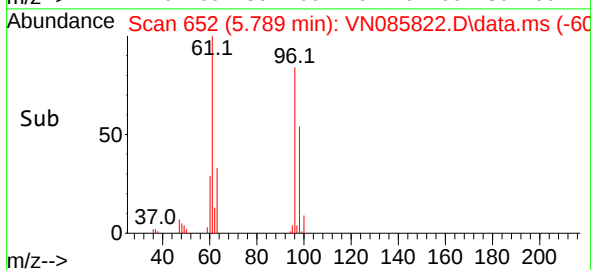
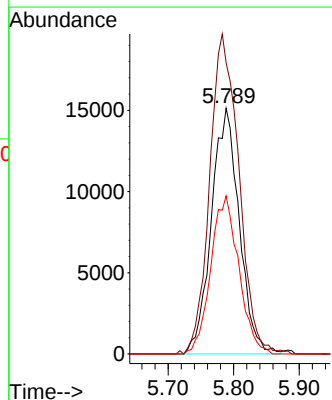
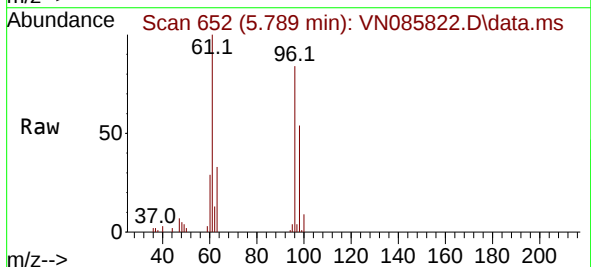




#24
 1,1-Dichloroethane
 Concen: 7.652 ug/l
 RT: 6.565 min Scan# 784
 Delta R.T. -0.000 min
 Lab File: VN085822.D
 Acq: 21 Feb 2025 23:01




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-04-021325


Tgt Ion: 63 Resp: 48248
 Ion Ratio Lower Upper
 63 100
 98 6.9 3.5 10.4
 100 5.9 2.4 7.2

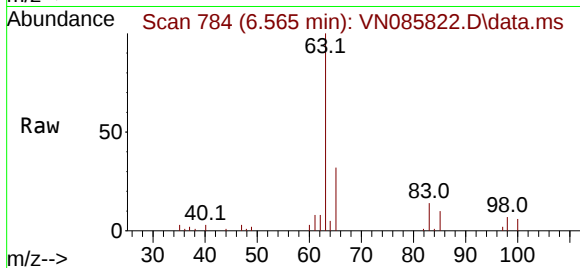

#27
 cis-1,2-Dichloroethene
 Concen: 1746.917 ug/l
 RT: 7.483 min Scan# 940
 Delta R.T. -0.000 min
 Lab File: VN085822.D
 Acq: 21 Feb 2025 23:01

Tgt Ion: 96 Resp: 6819018
 Ion Ratio Lower Upper
 96 100
 61 125.6 0.0 280.6
 98 63.7 0.0 128.6


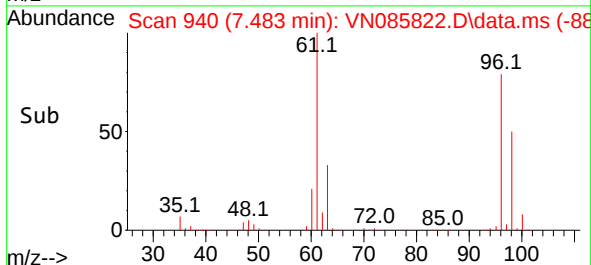
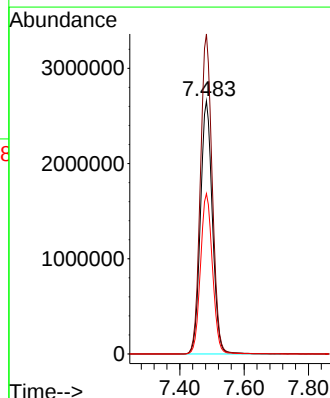
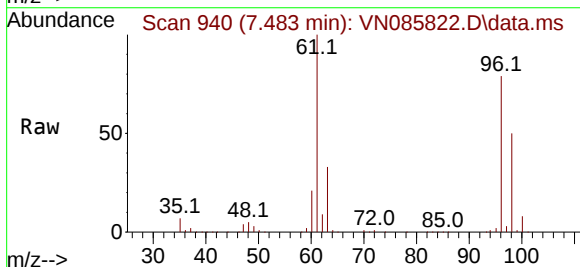




#29
Tetrahydrofuran
Concen: 0.837 ug/l
RT: 7.835 min Scan# 1000
Delta R.T. 0.006 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01




Instrument :
MSVOA_N
ClientSampleId :
MW-04-021325


Tgt Ion: 42 Resp: 930
Ion Ratio Lower Upper
42 100
72 5.8 40.0 60.0#
71 6.5 37.0 55.4#

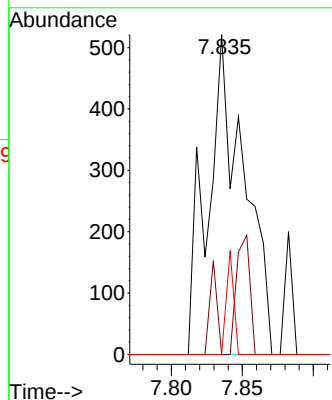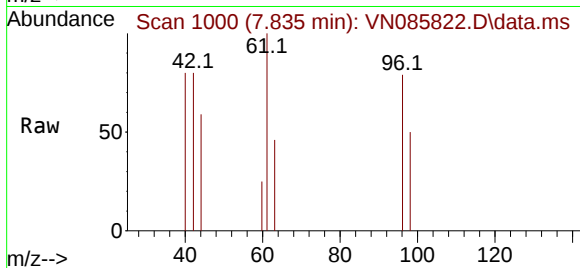

#30
Chloroform
Concen: 0.938 ug/l
RT: 7.953 min Scan# 1020
Delta R.T. -0.006 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01

Tgt Ion: 83 Resp: 6184
Ion Ratio Lower Upper
83 100
85 60.9 50.9 76.3


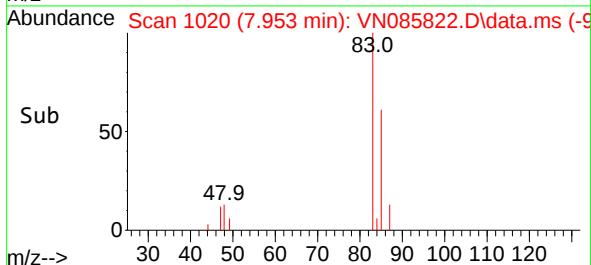
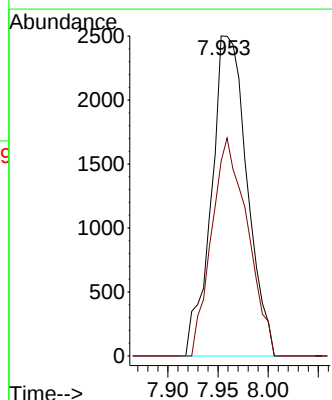
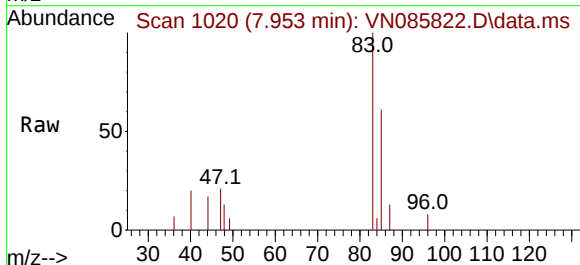




#31
Cyclohexane
Concen: 1.091 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.029 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01




Instrument :
MSVOA_N
ClientSampleId :
MW-04-021325


Tgt Ion: 56 Resp: 5761
Ion Ratio Lower Upper
56 100
69 217.4 25.8 38.6#
84 158.7 74.5 111.7#

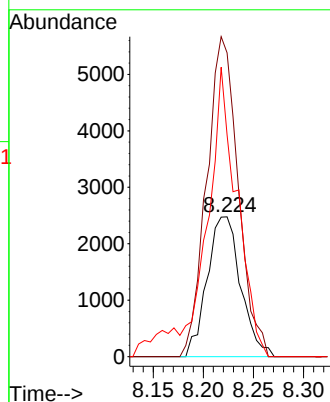

#32
1,1,1-Trichloroethane
Concen: 13.581 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01

Tgt Ion: 97 Resp: 79594
Ion Ratio Lower Upper
97 100
99 57.3 50.4 75.6
61 44.9 35.5 53.3

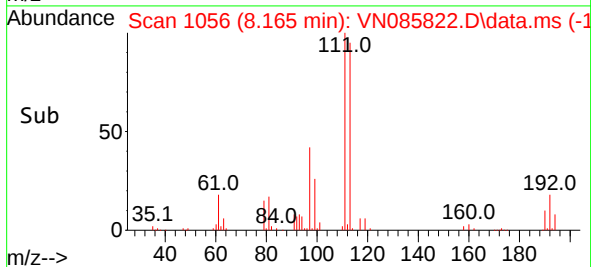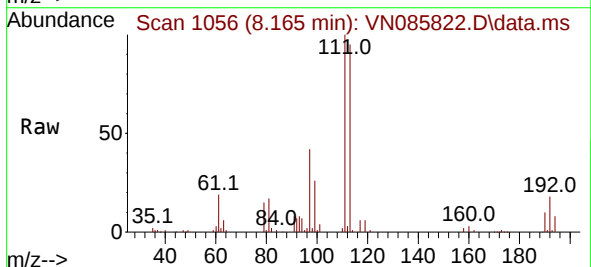

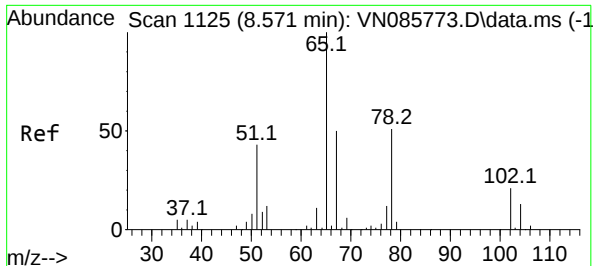

#33

1,2-Dichloroethane-d4

Concen: 52.021 ug/l

RT: 8.577 min Scan# 1125

Delta R.T. 0.006 min

Lab File: VN085822.D

Acq: 21 Feb 2025 23:01

Instrument :

MSVOA_N

ClientSampleId :





MW-04-021325

Tgt Ion: 65 Resp: 192280

Ion Ratio Lower Upper

65 100

67 53.1 0.0 106.2

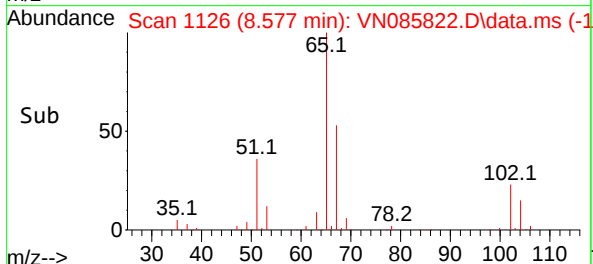

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1215

Delta R.T. 0.006 min

Lab File: VN085822.D

Acq: 21 Feb 2025 23:01




Tgt Ion: 114 Resp: 501960


Ion Ratio Lower Upper

114 100

63 20.1 0.0 39.2

88 16.5 0.0 30.0


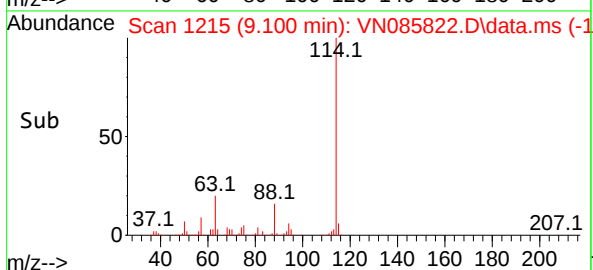

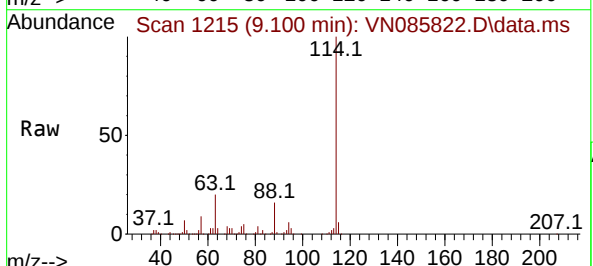


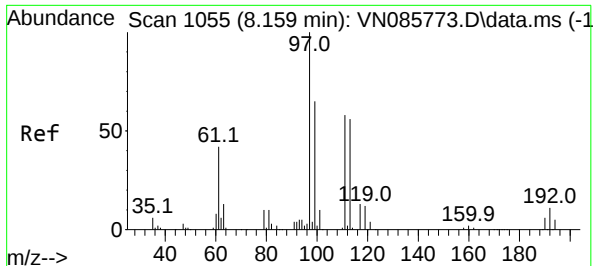

#35
Dibromofluoromethane
Concen: 52.376 ug/l
RT: 8.159 min Scan# 1055
Delta R.T. -0.000 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01




Instrument :
MSVOA_N
ClientSampleId :
MW-04-021325


Tgt Ion:113 Resp: 172034
Ion Ratio Lower Upper
113 100
111 102.9 82.2 123.4
192 19.0 14.7 22.1

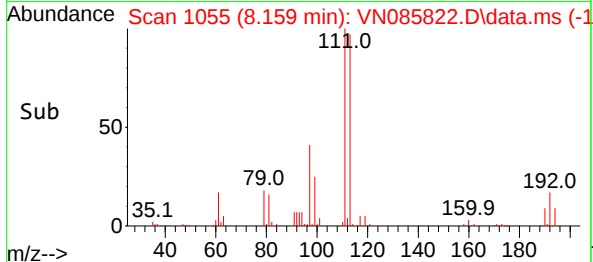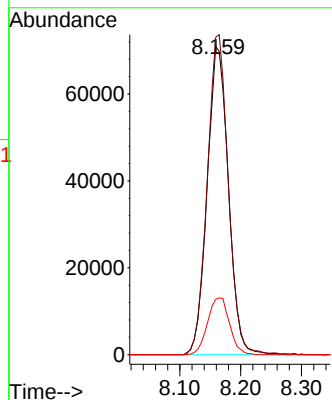

#36
1,1-Dichloropropene
Concen: 0.440 ug/l
RT: 8.377 min Scan# 1092
Delta R.T. 0.012 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01


Tgt Ion: 75 Resp: 2044
Ion Ratio Lower Upper
75 100
110 19.0 17.3 52.0
77 7.0 24.6 37.0#

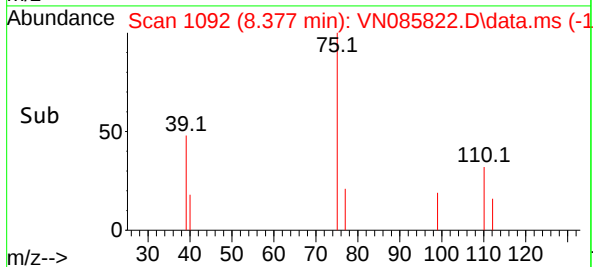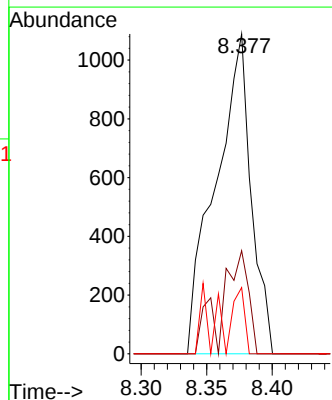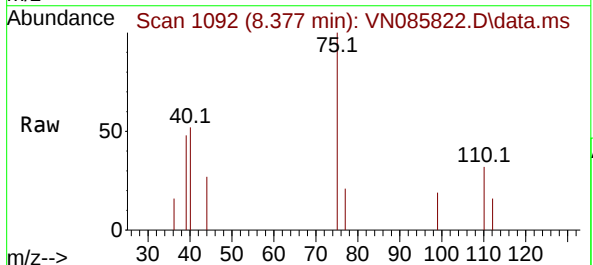



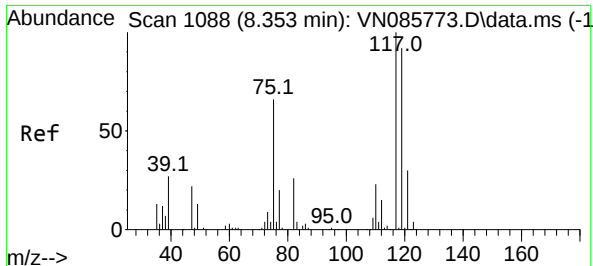


#38
Carbon Tetrachloride
Concen: 5.434 ug/l
RT: 8.224 min Scan# 11
Delta R.T. -0.129 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01

Instrument :
MSVOA_N
ClientSampleId :
MW-04-021325







Tgt Ion:117 Resp: 30012
Ion Ratio Lower Upper
117 100
119 4.2 73.8 110.6#
121 0.0 24.3 36.5#

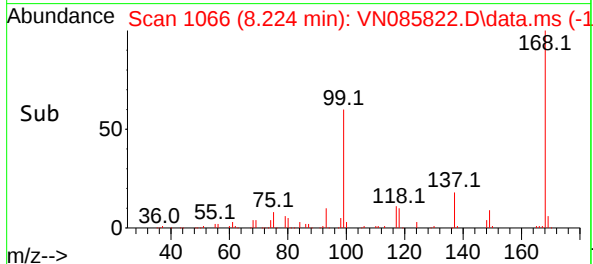

#39
Methylcyclohexane
Concen: 81.823 ug/l
RT: 9.353 min Scan# 1258
Delta R.T. -0.241 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01

Tgt Ion: 83 Resp: 373664
Ion Ratio Lower Upper
83 100
55 0.0 57.5 86.3#
98 199.7 39.2 58.8#


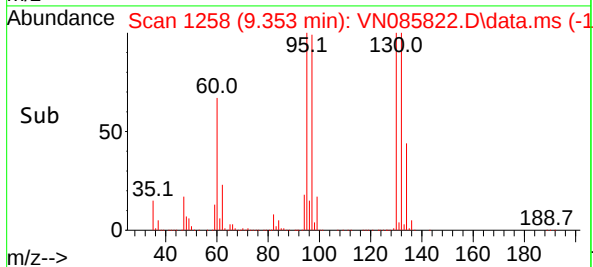

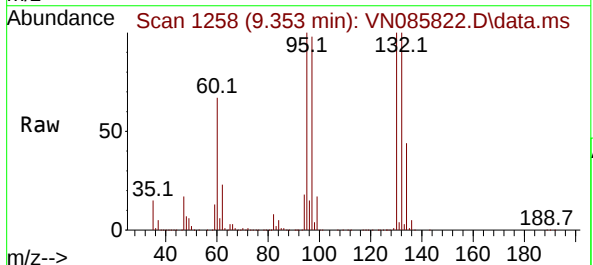


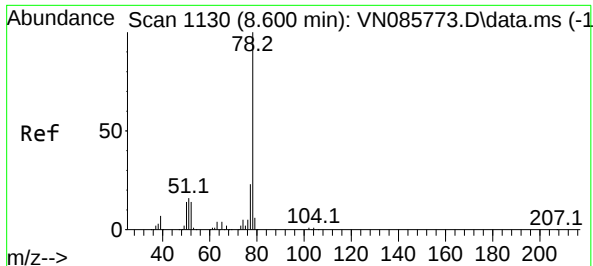

#40
Benzene
Concen: 0.782 ug/l
RT: 8.606 min Scan# 1130
Delta R.T. 0.006 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01




Instrument :
MSVOA_N
ClientSampleId :
MW-04-021325


Tgt Ion: 78 Resp: 11646
Ion Ratio Lower Upper
78 100
77 20.8 18.3 27.5

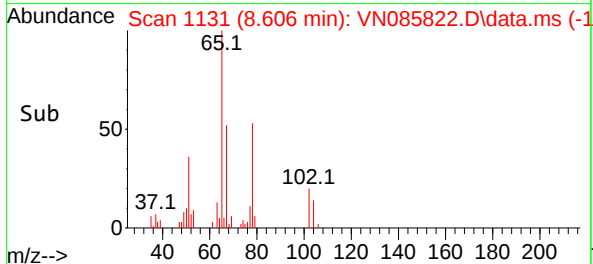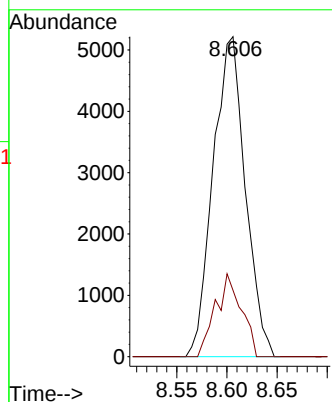

#43
Isopropyl Acetate
Concen: 1.016 ug/l
RT: 8.665 min Scan# 1141
Delta R.T. -0.018 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01

Tgt Ion: 43 Resp: 10412
Ion Ratio Lower Upper
43 100
61 1.2 22.6 34.0#
87 0.0 11.8 17.8#


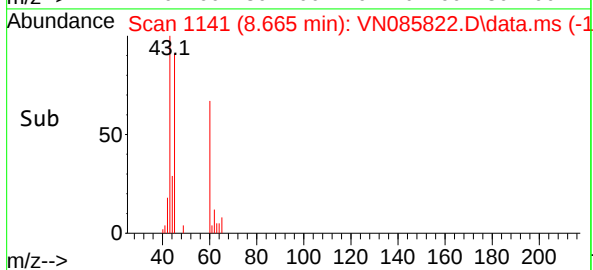
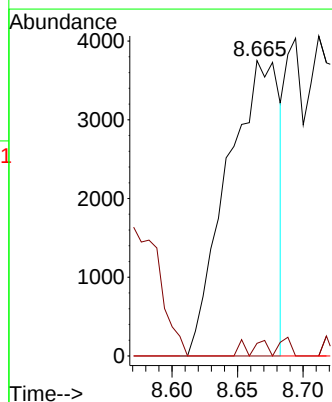
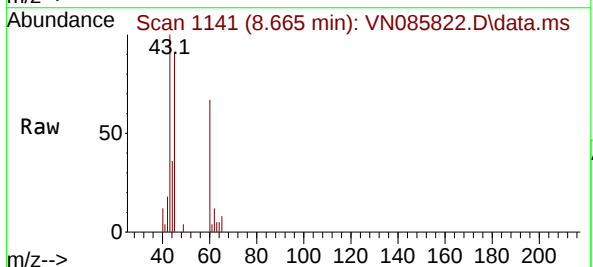


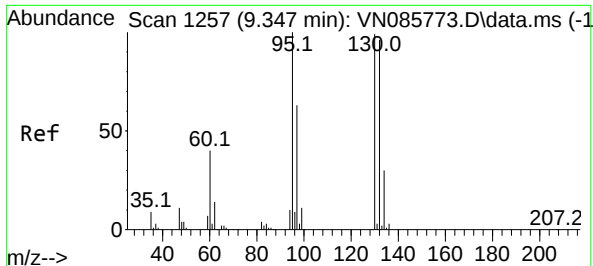

#44
Trichloroethene
Concen: 6208.955 ug/l
RT: 9.341 min Scan# 1256
Delta R.T. -0.006 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01




Instrument :
MSVOA_N
ClientSampleId :
MW-04-021325


Tgt Ion:130 Resp:22713356
Ion Ratio Lower Upper
130 100
95 100.0 0.0 202.6

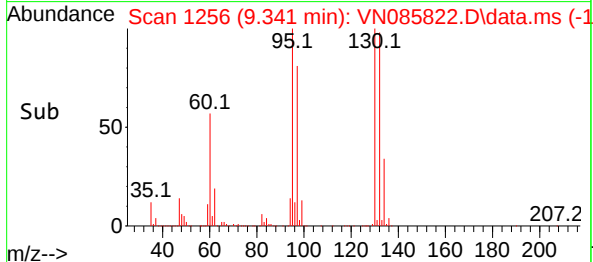

#45
1,2-Dichloropropane
Concen: 21.783 ug/l
RT: 9.347 min Scan# 1257
Delta R.T. -0.271 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01

Tgt Ion: 63 Resp: 78340
Ion Ratio Lower Upper
63 100
65 504.2 25.1 37.7#

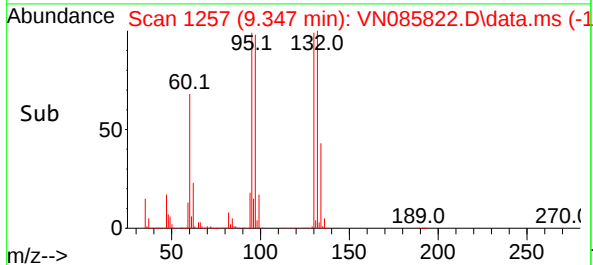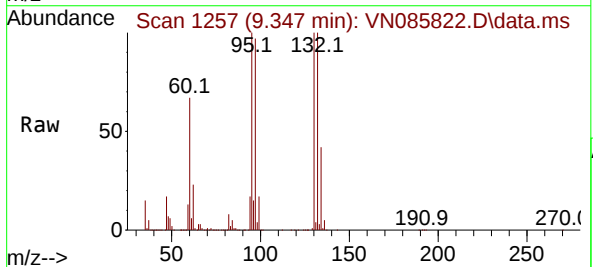

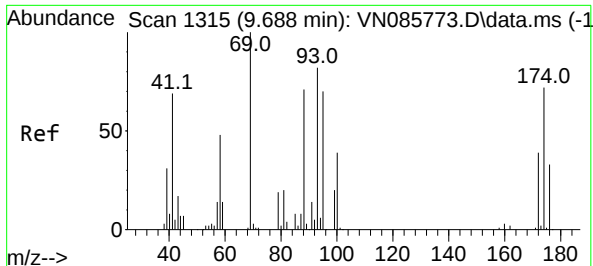

#49

1,4-Dioxane

Concen: 24.655 ug/l

RT: 9.700 min Scan# 1

Delta R.T. 0.012 min

Lab File: VN085822.D

Acq: 21 Feb 2025 23:01

Instrument :

MSVOA_N

ClientSampleId :

MW-04-021325





Tgt Ion: 88 Resp: 1332

Ion Ratio Lower Upper

88 100

43 70.3 18.6 27.8#

58 68.5 56.7 85.1

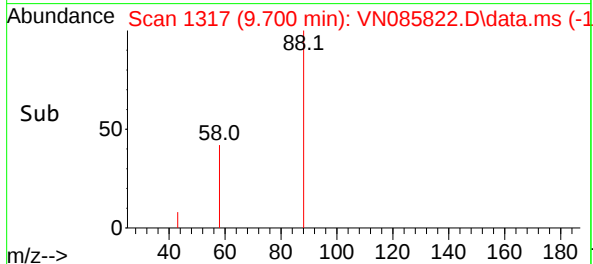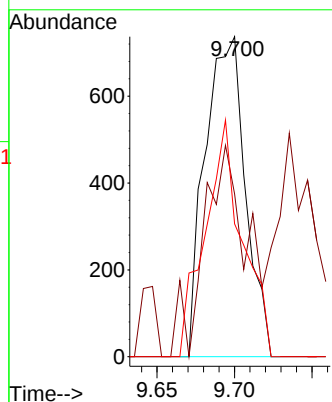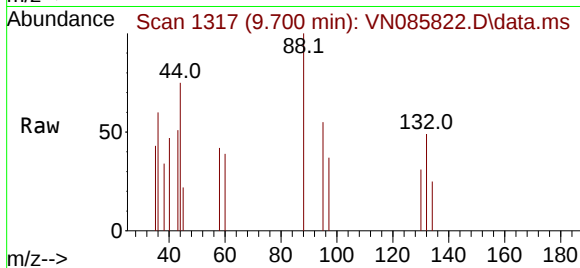

#50

Toluene-d8

Concen: 50.015 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. 0.006 min

Lab File: VN085822.D




Acq: 21 Feb 2025 23:01


Tgt Ion: 98 Resp: 597693

Ion Ratio Lower Upper

98 100

100 63.5 52.1 78.1



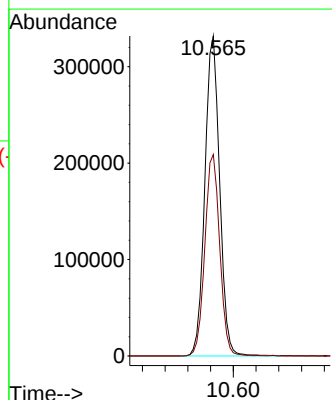
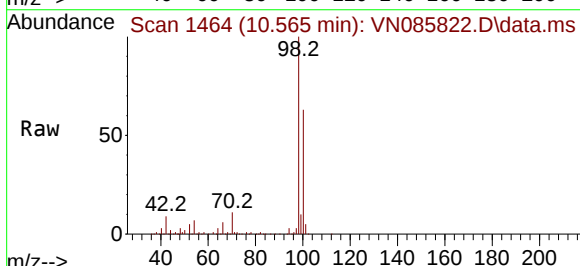




#55
1,1,2-Trichloroethane
Concen: 0.345 ug/l
RT: 11.012 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01




Instrument :
MSVOA_N
ClientSampleId :
MW-04-021325


Tgt Ion: 97	Resp: 1198
Ion Ratio	Lower Upper
97 100	
83 55.6	66.1 99.1#
85 31.1	44.7 67.1#
99 59.7	49.7 74.5



#60
Dibromochloromethane
Concen: 3.128 ug/l
RT: 11.100 min Scan# 1555
Delta R.T. -0.253 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01

Tgt Ion:129	Resp:	12647	
Ion	Ratio	Lower	Upper
129	100		
127	0.0	39.1	117.5#


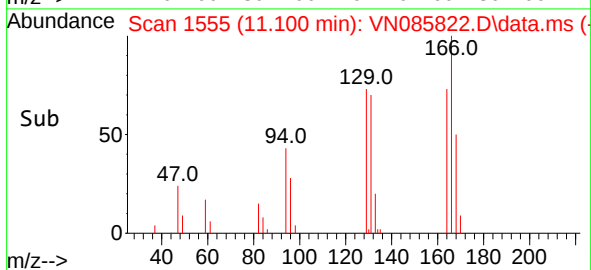

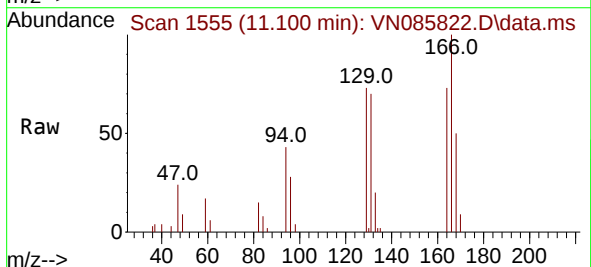




#62
4-Bromofluorobenzene
Concen: 45.811 ug/l
RT: 12.847 min Scan# 1851
Delta R.T. 0.006 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01




Instrument :
MSVOA_N
ClientSampleId :
MW-04-021325


Tgt Ion: 95 Resp: 180373
Ion Ratio Lower Upper
95 100
174 78.2 0.0 152.4
176 73.9 0.0 146.6



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. 0.006 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01

Tgt Ion: 117 Resp: 442801
Ion Ratio Lower Upper
117 100
82 55.6 45.7 68.5
119 31.3 26.2 39.2

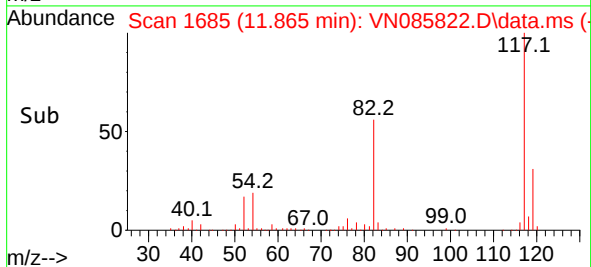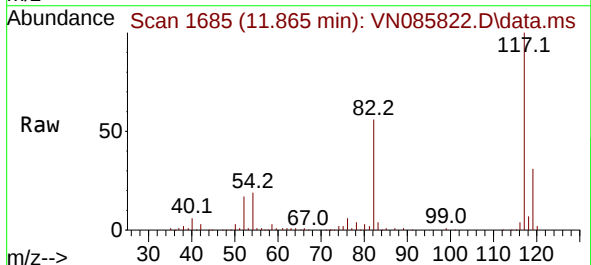



#64

Tetrachloroethene

Concen: 4.055 ug/l

RT: 11.100 min Scan# 1555

Delta R.T. -0.000 min

Lab File: VN085822.D

Acq: 21 Feb 2025 23:01

Instrument :

MSVOA_N

ClientSampleId :

MW-04-021325

Tgt Ion:164 Resp: 13909





Ion Ratio Lower Upper

164 100

166 137.6 107.2 160.8

129 99.8 80.7 121.1

131 96.1 74.6 112.0

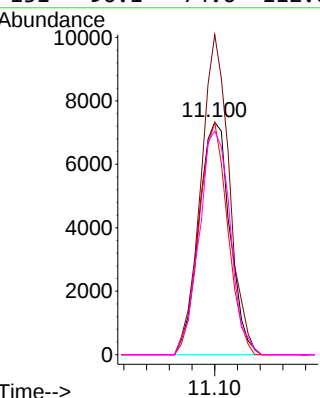

#65

Chlorobenzene

Concen: 0.349 ug/l

RT: 11.882 min Scan# 1688

Delta R.T. -0.000 min

Lab File: VN085822.D




Acq: 21 Feb 2025 23:01


Tgt Ion:112 Resp: 3536

Ion Ratio Lower Upper

112 100

114 26.5 24.3 36.5


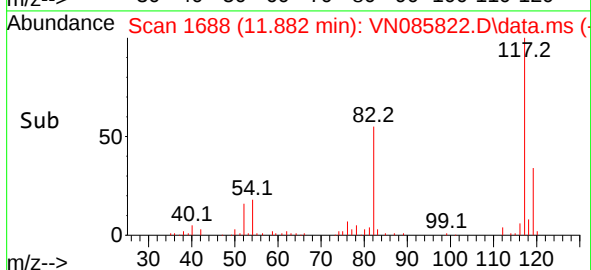
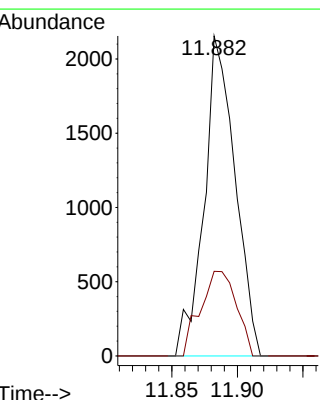



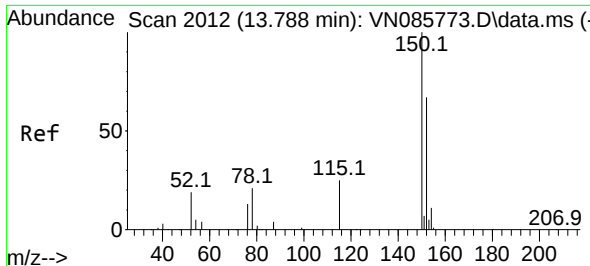

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.788 min Scan# 2012
 Delta R.T. -0.000 min
 Lab File: VN085822.D
 Acq: 21 Feb 2025 23:01




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-04-021325


Tgt Ion:152 Resp: 183668
 Ion Ratio Lower Upper
 152 100
 115 58.3 30.4 91.3
 150 155.8 0.0 345.4

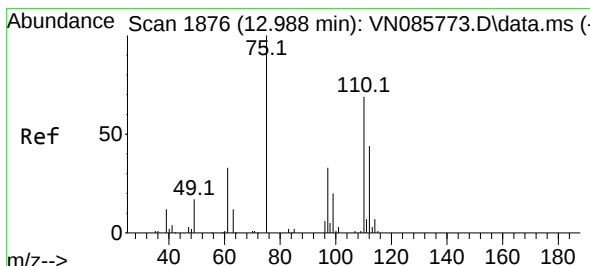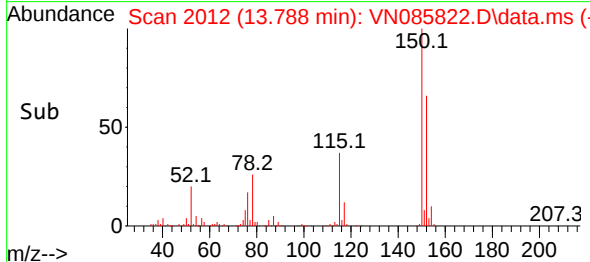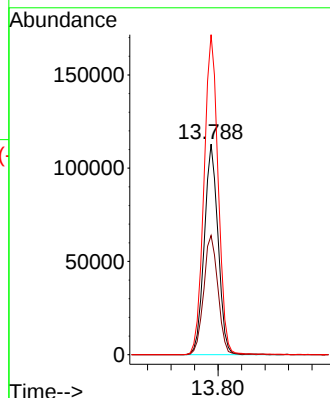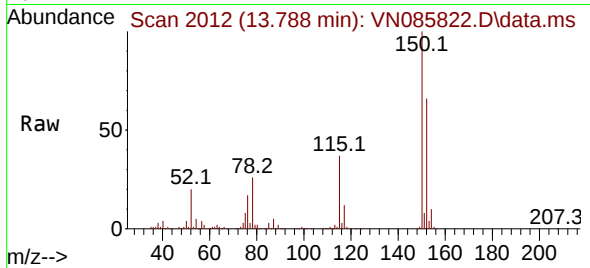

#76
 1,2,3-Trichloropropane
 Concen: 21.717 ug/l
 RT: 12.847 min Scan# 1852
 Delta R.T. -0.141 min
 Lab File: VN085822.D
 Acq: 21 Feb 2025 23:01

Tgt Ion: 75 Resp: 88605
 Ion Ratio Lower Upper
 75 100
 77 1.5 100.0 300.0#


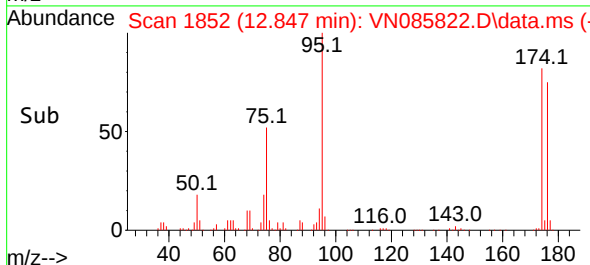

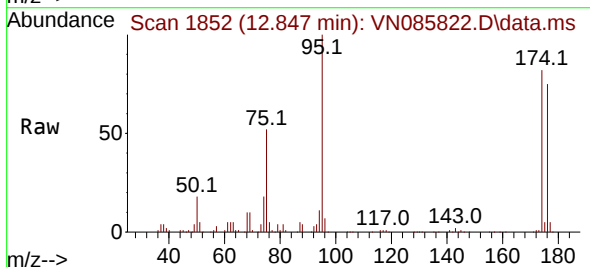




#78
n-propylbenzene
Concen: 5.032 ug/l
RT: 13.123 min Scan# 1899
Delta R.T. 0.094 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01




Instrument :
MSVOA_N
ClientSampleId :
MW-04-021325


Tgt Ion: 91 Resp: 72514
Ion Ratio Lower Upper
91 100
120 0.0 11.3 33.8#

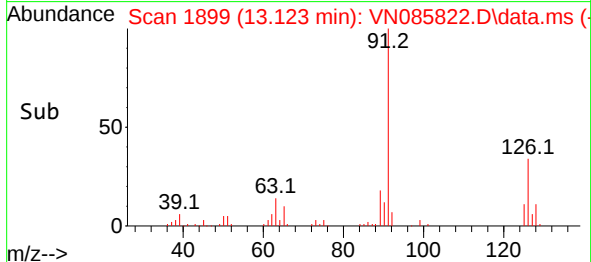

#79
2-Chlorotoluene
Concen: 7.531 ug/l
RT: 13.123 min Scan# 1899
Delta R.T. 0.006 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01

Tgt Ion: 91 Resp: 72514
Ion Ratio Lower Upper
91 100
126 33.0 16.4 49.1



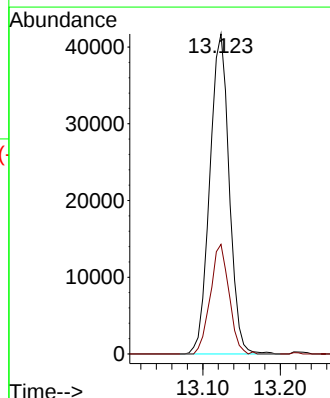





#81
trans-1,4-Dichloro-2-butene
Concen: 63.366 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.118 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01

Instrument :
MSVOA_N
ClientSampleId :
MW-04-021325

Tgt Ion: 75 Resp: 88605
Ion Ratio Lower Upper
75 100
53 0.0 74.2 111.4#
89 0.0 34.9 52.3#

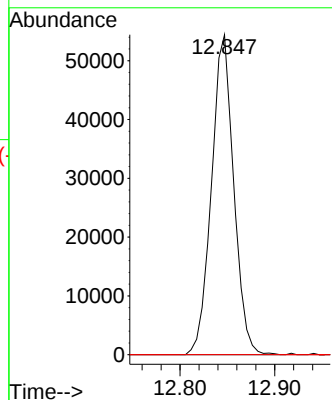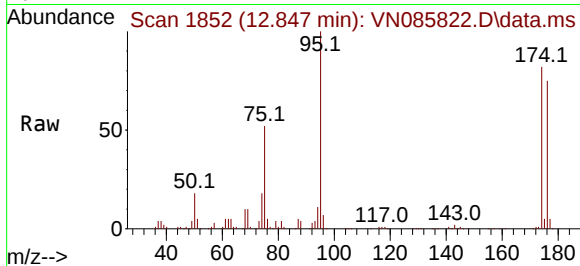

#82
4-Chlorotoluene
Concen: 7.597 ug/l
RT: 13.123 min Scan# 1899
Delta R.T. -0.094 min
Lab File: VN085822.D
Acq: 21 Feb 2025 23:01

Tgt Ion: 91 Resp: 72514
Ion Ratio Lower Upper
91 100
126 33.0 16.4 49.4

