


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022125\
Data File : VN085801.D
Acq On : 21 Feb 2025 14:10
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Title : SW846 8260
Last Update : Wed Feb 19 03:43:32 2025

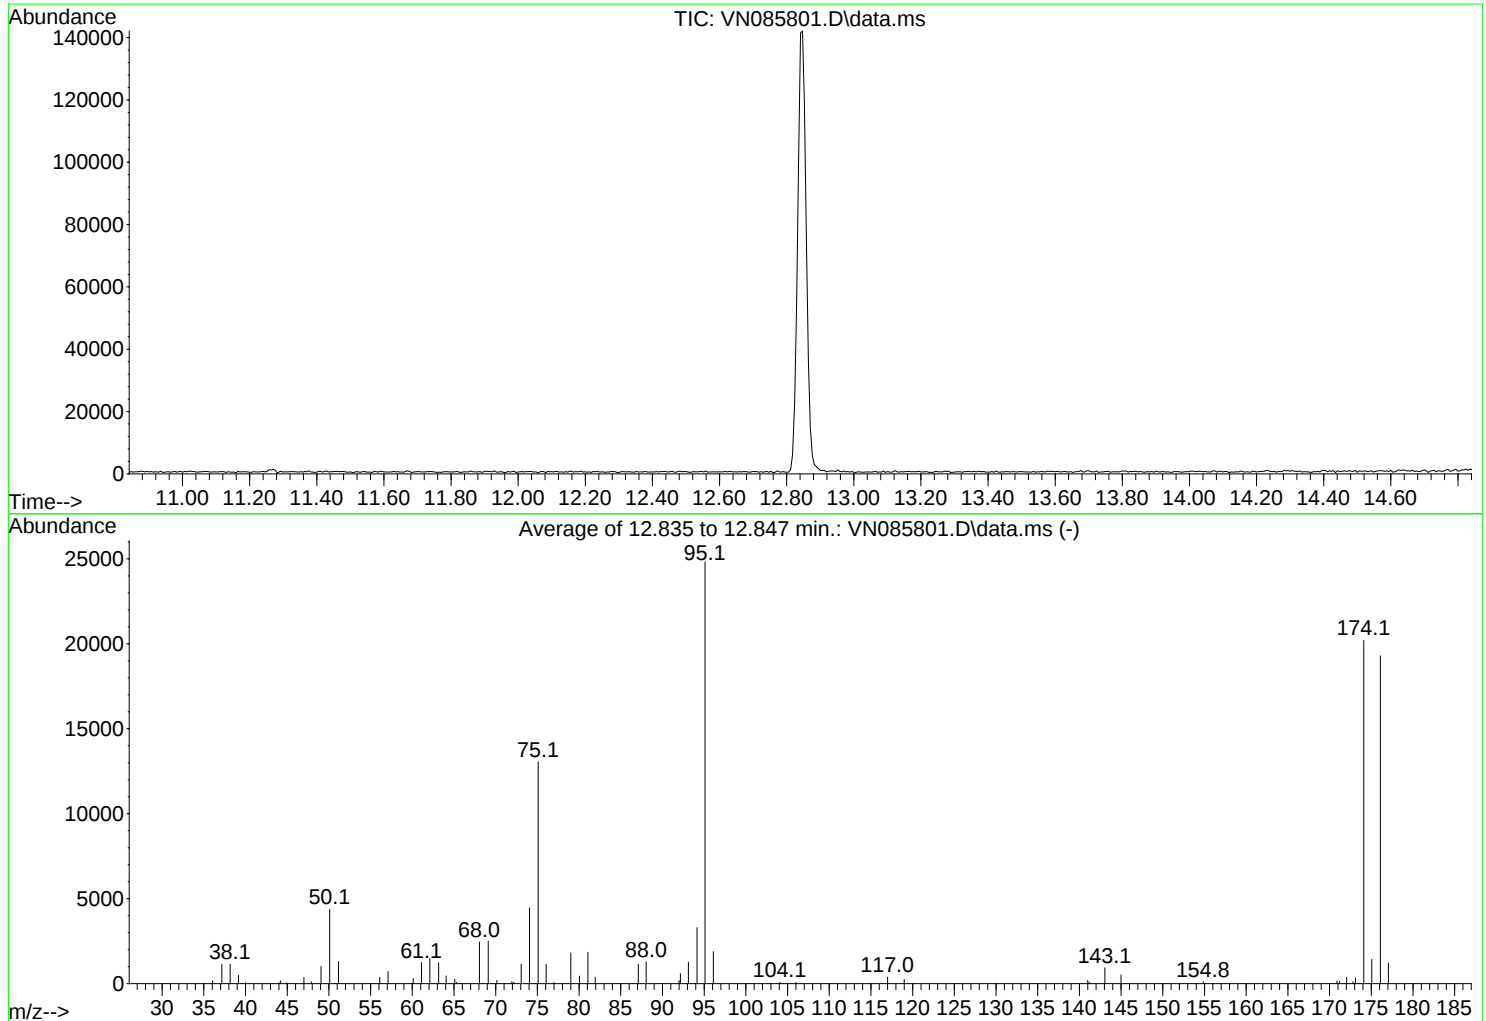

AutoFind: Scans 1850, 1851, 1852; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.6	4381	PASS
75	95	30	60	52.6	13051	PASS
95	95	100	100	100.0	24827	PASS
96	95	5	9	7.6	1881	PASS
173	174	0.00	2	1.7	339	PASS
174	95	50	100	81.4	20204	PASS
175	174	5	9	7.1	1432	PASS
176	174	95	101	95.5	19296	PASS
177	176	5	9	6.2	1205	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	174	50.10	4381	68.05	2450	80.05	431
37.15	1127	51.15	1305	69.10	2505	81.05	184
38.15	1151	56.10	363	70.15	198	81.95	38
39.15	494	57.10	719	71.95	114	87.10	113
40.00	62	60.10	298	72.20	81	88.05	1278
44.00	54	61.10	1243	73.05	1151	92.00	182
44.20	163	62.10	1475	74.05	4456	92.15	586
44.90	58	63.15	1236	75.10	13051	93.10	1275
47.00	365	64.05	451	76.05	1135	94.15	3297
47.90	108	65.10	265	77.00	65	95.10	24827
49.05	1021	65.30	79	79.00	1803	96.10	1881

Average of 12.835 to 12.847 min.: VN085801.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
104.10	82	172.05	379				
106.00	69	172.80	117				
117.00	381	173.10	339				
119.00	242	174.10	20204				
141.00	187	175.05	1432				
141.20	79	176.10	19296				
143.05	934	177.05	1205				
145.00	521						
154.85	109						
170.90	162						
171.20	133						

Instrument :

MSVOA_N

ClientSampleId :

BFB