


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN022219\
Data File : VN053903.D
Acq On : 22 Feb 2019 8:00
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022019W.M
Title : SW846 8260
Last Update : Thu Feb 21 03:36:07 2019

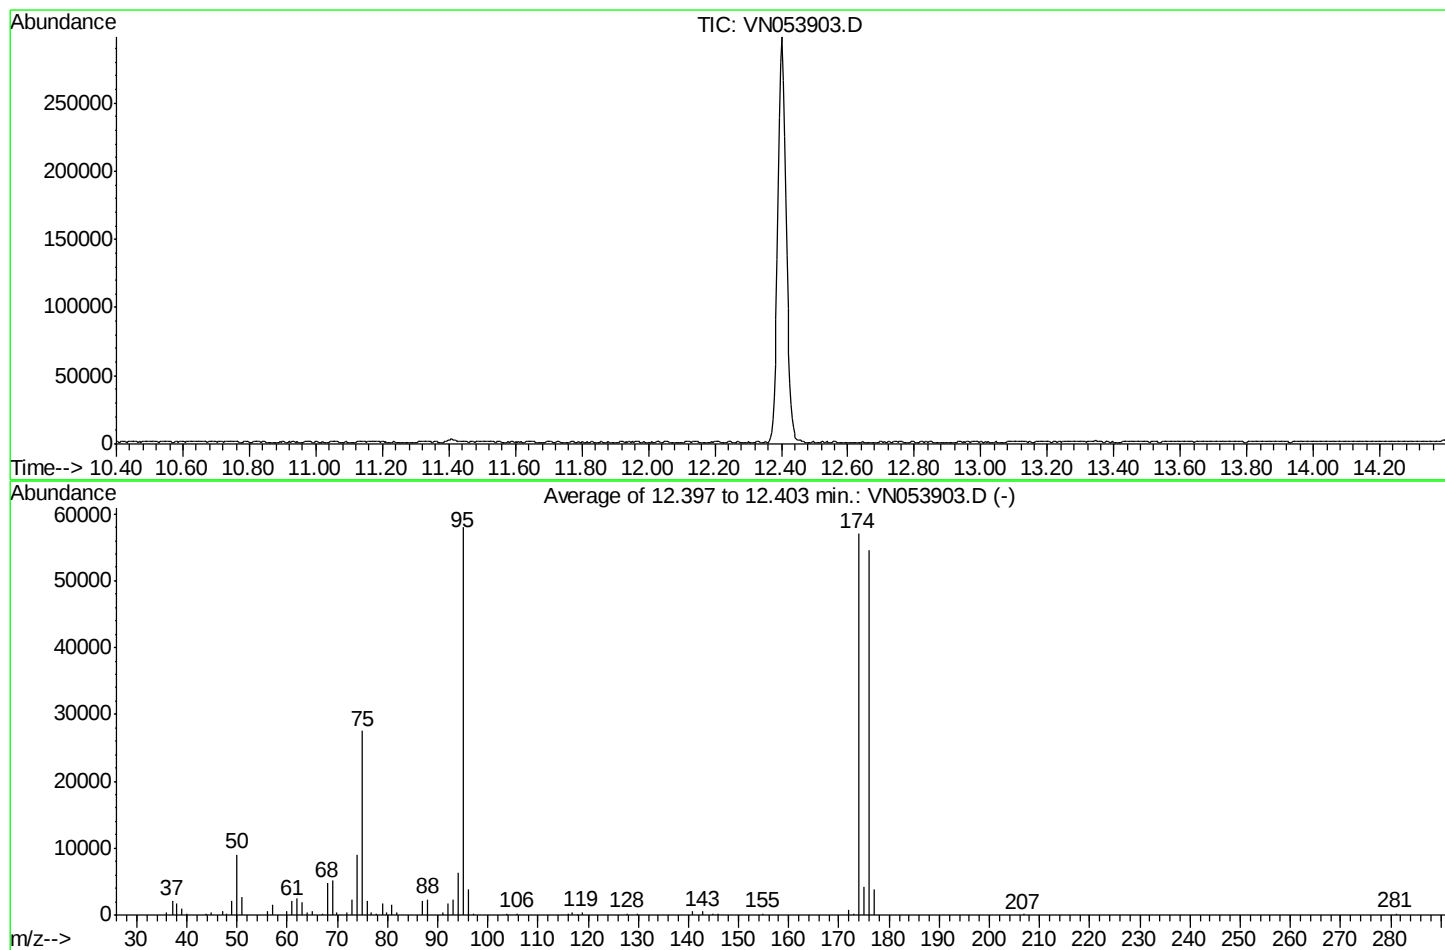

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	9090	PASS
75	95	30	60	47.5	27557	PASS
95	95	100	100	100.0	57984	PASS
96	95	5	9	6.5	3785	PASS
173	174	0.00	2	0.5	283	PASS
174	95	50	100	98.3	56994	PASS
175	174	5	9	7.5	4281	PASS
176	174	95	101	95.7	54538	PASS
177	176	5	9	7.1	3853	PASS