
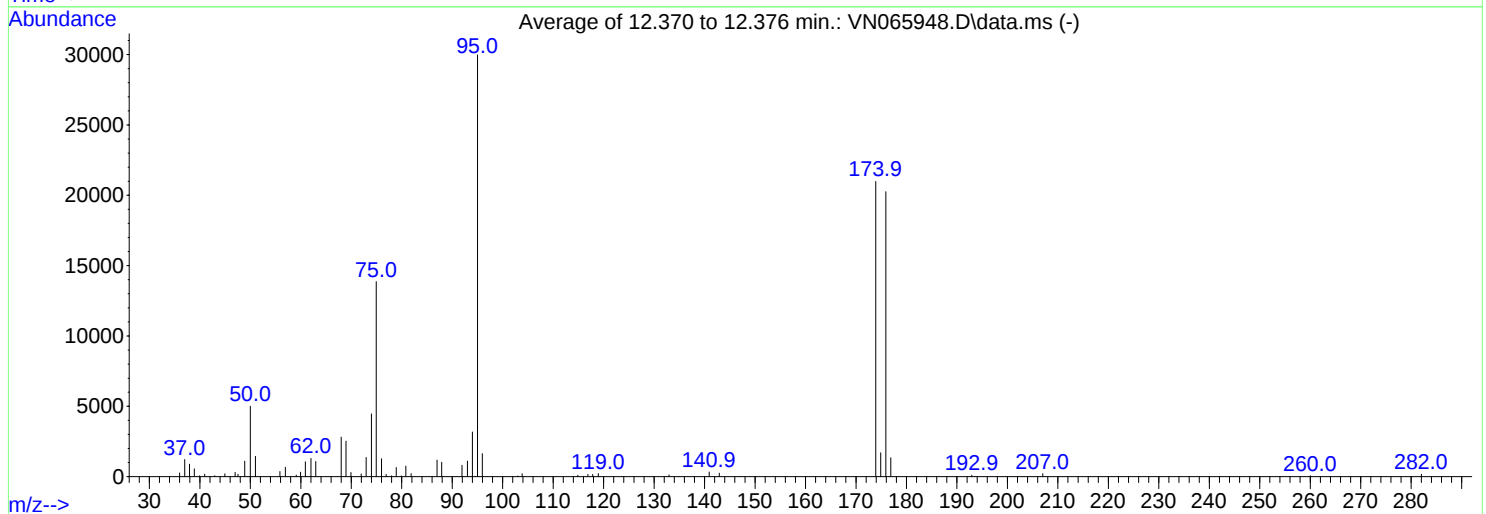


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022221\
 Data File : VN065948.D
 Acq On : 22 Feb 2021 10:02
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
 Title : SW846 8260
 Last Update : Wed Feb 17 15:48:13 2021

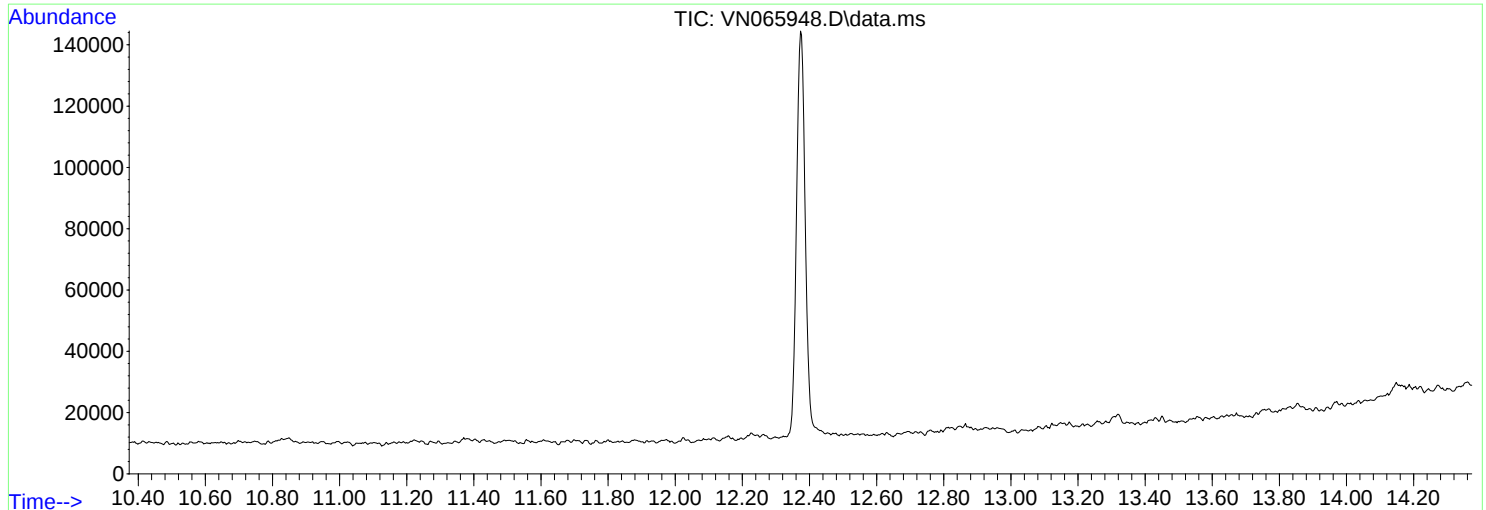

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	5001	PASS
75	95	30	60	46.3	13867	PASS
95	95	100	100	100.0	29981	PASS
96	95	5	9	5.5	1635	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.0	20987	PASS
175	174	5	9	8.1	1698	PASS
176	174	95	101	96.5	20261	PASS
177	176	5	9	6.6	1346	PASS