


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022222\
Data File : VN071018.D
Acq On : 22 Feb 2022 10:12
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
Title : SW846 8260
Last Update : Mon Feb 21 07:57:15 2022

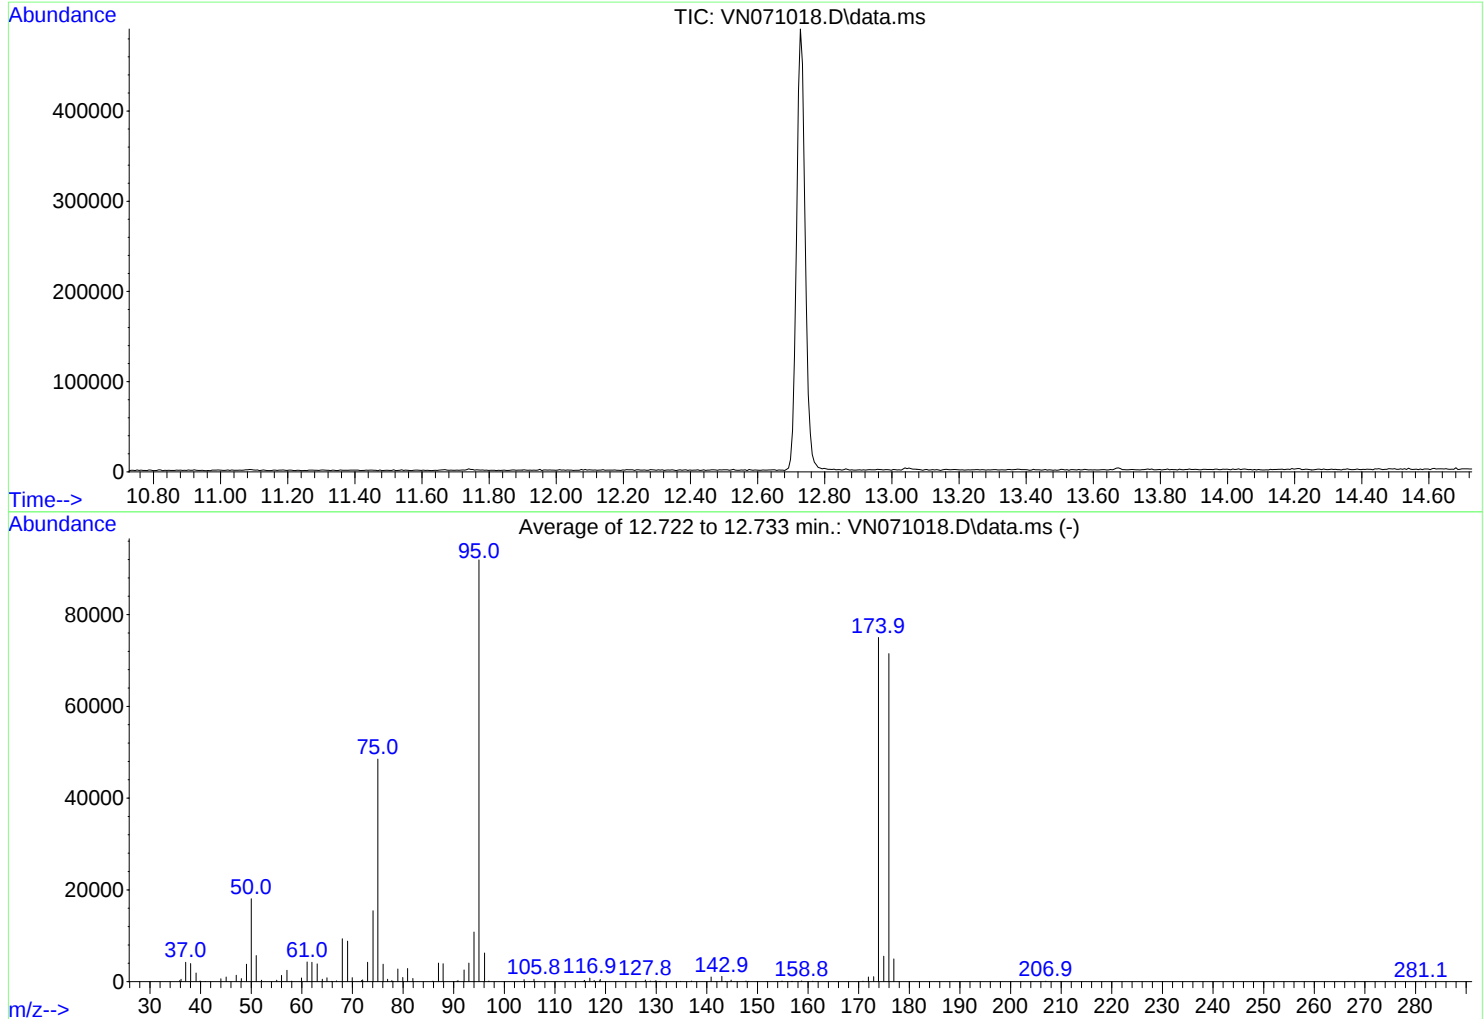

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	18080	PASS
75	95	30	60	52.8	48515	PASS
95	95	100	100	100.0	91941	PASS
96	95	5	9	6.8	6250	PASS
173	174	0.00	2	1.5	1094	PASS
174	95	50	100	81.6	75029	PASS
175	174	5	9	7.4	5537	PASS
176	174	95	101	95.3	71491	PASS
177	176	5	9	6.9	4940	PASS