

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022223\
 Data File : VN076764.D
 Acq On : 22 Feb 2023 12:09
 Operator : JC\MD
 Sample : VN0222MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0222MBL01

Quant Time: Feb 22 23:55:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 14 01:44:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	264851	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.107	114	477351	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.866	117	409868	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.795	152	155898	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	186308	50.943	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 101.880%	
35) Dibromofluoromethane	8.172	113	149103	47.696	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 95.400%	
50) Toluene-d8	10.572	98	559816	47.952	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 95.900%	
62) 4-Bromofluorobenzene	12.848	95	163578	42.305	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 84.600%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.372	50	942	0.257	ug/l	89
13) Acrolein	4.207	56	534	0.737	ug/l #	59
15) Acrylonitrile	5.719	53	416	0.243	ug/l #	35
16) Acetone	4.454	43	713	0.436	ug/l #	42
18) Methyl Acetate	5.066	43	1294	0.243	ug/l #	54
20) Methylene Chloride	5.295	84	2312	0.675	ug/l #	74
25) 2-Butanone	7.495	43	1573	0.653	ug/l #	51
29) Tetrahydrofuran	7.860	42	401	0.255	ug/l #	64
31) Cyclohexane	8.230	56	7575	1.320	ug/l #	26
36) 1,1-Dichloropropene	8.230	75	23929	5.298	ug/l #	46
38) Carbon Tetrachloride	8.225	117	28114	6.170	ug/l #	17
42) 1,2-Dichloroethane	8.678	62	1068	0.221	ug/l #	74
43) Isopropyl Acetate	8.707	43	4428	0.573	ug/l #	56
49) 1,4-Dioxane	9.719	88	67	1.056	ug/l #	1
51) 4-Methyl-2-Pentanone	10.448	43	1850	0.376	ug/l #	65
59) 2-Hexanone	11.195	43	3079	0.868	ug/l	97
71) Bromoform	12.854	173	1791	0.774	ug/l #	1
74) N-amyl acetate	12.489	43	1214	0.236	ug/l #	82
76) 1,2,3-Trichloropropane	12.848	75	93629	29.706	ug/l #	1
77) Bromobenzene	12.977	156	616	0.216	ug/l	65
81) trans-1,4-Dichloro-2-b...	12.848	75	93629	86.522	ug/l #	4
87) 1,3-Dichlorobenzene	13.736	146	1686	0.313	ug/l	96
88) 1,4-Dichlorobenzene	13.736	146	1686	0.314	ug/l	95
89) n-Butylbenzene	14.054	91	2156	0.260	ug/l	97
91) 1,2-Dichlorobenzene	14.101	146	1955	0.354	ug/l	86
92) 1,2-Dibromo-3-Chloropr...	14.730	75	248	0.309	ug/l #	24
93) 1,2,4-Trichlorobenzene	15.406	180	2513	0.912	ug/l	84
94) Hexachlorobutadiene	15.495	225	496	0.367	ug/l #	31
95) Naphthalene	15.642	128	11004	1.316	ug/l	98
96) 1,2,3-Trichlorobenzene	15.854	180	2865	1.073	ug/l	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022223\
Data File : VN076764.D
Acq On : 22 Feb 2023 12:09
Operator : JC\MD
Sample : VN0222MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0222MBL01

Quant Time: Feb 22 23:55:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 14 01:44:47 2023
Response via : Initial Calibration




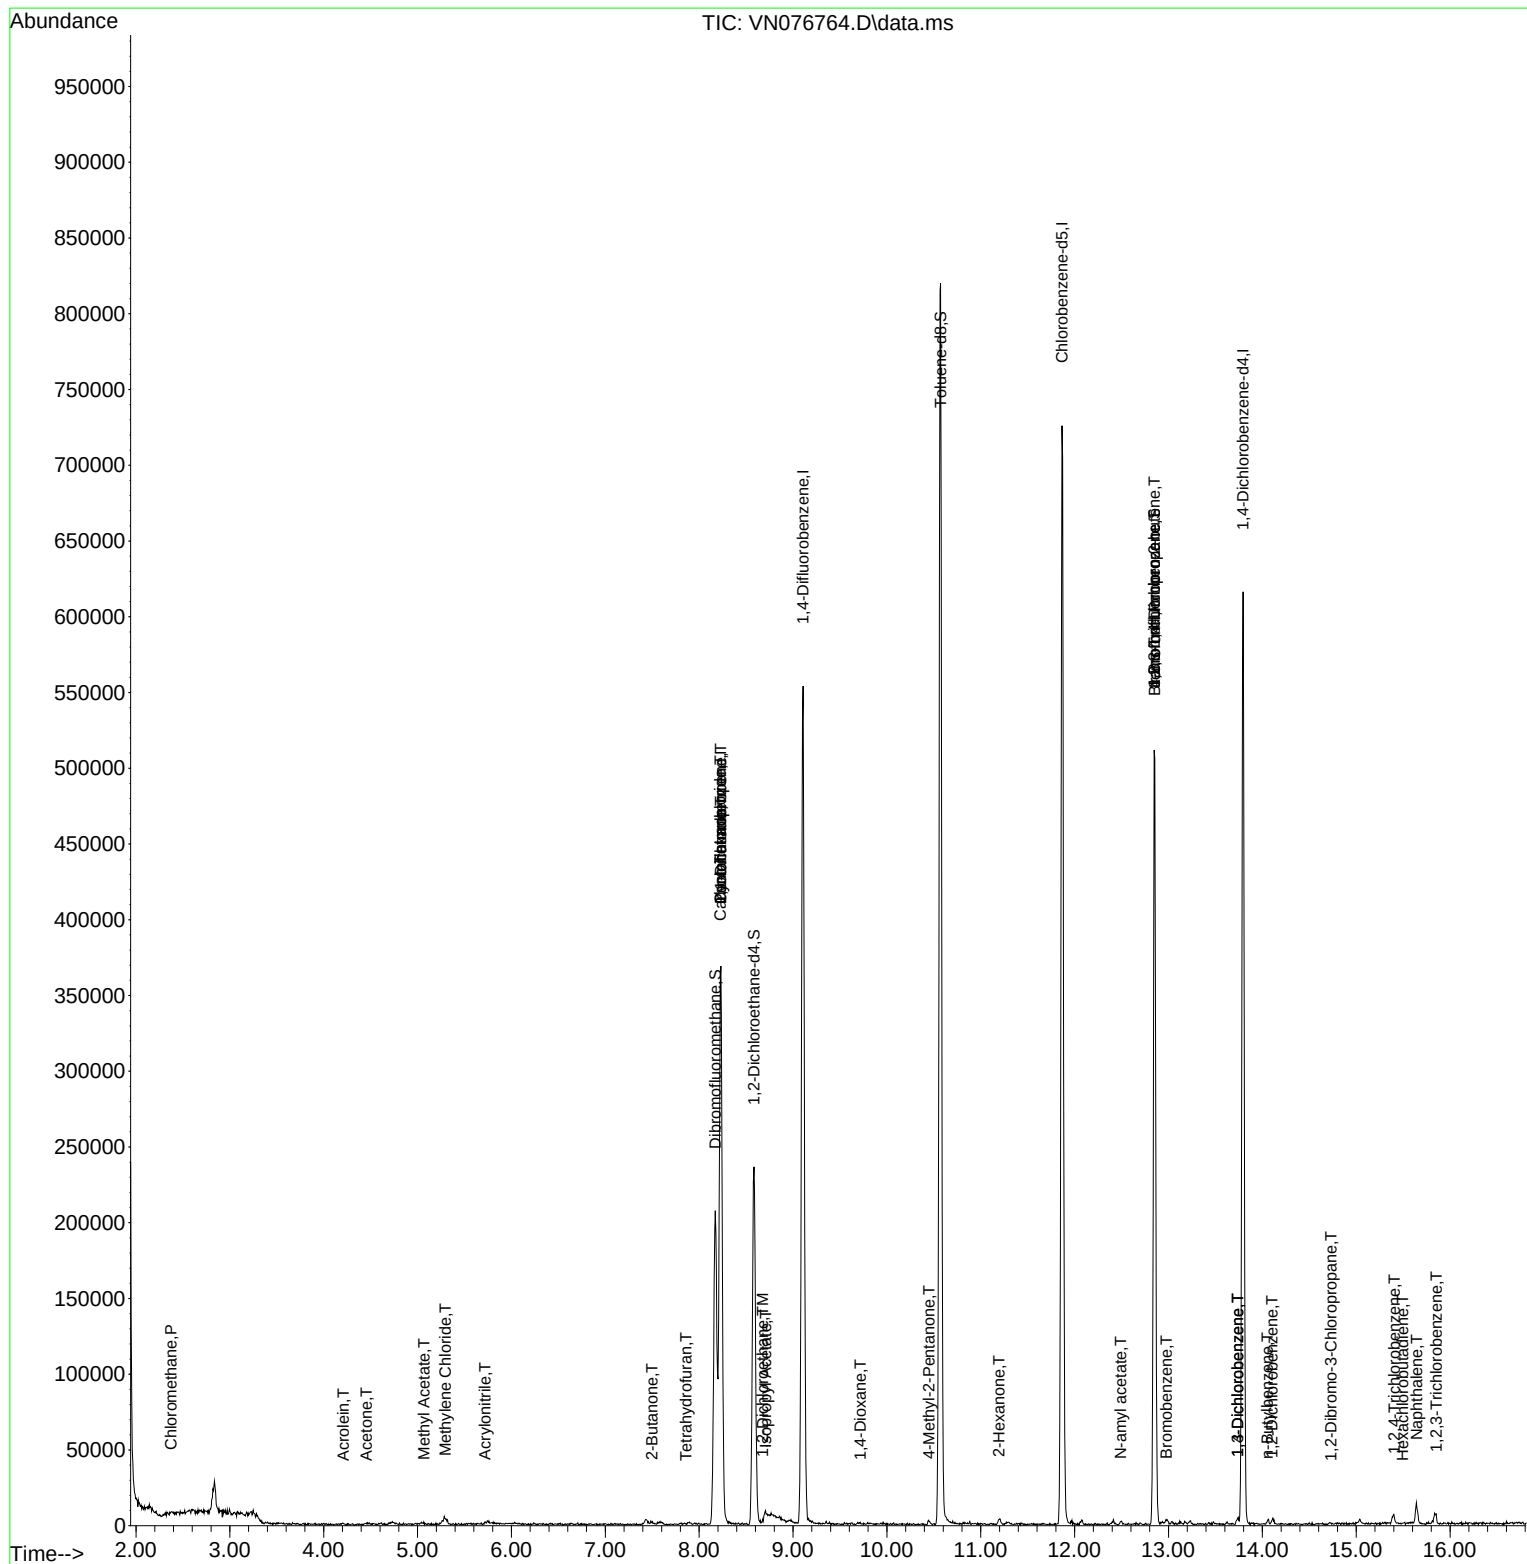




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 11
Delta R.T. -0.001 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09




Instrument :
MSVOA_N
ClientSampleId :
VN0222MBL01


Tgt Ion:168 Resp: 264851
Ion Ratio Lower Upper
168 100
99 57.0 44.8 67.2

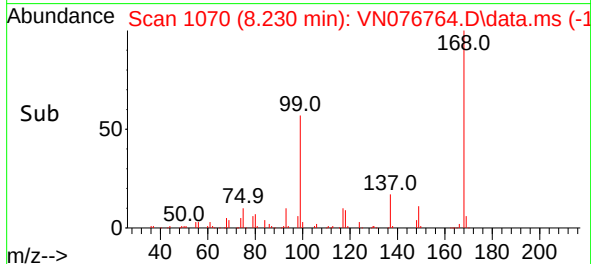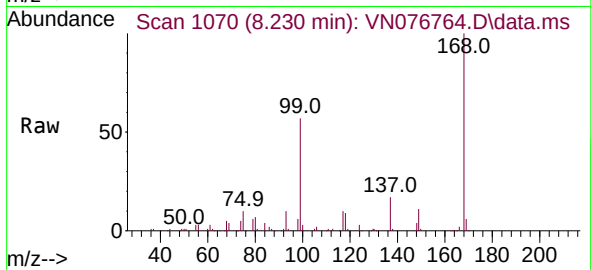

#3
Chloromethane
Concen: 0.257 ug/l
RT: 2.372 min Scan# 74
Delta R.T. -0.006 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09

Tgt Ion: 50 Resp: 942
Ion Ratio Lower Upper
50 100
52 25.0 24.7 37.1

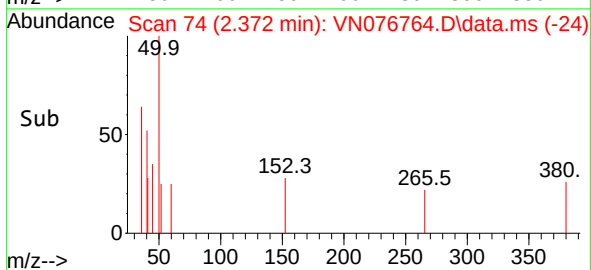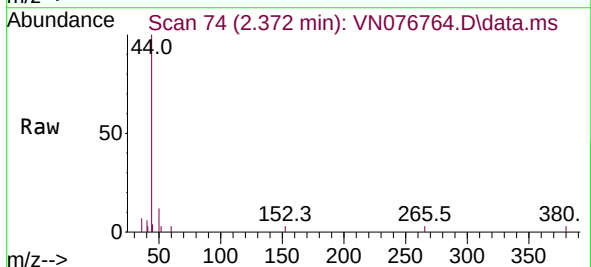



#13

Acrolein

Concen: 0.737 ug/l

RT: 4.207 min Scan# 386

Delta R.T. 0.017 min

Lab File: VN076764.D

Acq: 22 Feb 2023 12:09

Instrument :

MSVOA_N

ClientSampleId :





VN0222MBL01

Tgt Ion: 56 Resp: 534

Ion Ratio Lower Upper

56 100

55 36.7 56.3 84.5#

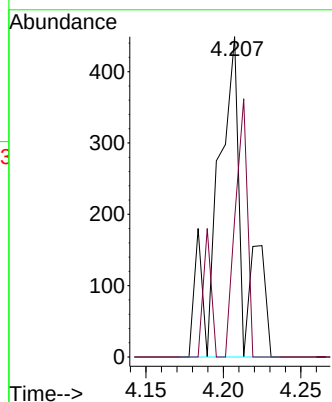

#15

Acrylonitrile

Concen: 0.243 ug/l

RT: 5.719 min Scan# 643

Delta R.T. -0.006 min

Lab File: VN076764.D

Acq: 22 Feb 2023 12:09




Tgt Ion: 53 Resp: 416


Ion Ratio Lower Upper

53 100

52 0.0 65.3 97.9#

51 33.4 29.2 43.8


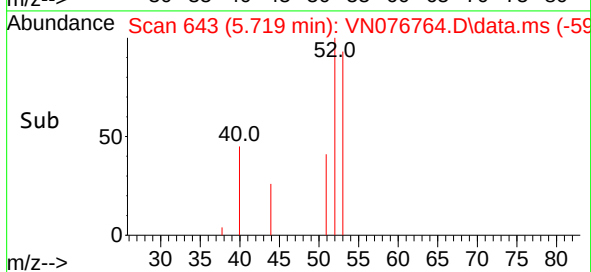
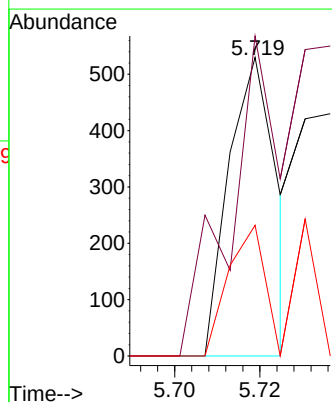





#16
Acetone
Concen: 0.436 ug/l
RT: 4.454 min Scan# 41
Delta R.T. 0.017 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09




Instrument :
MSVOA_N
ClientSampleId :
VN0222MBL01


Tgt Ion: 43 Resp: 713
Ion Ratio Lower Upper
43 100
58 0.0 25.9 38.9#

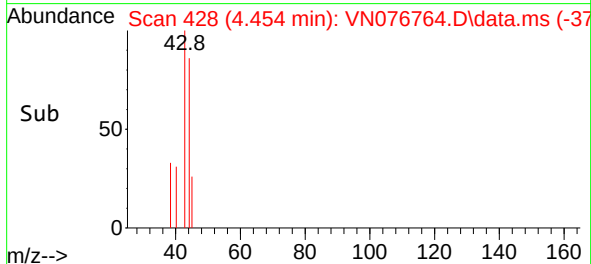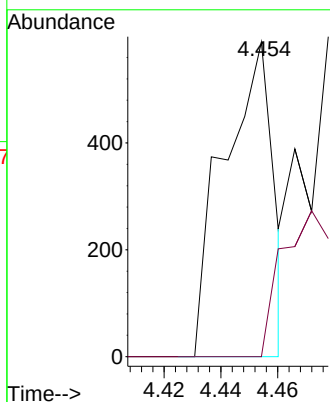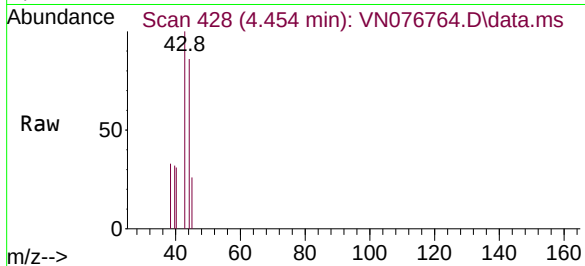

#18
Methyl Acetate
Concen: 0.243 ug/l
RT: 5.066 min Scan# 532
Delta R.T. 0.035 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09

Tgt Ion: 43 Resp: 1294
Ion Ratio Lower Upper
43 100
74 0.0 17.7 26.5#


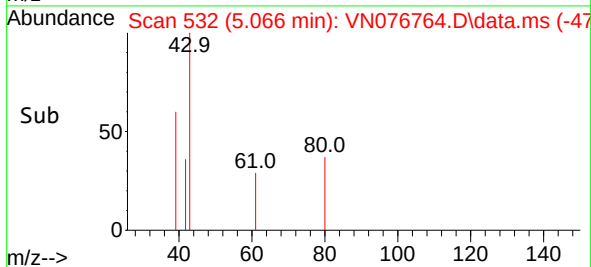

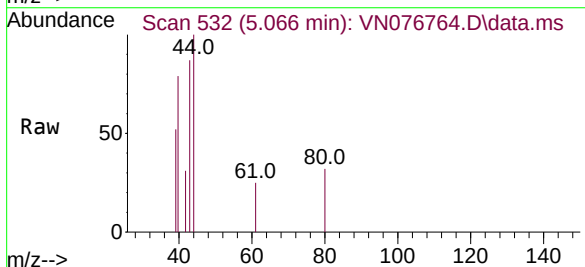




#20
Methylene Chloride
Concen: 0.675 ug/l
RT: 5.295 min Scan# 51
Delta R.T. 0.005 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09




Instrument :
MSVOA_N
ClientSampleId :
VN0222MBL01


Tgt Ion: 84 Resp: 2312
Ion Ratio Lower Upper
84 100
49 101.9 104.9 157.3#
51 11.7 33.8 50.8#
86 74.1 50.0 75.0

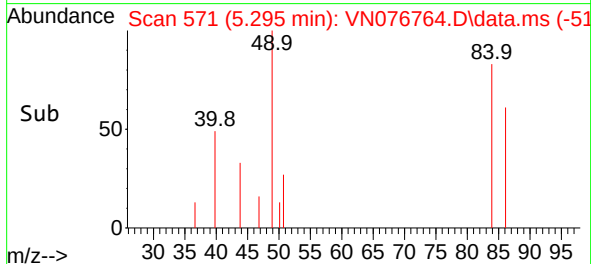

#25
2-Butanone
Concen: 0.653 ug/l
RT: 7.495 min Scan# 945
Delta R.T. 0.006 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09

Tgt Ion: 43 Resp: 1573
Ion Ratio Lower Upper
43 100
72 0.0 19.4 29.2#

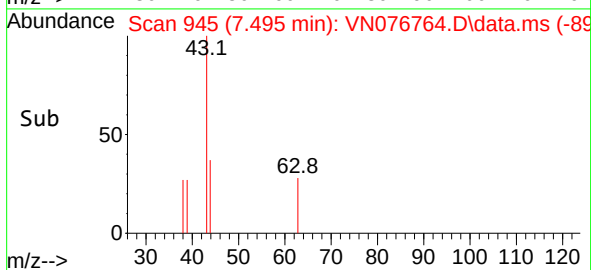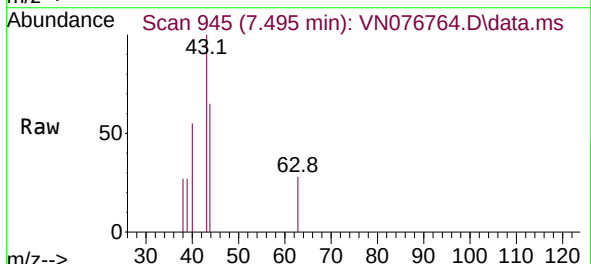



#29

Tetrahydrofuran

Concen: 0.255 ug/l

RT: 7.860 min Scan# 10

Delta R.T. 0.018 min

Lab File: VN076764.D

Acq: 22 Feb 2023 12:09

Instrument :

MSVOA_N

ClientSampleId :

VN0222MBL01





Tgt Ion: 42 Resp: 401

Ion Ratio Lower Upper

42 100

72 59.4 31.5 47.3#

71 61.3 29.8 44.8#

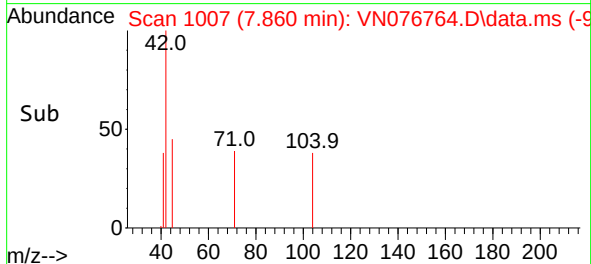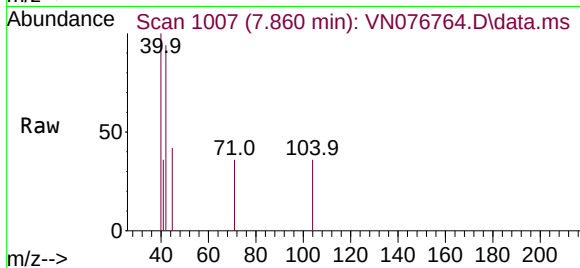

#31

Cyclohexane

Concen: 1.320 ug/l

RT: 8.230 min Scan# 1070

Delta R.T. -0.030 min

Lab File: VN076764.D

Acq: 22 Feb 2023 12:09




Tgt Ion: 56 Resp: 7575


Ion Ratio Lower Upper

56 100

69 114.7 21.6 32.4#

84 118.8 65.1 97.7#

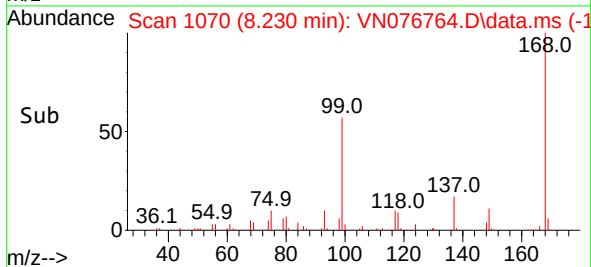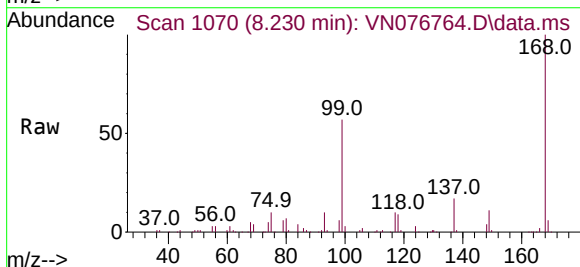

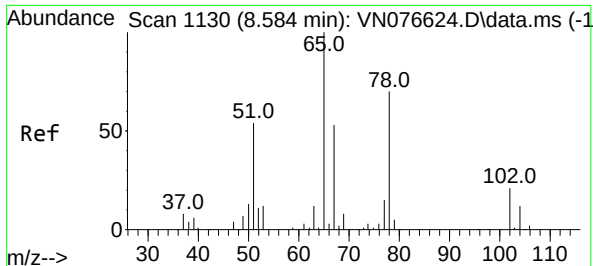

#33

1,2-Dichloroethane-d4

Concen: 50.943 ug/l

RT: 8.583 min Scan# 1130

Delta R.T. -0.001 min

Lab File: VN076764.D

Acq: 22 Feb 2023 12:09

Instrument :

MSVOA_N

ClientSampleId :





VN0222MBL01

Tgt Ion: 65 Resp: 186308

Ion Ratio Lower Upper

65 100

67 52.8 0.0 105.6

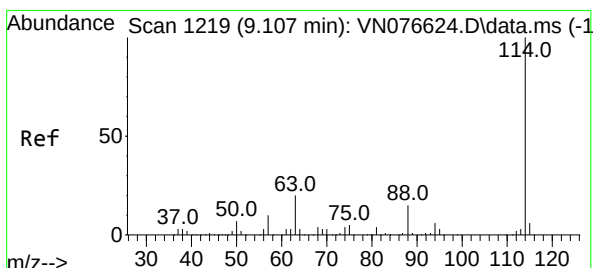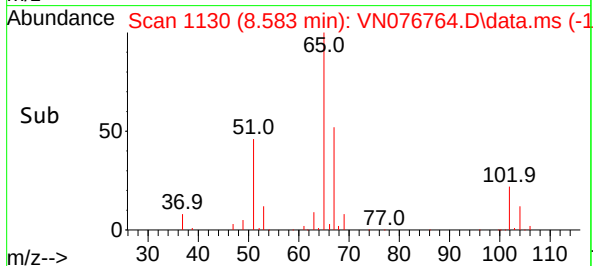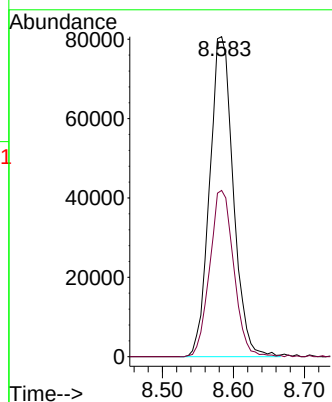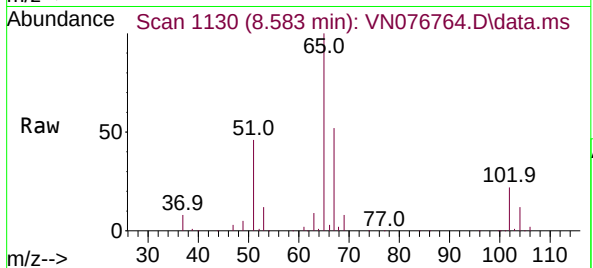

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.107 min Scan# 1219

Delta R.T. -0.000 min

Lab File: VN076764.D

Acq: 22 Feb 2023 12:09




Tgt Ion: 114 Resp: 477351


Ion Ratio Lower Upper

114 100

63 20.9 0.0 40.0

88 13.6 0.0 29.6

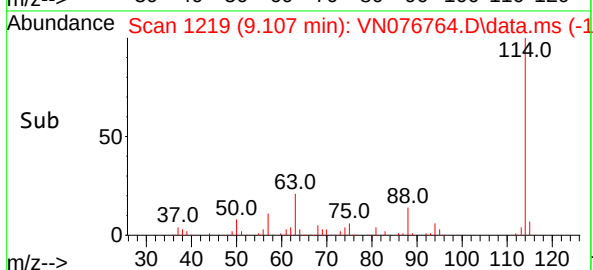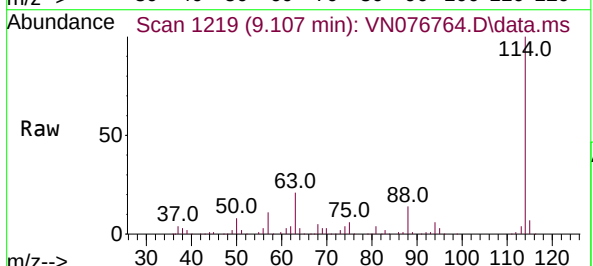

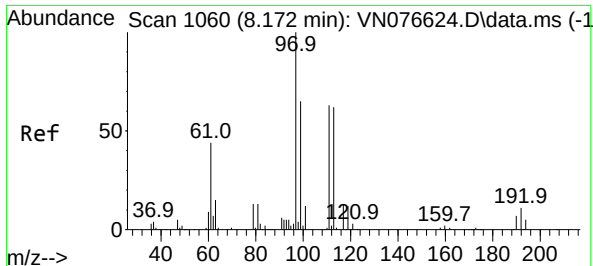

#35

Dibromofluoromethane

Concen: 47.696 ug/l

RT: 8.172 min Scan# 1060

Delta R.T. -0.000 min

Lab File: VN076764.D

Acq: 22 Feb 2023 12:09

Instrument :

MSVOA_N

ClientSampleId :

VN0222MBL01





Tgt Ion:113 Resp: 149103

Ion Ratio Lower Upper

113 100

111 100.3 83.1 124.7

192 16.9 15.6 23.4

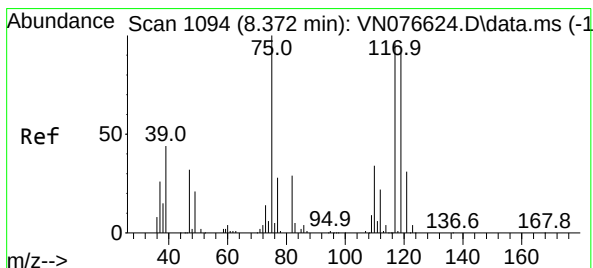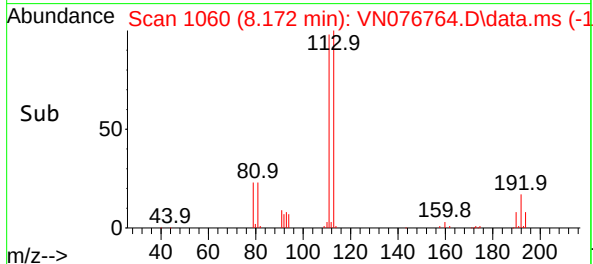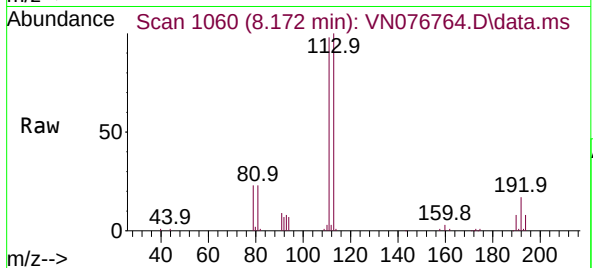

#36

1,1-Dichloropropene

Concen: 5.298 ug/l

RT: 8.230 min Scan# 1070

Delta R.T. -0.142 min

Lab File: VN076764.D

Acq: 22 Feb 2023 12:09




Tgt Ion: 75 Resp: 23929


Ion Ratio Lower Upper

75 100

110 4.2 17.5 52.5#

77 0.0 24.5 36.7#


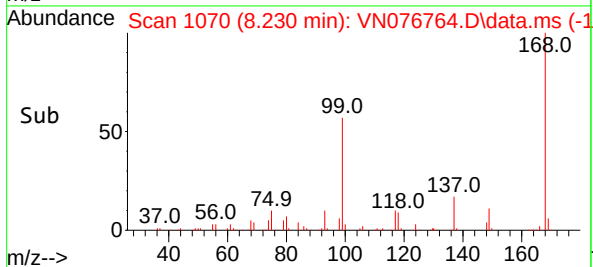

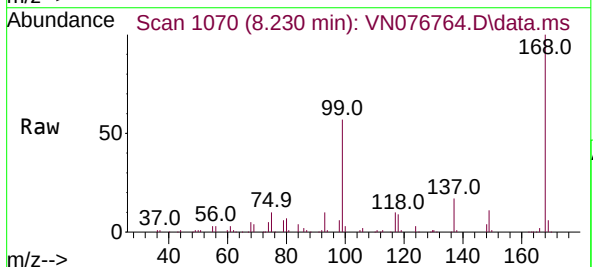


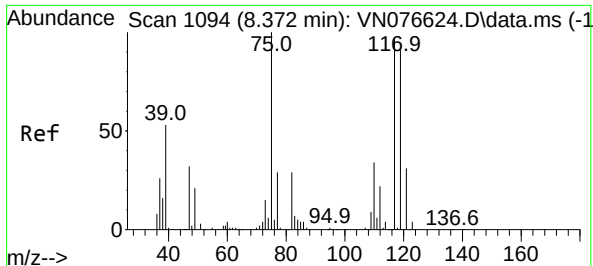

#38
Carbon Tetrachloride
Concen: 6.170 ug/l
RT: 8.225 min Scan# 1069
Delta R.T. -0.147 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09




Instrument :
MSVOA_N
ClientSampleId :
VN0222MBL01


Tgt Ion:117 Resp: 28114
Ion Ratio Lower Upper
117 100
119 5.6 75.4 113.0#
121 0.0 26.0 39.0#

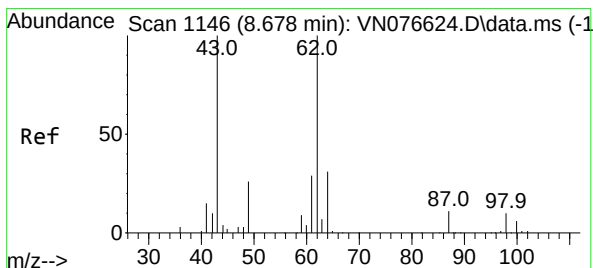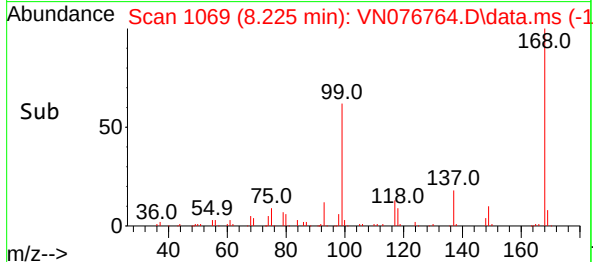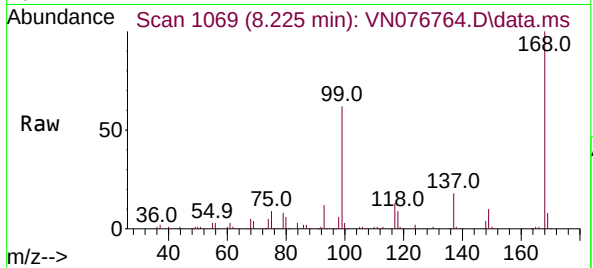

#42
1,2-Dichloroethane
Concen: 0.221 ug/l
RT: 8.678 min Scan# 1146
Delta R.T. -0.001 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09

Tgt Ion: 62 Resp: 1068
Ion Ratio Lower Upper
62 100
98 0.0 0.0 19.2

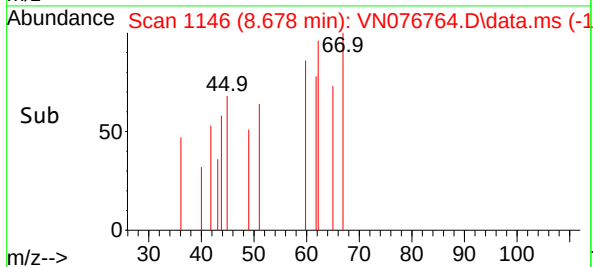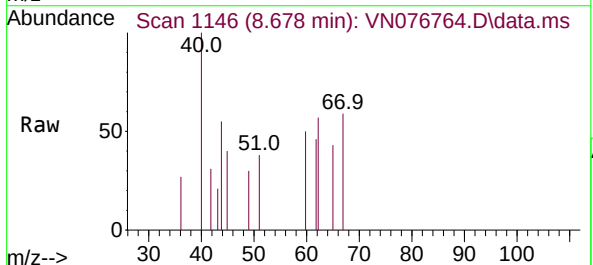

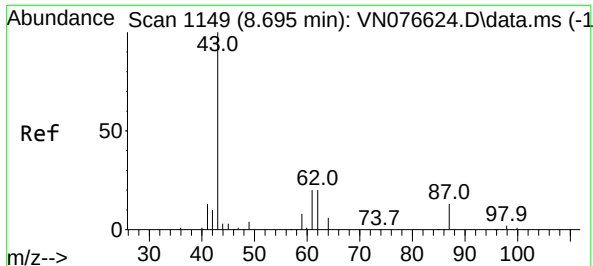

#43

Isopropyl Acetate

Concen: 0.573 ug/l

RT: 8.707 min Scan# 1151

Delta R.T. 0.012 min

Lab File: VN076764.D

Acq: 22 Feb 2023 12:09

Instrument :

MSVOA_N

ClientSampleId :

VN0222MBL01





Tgt Ion: 43 Resp: 4428

Ion Ratio Lower Upper

43 100

61 0.0 20.0 30.0#

87 0.0 9.9 14.9#

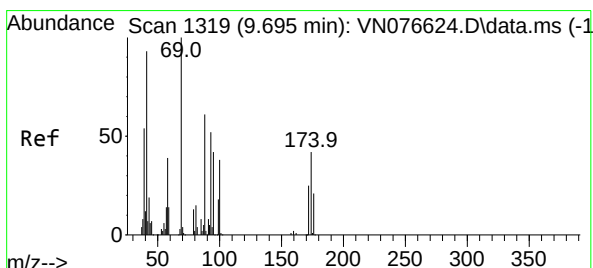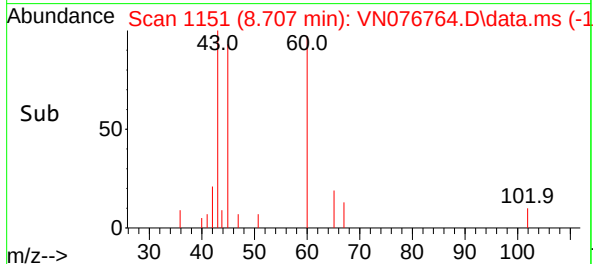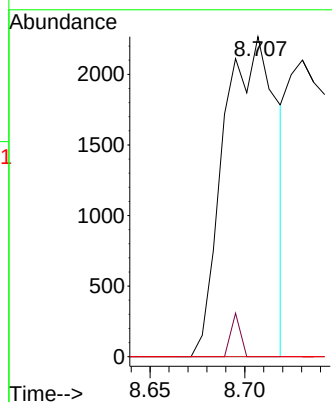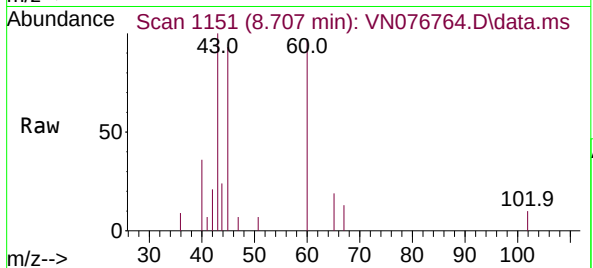

#49

1,4-Dioxane

Concen: 1.056 ug/l

RT: 9.719 min Scan# 1323

Delta R.T. 0.024 min

Lab File: VN076764.D

Acq: 22 Feb 2023 12:09




Tgt Ion: 88 Resp: 67


Ion Ratio Lower Upper

88 100

43 186.6 22.6 33.8#

58 173.1 57.6 86.4#


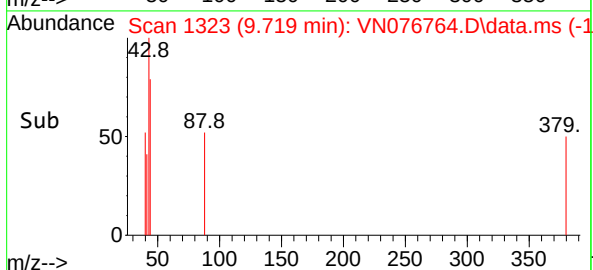

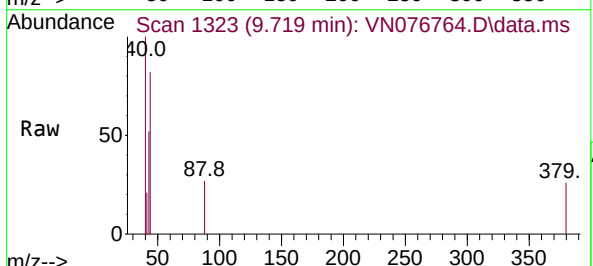




#50
Toluene-d8
Concen: 47.952 ug/l
RT: 10.572 min Scan# 1468
Delta R.T. 0.005 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09




Instrument :
MSVOA_N
ClientSampleId :
VN0222MBL01


Tgt Ion: 98 Resp: 559816
Ion Ratio Lower Upper
98 100
100 65.0 52.9 79.3

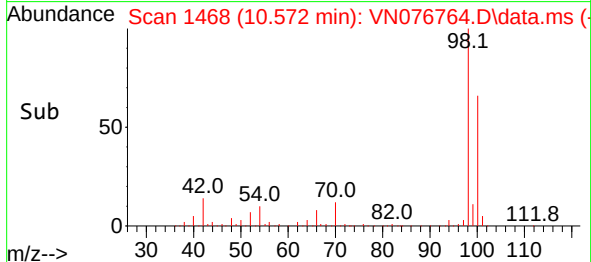

#51
4-Methyl-2-Pentanone
Concen: 0.376 ug/l
RT: 10.448 min Scan# 1447
Delta R.T. -0.000 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09

Tgt Ion: 43 Resp: 1850
Ion Ratio Lower Upper
43 100
58 16.1 29.5 44.3#


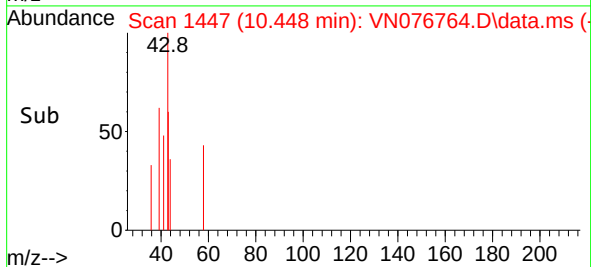

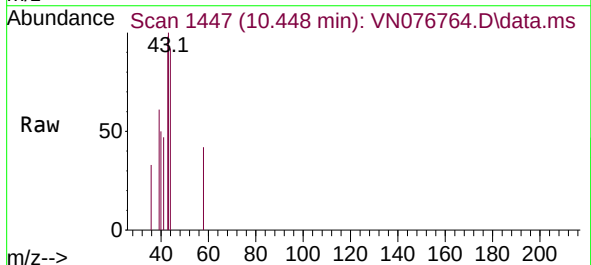




#59
2-Hexanone
Concen: 0.868 ug/l
RT: 11.195 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09




Instrument :
MSVOA_N
ClientSampleId :
VN0222MBL01


Tgt Ion: 43 Resp: 3079
Ion Ratio Lower Upper
43 100
58 52.9 25.4 76.0

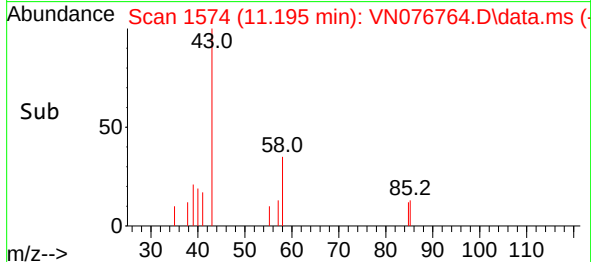

#62
4-Bromofluorobenzene
Concen: 42.305 ug/l
RT: 12.848 min Scan# 1855
Delta R.T. -0.000 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09

Tgt Ion: 95 Resp: 163578
Ion Ratio Lower Upper
95 100
174 76.7 0.0 169.2
176 75.8 0.0 163.4


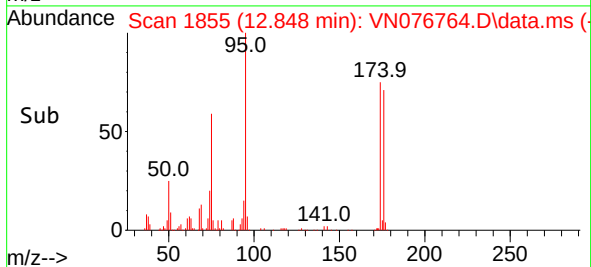

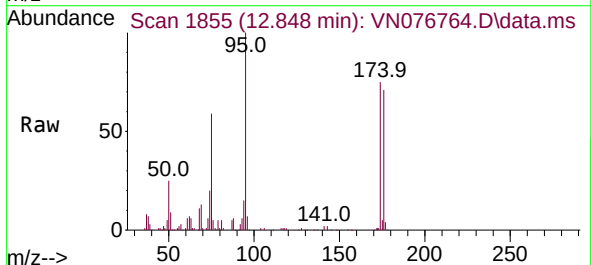


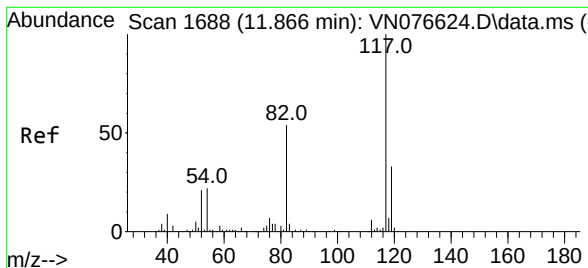

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.866 min Scan# 1177
Delta R.T. -0.000 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09




Instrument :
MSVOA_N
ClientSampleId :
VN0222MBL01


Tgt Ion:117 Resp: 409868
Ion Ratio Lower Upper
117 100
82 56.0 43.4 65.2
119 30.7 26.1 39.1

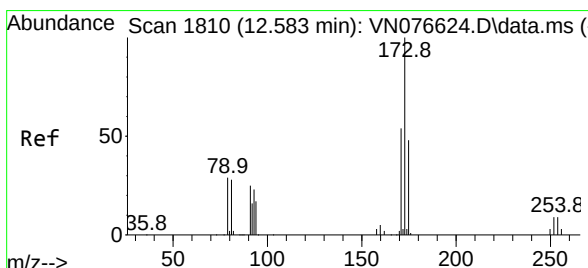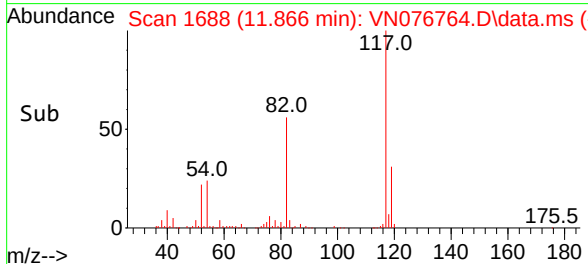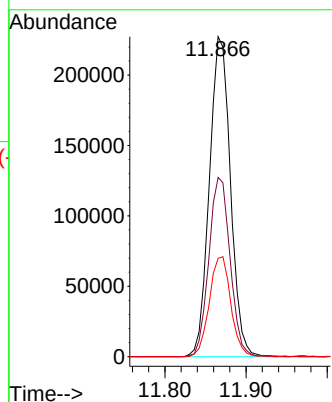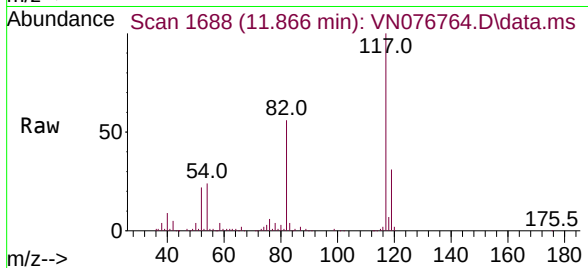

#71
Bromoform
Concen: 0.774 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.271 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09

Tgt Ion:173 Resp: 1791
Ion Ratio Lower Upper
173 100
175 435.4 24.9 74.7#
254 0.0 0.1 0.1#


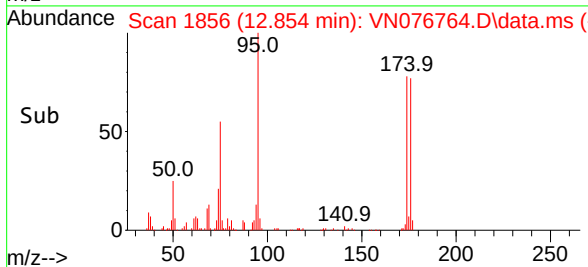
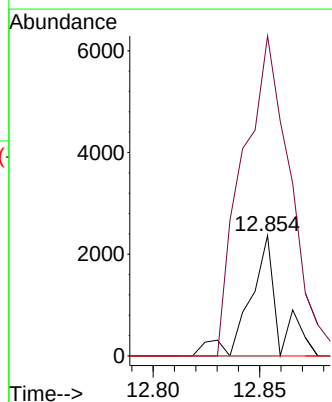
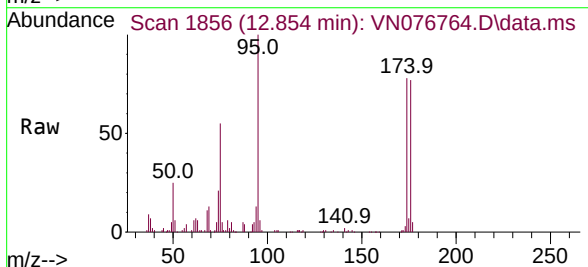




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.795 min Scan# 2016
Delta R.T. -0.000 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09




Instrument :
MSVOA_N
ClientSampleId :
VN0222MBL01


Tgt Ion:152 Resp: 155898
Ion Ratio Lower Upper
152 100
115 62.4 29.3 87.9
150 156.5 0.0 349.8

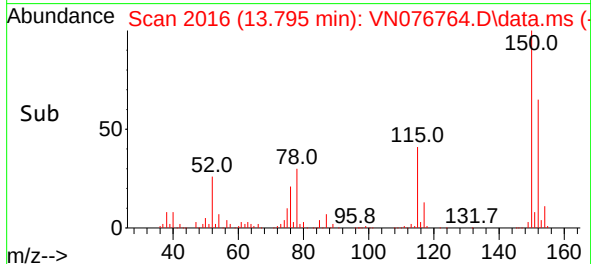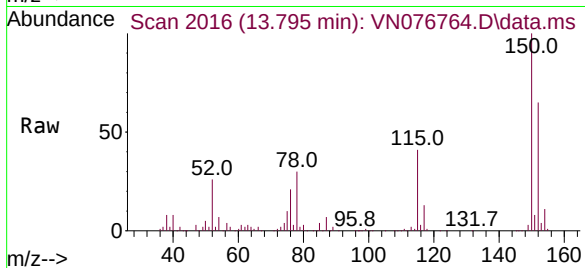

#74
N-ethyl acetate
Concen: 0.236 ug/l
RT: 12.489 min Scan# 1794
Delta R.T. -0.006 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09

Tgt Ion: 43 Resp: 1214
Ion Ratio Lower Upper
43 100
70 36.7 30.5 45.7
55 8.6 17.8 26.8#
61 6.1 17.8 26.8#


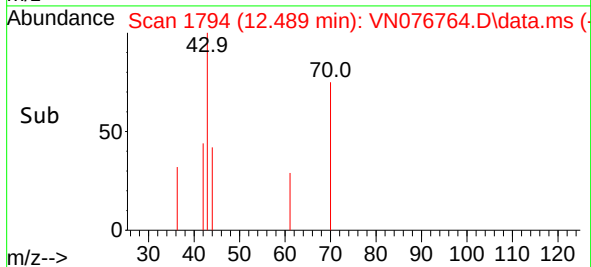

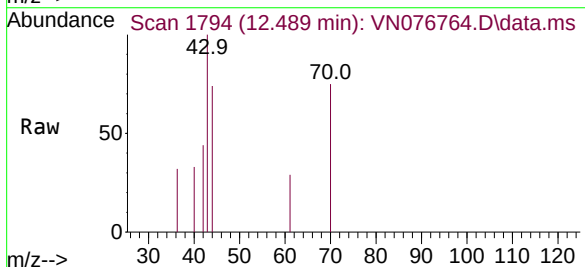


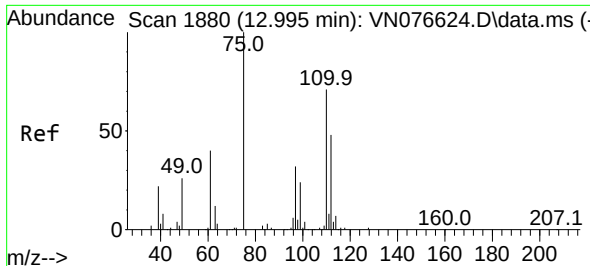

#76
1,2,3-Trichloropropane
Concen: 29.706 ug/l
RT: 12.848 min Scan# 1855
Delta R.T. -0.147 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09




Instrument :
MSVOA_N
ClientSampleId :
VN0222MBL01


Tgt Ion: 75 Resp: 93629
Ion Ratio Lower Upper
75 100
77 1.6 93.1 279.3#

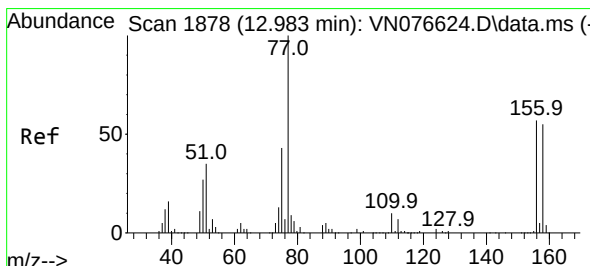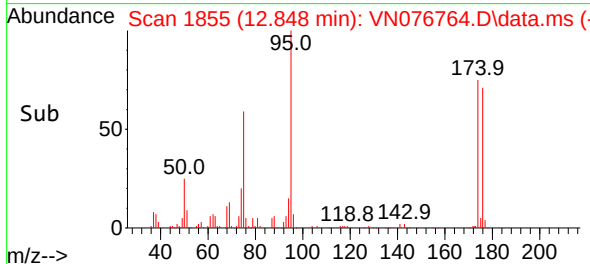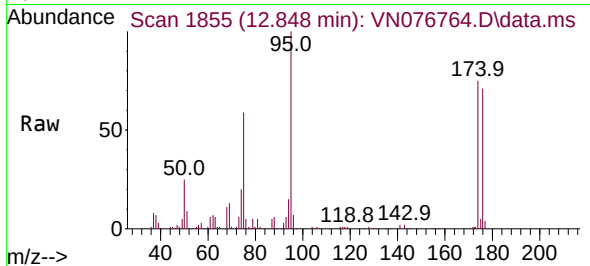

#77
Bromobenzene
Concen: 0.216 ug/l
RT: 12.977 min Scan# 1877
Delta R.T. -0.006 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09

Tgt Ion: 156 Resp: 616
Ion Ratio Lower Upper
156 100
77 261.0 102.8 308.4
158 130.4 48.9 146.6


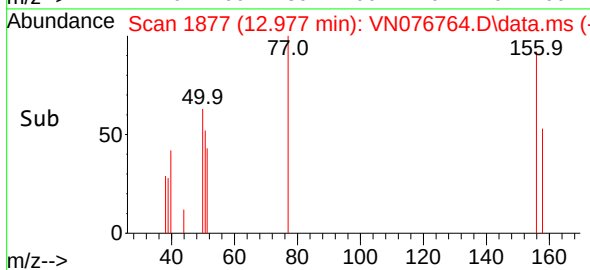

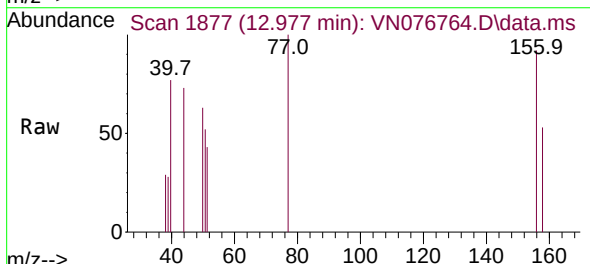




#81
 trans-1,4-Dichloro-2-butene
 Concen: 86.522 ug/l
 RT: 12.848 min Scan# 1836
 Delta R.T. 0.112 min
 Lab File: VN076764.D
 Acq: 22 Feb 2023 12:09




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0222MBL01


Tgt Ion: 75 Resp: 93629
 Ion Ratio Lower Upper
 75 100
 53 0.1 92.1 138.1#
 89 0.1 37.5 56.3#

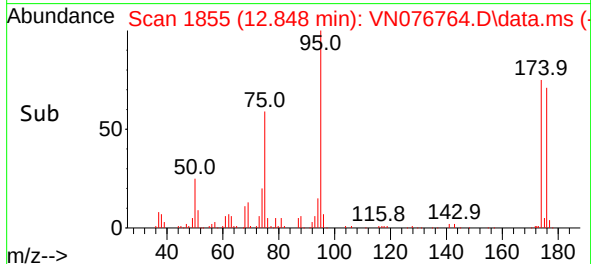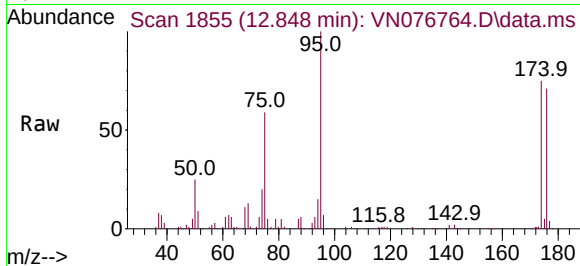

#87
 1,3-Dichlorobenzene
 Concen: 0.313 ug/l
 RT: 13.736 min Scan# 2006
 Delta R.T. 0.000 min
 Lab File: VN076764.D
 Acq: 22 Feb 2023 12:09

Tgt Ion: 146 Resp: 1686
 Ion Ratio Lower Upper
 146 100
 111 35.1 19.8 59.4
 148 62.2 32.0 96.2


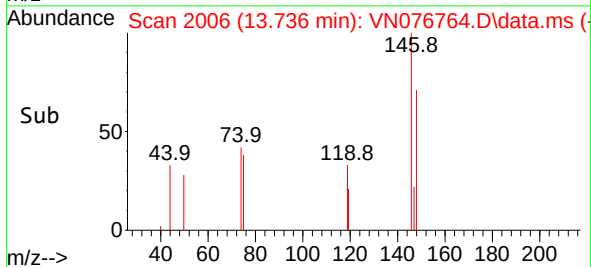

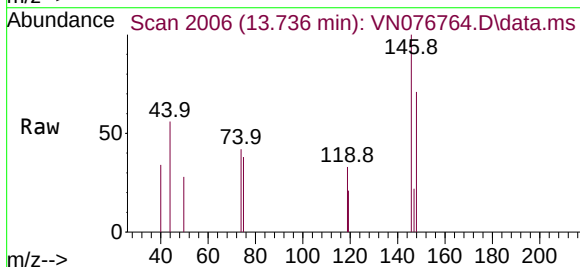




#88
1,4-Dichlorobenzene
Concen: 0.314 ug/l
RT: 13.736 min Scan# 2006
Delta R.T. -0.077 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09




Instrument :
MSVOA_N
ClientSampleId :
VN0222MBL01


Tgt Ion:	146	Resp:	1686
Ion	Ratio	Lower	Upper
146	100		
111	35.1	19.4	58.1
148	62.2	32.7	98.1

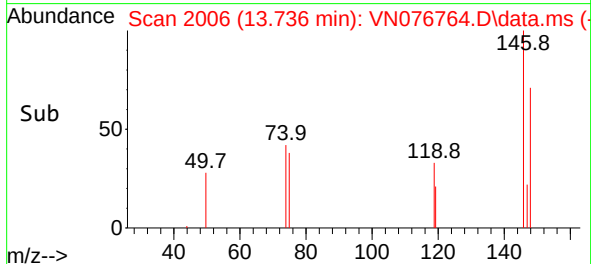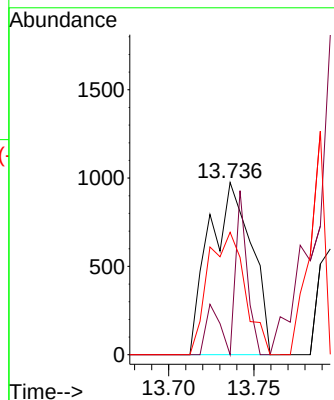

#89
n-Butylbenzene
Concen: 0.260 ug/l
RT: 14.054 min Scan# 2060
Delta R.T. -0.006 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09

Tgt Ion:	91	Resp:	2156
Ion	Ratio	Lower	Upper
91	100		
92	54.3	26.4	79.0
134	24.4	13.2	39.5


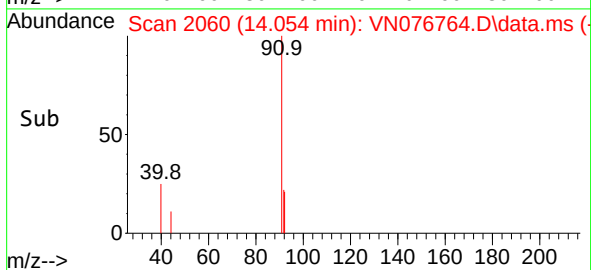
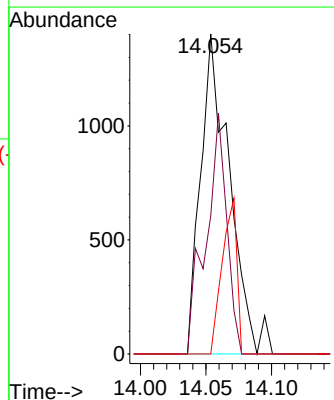
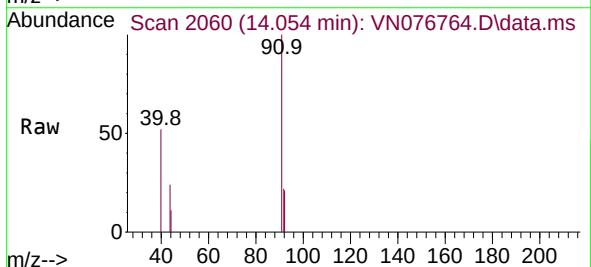




#91
1,2-Dichlorobenzene
Concen: 0.354 ug/l
RT: 14.101 min Scan# 2068
Delta R.T. -0.006 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09




Instrument :
MSVOA_N
ClientSampleId :
VN0222MBL01


Tgt Ion:146 Resp: 1955
Ion Ratio Lower Upper
146 100
111 35.4 20.0 59.9
148 49.9 32.4 97.2

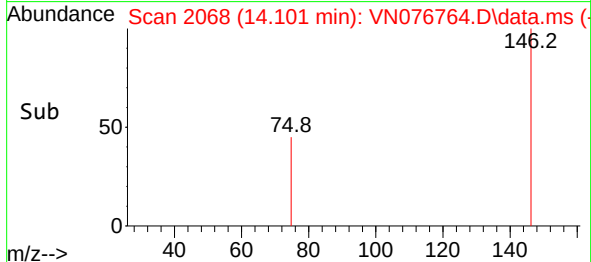

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.309 ug/l
RT: 14.730 min Scan# 2175
Delta R.T. 0.006 min
Lab File: VN076764.D
Acq: 22 Feb 2023 12:09

Tgt Ion: 75 Resp: 248
Ion Ratio Lower Upper
75 100
155 49.2 43.4 130.2
157 0.0 55.2 165.6#

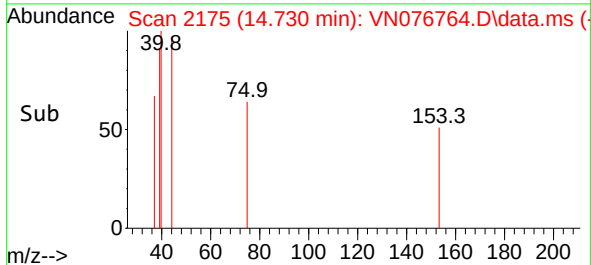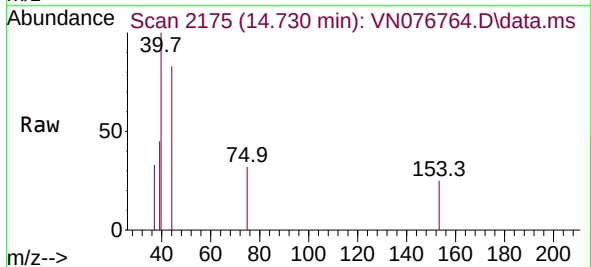



#93

1,2,4-Trichlorobenzene

Concen: 0.912 ug/l

RT: 15.406 min Scan# 21

Delta R.T. 0.011 min

Lab File: VN076764.D

Acq: 22 Feb 2023 12:09

Instrument :

MSVOA_N

ClientSampleId :

VN0222MBL01





Tgt Ion:180 Resp: 2513

Ion Ratio Lower Upper

180 100

182 83.0 48.0 144.0

145 17.9 15.2 45.6



#94

Hexachlorobutadiene

Concen: 0.367 ug/l

RT: 15.495 min Scan# 2305

Delta R.T. -0.012 min

Lab File: VN076764.D

Acq: 22 Feb 2023 12:09




Tgt Ion:225 Resp: 496


Ion Ratio Lower Upper

225 100

223 0.0 31.6 95.0#

227 18.3 31.3 93.9#

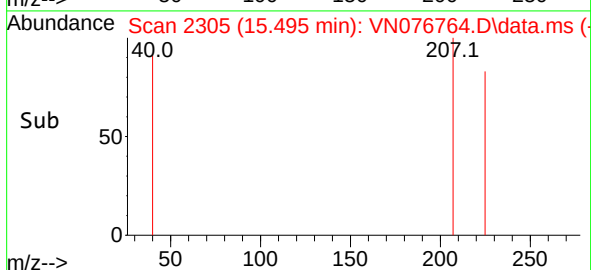

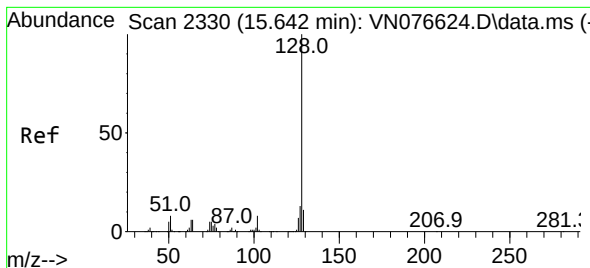

#95

Naphthalene

Concen: 1.316 ug/l

RT: 15.642 min Scan# 21

Delta R.T. -0.000 min

Lab File: VN076764.D

Acq: 22 Feb 2023 12:09

Instrument :

MSVOA_N

ClientSampleId :

VN0222MBL01





Tgt Ion:128 Resp: 11004

Ion Ratio Lower Upper

128 100

127 14.2 10.6 16.0

129 10.2 8.6 13.0

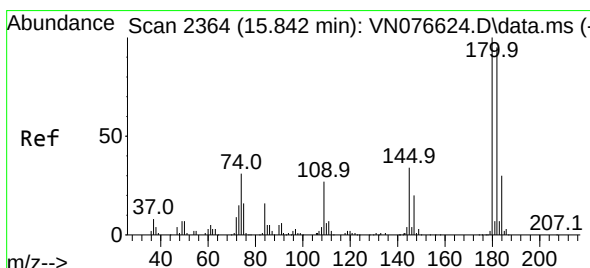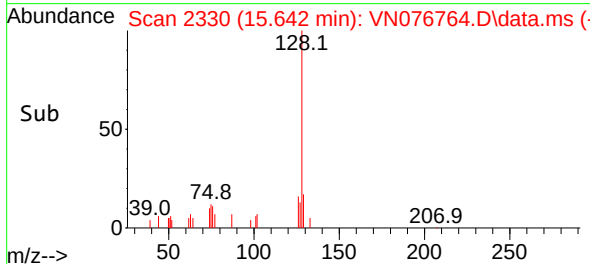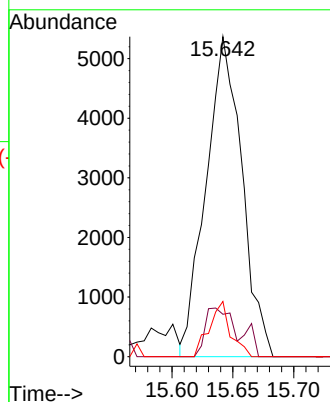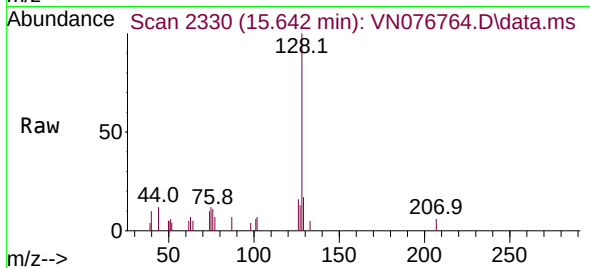

#96

1,2,3-Trichlorobenzene

Concen: 1.073 ug/l

RT: 15.854 min Scan# 2366

Delta R.T. 0.011 min

Lab File: VN076764.D

Acq: 22 Feb 2023 12:09

Tgt Ion:180 Resp: 2865

Ion Ratio Lower Upper

180 100

182 76.5 46.7 140.1

145 27.6 16.0 47.9

