
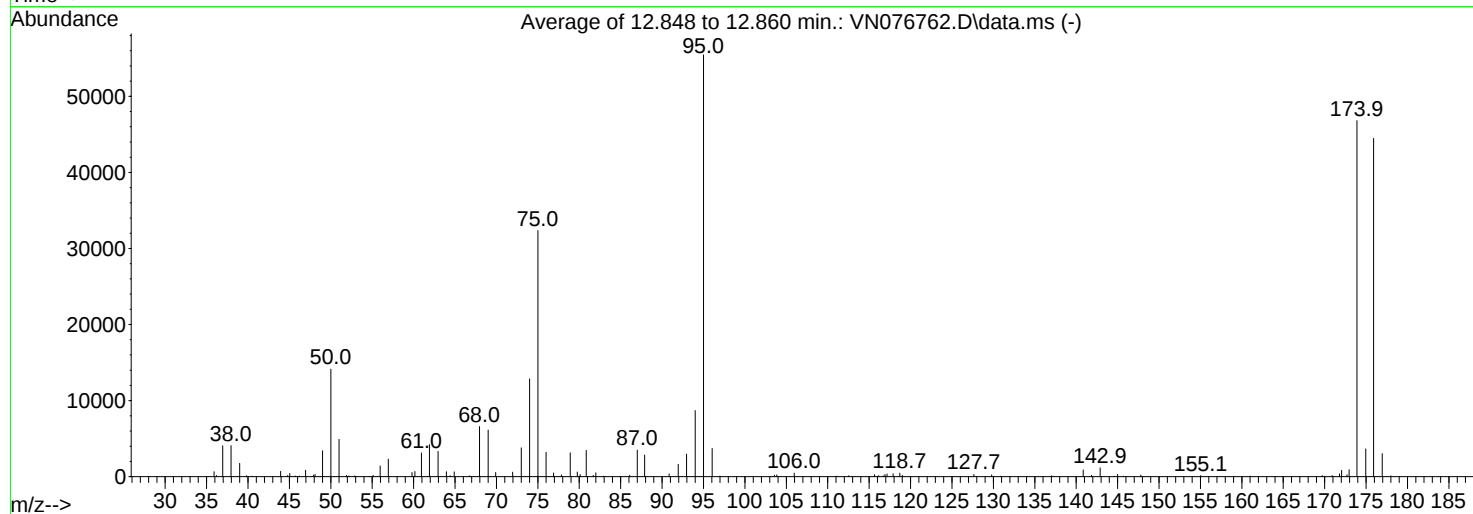


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022223\
Data File : VN076762.D
Acq On : 22 Feb 2023 10:23
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
Title : SW846 8260
Last Update : Tue Feb 14 01:44:47 2023

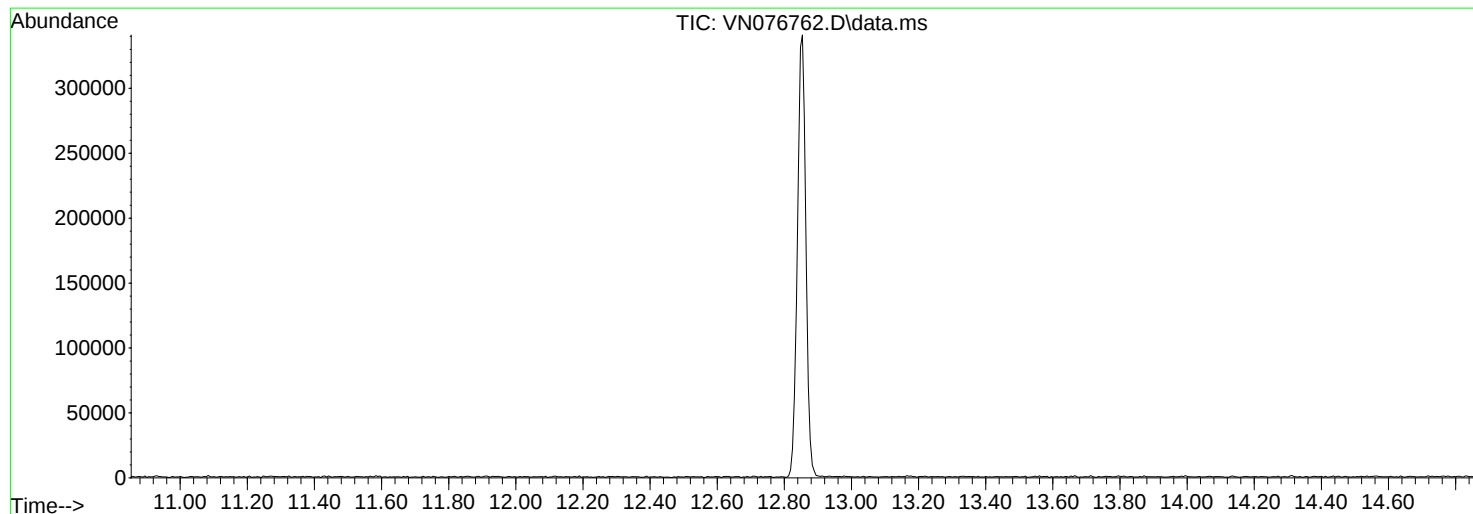

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.5	14130	PASS
75	95	30	60	58.3	32360	PASS
95	95	100	100	100.0	55459	PASS
96	95	5	9	6.7	3694	PASS
173	174	0.00	2	1.9	908	PASS
174	95	50	100	84.4	46803	PASS
175	174	5	9	7.8	3643	PASS
176	174	95	101	95.0	44477	PASS
177	176	5	9	6.8	3037	PASS

Average of 12.848 to 12.860 min.: VN076762.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	662	46.20	89	55.10	168	66.70	111
36.20	159	46.95	852	55.95	1421	66.90	7
36.95	4067	47.90	204	56.95	2299	67.95	658
37.95	4079	48.10	302	59.80	549	69.00	612
39.00	1754	49.00	3405	60.15	683	69.90	554
39.80	136	50.00	14130	60.95	3118	71.95	582
40.50	56	51.00	4904	61.90	4211	73.00	3794
43.95	702	51.90	173	62.95	3317	74.00	12862
44.80	149	52.20	86	63.95	661	75.00	32360
45.05	428	52.90	99	64.40	132	76.00	3208
45.70	78	54.70	51	64.90	626	76.90	477

Average of 12.848 to 12.860 min.: VN076762.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.85	233	90.85	359	112.55	134	130.90	68
78.90	3140	91.95	1626	115.65	258	137.05	129
79.75	614	92.95	2962	116.15	126	140.85	893
80.10	264	94.00	8685	116.70	104	141.85	170
80.85	3448	95.00	55459	116.90	296	142.90	1169
81.70	175	96.05	3694	117.15	349	144.60	66
82.00	507	97.00	63	117.90	388	145.00	297
82.90	57	103.55	187	118.70	466	145.70	60
86.10	192	103.85	239	119.00	163	147.80	204
87.00	3503	105.95	473	127.65	302	155.05	143
87.90	2849	111.10	75	129.80	228	161.00	86

Average of 12.848 to 12.860 min.: VN076762.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
169.70	138						
170.90	147						
171.80	354						
172.05	822						
172.70	254						
172.95	908						
173.90	46803						
174.95	3643						
175.90	44477						
176.95	3037						
178.00	112						

Instrument :

MSVOA_N

ClientSampleId :

BFB