
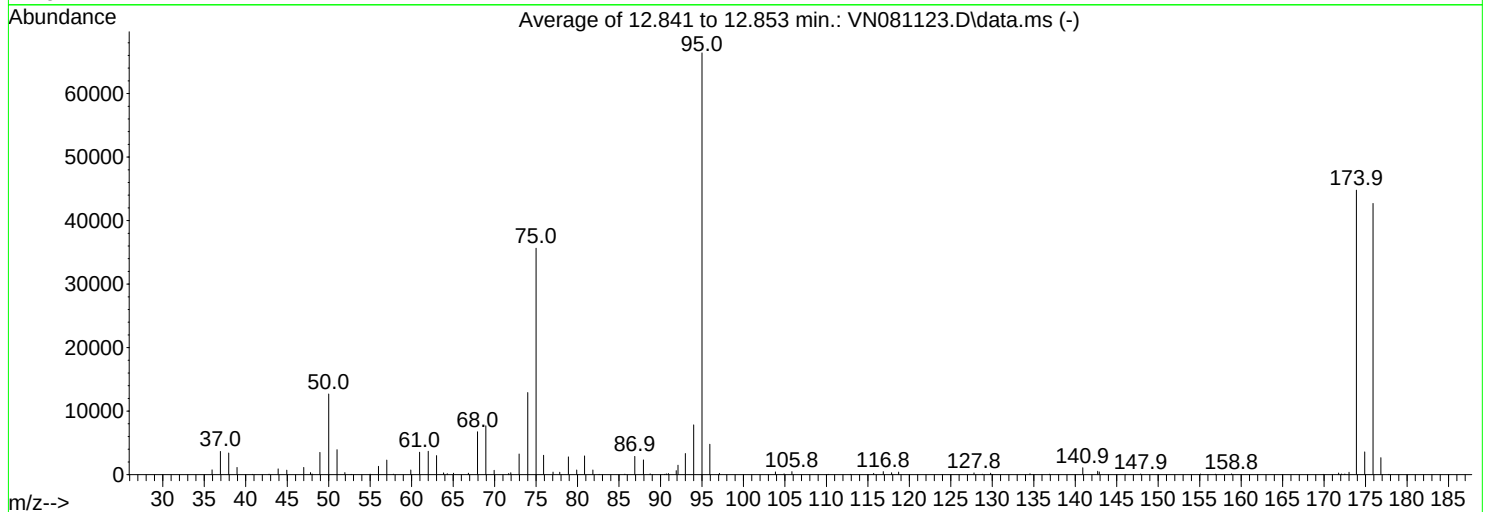


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022224\
Data File : VN081123.D
Acq On : 22 Feb 2024 09:39
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
Title : SW846 8260
Last Update : Fri Feb 16 23:45:20 2024

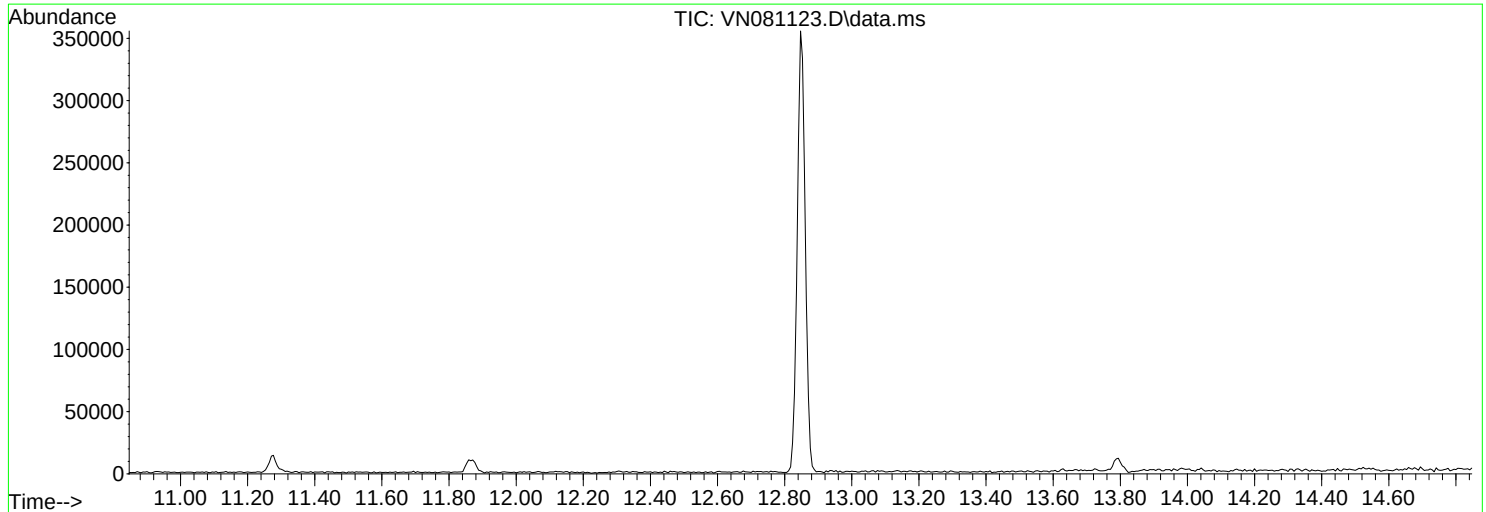

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	12705	PASS
75	95	30	60	53.7	35648	PASS
95	95	100	100	100.0	66408	PASS
96	95	5	9	7.2	4793	PASS
173	174	0.00	2	0.9	390	PASS
174	95	50	100	67.5	44803	PASS
175	174	5	9	8.0	3574	PASS
176	174	95	101	95.3	42701	PASS
177	176	5	9	6.2	2664	PASS

Average of 12.841 to 12.853 min.: VN081123.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	754	48.95	3505	62.00	3673	72.95	3251
36.95	3662	50.00	12705	63.00	2990	74.00	1293
37.95	3393	51.00	3933	63.85	269	75.00	3564
38.95	1125	51.95	325	64.30	156	75.90	3041
40.80	56	52.70	62	65.05	220	77.05	409
42.80	88	55.00	65	66.85	229	77.85	378
43.90	921	56.00	1315	67.95	6757	78.90	2805
44.95	712	57.00	2294	68.95	7673	79.90	737
47.00	1143	57.80	89	69.95	692	80.85	2937
47.80	335	59.90	733	71.70	178	81.85	725
48.00	100	60.95	3535	71.95	311	82.60	50

Average of 12.841 to 12.853 min.: VN081123.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.70	91	95.00	66408	118.70	398	155.10	115
86.90	2876	95.95	4793	127.80	279	156.90	76
87.95	2311	97.10	205	128.80	79	158.85	128
88.75	124	103.85	435	129.80	236	169.90	51
90.50	52	104.90	136	134.55	144	171.75	246
90.70	116	105.85	480	136.90	66	172.10	102
90.95	169	110.20	51	140.90	1081	172.50	110
91.90	641	112.90	52	142.70	523	173.00	390
92.10	1485	115.70	202	142.90	429	173.90	44803
93.00	3336	116.85	477	146.10	54	174.90	3574
94.00	7833	117.85	311	147.90	114	175.90	42701

Average of 12.841 to 12.853 min.: VN081123.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.85	2664						
177.80	51						

Instrument :
MSVOA_N
ClientSampleId :
BFB