

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022321\
 Data File : VN065981.D
 Acq On : 23 Feb 2021 13:19
 Operator : JC/MD
 Sample : PB134775TB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Feb 24 00:33:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 17 15:48:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.630	168	144525	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.550	114	238009	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	217743	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.315	152	89374	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.990	65	93225	46.13	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	92.26%		
35) Dibromofluoromethane	7.553	113	71635	48.63	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	97.26%		
50) Toluene-d8	10.058	98	293417	48.53	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	97.06%		
62) 4-Bromofluorobenzene	12.373	95	104450	46.02	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	92.04%		
Target Compounds						Qvalue
3) Chloromethane	2.055	50	1424	0.60	ug/l #	83
11) Tert butyl alcohol	4.733	59	414	1.47	ug/l #	73
13) Acrolein	3.586	56	2267	8.82	ug/l	96
16) Acetone	3.791	43	25228	38.38	ug/l	99
18) Methyl Acetate	4.290	43	486	0.29	ug/l #	51
20) Methylene Chloride	4.521	84	8644	4.61	ug/l	95
21) trans-1,2-Dichloroethene	5.000	96	344	0.20	ug/l #	1
25) 2-Butanone	6.798	43	2740	2.74	ug/l #	89
29) Tetrahydrofuran	7.171	42	677	0.98	ug/l #	42
31) Cyclohexane	7.627	56	2734	0.91	ug/l #	1
36) 1,1-Dichloropropene	7.630	75	11478	4.89	ug/l #	48
37) Ethyl Acetate	6.798	43	2740	1.29	ug/l #	68
38) Carbon Tetrachloride	7.630	117	14810	6.79	ug/l #	17
41) Methacrylonitrile	7.190	41	339	0.33	ug/l #	100
43) Isopropyl Acetate	8.129	43	10181	3.01	ug/l #	88
45) 1,2-Dichloropropane	9.232	63	664	0.36	ug/l #	44
48) Methyl methacrylate	9.142	41	2694	1.57	ug/l #	10
51) 4-Methyl-2-Pentanone	9.949	43	4188	2.04	ug/l	87
53) t-1,3-Dichloropropene	10.363	75	61	2.00	ug/l #	42
54) cis-1,3-Dichloropropene	9.871	75	18297	6.45	ug/l #	59
56) Ethyl methacrylate	10.193	69	1160	0.47	ug/l	89
57) 1,3-Dichloropropane	10.733	76	9843	3.37	ug/l #	43
59) 2-Hexanone	10.733	43	127173	86.87	ug/l #	50
74) N-amyl acetate	11.852	43	6793	2.68	ug/l #	49
76) 1,2,3-Trichloropropane	12.373	75	53588	24.96	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.704	105	2904	0.47	ug/l	90
81) trans-1,4-Dichloro-2-b...	12.373	75	53588	79.54	ug/l #	12
92) 1,2-Dibromo-3-Chloropr...	14.222	75	57	0.98	ug/l #	1
93) 1,2,4-Trichlorobenzene	14.878	180	353	2.67	ug/l	97
95) Naphthalene	15.103	128	1964	3.41	ug/l #	79
96) 1,2,3-Trichlorobenzene	15.289	180	439	2.43	ug/l #	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022321\
Data File : VN065981.D
Acq On : 23 Feb 2021 13:19
Operator : JC/MD
Sample : PB134775TB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Feb 24 00:33:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 17 15:48:13 2021
Response via : Initial Calibration




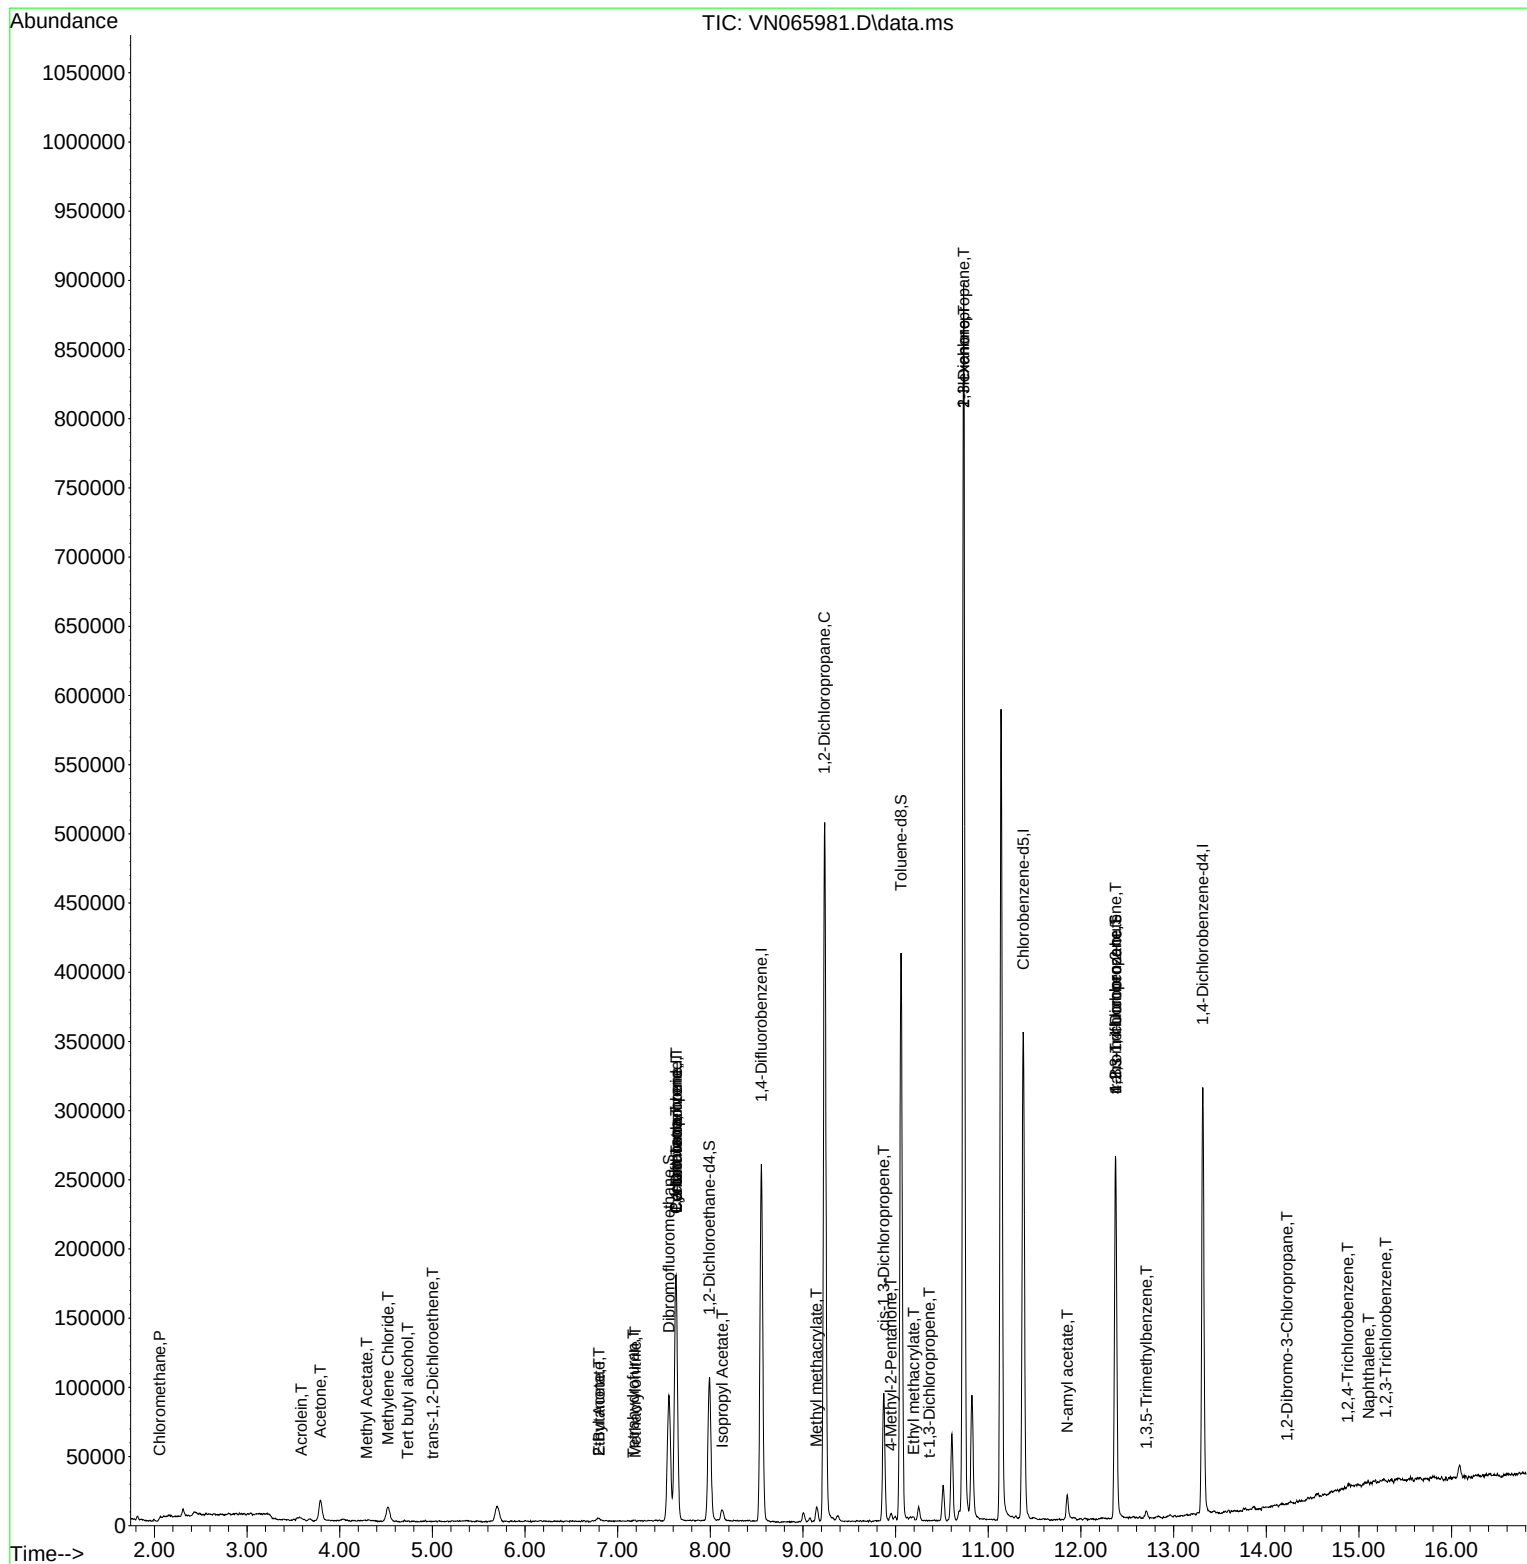




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.630 min Scan# 1832
Delta R.T. 0.003 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 144525
Ion Ratio Lower Upper
168 100
99 60.5 42.6 63.8

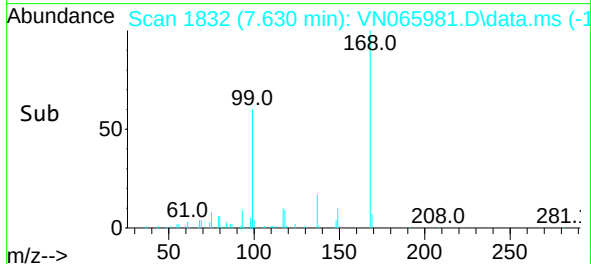

#3
Chloromethane
Concen: 0.60 ug/l
RT: 2.055 min Scan# 98
Delta R.T. 0.006 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion: 50 Resp: 1424
Ion Ratio Lower Upper
50 100
52 22.6 25.8 38.8#

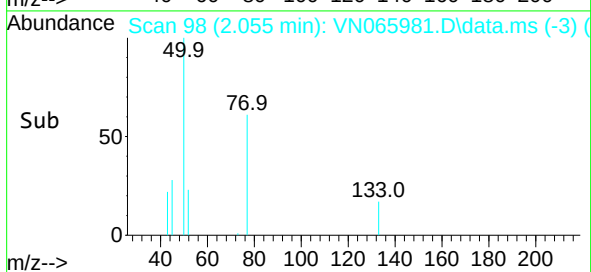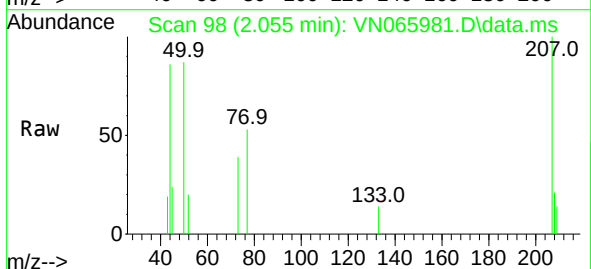







#11

Tert butyl alcohol
Concen: 1.47 ug/l
RT: 4.733 min Scan# 931
Delta R.T. -0.042 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Instrument :
MSVOA_N
ClientSampled :

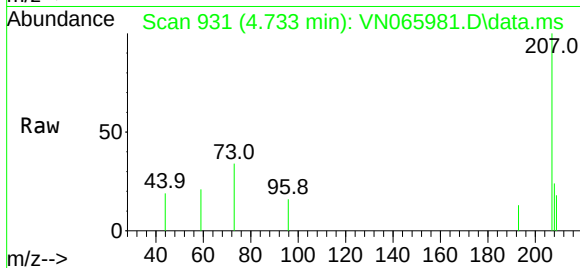




Tgt Ion: 59 Resp: 414
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#

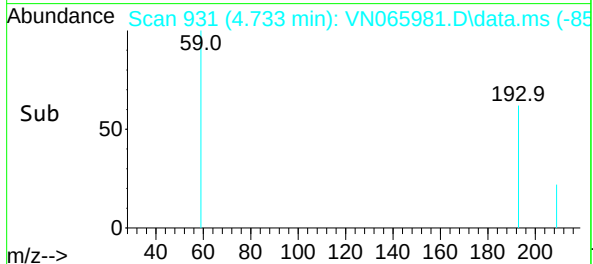


#13

Acrolein
Concen: 8.82 ug/l
RT: 3.586 min Scan# 574
Delta R.T. 0.010 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion: 56 Resp: 2267
Ion Ratio Lower Upper
56 100
55 73.4 56.0 84.0


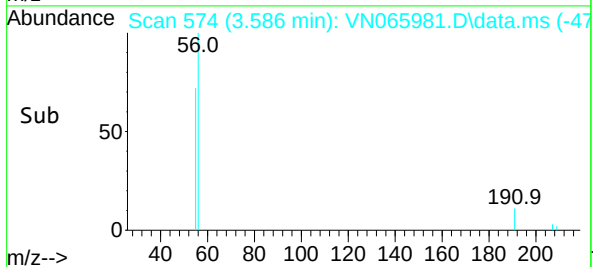

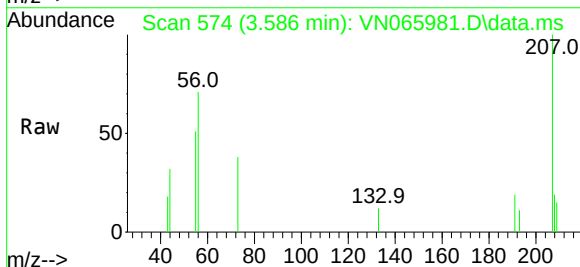




#16
Acetone
Concen: 38.38 ug/l
RT: 3.791 min Scan# 638
Delta R.T. 0.003 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 25228
Ion Ratio Lower Upper
43 100
58 34.5 27.0 40.6

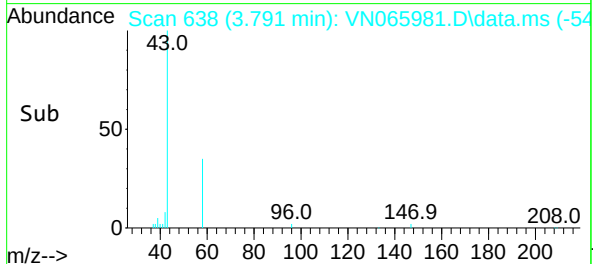

#18
Methyl Acetate
Concen: 0.29 ug/l
RT: 4.290 min Scan# 793
Delta R.T. -0.003 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19


Tgt Ion: 43 Resp: 486
Ion Ratio Lower Upper
43 100
74 0.0 19.5 29.3#

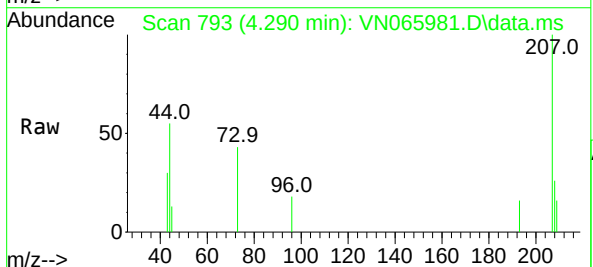






#20
Methylene Chloride
Concen: 4.61 ug/l
RT: 4.521 min Scan# 865
Delta R.T. 0.016 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 84 Resp: 8644

Ion	Ratio	Lower	Upper
84	100		
49	117.7	94.6	141.8
51	40.8	29.9	44.9
86	73.4	51.4	77.2

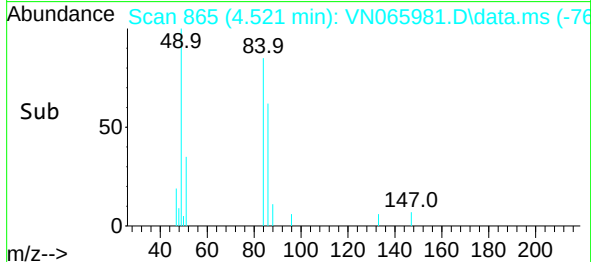
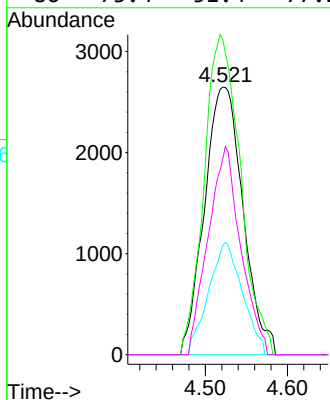



#21
trans-1,2-Dichloroethene
Concen: 0.20 ug/l
RT: 5.000 min Scan# 1014
Delta R.T. 0.009 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19



Tgt Ion: 96 Resp: 344

Ion	Ratio	Lower	Upper
96	100		
61	0.0	104.9	157.3#
98	0.0	51.8	77.8#



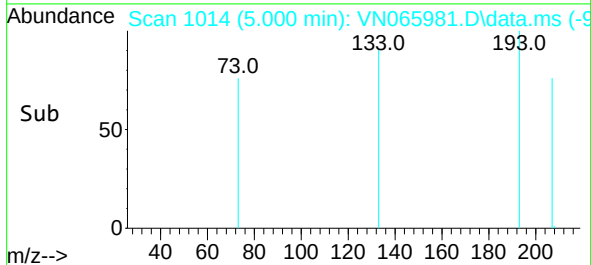
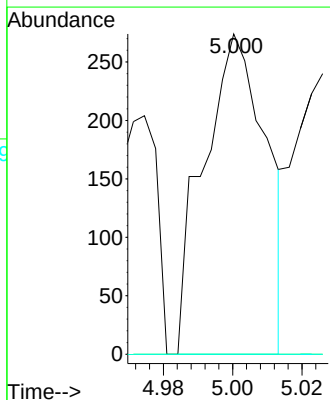




#25
2-Butanone
Concen: 2.74 ug/l
RT: 6.798 min Scan# 1573
Delta R.T. -0.000 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 2740
Ion Ratio Lower Upper
43 100
72 23.0 23.1 34.7#

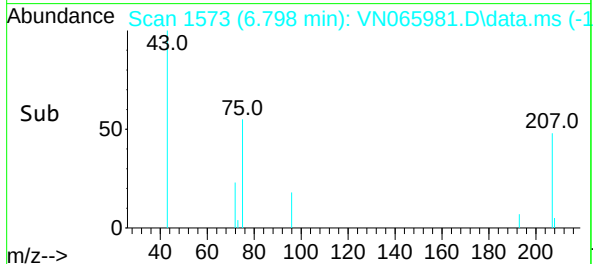

#29
Tetrahydrofuran
Concen: 0.98 ug/l
RT: 7.171 min Scan# 1689
Delta R.T. -0.003 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion: 42 Resp: 677
Ion Ratio Lower Upper
42 100
72 8.7 36.6 55.0#
71 4.4 34.3 51.5#


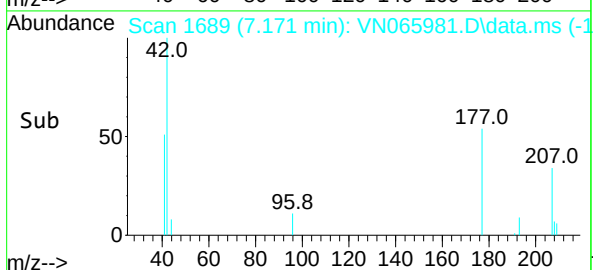






#31
Cyclohexane
Concen: 0.91 ug/l
RT: 7.627 min Scan# 1831
Delta R.T. 0.016 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 2734
Ion Ratio Lower Upper
56 100
69 190.5 26.6 39.8#
84 133.1 70.4 105.6#

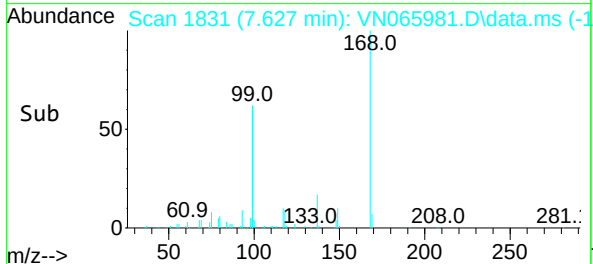

#33
1,2-Dichloroethane-d4
Concen: 46.13 ug/l
RT: 7.990 min Scan# 1944
Delta R.T. 0.003 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion: 65 Resp: 93225
Ion Ratio Lower Upper
65 100
67 52.3 0.0 107.2

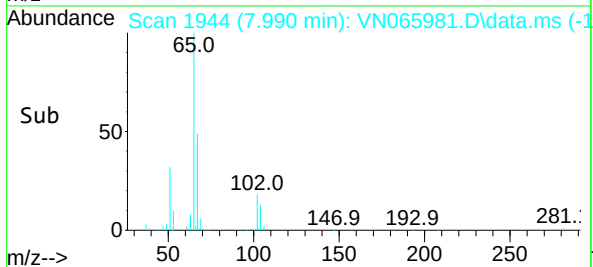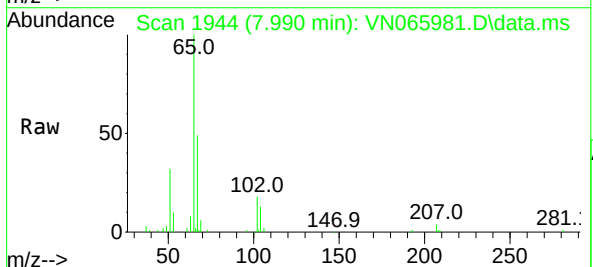







#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.550 min Scan# 2118
Delta R.T. -0.000 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Instrument :
MSVOA_N
ClientSampleId :




Tgt Ion:	114	Resp:	238009
Ion	Ratio	Lower	Upper
114	100		
63	21.3	0.0	38.6
88	17.3	0.0	30.6

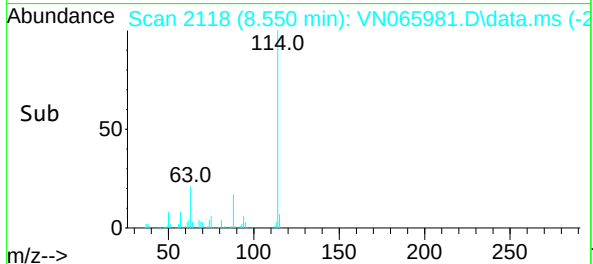


#35

Dibromofluoromethane
Concen: 48.63 ug/l
RT: 7.553 min Scan# 1808
Delta R.T. 0.003 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion:	113	Resp:	71635
Ion	Ratio	Lower	Upper
113	100		
111	102.9	82.2	123.2
192	18.6	15.4	23.0


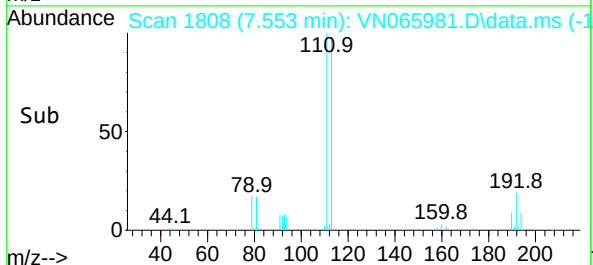
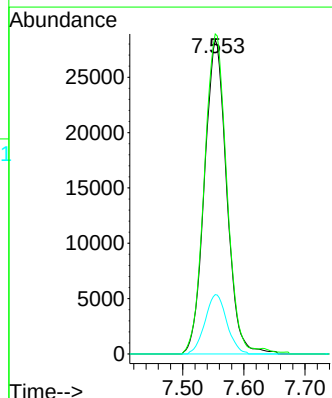
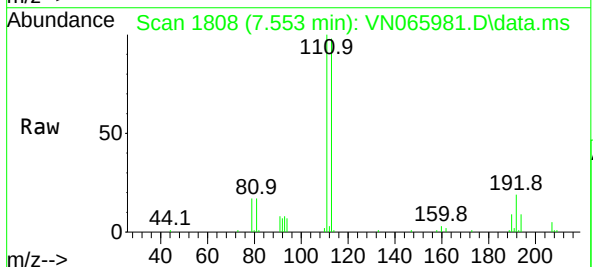




#36
1,1-Dichloropropene
Concen: 4.89 ug/l
RT: 7.630 min Scan# 1832
Delta R.T. -0.123 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 11478
Ion Ratio Lower Upper
75 100
110 8.2 18.2 54.6#
77 0.0 24.9 37.3#

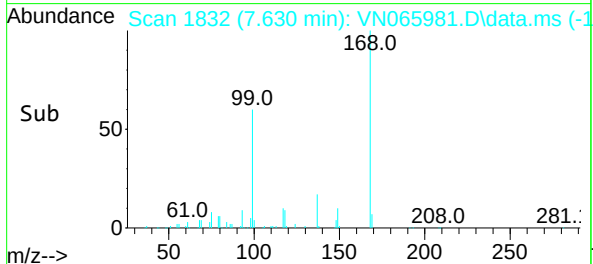

#37
Ethyl Acetate
Concen: 1.29 ug/l
RT: 6.798 min Scan# 1573
Delta R.T. -0.093 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion: 43 Resp: 2740
Ion Ratio Lower Upper
43 100
61 0.0 11.6 17.4#
70 0.0 8.6 13.0#


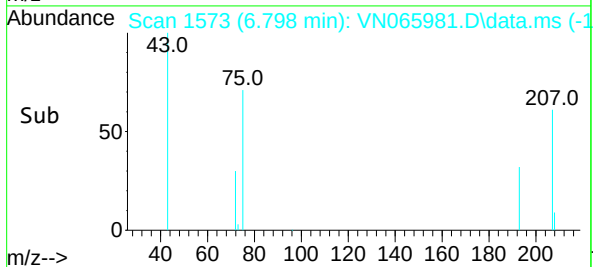

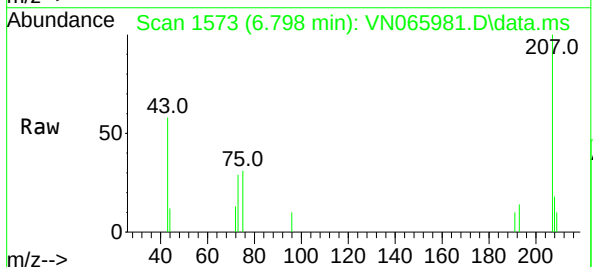




#38
Carbon Tetrachloride
Concen: 6.79 ug/l
RT: 7.630 min Scan# 1832
Delta R.T. -0.104 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 14810
Ion Ratio Lower Upper
117 100
119 5.9 76.0 114.0#
121 0.0 24.5 36.7#

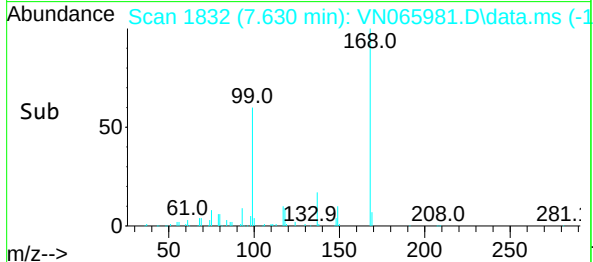

#41
Methacrylonitrile
Concen: 0.33 ug/l
RT: 7.190 min Scan# 1695
Delta R.T. 0.061 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion: 41 Resp: 339
Ion Ratio Lower Upper
41 100
39 0.0 0.0 0.0
67 0.0 0.0 0.0
52 0.0 0.0 0.0

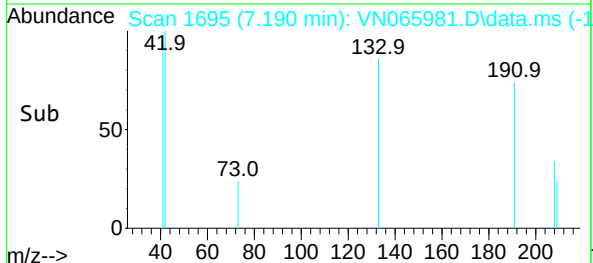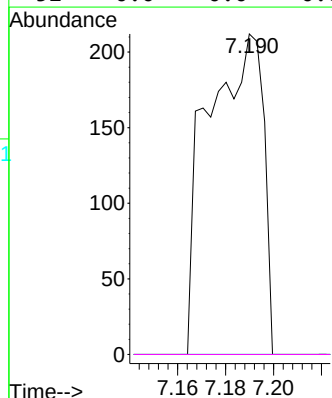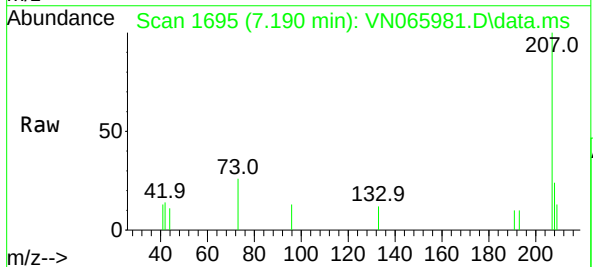







#43

Isopropyl Acetate
Concen: 3.01 ug/l
RT: 8.129 min Scan# 1987
Delta R.T. -0.003 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Instrument :
MSVOA_N
ClientSampled :






Tgt Ion:	43	Resp:	10181
Ion	Ratio	Lower	Upper
43	100		
61	19.2	22.5	33.7#
87	13.6	11.1	16.7

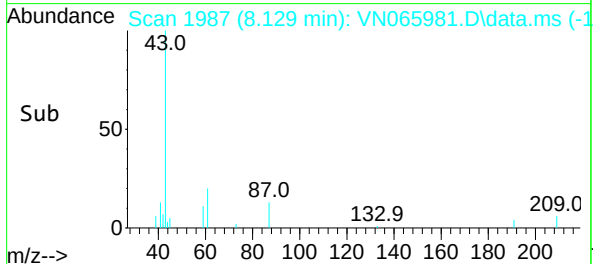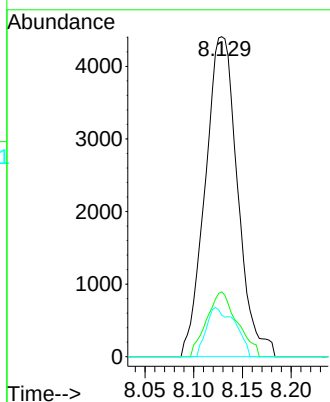


#45

1,2-Dichloropropane
Concen: 0.36 ug/l
RT: 9.232 min Scan# 2330
Delta R.T. 0.148 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion:	63	Resp:	664
Ion	Ratio	Lower	Upper
63	100		
65	0.0	24.9	37.3#


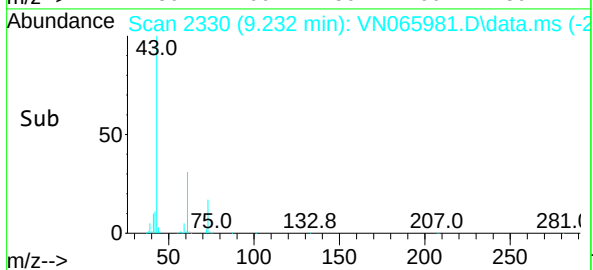
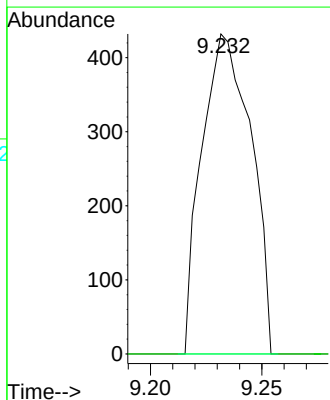
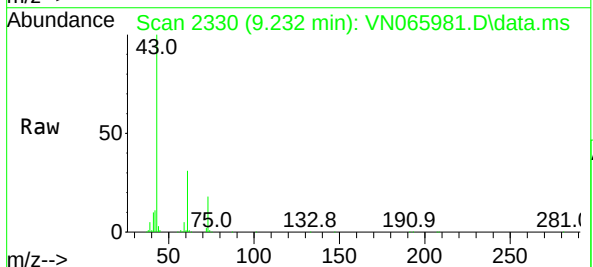




#48
Methyl methacrylate
Concen: 1.57 ug/l
RT: 9.142 min Scan# 2302
Delta R.T. -0.026 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 41 Resp: 2694
Ion Ratio Lower Upper
41 100
69 0.0 75.9 113.9#
39 0.0 46.6 69.8#

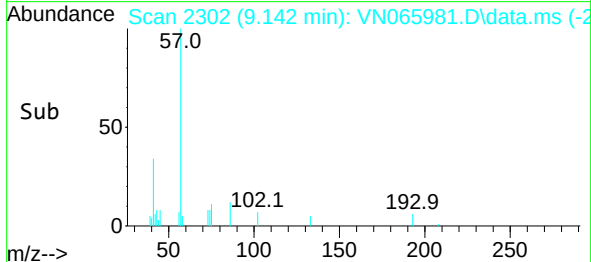

#50
Toluene-d8
Concen: 48.53 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. -0.000 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion: 98 Resp: 293417
Ion Ratio Lower Upper
98 100
100 65.3 50.5 75.7




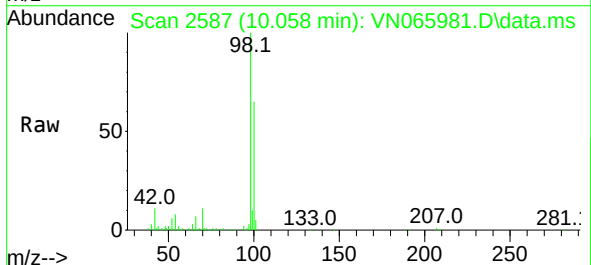




#51
4-Methyl-2-Pentanone
Concen: 2.04 ug/l
RT: 9.949 min Scan# 2553
Delta R.T. -0.003 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 4188
Ion Ratio Lower Upper
43 100
58 32.6 32.5 48.7

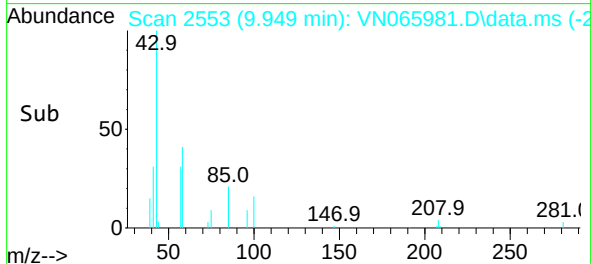

#53
t-1,3-Dichloropropene
Concen: 2.00 ug/l
RT: 10.363 min Scan# 2682
Delta R.T. 0.012 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion: 75 Resp: 61
Ion Ratio Lower Upper
75 100
77 0.0 26.2 39.4#









#54
cis-1,3-Dichloropropene
Concen: 6.45 ug/l
RT: 9.871 min Scan# 2529
Delta R.T. 0.064 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 18297
Ion Ratio Lower Upper
75 100
77 2.1 24.9 37.3#
39 23.3 36.2 54.4#

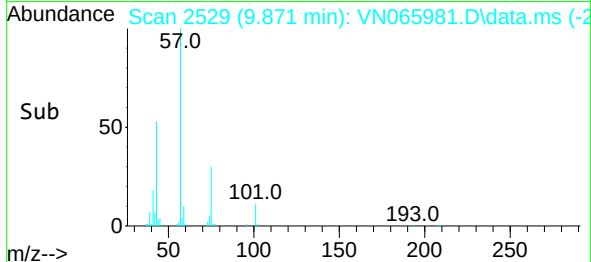

#56
Ethyl methacrylate
Concen: 0.47 ug/l
RT: 10.193 min Scan# 2629
Delta R.T. -0.206 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion: 69 Resp: 1160
Ion Ratio Lower Upper
69 100
41 53.6 49.6 74.4
39 42.0 28.0 42.0


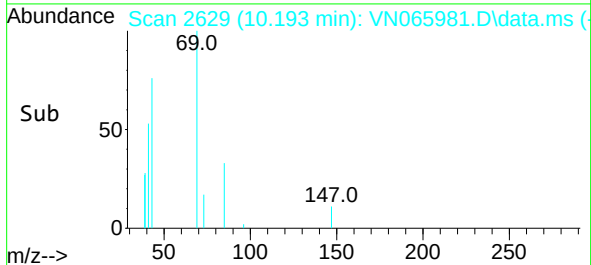






#57
1,3-Dichloropropane
Concen: 3.37 ug/l
RT: 10.733 min Scan# 2797
Delta R.T. 0.057 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 76 Resp: 9843
Ion Ratio Lower Upper
76 100
78 0.0 25.7 38.5#



#59
2-Hexanone
Concen: 86.87 ug/l
RT: 10.733 min Scan# 2797
Delta R.T. 0.012 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion: 43 Resp: 127173
Ion Ratio Lower Upper
43 100
58 19.8 28.1 84.3#


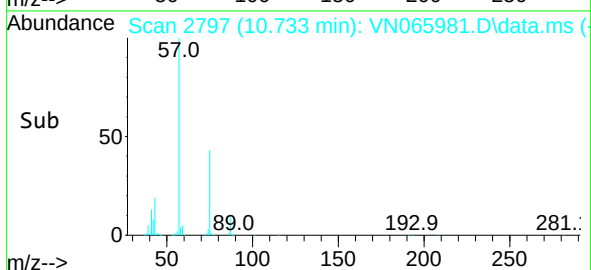






#62
4-Bromofluorobenzene
Concen: 46.02 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.003 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 104450
Ion Ratio Lower Upper
95 100
174 72.5 0.0 169.0
176 68.3 0.0 162.4

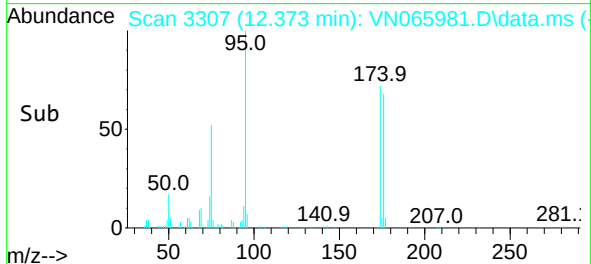

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion: 117 Resp: 217743
Ion Ratio Lower Upper
117 100
82 57.2 43.7 65.5
119 31.9 26.1 39.1







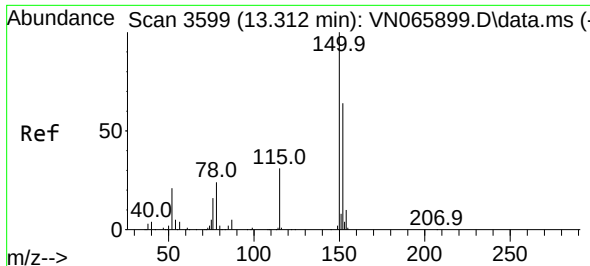

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.315 min Scan# 3600
Delta R.T. 0.003 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:152 Resp: 89374
Ion Ratio Lower Upper
152 100
115 61.5 28.5 85.6
150 156.0 0.0 347.6

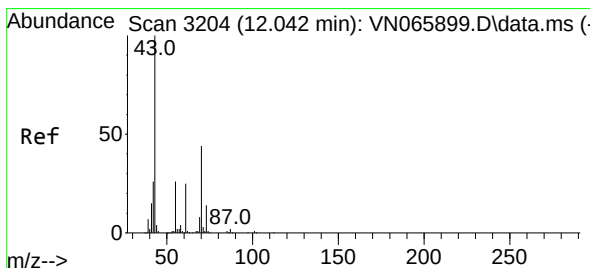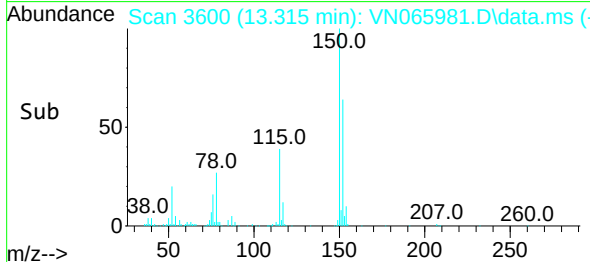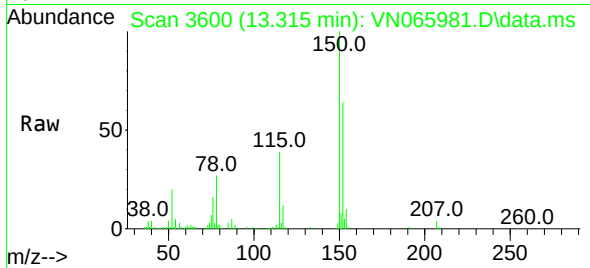

#74
N-ethyl acetate
Concen: 2.68 ug/l
RT: 11.852 min Scan# 3145
Delta R.T. -0.190 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion: 43 Resp: 6793
Ion Ratio Lower Upper
43 100
70 0.0 34.4 51.6#
55 1.0 20.7 31.1#
61 11.5 19.1 28.7#


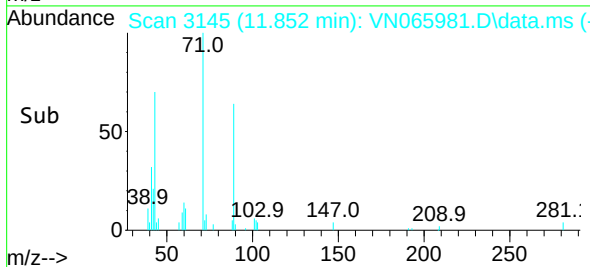

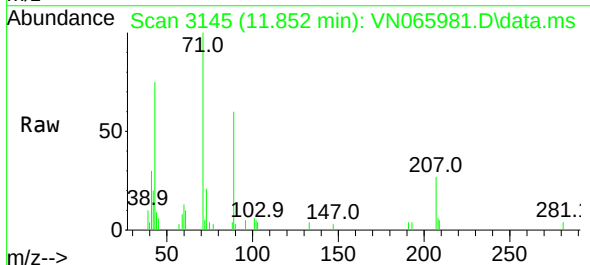




#76
1,2,3-Trichloropropane
Concen: 24.96 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. -0.151 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 53588
Ion Ratio Lower Upper
75 100
77 2.1 0.0 0.0#

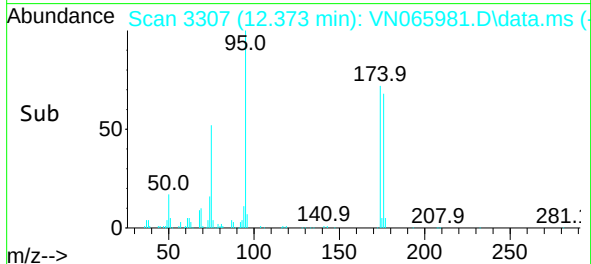

#80
1,3,5-Trimethylbenzene
Concen: 0.47 ug/l
RT: 12.704 min Scan# 3410
Delta R.T. 0.003 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19

Tgt Ion: 105 Resp: 2904
Ion Ratio Lower Upper
105 100
120 41.8 24.3 72.8


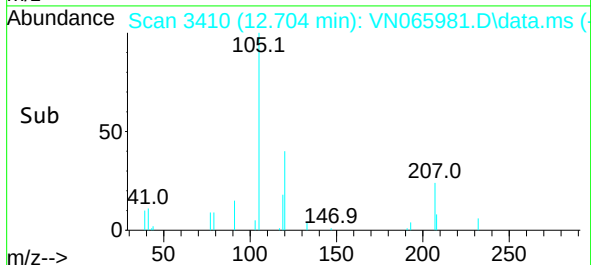






#81
 trans-1,4-Dichloro-2-butene
 Concen: 79.54 ug/l
 RT: 12.373 min Scan# 3307
 Delta R.T. 0.103 min
 Lab File: VN065981.D
 Acq: 23 Feb 2021 13:19




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 75 Resp: 53588
 Ion Ratio Lower Upper
 75 100
 53 0.0 74.6 111.8#
 89 0.1 35.8 53.8#

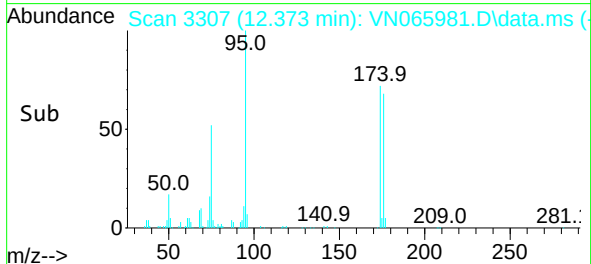

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.98 ug/l
 RT: 14.222 min Scan# 3882
 Delta R.T. -0.016 min
 Lab File: VN065981.D
 Acq: 23 Feb 2021 13:19

Tgt Ion: 75 Resp: 57
 Ion Ratio Lower Upper
 75 100
 155 0.0 44.1 132.4#
 157 0.0 56.0 168.2#


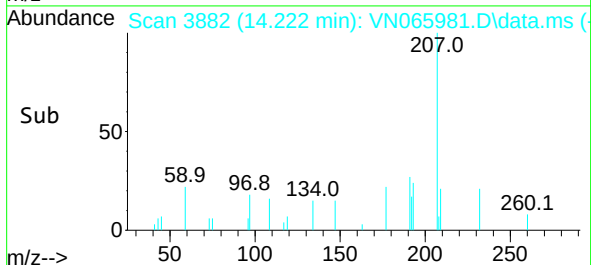






#93
1,2,4-Trichlorobenzene
Concen: 2.67 ug/l
RT: 14.878 min Scan# 4086
Delta R.T. -0.000 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:	180	Resp:	353
Ion	Ratio	Lower	Upper
180	100		
182	92.6	47.3	142.0
145	35.1	15.6	46.8

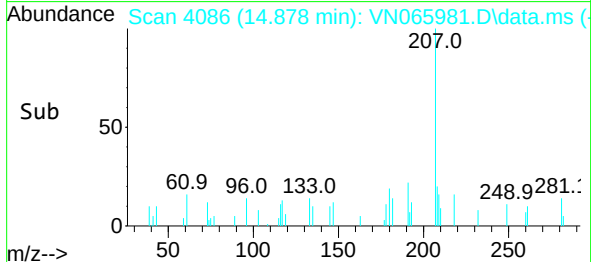

#95
Naphthalene
Concen: 3.41 ug/l
RT: 15.103 min Scan# 4156
Delta R.T. 0.006 min
Lab File: VN065981.D
Acq: 23 Feb 2021 13:19


Tgt Ion:	128	Resp:	1964
Ion	Ratio	Lower	Upper
128	100		
127	7.2	10.2	15.2#
129	0.0	8.6	13.0#

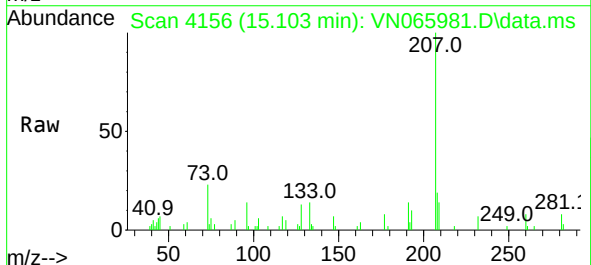



#96
 1,2,3-Trichlorobenzene
 Concen: 2.43 ug/l
 RT: 15.289 min Scan# 4214
 Delta R.T. 0.012 min
 Lab File: VN065981.D
 Acq: 23 Feb 2021 13:19

Instrument :
 MSVOA_N
 ClientSampleId :

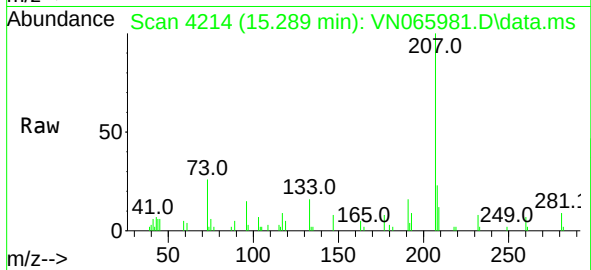

Tgt Ion:180 Resp: 439
 Ion Ratio Lower Upper
 180 100
 182 86.8 47.4 142.3
 145 0.0 16.5 49.5#

