
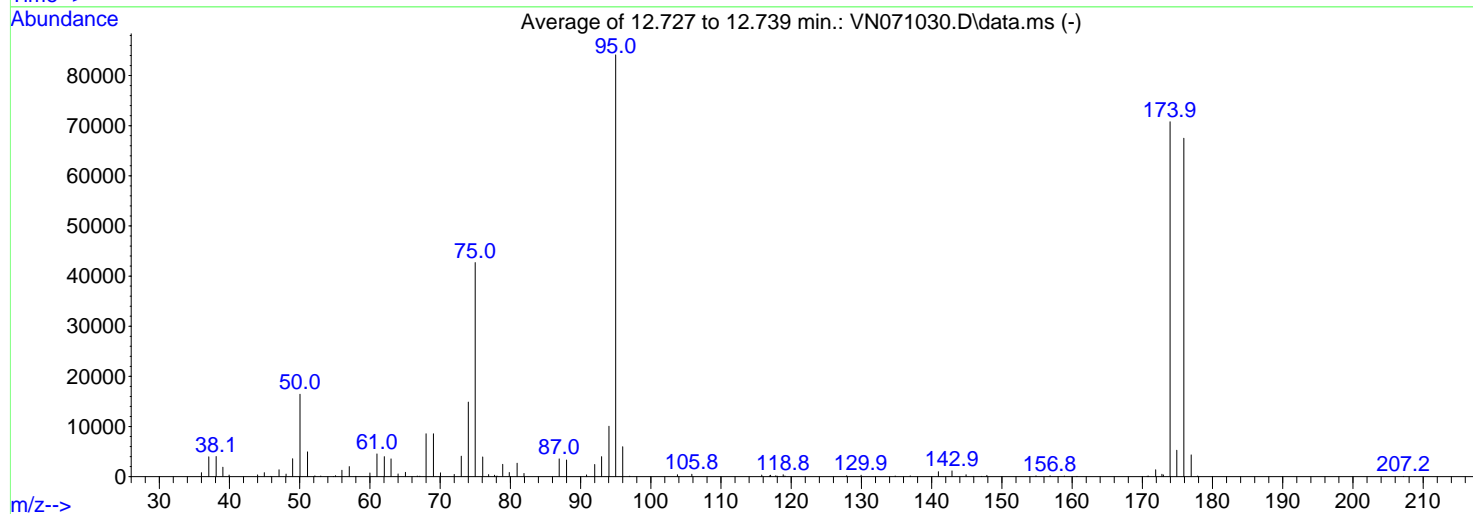


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022322\
 Data File : VN071030.D
 Acq On : 23 Feb 2022 10:24
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
 Title : SW846 8260
 Last Update : Mon Feb 21 07:57:15 2022

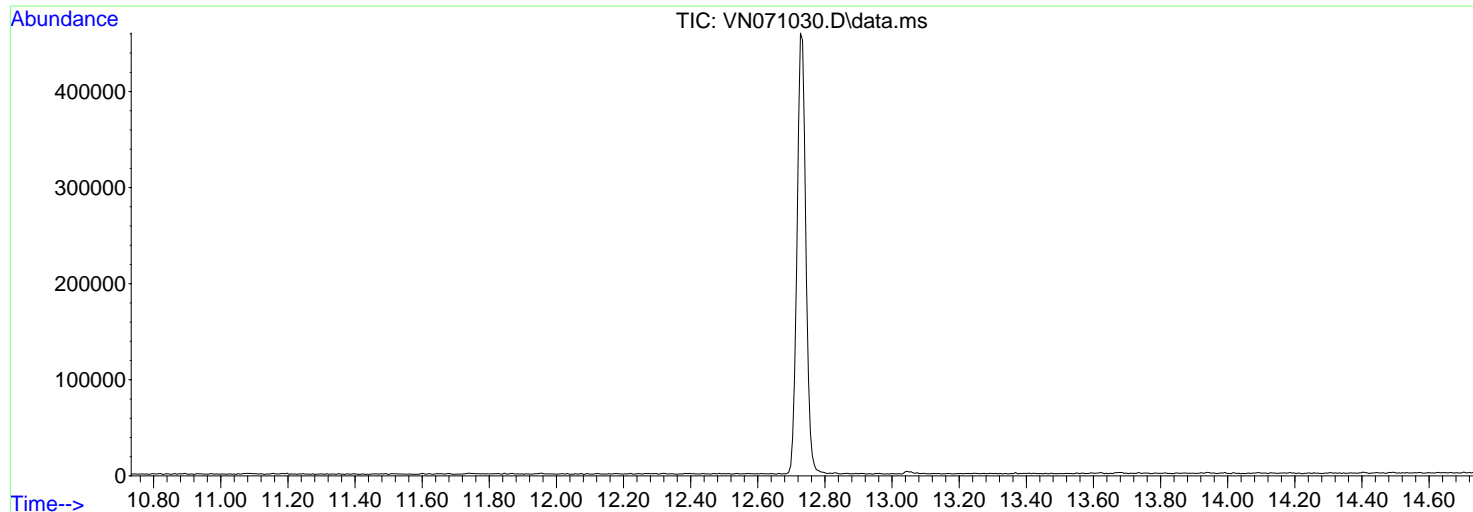

AutoFind: Scans 1826, 1827, 1828; Background Corrected with Scan 1817

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50 | 95 | 15 | 40 | 19.5 | 16434 | PASS |
| 75 | 95 | 30 | 60 | 50.8 | 42712 | PASS |
| 95 | 95 | 100 | 100 | 100.0 | 84136 | PASS |
| 96 | 95 | 5 | 9 | 7.1 | 5963 | PASS |
| 173 | 174 | 0.00 | 2 | 0.7 | 482 | PASS |
| 174 | 95 | 50 | 100 | 84.1 | 70779 | PASS |
| 175 | 174 | 5 | 9 | 7.4 | 5261 | PASS |
| 176 | 174 | 95 | 101 | 95.4 | 67509 | PASS |
| 177 | 176 | 5 | 9 | 6.4 | 4339 | PASS |