

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022323\
 Data File : VN076794.D
 Acq On : 23 Feb 2023 15:37
 Operator : JC\MD
 Sample : 01664-01DL 4X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-10-0222DL

Quant Time: Feb 24 01:35:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 14 01:44:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.231	168	307601	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.107	114	537259	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.866	117	473602	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.795	152	195589	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.584	65	217258	51.149	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 102.300%			
35) Dibromofluoromethane	8.172	113	161973	46.036	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 92.080%			
50) Toluene-d8	10.572	98	666726	50.741	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 101.480%			
62) 4-Bromofluorobenzene	12.848	95	198932	45.711	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 91.420%			
Target Compounds						Qvalue
11) Tert butyl alcohol	5.513	59	6345	11.317	ug/l #	71
15) Acrylonitrile	5.813	53	3181	1.599	ug/l #	26
16) Acetone	4.443	43	5974	3.149	ug/l #	55
19) Methyl tert-butyl Ether	5.801	73	275708	25.757	ug/l	100
20) Methylene Chloride	5.272	84	1261	0.317	ug/l #	55
25) 2-Butanone	7.507	43	1052	0.376	ug/l #	51
29) Tetrahydrofuran	7.854	42	379	0.207	ug/l #	37
31) Cyclohexane	8.266	56	40170	6.029	ug/l	97
36) 1,1-Dichloropropene	8.231	75	27849	5.478	ug/l #	49
38) Carbon Tetrachloride	8.231	117	31415	6.126	ug/l #	17
39) Methylcyclohexane	9.607	83	18162	3.143	ug/l	99
48) Methyl methacrylate	9.607	41	8372	2.027	ug/l #	52
51) 4-Methyl-2-Pentanone	10.448	43	5012	0.905	ug/l	97
55) 1,1,2-Trichloroethane	11.013	97	2025	0.528	ug/l #	16
59) 2-Hexanone	11.060	43	5318	1.332	ug/l	77
67) Ethyl Benzene	11.966	91	23152	1.354	ug/l	97
68) m/p-Xylenes	12.077	106	19140	2.904	ug/l	90
69) o-Xylene	12.401	106	6768	1.053	ug/l	96
71) Bromoform	12.854	173	2204	0.824	ug/l #	1
73) Isopropylbenzene	12.695	105	3699	0.258	ug/l	93
76) 1,2,3-Trichloropropane	12.848	75	110171	27.861	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.136	105	15725	1.327	ug/l	73
81) trans-1,4-Dichloro-2-b...	12.848	75	110171	81.148	ug/l #	4
83) tert-Butylbenzene	13.483	119	7707	0.719	ug/l #	48
84) 1,2,4-Trimethylbenzene	13.483	105	62863	5.324	ug/l	96
85) sec-Butylbenzene	13.483	105	62863	4.201	ug/l #	55
86) p-Isopropyltoluene	13.736	119	2793	0.234	ug/l	91
89) n-Butylbenzene	13.995	91	17575	1.691	ug/l #	45
90) Hexachloroethane	14.330	117	7483	2.991	ug/l #	14
95) Naphthalene	15.648	128	9930	0.946	ug/l #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022323\
Data File : VN076794.D
Acq On : 23 Feb 2023 15:37
Operator : JC\MD
Sample : 01664-01DL 4X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL

Quant Time: Feb 24 01:35:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 14 01:44:47 2023
Response via : Initial Calibration




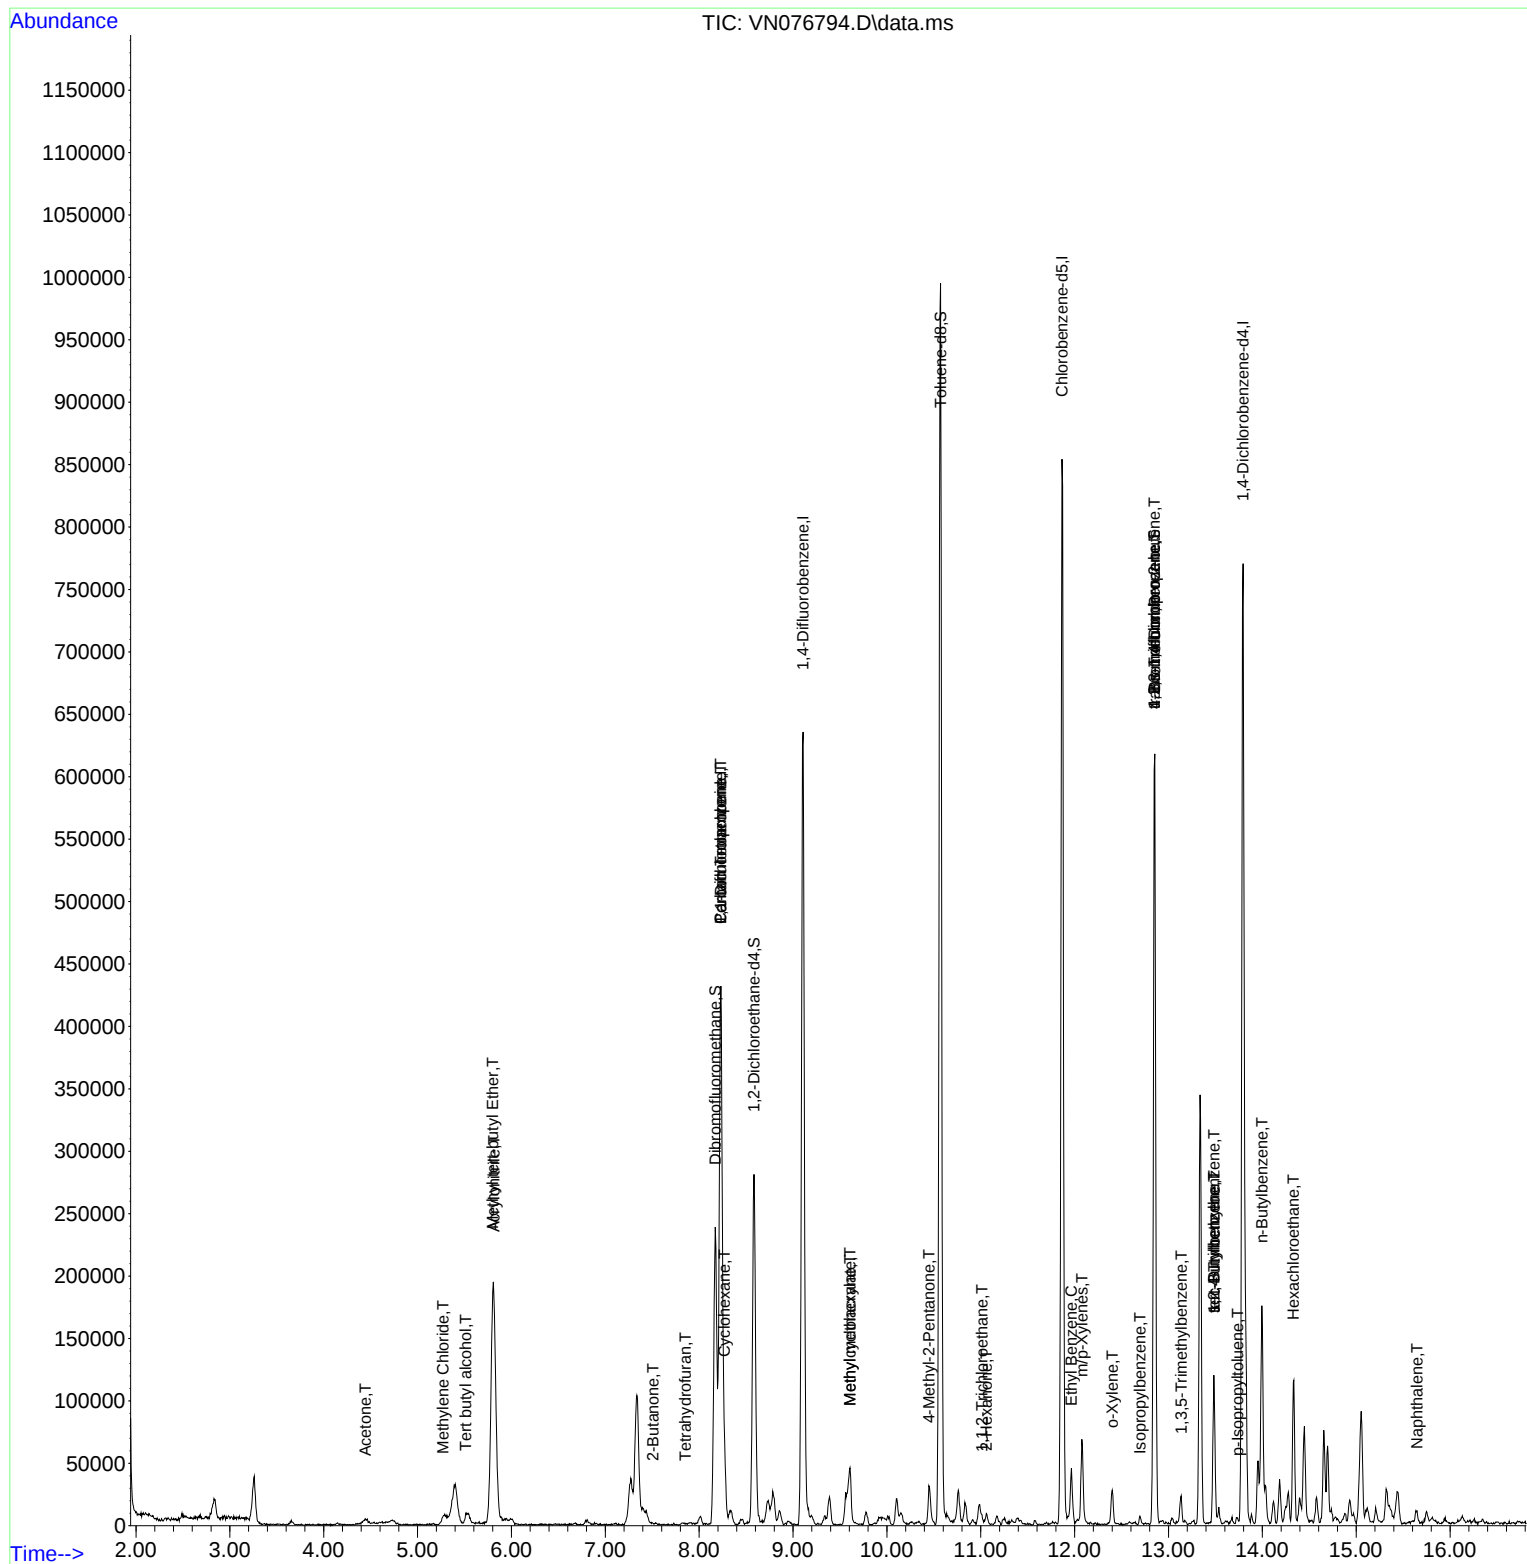


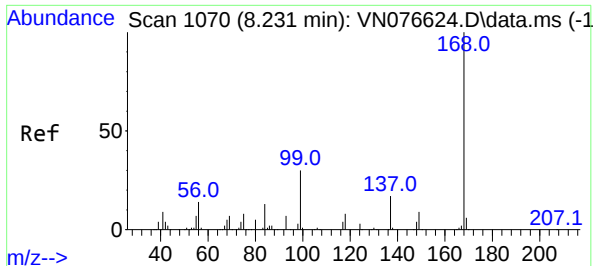

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.231 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion:168 Resp: 307601
Ion Ratio Lower Upper
168 100
99 57.6 44.8 67.2

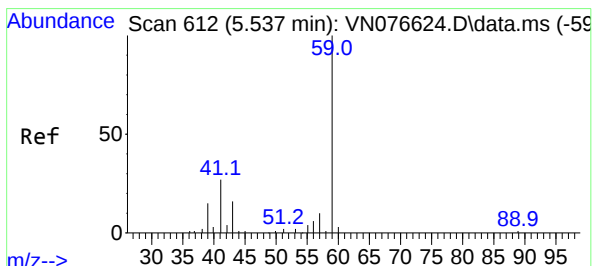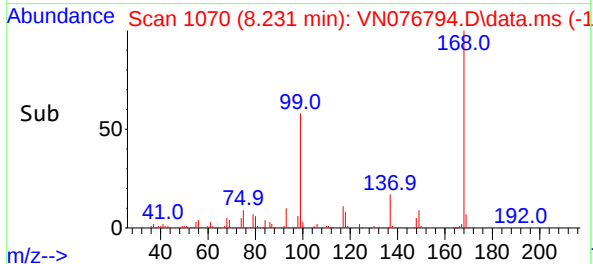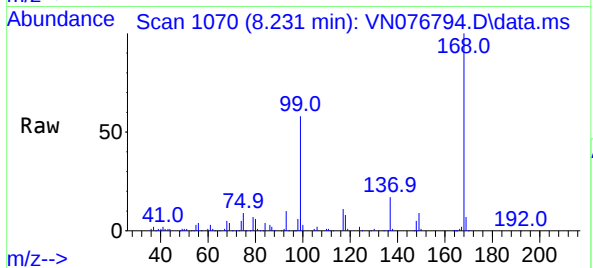

#11
Tert butyl alcohol
Concen: 11.317 ug/l
RT: 5.513 min Scan# 608
Delta R.T. -0.024 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion: 59 Resp: 6345
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#


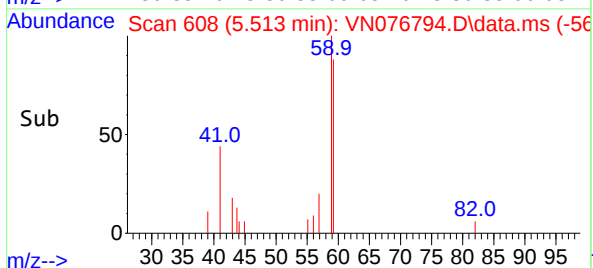

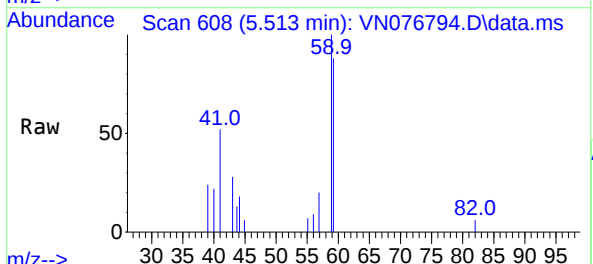




#15
Acrylonitrile
Concen: 1.599 ug/l
RT: 5.813 min Scan# 61
Delta R.T. 0.088 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion: 53 Resp: 3181
Ion Ratio Lower Upper
53 100
52 10.8 65.3 97.9#
51 0.0 29.2 43.8#



#16
Acetone
Concen: 3.149 ug/l
RT: 4.443 min Scan# 426
Delta R.T. 0.006 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion: 43 Resp: 5974
Ion Ratio Lower Upper
43 100
58 7.1 25.9 38.9#

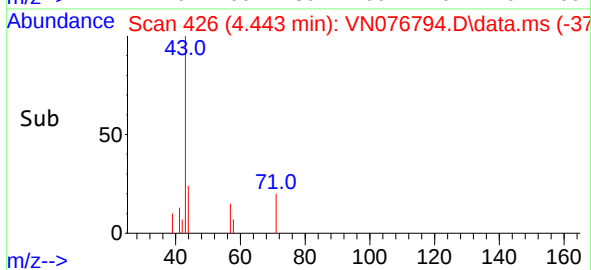



#19

Methyl tert-butyl Ether

Concen: 25.757 ug/l

RT: 5.801 min Scan# 61

Delta R.T. -0.006 min

Lab File: VN076794.D

Acq: 23 Feb 2023 15:37

Instrument :

MSVOA_N

ClientSampleId :





MW-10-0222DL

Tgt Ion: 73 Resp: 275708

Ion Ratio Lower Upper

73 100

57 23.8 19.0 28.4

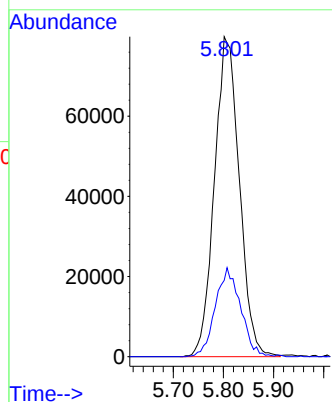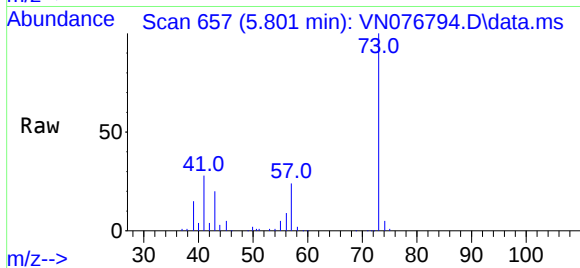

#20

Methylene Chloride

Concen: 0.317 ug/l

RT: 5.272 min Scan# 567

Delta R.T. -0.018 min

Lab File: VN076794.D

Acq: 23 Feb 2023 15:37

Tgt Ion: 84 Resp: 1261




Ion Ratio Lower Upper


84 100

49 68.9 104.9 157.3#

51 26.6 33.8 50.8#

86 30.3 50.0 75.0#


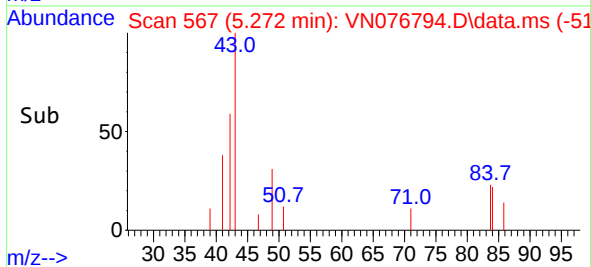

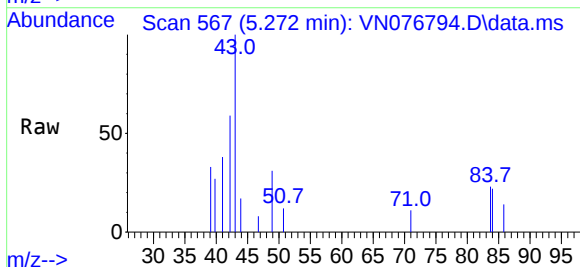




#25
2-Butanone
Concen: 0.376 ug/l
RT: 7.507 min Scan# 94
Delta R.T. 0.018 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion: 43 Resp: 1052
Ion Ratio Lower Upper
43 100
72 0.0 19.4 29.2#



#29
Tetrahydrofuran
Concen: 0.207 ug/l
RT: 7.854 min Scan# 1006
Delta R.T. 0.012 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion: 42 Resp: 379
Ion Ratio Lower Upper
42 100
72 0.0 31.5 47.3#
71 0.0 29.8 44.8#


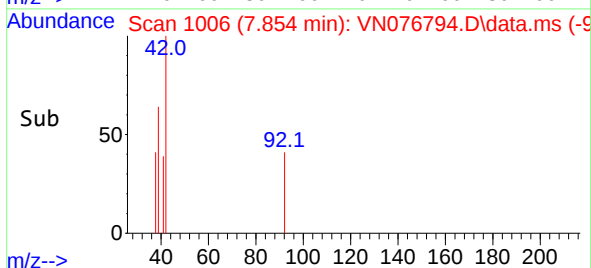
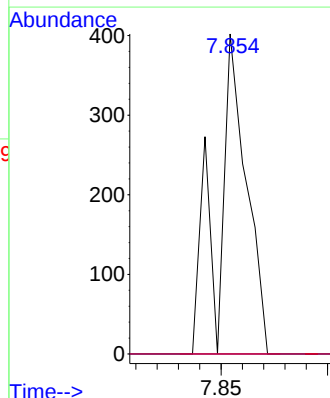



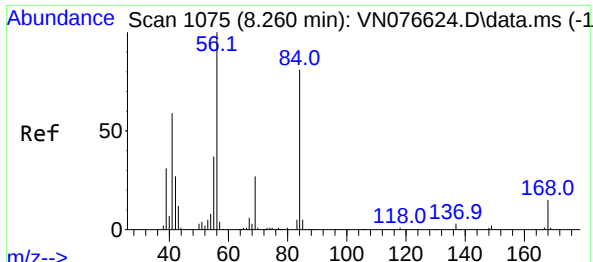

#31
Cyclohexane
Concen: 6.029 ug/l
RT: 8.266 min Scan# 1075
Delta R.T. 0.006 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion: 56 Resp: 40170
Ion Ratio Lower Upper
56 100
69 29.4 21.6 32.4
84 83.9 65.1 97.7

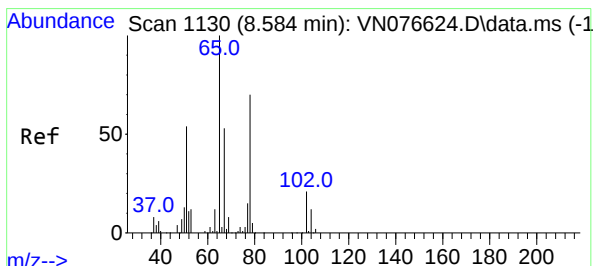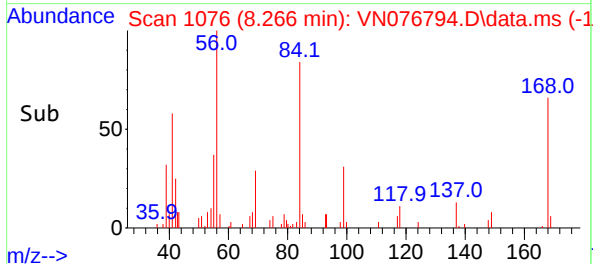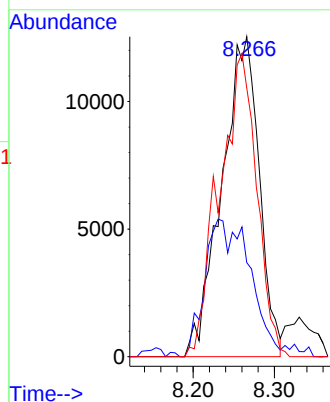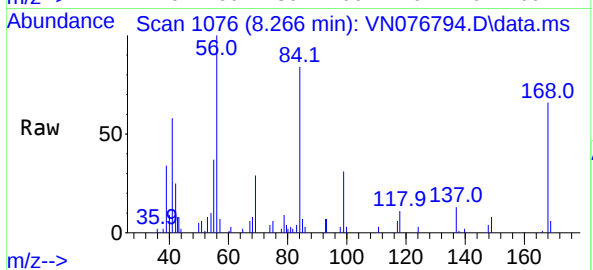

#33
1,2-Dichloroethane-d4
Concen: 51.149 ug/l
RT: 8.584 min Scan# 1130
Delta R.T. -0.000 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion: 65 Resp: 217258
Ion Ratio Lower Upper
65 100
67 52.6 0.0 105.6


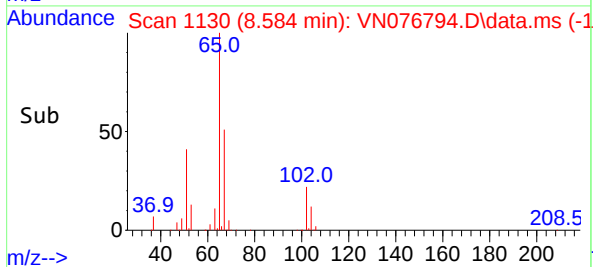
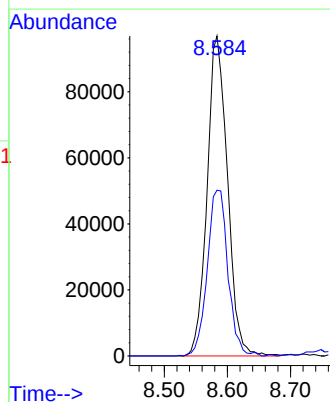
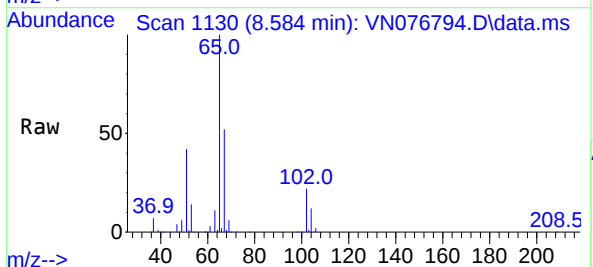


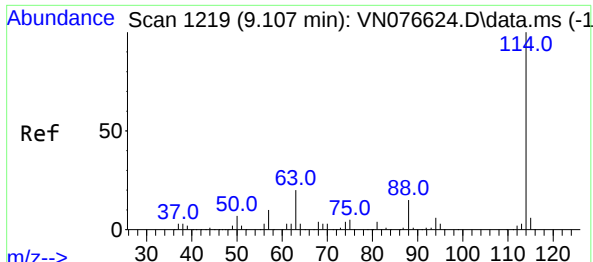

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.107 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion:114 Resp: 537259
Ion Ratio Lower Upper
114 100
63 21.7 0.0 40.0
88 14.5 0.0 29.6

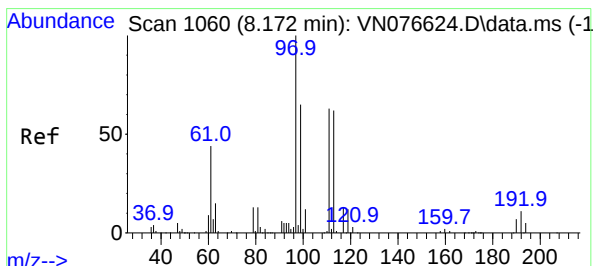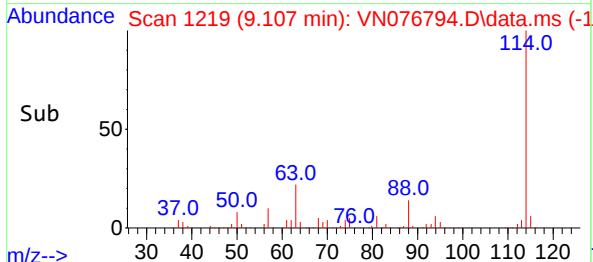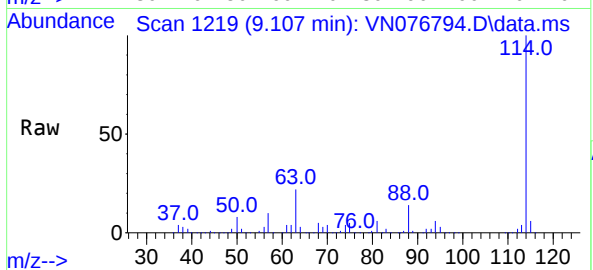

#35
Dibromofluoromethane
Concen: 46.036 ug/l
RT: 8.172 min Scan# 1060
Delta R.T. -0.000 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion:113 Resp: 161973
Ion Ratio Lower Upper
113 100
111 103.6 83.1 124.7
192 18.9 15.6 23.4


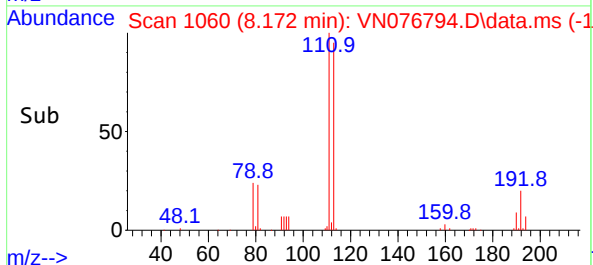

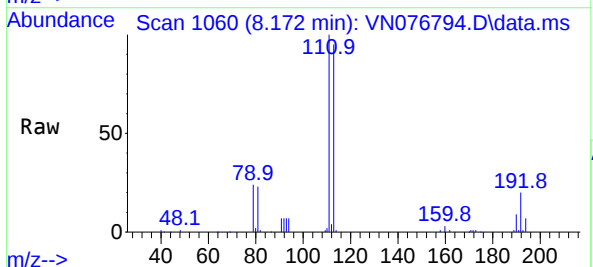


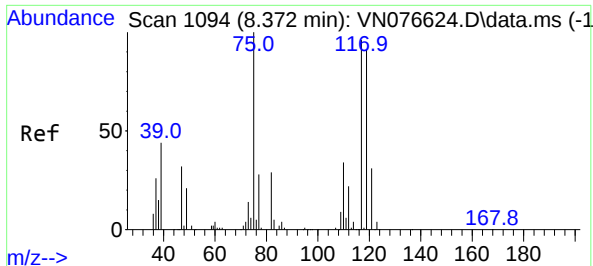

#36
1,1-Dichloropropene
Concen: 5.478 ug/l
RT: 8.231 min Scan# 1070
Delta R.T. -0.141 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion: 75 Resp: 27849
Ion Ratio Lower Upper
75 100
110 7.4 17.5 52.5#
77 0.9 24.5 36.7#

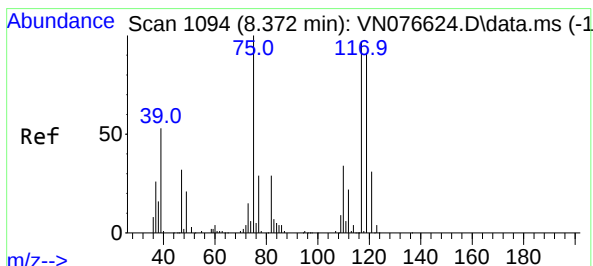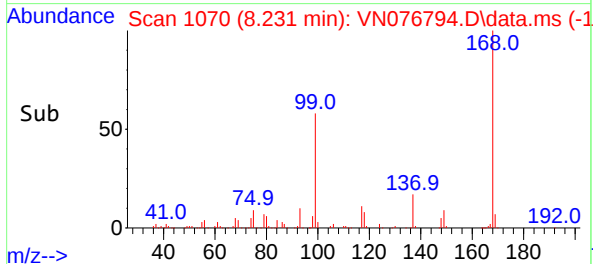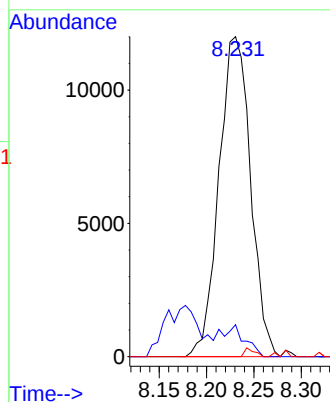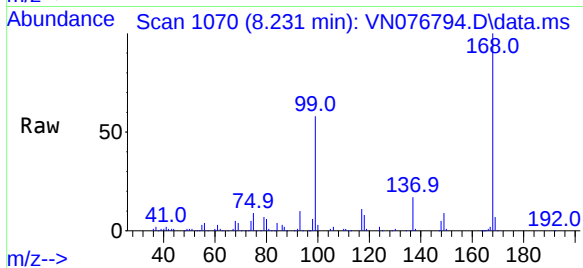

#38
Carbon Tetrachloride
Concen: 6.126 ug/l
RT: 8.231 min Scan# 1070
Delta R.T. -0.141 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion: 117 Resp: 31415
Ion Ratio Lower Upper
117 100
119 5.3 75.4 113.0#
121 0.0 26.0 39.0#


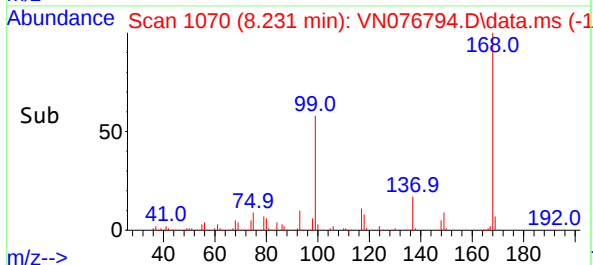

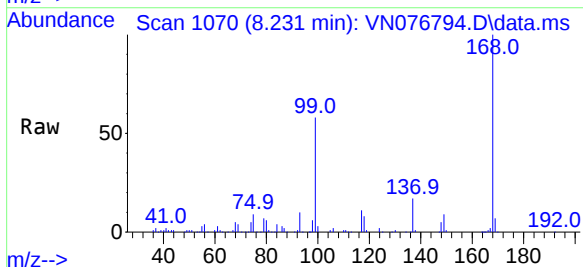


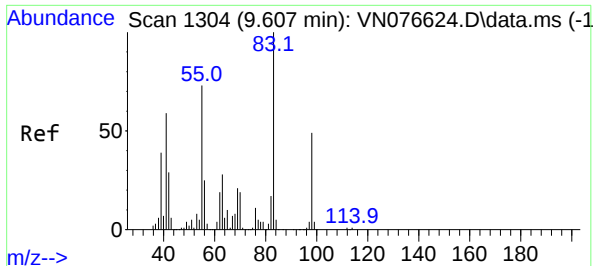

#39
Methylcyclohexane
Concen: 3.143 ug/l
RT: 9.607 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion:	83	Resp:	18162
Ion	Ratio	Lower	Upper
83	100		
55	71.6	58.6	88.0
98	49.0	39.4	59.2

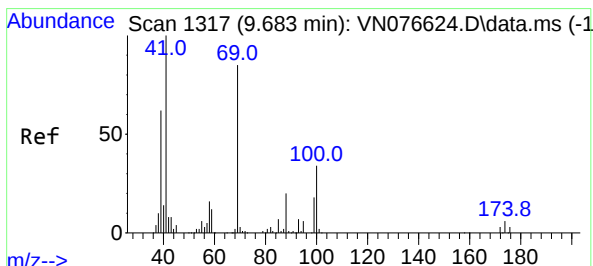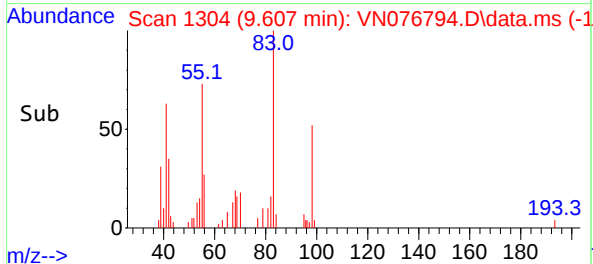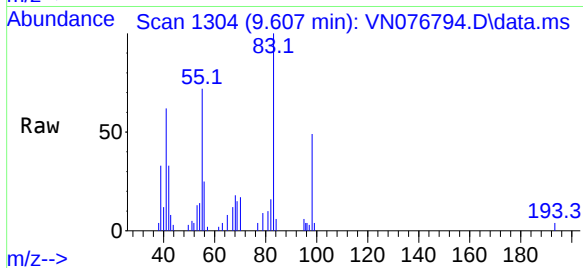

#48
Methyl methacrylate
Concen: 2.027 ug/l
RT: 9.607 min Scan# 1304
Delta R.T. -0.076 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion:	41	Resp:	8372
Ion	Ratio	Lower	Upper
41	100		
69	43.0	65.4	98.0#
39	103.7	49.3	73.9#


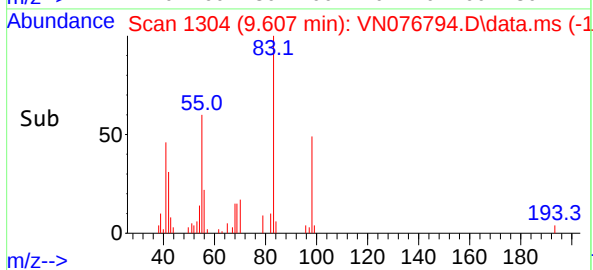

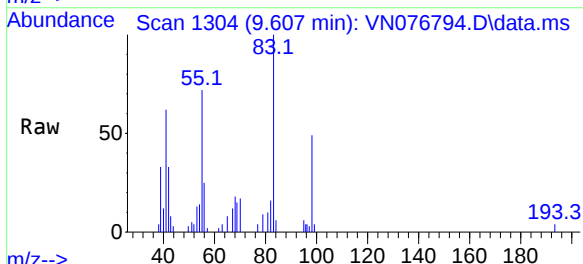




#50
Toluene-d8
Concen: 50.741 ug/l
RT: 10.572 min Scan# 1468
Delta R.T. 0.006 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion: 98 Resp: 666726
Ion Ratio Lower Upper
98 100
100 63.2 52.9 79.3

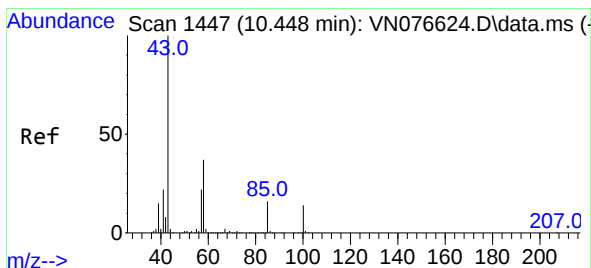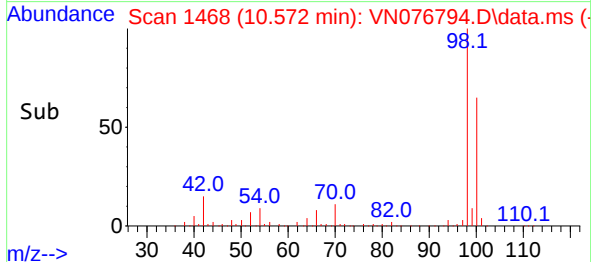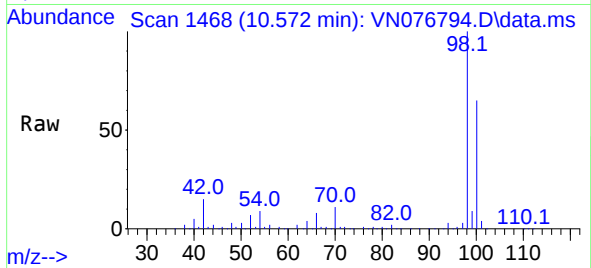

#51
4-Methyl-2-Pentanone
Concen: 0.905 ug/l
RT: 10.448 min Scan# 1447
Delta R.T. 0.000 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion: 43 Resp: 5012
Ion Ratio Lower Upper
43 100
58 35.0 29.5 44.3

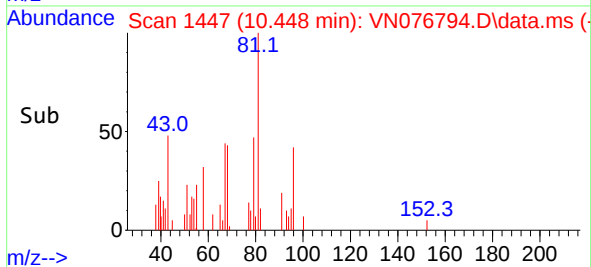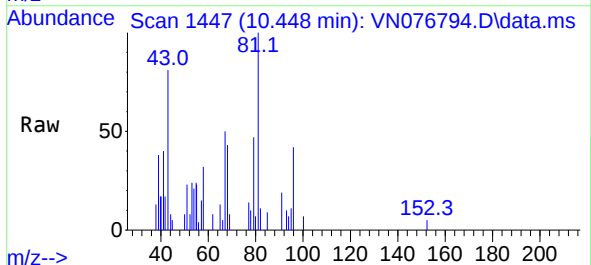







#55
1,1,2-Trichloroethane
Concen: 0.528 ug/l
RT: 11.013 min Scan# 1151
Delta R.T. -0.006 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL

Tgt Ion: 97 Resp: 2025




Ion	Ratio	Lower	Upper
97	100		
83	0.0	67.3	100.9#
85	0.0	43.2	64.8#
99	0.0	49.0	73.4#

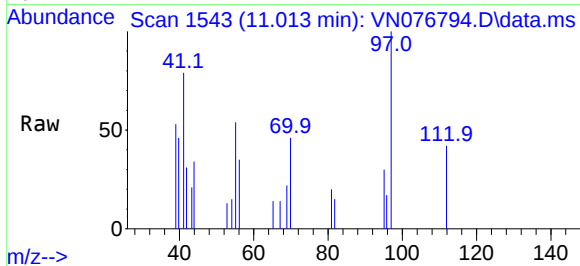


#59
2-Hexanone
Concen: 1.332 ug/l
RT: 11.060 min Scan# 1551
Delta R.T. -0.135 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion: 43 Resp: 5318

Ion	Ratio	Lower	Upper
43	100		
58	35.1	25.4	76.0


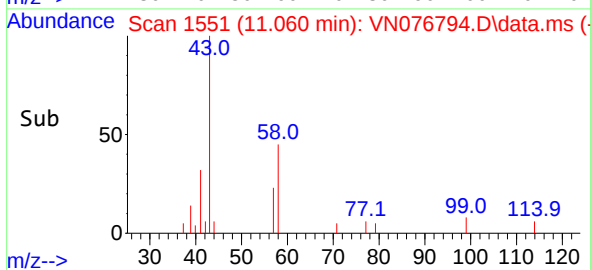

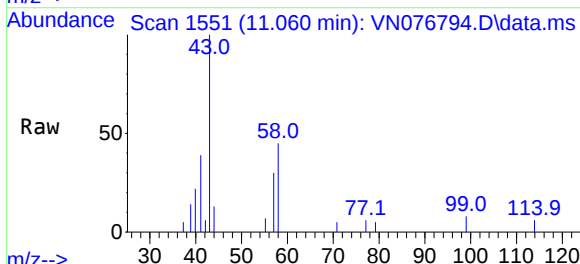


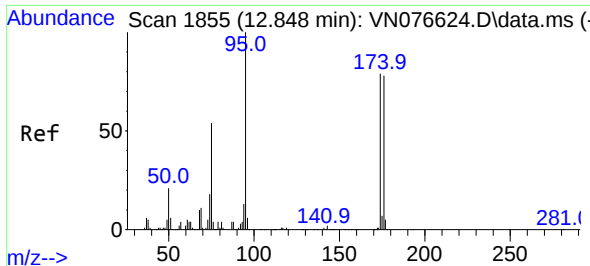

#62
4-Bromofluorobenzene
Concen: 45.711 ug/l
RT: 12.848 min Scan# 1855
Delta R.T. 0.000 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion: 95 Resp: 198932
Ion Ratio Lower Upper
95 100
174 77.5 0.0 169.2
176 73.2 0.0 163.4

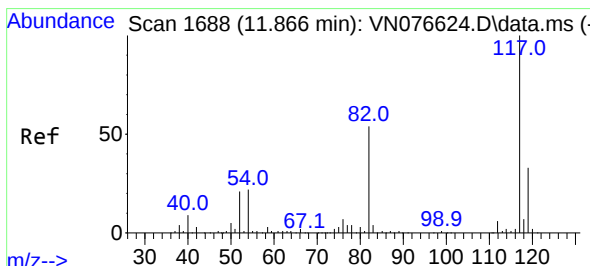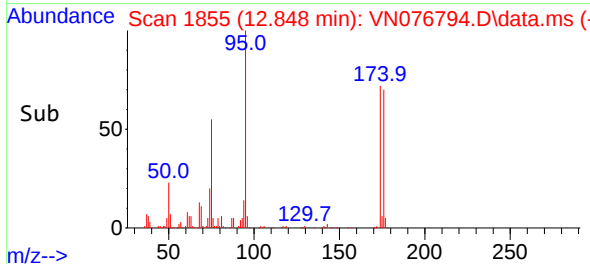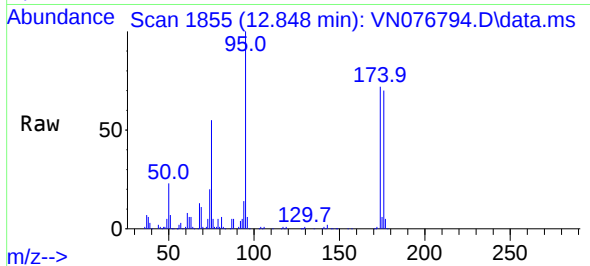

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.866 min Scan# 1688
Delta R.T. -0.000 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion: 117 Resp: 473602
Ion Ratio Lower Upper
117 100
82 57.1 43.4 65.2
119 31.3 26.1 39.1


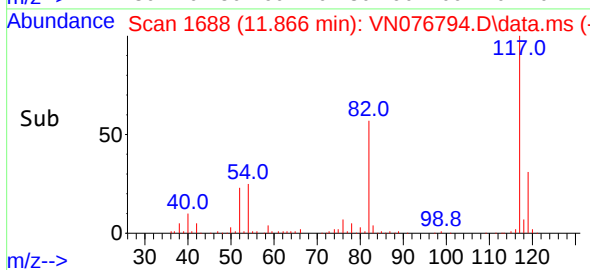

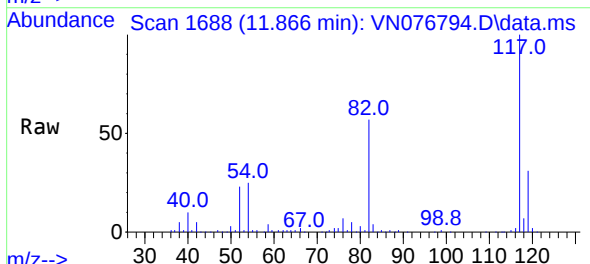


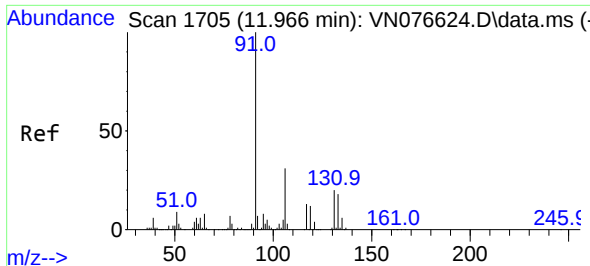

#67
Ethyl Benzene
Concen: 1.354 ug/l
RT: 11.966 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion: 91 Resp: 23152
Ion Ratio Lower Upper
91 100
106 30.0 25.1 37.7

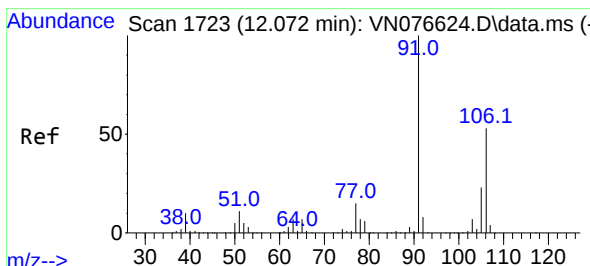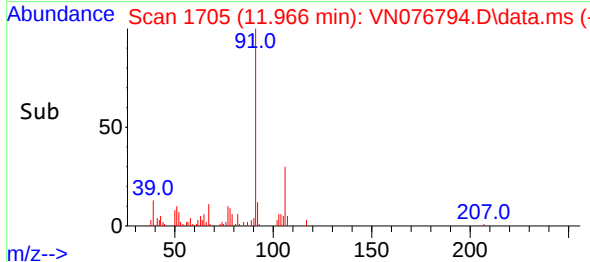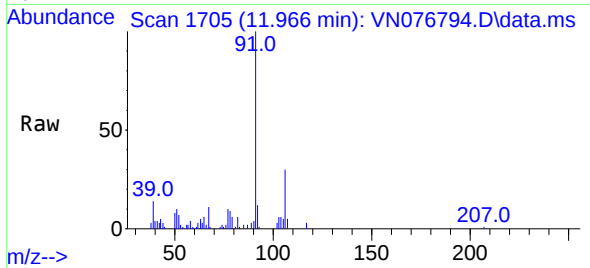

#68
m/p-Xylenes
Concen: 2.904 ug/l
RT: 12.077 min Scan# 1724
Delta R.T. 0.005 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion:106 Resp: 19140
Ion Ratio Lower Upper
106 100
91 178.8 154.7 232.1


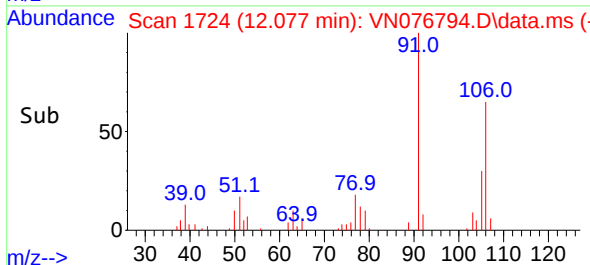
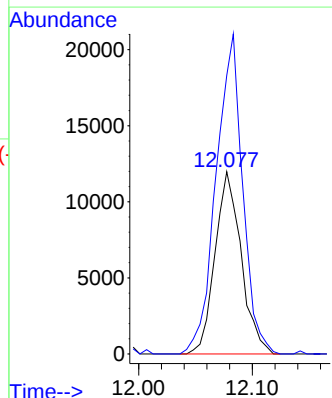
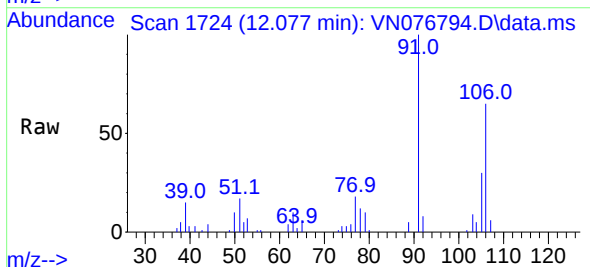




#69
o-Xylene
Concen: 1.053 ug/l
RT: 12.401 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion:106 Resp: 6768
Ion Ratio Lower Upper
106 100
91 217.7 105.8 317.4



#71
Bromoform
Concen: 0.824 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.271 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion:173 Resp: 2204
Ion Ratio Lower Upper
173 100
175 514.2 24.9 74.7#
254 0.0 0.1 0.1#


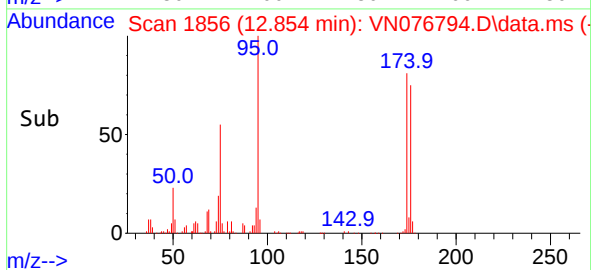






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.795 min Scan# 2016
Delta R.T. 0.000 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion:152 Resp: 195589
Ion Ratio Lower Upper
152 100
115 60.1 29.3 87.9
150 158.8 0.0 349.8

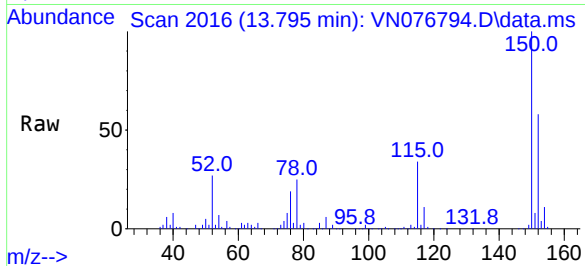

#73
Isopropylbenzene
Concen: 0.258 ug/l
RT: 12.695 min Scan# 1829
Delta R.T. 0.000 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion:105 Resp: 3699
Ion Ratio Lower Upper
105 100
120 30.8 13.7 41.0


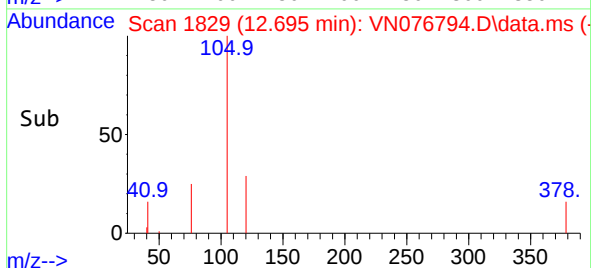
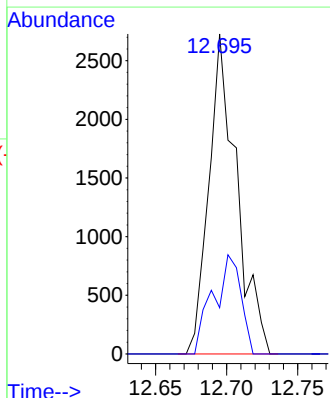
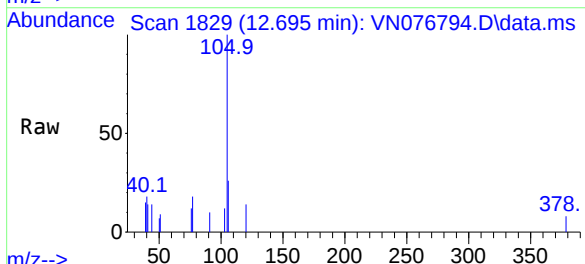


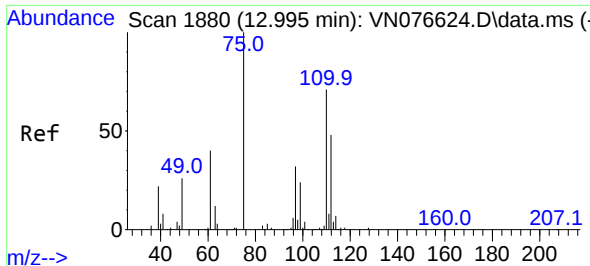

#76
1,2,3-Trichloropropane
Concen: 27.861 ug/l
RT: 12.848 min Scan# 11
Delta R.T. -0.147 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion: 75 Resp: 110171
Ion Ratio Lower Upper
75 100
77 1.0 93.1 279.3#

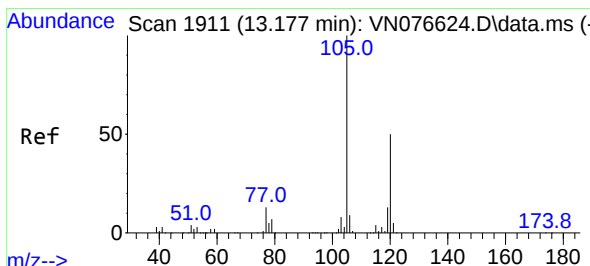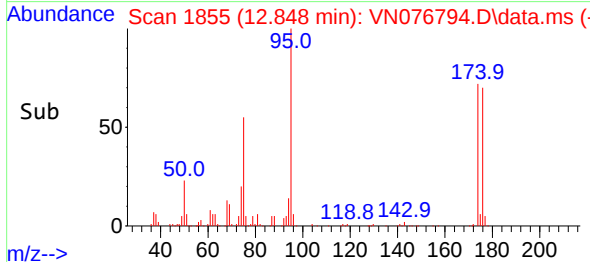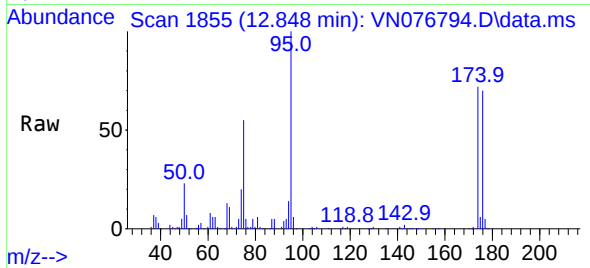

#80
1,3,5-Trimethylbenzene
Concen: 1.327 ug/l
RT: 13.136 min Scan# 1904
Delta R.T. -0.041 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion: 105 Resp: 15725
Ion Ratio Lower Upper
105 100
120 31.4 25.1 75.4


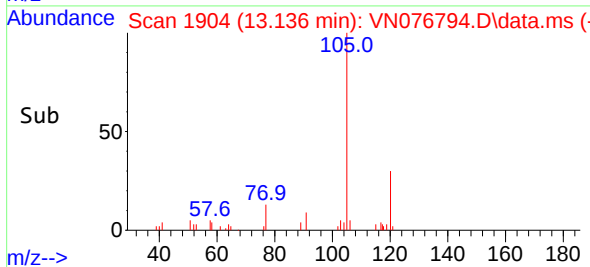

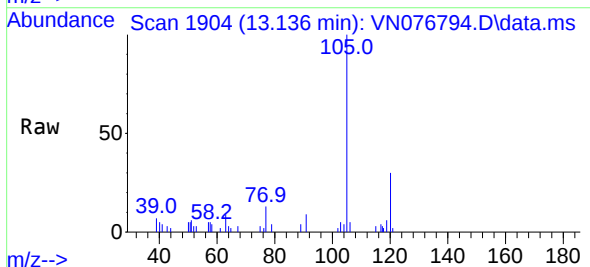




#81
trans-1,4-Dichloro-2-butene
Concen: 81.148 ug/l
RT: 12.848 min Scan# 1855
Delta R.T. 0.112 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion: 75 Resp: 110171
Ion Ratio Lower Upper
75 100
53 0.3 92.1 138.1#
89 0.0 37.5 56.3#

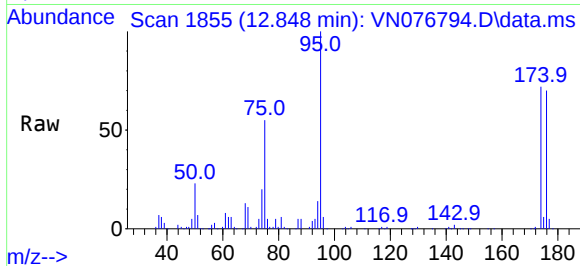

#83
tert-Butylbenzene
Concen: 0.719 ug/l
RT: 13.483 min Scan# 1963
Delta R.T. 0.041 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion: 119 Resp: 7707
Ion Ratio Lower Upper
119 100
91 104.7 32.0 96.2#
134 0.0 13.8 41.4#


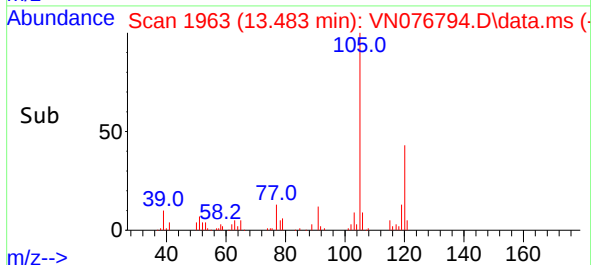
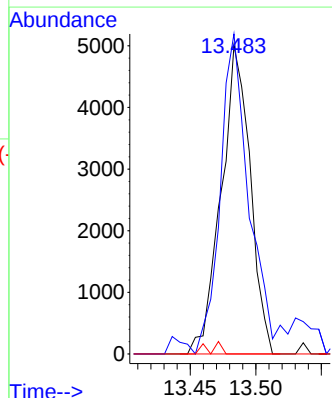
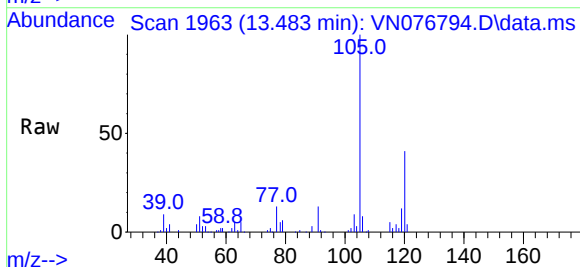




#84
1,2,4-Trimethylbenzene
Concen: 5.324 ug/l
RT: 13.483 min Scan# 1963
Delta R.T. 0.000 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37




Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL


Tgt Ion:105 Resp: 62863
Ion Ratio Lower Upper
105 100
120 43.6 23.0 69.0



#85
sec-Butylbenzene
Concen: 4.201 ug/l
RT: 13.483 min Scan# 1963
Delta R.T. -0.136 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion:105 Resp: 62863
Ion Ratio Lower Upper
105 100
134 0.0 10.5 31.5#

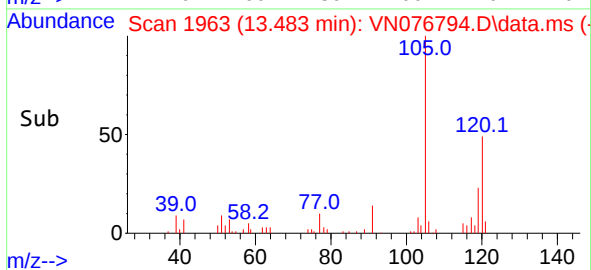







#86
p-Isopropyltoluene
Concen: 0.234 ug/l
RT: 13.736 min Scan# 2005
Delta R.T. 0.006 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL

Tgt Ion:119 Resp: 2793




Ion	Ratio	Lower	Upper
119	100		
134	26.6	13.4	40.1
91	32.3	11.7	35.0

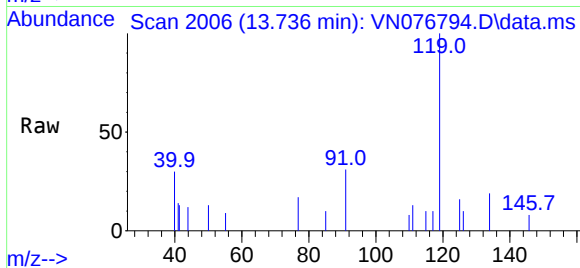


#89
n-Butylbenzene
Concen: 1.691 ug/l
RT: 13.995 min Scan# 2050
Delta R.T. -0.065 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion: 91 Resp: 17575

Ion	Ratio	Lower	Upper
91	100		
92	12.2	26.4	79.0#
134	0.0	13.2	39.5#


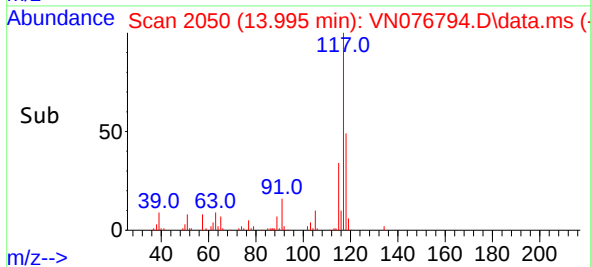

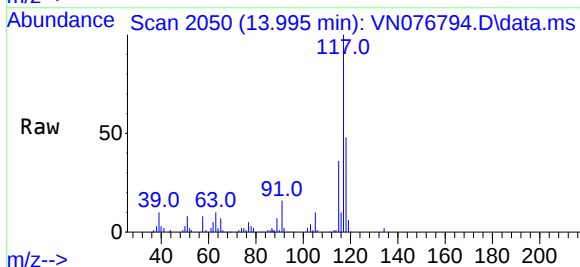




#90
Hexachloroethane
Concen: 2.991 ug/l
RT: 14.330 min Scan# 2108
Delta R.T. -0.006 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Instrument :
MSVOA_N
ClientSampleId :
MW-10-0222DL

Tgt Ion:117 Resp: 7483
Ion Ratio Lower Upper
117 100
201 0.0 35.5 106.7#

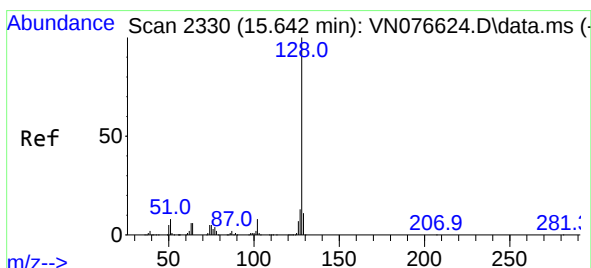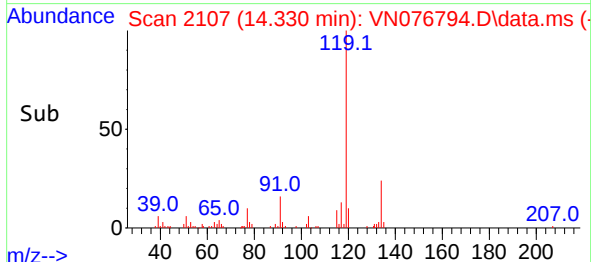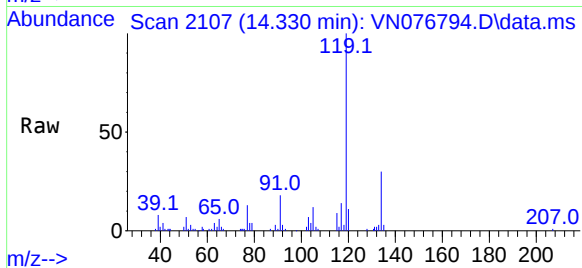

#95
Naphthalene
Concen: 0.946 ug/l
RT: 15.648 min Scan# 2331
Delta R.T. 0.006 min
Lab File: VN076794.D
Acq: 23 Feb 2023 15:37

Tgt Ion:128 Resp: 9930
Ion Ratio Lower Upper
128 100
127 13.0 10.6 16.0
129 0.0 8.6 13.0#

