
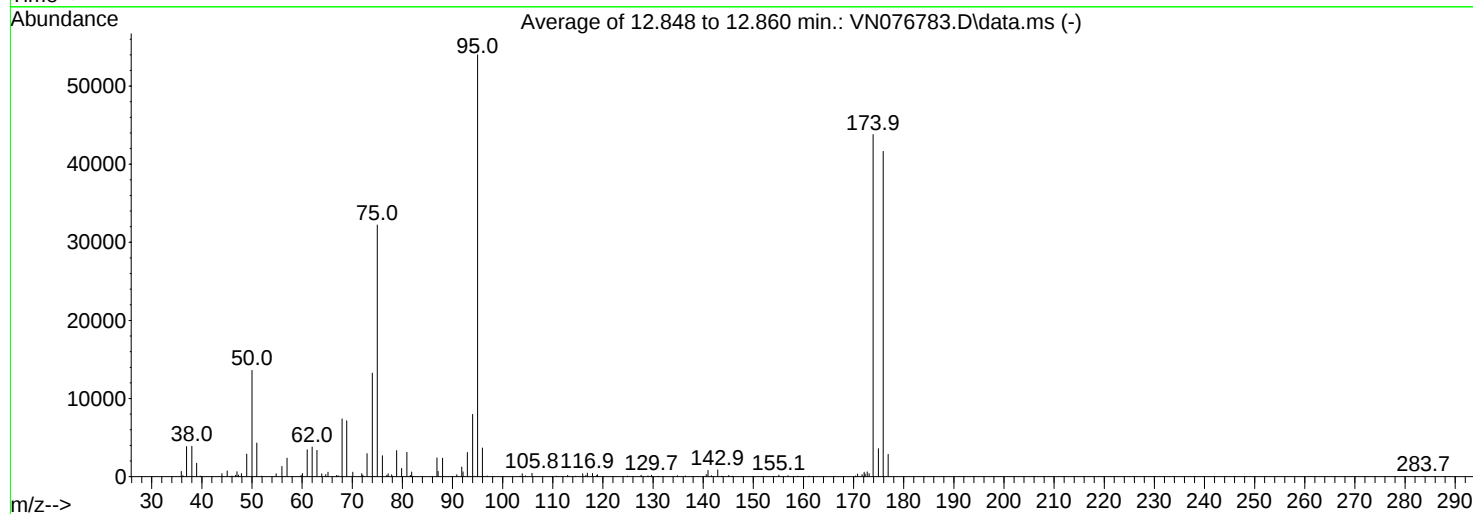


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022323\
Data File : VN076783.D
Acq On : 23 Feb 2023 09:46
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
Title : SW846 8260
Last Update : Tue Feb 14 01:44:47 2023

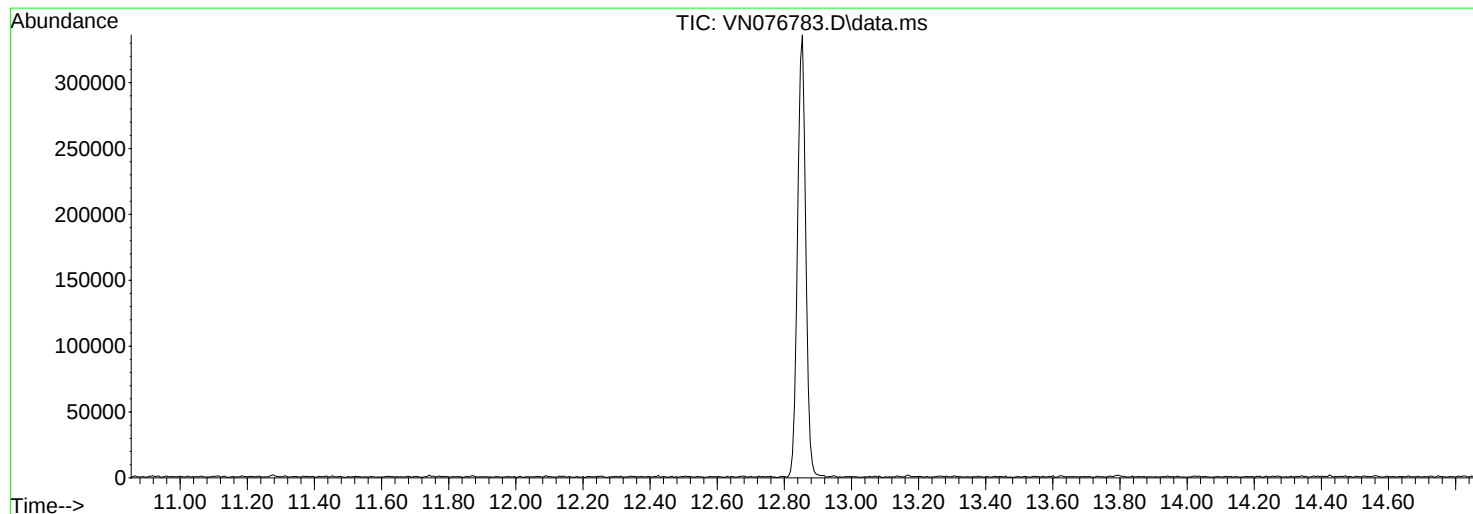

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.2	13602	PASS
75	95	30	60	59.7	32221	PASS
95	95	100	100	100.0	54000	PASS
96	95	5	9	6.8	3664	PASS
173	174	0.00	2	1.4	621	PASS
174	95	50	100	81.1	43795	PASS
175	174	5	9	8.2	3593	PASS
176	174	95	101	95.1	41640	PASS
177	176	5	9	6.9	2855	PASS

Average of 12.848 to 12.860 min.: VN076783.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	682	47.00	630	60.05	414	70.10	571
36.20	146	47.30	208	61.00	3443	71.90	381
36.95	3844	47.90	401	62.00	3795	72.10	181
38.00	3884	48.95	2889	62.95	3370	72.95	296
38.95	1712	50.00	13602	63.90	370	74.00	13263
39.65	93	50.95	4307	64.70	271	75.00	32221
44.00	392	51.90	69	65.15	571	76.00	2677
45.05	742	54.80	361	66.85	135	76.90	178
45.70	50	55.95	1319	67.15	118	77.15	372
46.00	82	57.00	2376	67.95	7395	77.85	247
46.70	160	59.80	166	68.90	7155	78.85	3332

Average of 12.848 to 12.860 min.: VN076783.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.85	1040	94.00	7971	115.95	363	134.85	127
80.90	3111	95.00	54000	116.60	150	136.50	75
81.60	162	95.95	3664	116.90	445	140.60	261
81.85	588	96.90	79	117.90	405	140.95	790
86.90	2390	103.50	72	118.70	127	141.65	116
87.10	680	103.90	377	118.90	257	142.90	870
88.00	2348	104.55	110	124.90	74	143.70	65
90.85	251	105.85	439	127.60	183	145.10	157
91.85	1236	110.80	53	129.00	107	145.80	69
92.10	619	112.95	158	129.70	186	155.10	198
92.95	3084	114.60	71	131.00	50	156.90	121

Average of 12.848 to 12.860 min.: VN076783.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
158.90	55	175.90	41640				
161.10	64	176.90	2855				
170.40	78	283.70	50				
170.80	334						
171.70	276						
172.10	582						
172.30	338						
172.70	621						
173.10	381						
173.90	43795						
174.95	3593						