

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022324\
 Data File : VN081174.D
 Acq On : 23 Feb 2024 21:21
 Operator : JC\MD
 Sample : P1574-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-4

Quant Time: Feb 23 22:06:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 16 23:45:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	269949	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	534457	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	486667	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	186954	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	179516	54.254	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 108.500%	
35) Dibromofluoromethane	8.171	113	147935	48.950	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 97.900%	
50) Toluene-d8	10.571	98	494667	46.084	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 92.160%	
62) 4-Bromofluorobenzene	12.853	95	175817	43.591	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 87.180%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.359	50	801	Below Cal		92
5) Bromomethane	2.983	94	815	0.296 ug/l	#	6
6) Chloroethane	3.130	64	188	Below Cal	#	42
11) Tert butyl alcohol	5.524	59	2258	3.711 ug/l		97
13) Acrolein	4.171	56	424	1.300 ug/l		85
16) Acetone	4.430	43	66063	50.742 ug/l		98
17) Carbon Disulfide	4.724	76	2109	0.248 ug/l	#	78
18) Methyl Acetate	5.024	43	6108	1.923 ug/l		98
20) Methylene Chloride	5.283	84	19588	4.979 ug/l		85
25) 2-Butanone	7.488	43	6535	3.107 ug/l	#	58
29) Tetrahydrofuran	7.859	42	5857	4.171 ug/l	#	61
31) Cyclohexane	8.230	56	7194	1.259 ug/l	#	1
36) 1,1-Dichloropropene	8.230	75	23063	4.454 ug/l	#	53
37) Ethyl Acetate	7.565	43	8178	1.750 ug/l	#	82
38) Carbon Tetrachloride	8.224	117	31218	5.959 ug/l	#	18
40) Benzene	8.606	78	3581	0.239 ug/l	#	80
42) 1,2-Dichloroethane	8.694	62	1774	0.339 ug/l	#	75
43) Isopropyl Acetate	8.694	43	503783	61.643 ug/l	#	79
45) 1,2-Dichloropropane	9.741	63	3208	0.856 ug/l	#	42
48) Methyl methacrylate	9.671	41	8393	2.207 ug/l	#	48
49) 1,4-Dioxane	9.718	88	53	Below Cal	#	18
51) 4-Methyl-2-Pentanone	10.447	43	23337	4.964 ug/l	#	81
52) Toluene	10.629	92	2714	0.286 ug/l		94
53) t-1,3-Dichloropropene	10.729	75	2295	0.399 ug/l	#	64
54) cis-1,3-Dichloropropene	10.359	75	95743	15.415 ug/l	#	60
57) 1,3-Dichloropropane	11.206	76	12600	1.997 ug/l	#	45
59) 2-Hexanone	11.171	43	247621	66.436 ug/l	#	26
74) N-amyl acetate	12.488	43	1812	0.262 ug/l	#	56
76) 1,2,3-Trichloropropane	12.853	75	96974	22.830 ug/l	#	1
81) trans-1,4-Dichloro-2-b...	12.853	75	96974	58.762 ug/l	#	14
95) Naphthalene	15.647	128	6750	0.497 ug/l	#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022324\
Data File : VN081174.D
Acq On : 23 Feb 2024 21:21
Operator : JC\MD
Sample : P1574-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SB-4

Quant Time: Feb 23 22:06:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 16 23:45:20 2024
Response via : Initial Calibration




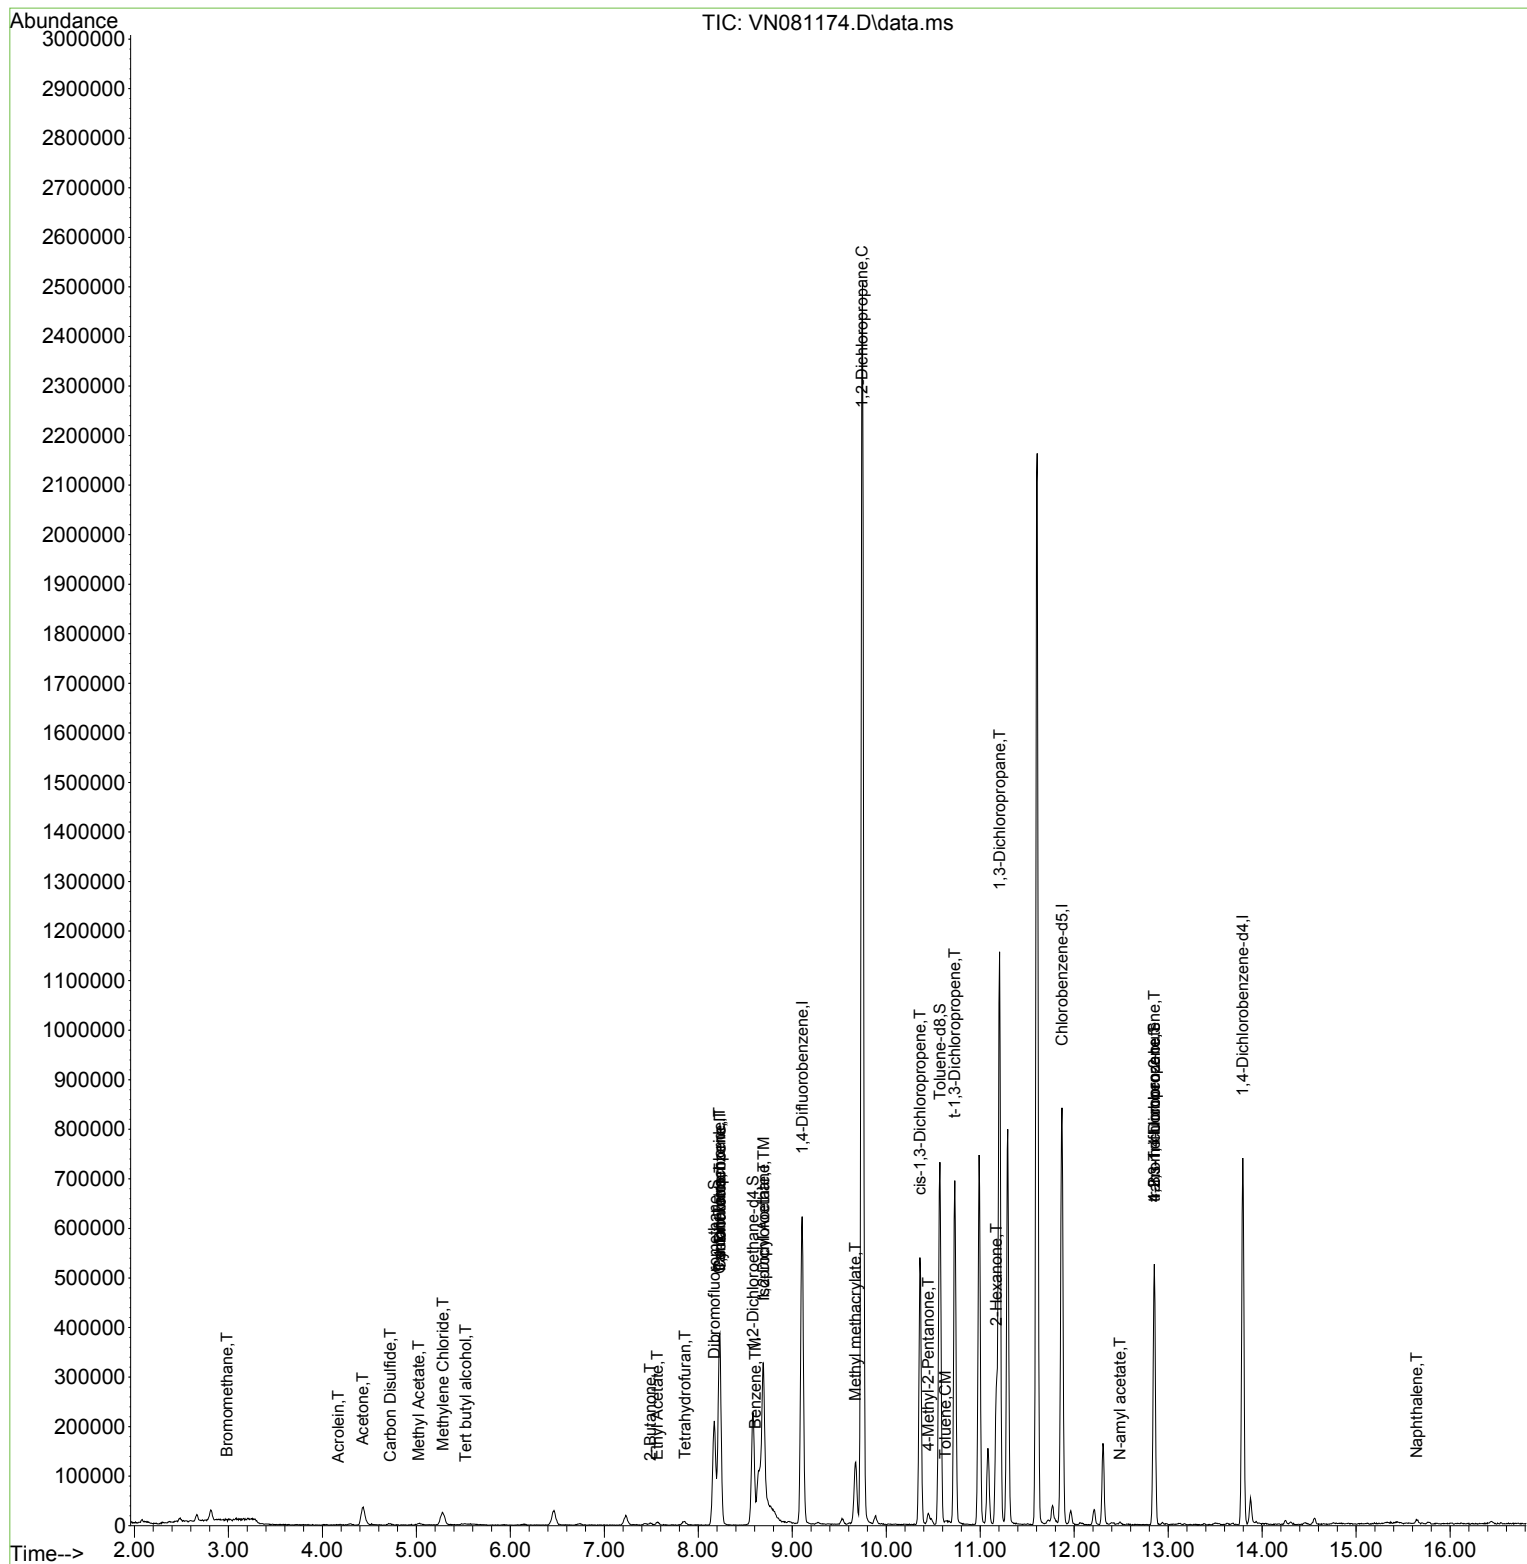




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion:168 Resp: 269949
Ion Ratio Lower Upper
168 100
99 61.5 59.9 89.9



#3
Chloromethane
Concen: Below Cal
RT: 2.359 min Scan# 69
Delta R.T. -0.006 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21

Tgt Ion: 50 Resp: 801
Ion Ratio Lower Upper
50 100
52 26.9 25.0 37.4




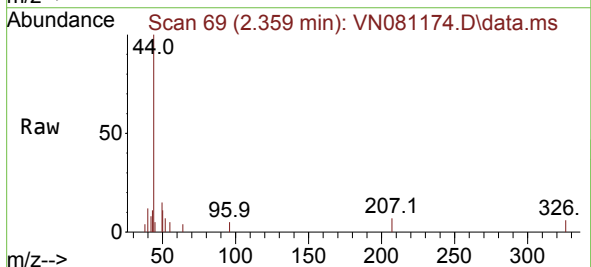




#5
Bromomethane
Concen: 0.296 ug/l
RT: 2.983 min Scan# 11
Delta R.T. 0.029 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 94 Resp: 815
Ion Ratio Lower Upper
94 100
96 0.0 69.2 103.8#



#6
Chloroethane
Concen: Below Cal
RT: 3.130 min Scan# 200
Delta R.T. 0.012 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21

Tgt Ion: 64 Resp: 188
Ion Ratio Lower Upper
64 100
66 0.0 26.4 39.6#

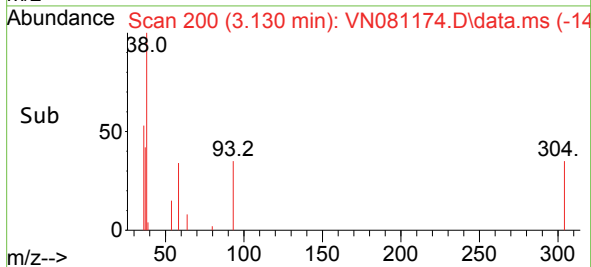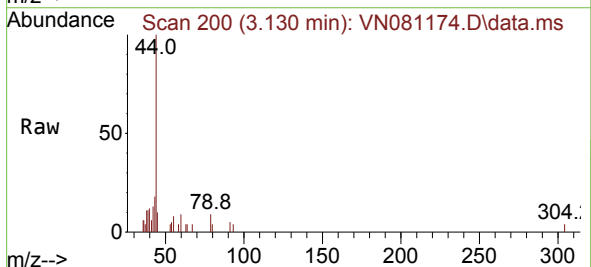



#11

Tert butyl alcohol

Concen: 3.711 ug/l

RT: 5.524 min Scan# 605

Delta R.T. 0.012 min

Lab File: VN081174.D

Acq: 23 Feb 2024 21:21

Instrument :

MSVOA_N

ClientSampleId :





SB-4

Tgt Ion: 59 Resp: 2258

Ion Ratio Lower Upper

59 100

57 9.6 8.6 12.8



#13

Acrolein

Concen: 1.300 ug/l

RT: 4.171 min Scan# 377

Delta R.T. -0.006 min

Lab File: VN081174.D




Acq: 23 Feb 2024 21:21


Tgt Ion: 56 Resp: 424

Ion Ratio Lower Upper

56 100

55 56.6 55.3 82.9









#16
Acetone
Concen: 50.742 ug/l
RT: 4.430 min Scan# 419
Delta R.T. 0.012 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 43 Resp: 66063
Ion Ratio Lower Upper
43 100
58 29.8 24.8 37.2



#17
Carbon Disulfide
Concen: 0.248 ug/l
RT: 4.724 min Scan# 471
Delta R.T. 0.012 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21

Tgt Ion: 76 Resp: 2109
Ion Ratio Lower Upper
76 100
78 0.0 6.3 9.5#









#18
Methyl Acetate
Concen: 1.923 ug/l
RT: 5.024 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 43 Resp: 6108
Ion Ratio Lower Upper
43 100
74 22.4 17.3 25.9

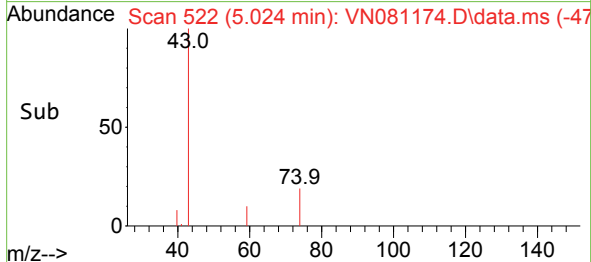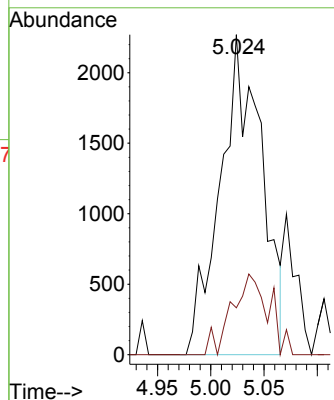

#20
Methylene Chloride
Concen: 4.979 ug/l
RT: 5.283 min Scan# 566
Delta R.T. 0.006 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21

Tgt Ion: 84 Resp: 19588
Ion Ratio Lower Upper
84 100
49 112.0 108.1 162.1
51 39.7 32.9 49.3
86 70.4 48.6 73.0


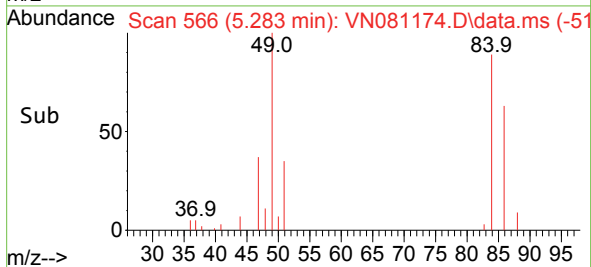
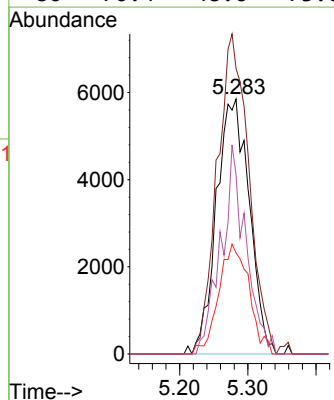
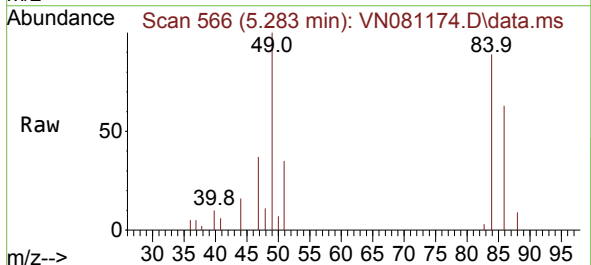




#25
2-Butanone
Concen: 3.107 ug/l
RT: 7.488 min Scan# 941
Delta R.T. 0.012 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 43 Resp: 6535
Ion Ratio Lower Upper
43 100
72 45.4 19.5 29.3#



#29
Tetrahydrofuran
Concen: 4.171 ug/l
RT: 7.859 min Scan# 1004
Delta R.T. 0.023 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21

Tgt Ion: 42 Resp: 5857
Ion Ratio Lower Upper
42 100
72 0.0 31.1 46.7#
71 42.1 28.3 42.5


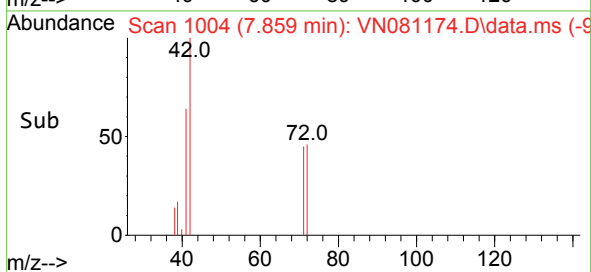

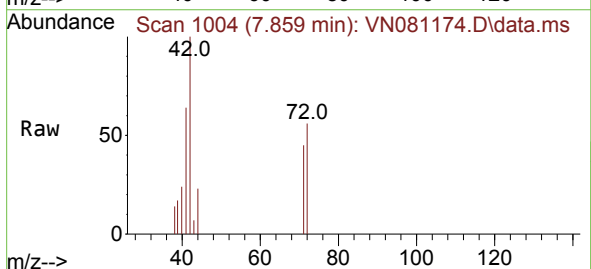




#31
Cyclohexane
Concen: 1.259 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.029 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 56 Resp: 7194
Ion Ratio Lower Upper
56 100
69 174.1 20.1 30.1#
84 104.3 56.9 85.3#

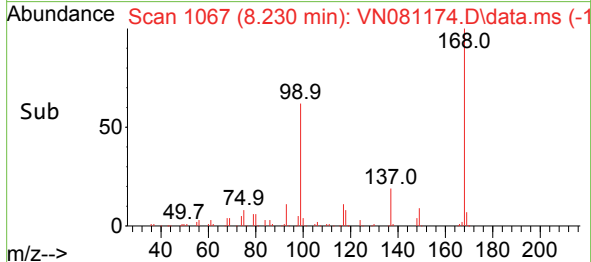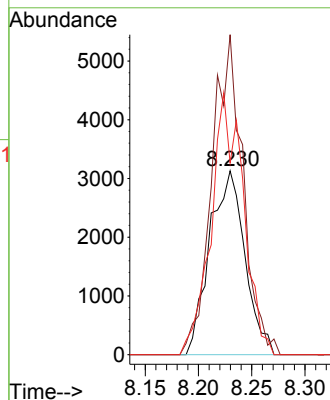

#33
1,2-Dichloroethane-d4
Concen: 54.254 ug/l
RT: 8.583 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21

Tgt Ion: 65 Resp: 179516
Ion Ratio Lower Upper
65 100
67 52.4 0.0 102.4

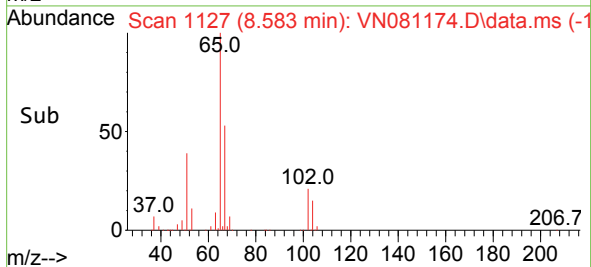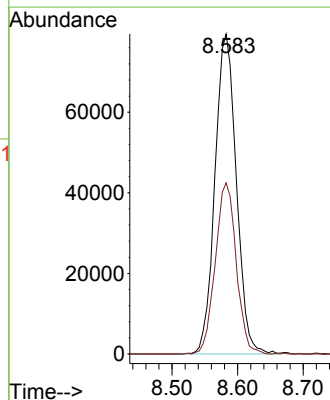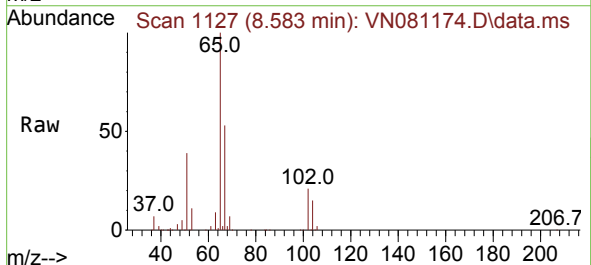



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN081174.D

Acq: 23 Feb 2024 21:21

Instrument :

MSVOA_N

ClientSampleId :

SB-4





Tgt Ion:114 Resp: 534457

Ion Ratio Lower Upper

114 100

63 20.5 0.0 48.0

88 16.6 0.0 34.8

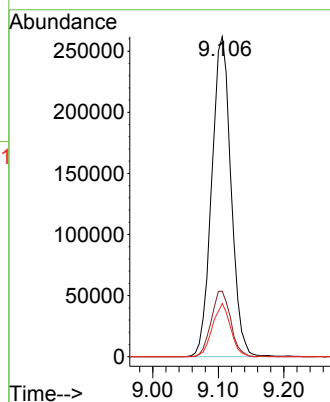

#35

Dibromofluoromethane

Concen: 48.950 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VN081174.D

Acq: 23 Feb 2024 21:21




Tgt Ion:113 Resp: 147935


Ion Ratio Lower Upper

113 100

111 104.2 82.2 123.4

192 15.2 12.5 18.7

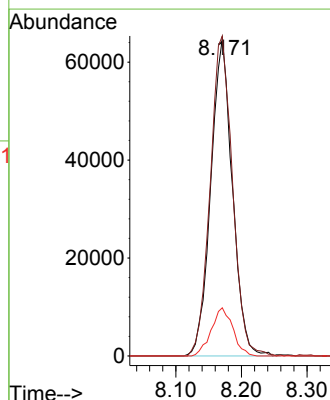



#36

1,1-Dichloropropene

Concen: 4.454 ug/l

RT: 8.230 min Scan# 1

Delta R.T. -0.141 min

Lab File: VN081174.D

Acq: 23 Feb 2024 21:21

Instrument :

MSVOA_N

ClientSampleId :

SB-4





Tgt Ion: 75 Resp: 23063

Ion Ratio Lower Upper

75 100

110 11.7 16.0 48.0#

77 0.3 25.8 38.6#



#37

Ethyl Acetate

Concen: 1.750 ug/l

RT: 7.565 min Scan# 954

Delta R.T. 0.006 min

Lab File: VN081174.D

Acq: 23 Feb 2024 21:21




Tgt Ion: 43 Resp: 8178


Ion Ratio Lower Upper

43 100

61 8.5 10.6 15.8#

70 0.0 8.0 12.0#

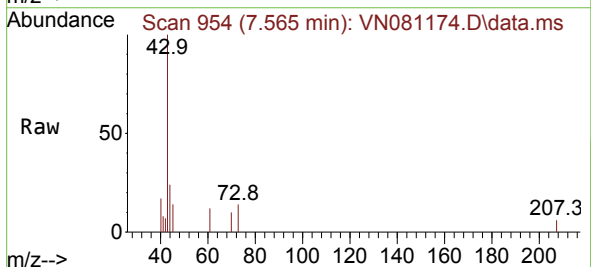



#38

Carbon Tetrachloride

Concen: 5.959 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.135 min

Lab File: VN081174.D

Acq: 23 Feb 2024 21:21

Instrument :

MSVOA_N

ClientSampleId :

SB-4





Tgt Ion:117 Resp: 31218

Ion Ratio Lower Upper

117 100

119 5.0 73.4 110.2#

121 0.0 24.4 36.6#

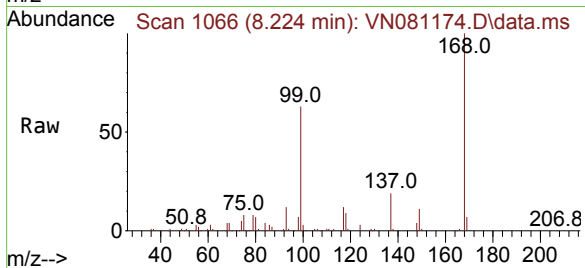

#40

Benzene

Concen: 0.239 ug/l

RT: 8.606 min Scan# 1131

Delta R.T. -0.000 min

Lab File: VN081174.D




Acq: 23 Feb 2024 21:21


Tgt Ion: 78 Resp: 3581

Ion Ratio Lower Upper

78 100

77 15.6 20.4 30.6#

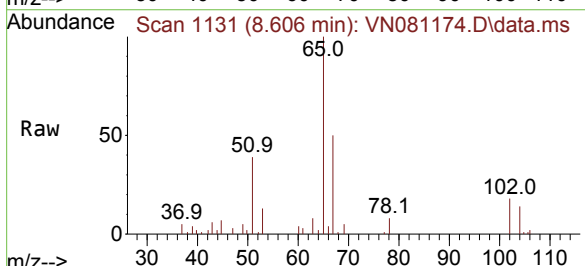



#42

1,2-Dichloroethane

Concen: 0.339 ug/l

RT: 8.694 min Scan# 1146

Delta R.T. 0.023 min

Lab File: VN081174.D

Acq: 23 Feb 2024 21:21

Instrument :

MSVOA_N

ClientSampleId :





SB-4

Tgt Ion: 62 Resp: 1774

Ion Ratio Lower Upper

62 100

98 0.0 0.0 18.0

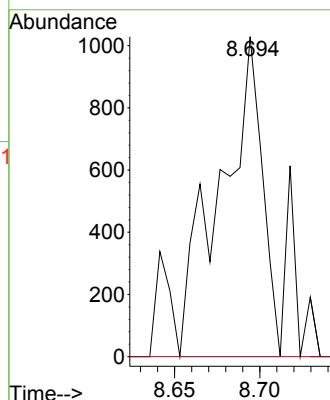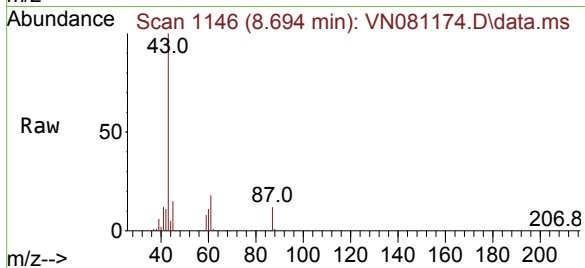

#43

Isopropyl Acetate

Concen: 61.643 ug/l

RT: 8.694 min Scan# 1146

Delta R.T. 0.006 min

Lab File: VN081174.D

Acq: 23 Feb 2024 21:21




Tgt Ion: 43 Resp: 503783


Ion Ratio Lower Upper

43 100

61 11.7 19.9 29.9#

87 8.2 9.0 13.6#


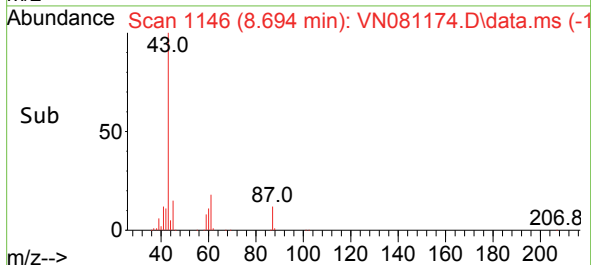
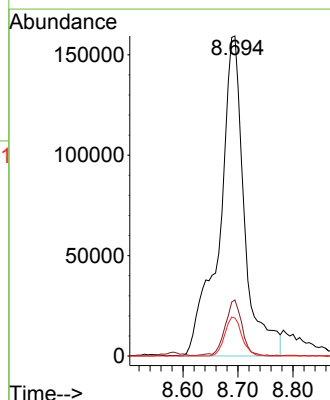
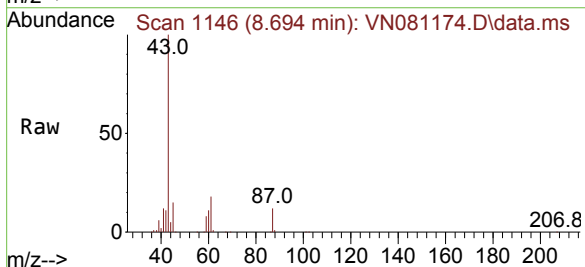




#45
1,2-Dichloropropane
Concen: 0.856 ug/l
RT: 9.741 min Scan# 11
Delta R.T. 0.118 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 63 Resp: 3208
Ion Ratio Lower Upper
63 100
65 0.0 26.1 39.1#

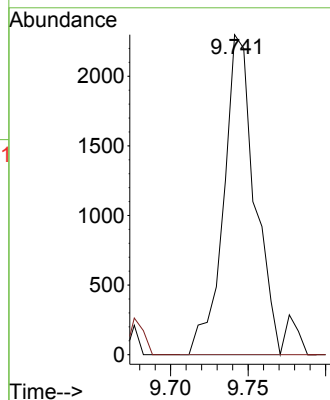

#48
Methyl methacrylate
Concen: 2.207 ug/l
RT: 9.671 min Scan# 1312
Delta R.T. -0.012 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21

Tgt Ion: 41 Resp: 8393
Ion Ratio Lower Upper
41 100
69 0.0 62.2 93.2#
39 61.5 47.6 71.4

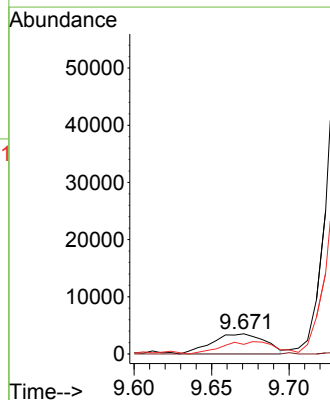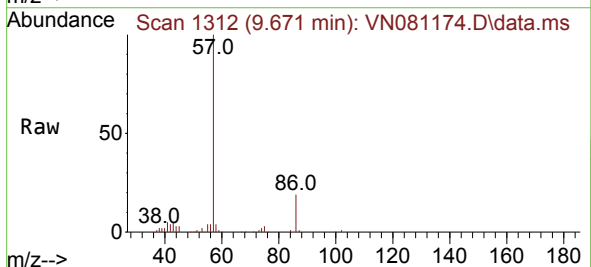



#49

1,4-Dioxane

Concen: Below Cal

RT: 9.718 min Scan# 11

Delta R.T. 0.024 min

Lab File: VN081174.D

Acq: 23 Feb 2024 21:21

Instrument :

MSVOA_N

ClientSampleId :

SB-4





Tgt Ion: 88 Resp: 53

Ion Ratio Lower Upper

88 100

43 0.0 30.1 45.1#

58 0.0 63.9 95.9#



#50

Toluene-d8

Concen: 46.084 ug/l

RT: 10.571 min Scan# 1465

Delta R.T. 0.006 min

Lab File: VN081174.D




Acq: 23 Feb 2024 21:21


Tgt Ion: 98 Resp: 494667

Ion Ratio Lower Upper

98 100

100 65.0 51.4 77.0


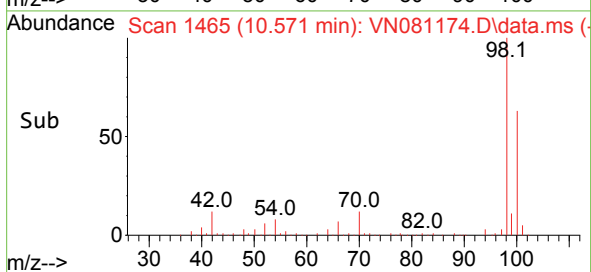




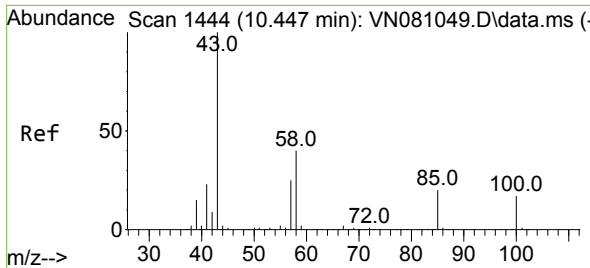

#51
4-Methyl-2-Pentanone
Concen: 4.964 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. -0.000 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 43 Resp: 23337
Ion Ratio Lower Upper
43 100
58 25.3 29.4 44.0#

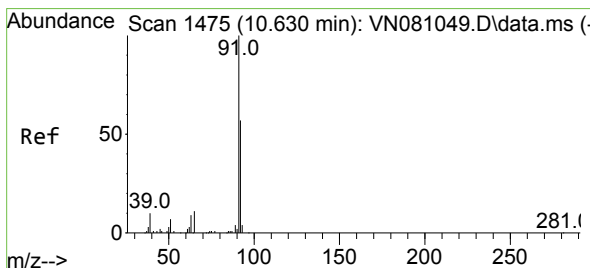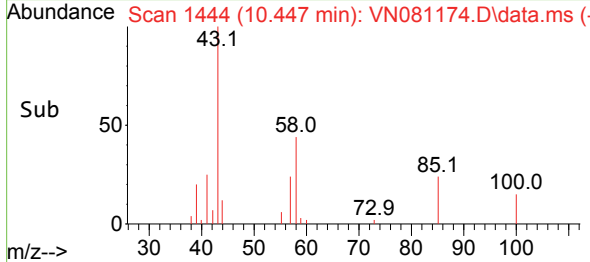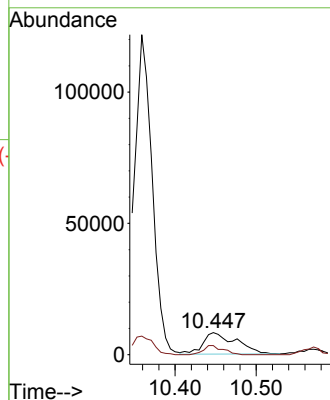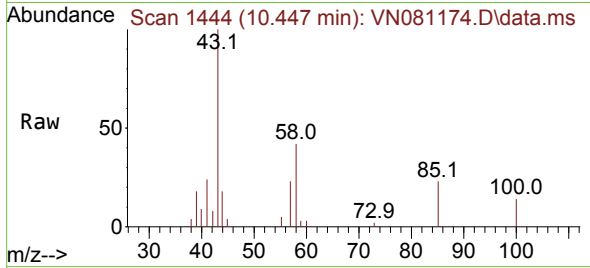

#52
Toluene
Concen: 0.286 ug/l
RT: 10.629 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21

Tgt Ion: 92 Resp: 2714
Ion Ratio Lower Upper
92 100
91 182.5 139.4 209.0


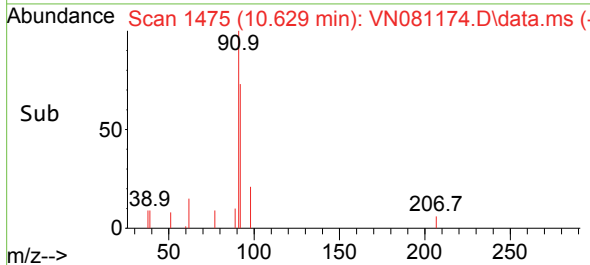
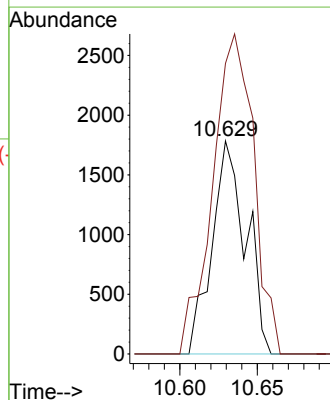
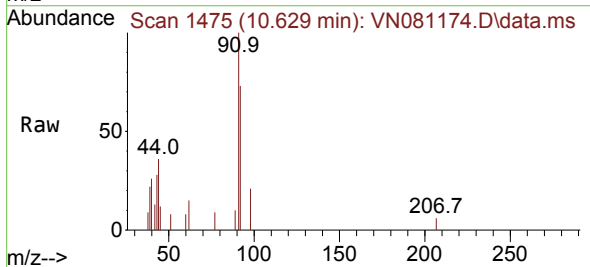




#53
t-1,3-Dichloropropene
Concen: 0.399 ug/l
RT: 10.729 min Scan# 1492
Delta R.T. -0.106 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 75 Resp: 2295
Ion Ratio Lower Upper
75 100
77 11.6 25.5 38.3#



#54
cis-1,3-Dichloropropene
Concen: 15.415 ug/l
RT: 10.359 min Scan# 1429
Delta R.T. 0.047 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21

Tgt Ion: 75 Resp: 95743
Ion Ratio Lower Upper
75 100
77 0.0 23.3 34.9#
39 32.2 44.6 66.8#




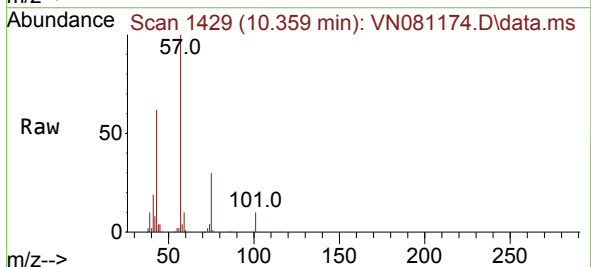


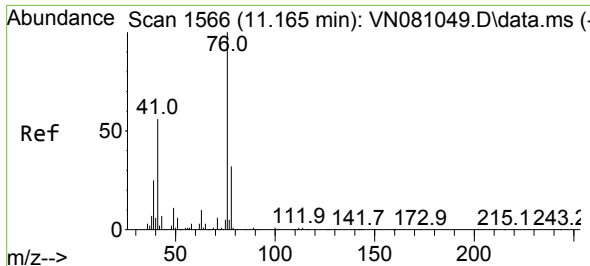

#57
1,3-Dichloropropane
Concen: 1.997 ug/l
RT: 11.206 min Scan# 1573
Delta R.T. 0.041 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 76 Resp: 12600
Ion Ratio Lower Upper
76 100
78 1.1 25.5 38.3#

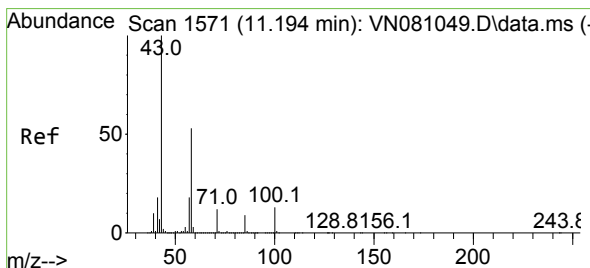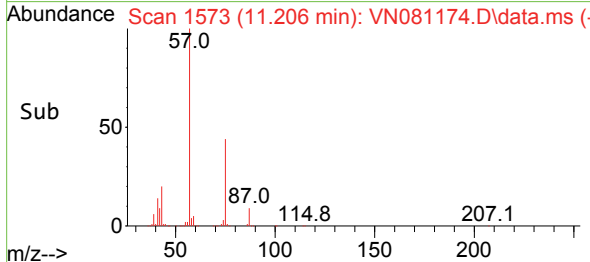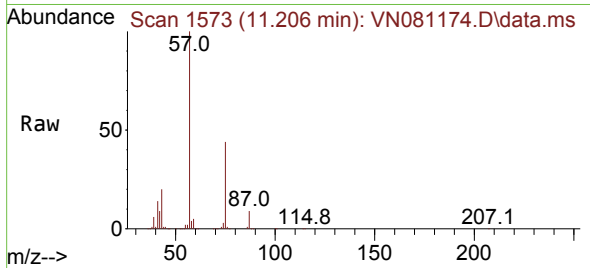

#59
2-Hexanone
Concen: 66.436 ug/l
RT: 11.171 min Scan# 1567
Delta R.T. -0.024 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21

Tgt Ion: 43 Resp: 247621
Ion Ratio Lower Upper
43 100
58 0.0 25.9 77.8#


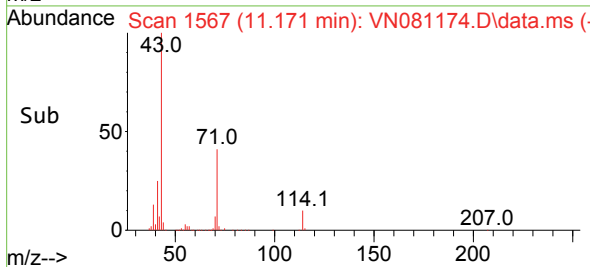

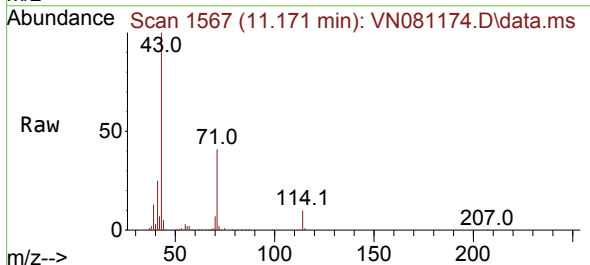


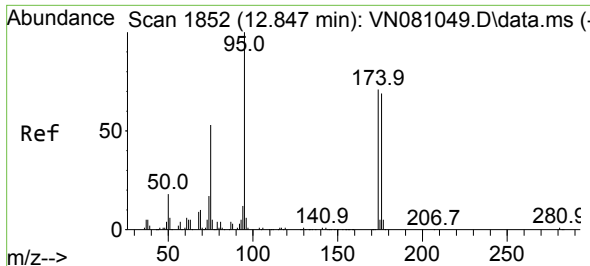

#62
4-Bromofluorobenzene
Concen: 43.591 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 95	Resp: 175817
Ion Ratio	Lower Upper
95 100	
174 74.6	0.0 120.4
176 69.8	0.0 121.0

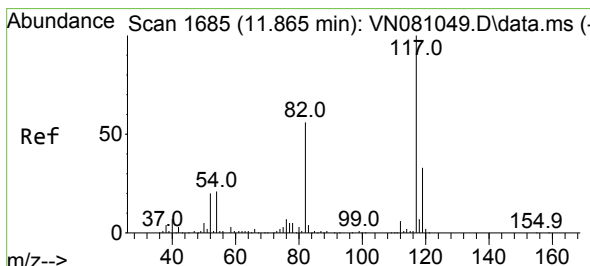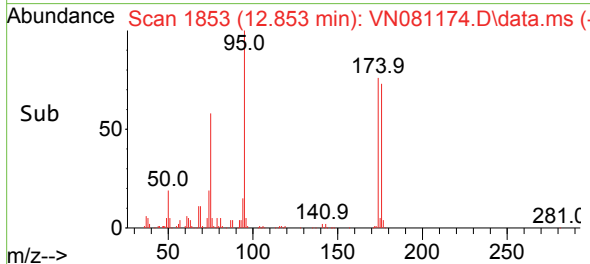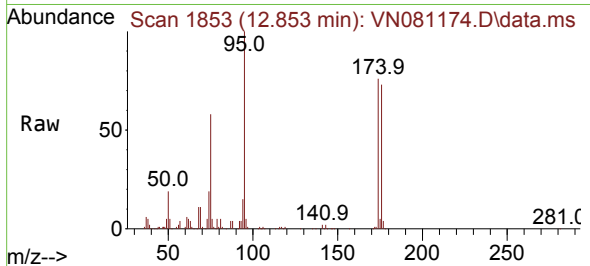

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. 0.006 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21

Tgt Ion: 117	Resp: 486667
Ion Ratio	Lower Upper
117 100	
82 55.4	52.7 79.1
119 31.9	25.3 37.9


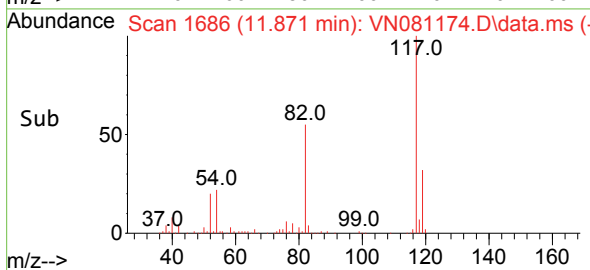

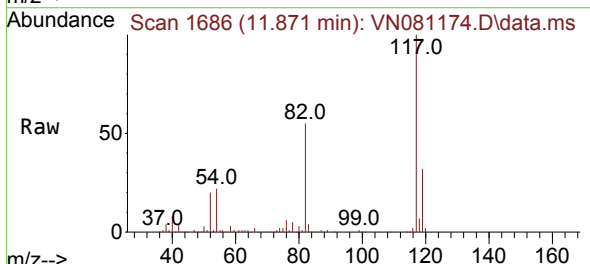




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion:152 Resp: 186954
Ion Ratio Lower Upper
152 100
115 65.2 32.3 96.8
150 163.8 0.0 339.8



#74
N-ethyl acetate
Concen: 0.262 ug/l
RT: 12.488 min Scan# 1791
Delta R.T. -0.006 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21

Tgt Ion: 43 Resp: 1812
Ion Ratio Lower Upper
43 100
70 0.0 30.1 45.1#
55 16.4 17.0 25.4#
61 0.0 17.5 26.3#




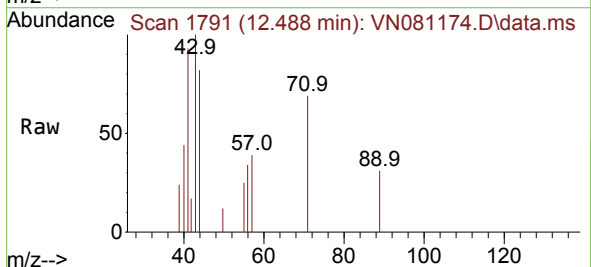


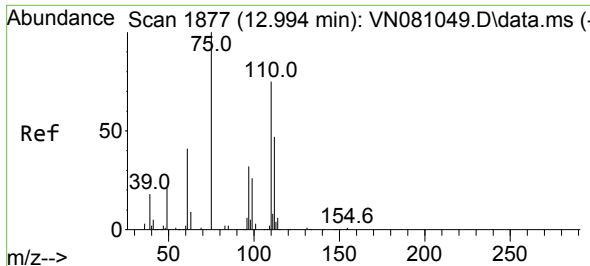

#76
1,2,3-Trichloropropane
Concen: 22.830 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.141 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 75 Resp: 96974
Ion Ratio Lower Upper
75 100
77 1.8 91.0 272.8#

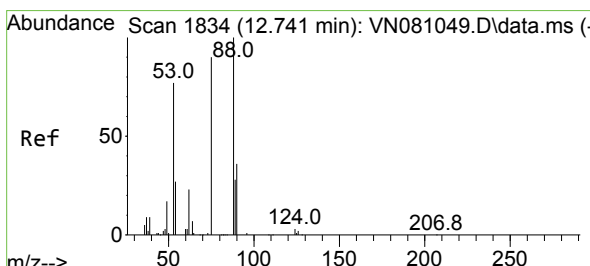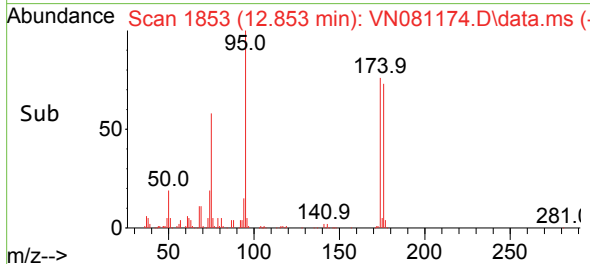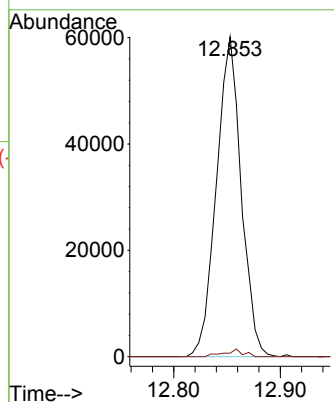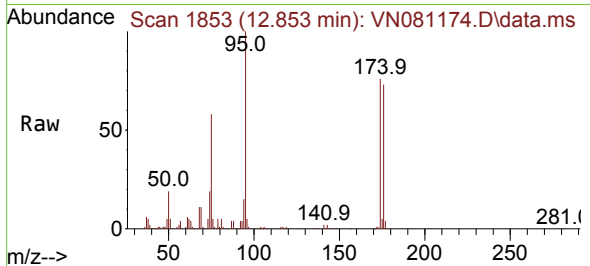

#81
trans-1,4-Dichloro-2-butene
Concen: 58.762 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.112 min
Lab File: VN081174.D
Acq: 23 Feb 2024 21:21

Tgt Ion: 75 Resp: 96974
Ion Ratio Lower Upper
75 100
53 0.0 71.4 107.2#
89 0.0 33.4 50.0#

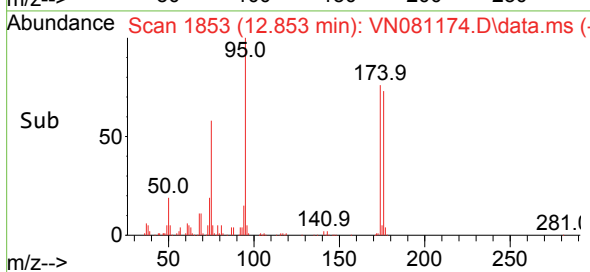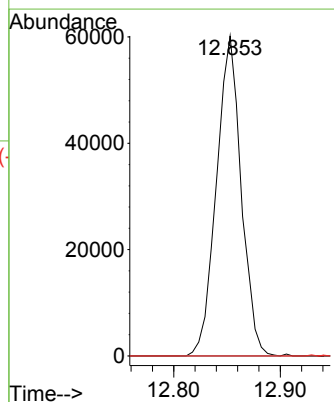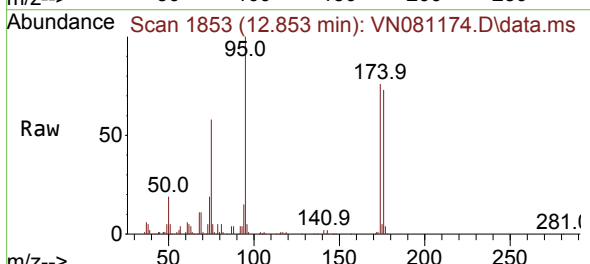



#95
 Naphthalene
 Concen: 0.497 ug/l
 RT: 15.647 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VN081174.D
 Acq: 23 Feb 2024 21:21

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-4

Tgt Ion:128 Resp: 6750
 Ion Ratio Lower Upper
 128 100
 127 13.1 10.0 15.0
 129 13.4 8.7 13.1#

