

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022324\
 Data File : VN081176.D
 Acq On : 23 Feb 2024 22:09
 Operator : JC\MD
 Sample : P1574-06
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-6

Quant Time: Feb 24 01:11:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 16 23:45:20 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	279141	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	546519	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	496145	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	195836	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	175140	51.188	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	102.380%
35) Dibromofluoromethane	8.171	113	149351	48.327	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.660%
50) Toluene-d8	10.571	98	486881	44.358	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	88.720%
62) 4-Bromofluorobenzene	12.853	95	177564	43.052	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	86.100%
Target Compounds						
					Qvalue	
3) Chloromethane	2.359	50	802	Below Cal	#	43
5) Bromomethane	2.977	94	644	0.226	ug/l	88
6) Chloroethane	3.124	64	379	Below Cal	#	42
11) Tert butyl alcohol	5.518	59	2313	3.676	ug/l	# 72
13) Acrolein	4.183	56	968	2.870	ug/l	97
16) Acetone	4.430	43	69293	51.470	ug/l	95
17) Carbon Disulfide	4.724	76	2220	0.252	ug/l	# 78
18) Methyl Acetate	5.030	43	7099	2.162	ug/l	# 82
20) Methylene Chloride	5.283	84	19785	4.841	ug/l	# 82
25) 2-Butanone	7.500	43	6068	2.790	ug/l	# 87
29) Tetrahydrofuran	7.847	42	5567	3.834	ug/l	96
31) Cyclohexane	8.230	56	7706	1.304	ug/l	# 1
36) 1,1-Dichloropropene	8.224	75	25077	4.736	ug/l	# 51
37) Ethyl Acetate	7.559	43	8803	1.842	ug/l	96
38) Carbon Tetrachloride	8.224	117	31133	5.812	ug/l	# 17
40) Benzene	8.612	78	5279	0.344	ug/l	# 86
41) Methacrylonitrile	7.847	41	2891	1.063	ug/l	# 49
42) 1,2-Dichloroethane	8.682	62	2303	0.431	ug/l	# 75
43) Isopropyl Acetate	8.688	43	572637	68.522	ug/l	# 77
48) Methyl methacrylate	9.665	41	8573	2.205	ug/l	# 51
49) 1,4-Dioxane	9.694	88	101	Below Cal	#	1
51) 4-Methyl-2-Pentanone	10.447	43	23842	4.959	ug/l	# 77
52) Toluene	10.635	92	3061	0.316	ug/l	76
53) t-1,3-Dichloropropene	10.724	75	2053	0.349	ug/l	# 82
54) cis-1,3-Dichloropropene	10.359	75	99978	15.741	ug/l	# 61
57) 1,3-Dichloropropane	11.200	76	12327	1.911	ug/l	# 43
59) 2-Hexanone	11.171	43	209550	54.981	ug/l	# 26
74) N-amyl acetate	12.494	43	2435	0.336	ug/l	# 50
76) 1,2,3-Trichloropropane	12.853	75	96272	21.636	ug/l	# 1
81) trans-1,4-Dichloro-2-b...	12.853	75	96272	55.691	ug/l	# 14


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022324\
Data File : VN081176.D
Acq On : 23 Feb 2024 22:09
Operator : JC\MD
Sample : P1574-06
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SB-6

Quant Time: Feb 24 01:11:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 16 23:45:20 2024
Response via : Initial Calibration

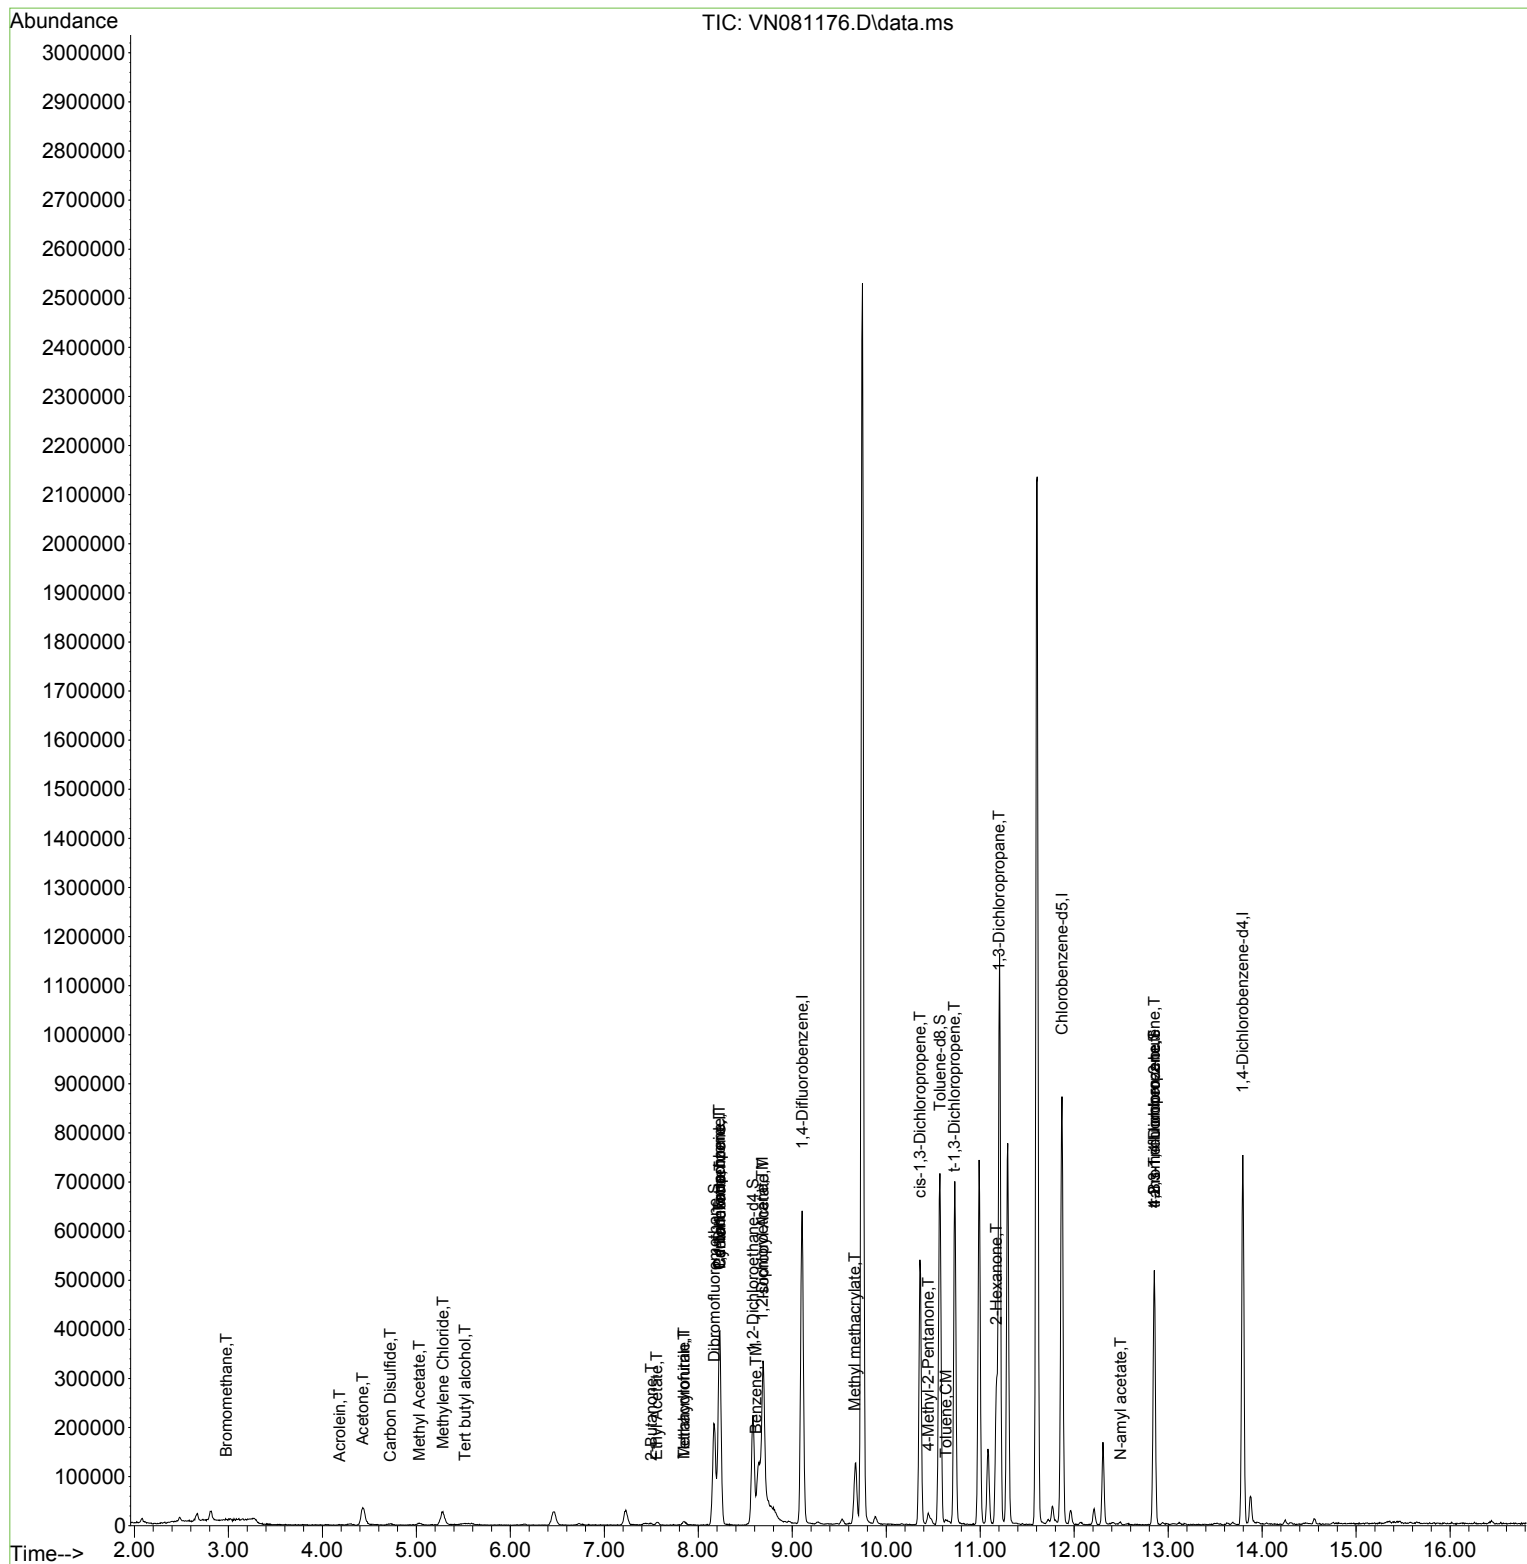



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.230 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN081176.D

Acq: 23 Feb 2024 22:09

Instrument :

MSVOA_N

ClientSampleId :





SB-6

Tgt Ion:168 Resp: 279141

Ion Ratio Lower Upper

168 100

99 66.5 59.9 89.9

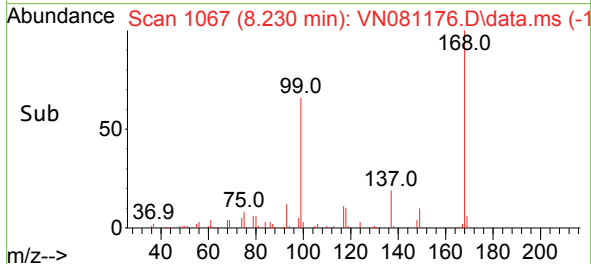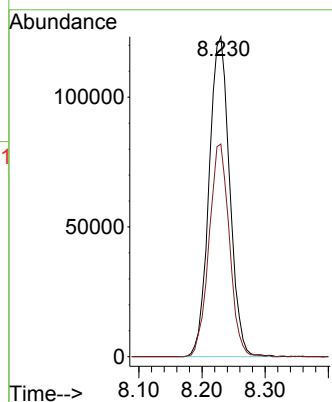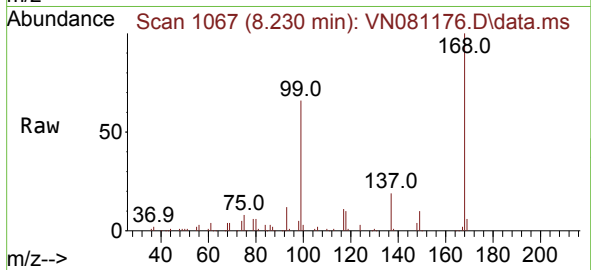

#3

Chloromethane

Concen: Below Cal

RT: 2.359 min Scan# 69

Delta R.T. -0.006 min

Lab File: VN081176.D




Acq: 23 Feb 2024 22:09


Tgt Ion: 50 Resp: 802

Ion Ratio Lower Upper

50 100

52 0.0 25.0 37.4#

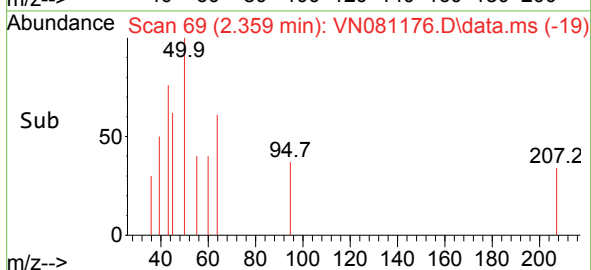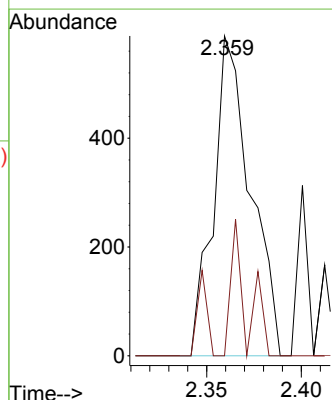



#5

Bromomethane

Concen: 0.226 ug/l

RT: 2.977 min Scan# 11

Delta R.T. 0.023 min

Lab File: VN081176.D

Acq: 23 Feb 2024 22:09

Instrument :

MSVOA_N

ClientSampleId :





SB-6

Tgt Ion: 94 Resp: 644

Ion Ratio Lower Upper

94 100

96 97.6 69.2 103.8

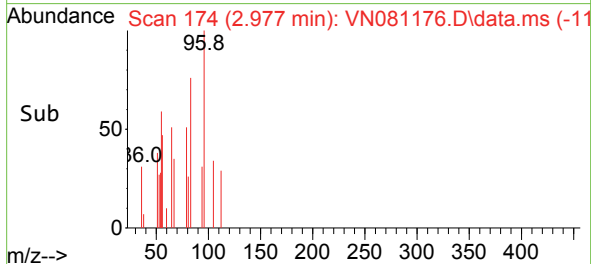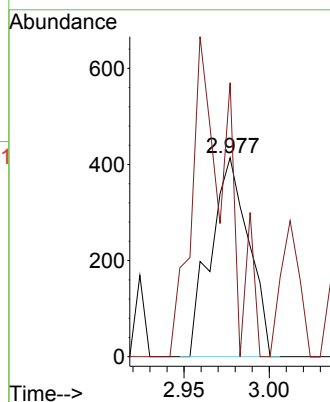

#6

Chloroethane

Concen: Below Cal

RT: 3.124 min Scan# 199

Delta R.T. 0.006 min

Lab File: VN081176.D




Acq: 23 Feb 2024 22:09


Tgt Ion: 64 Resp: 379

Ion Ratio Lower Upper

64 100

66 0.0 26.4 39.6#


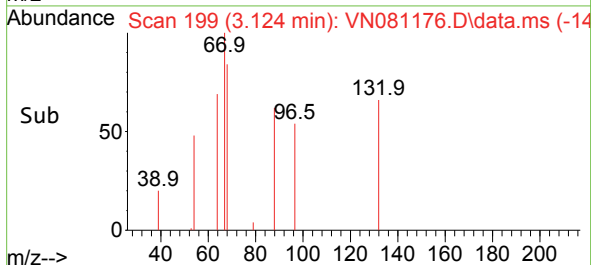

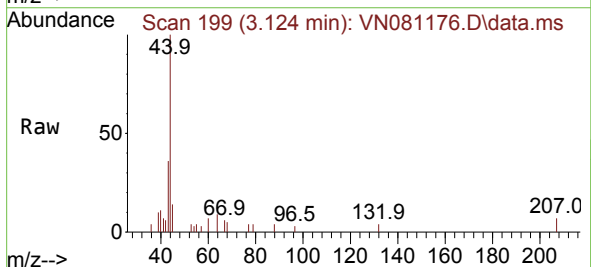




#11
Tert butyl alcohol
Concen: 3.676 ug/l
RT: 5.518 min Scan# 605
Delta R.T. 0.006 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09




Instrument :
MSVOA_N
ClientSampleId :
SB-6


Tgt Ion: 59 Resp: 2313
Ion Ratio Lower Upper
59 100
57 0.0 8.6 12.8#

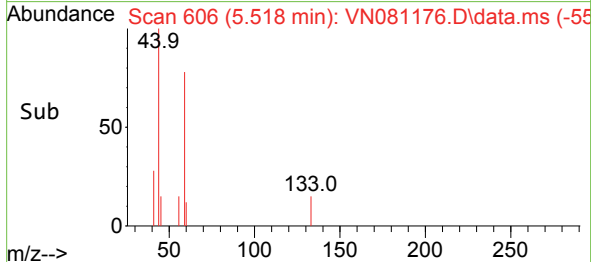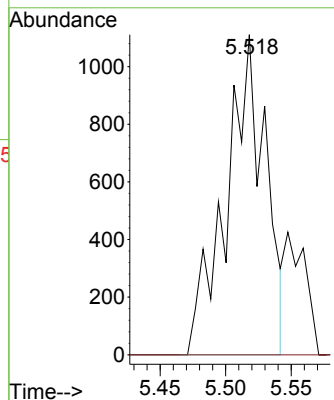

#13
Acrolein
Concen: 2.870 ug/l
RT: 4.183 min Scan# 379
Delta R.T. 0.006 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09

Tgt Ion: 56 Resp: 968
Ion Ratio Lower Upper
56 100
55 71.3 55.3 82.9


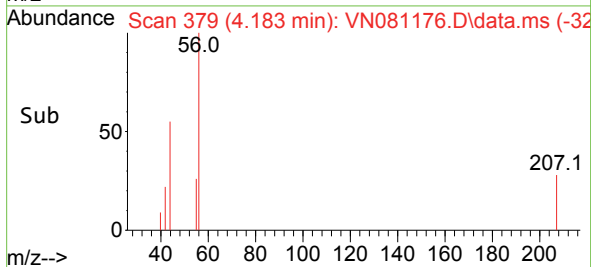
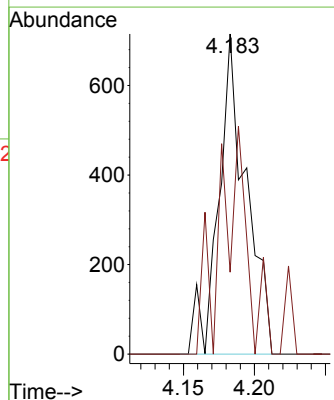
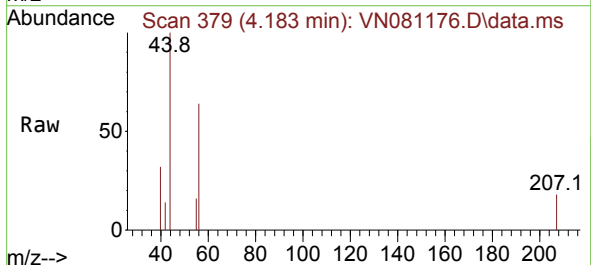




#16
Acetone
Concen: 51.470 ug/l
RT: 4.430 min Scan# 419
Delta R.T. 0.012 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09




Instrument :
MSVOA_N
ClientSampleId :
SB-6


Tgt Ion: 43 Resp: 69293
Ion Ratio Lower Upper
43 100
58 33.5 24.8 37.2

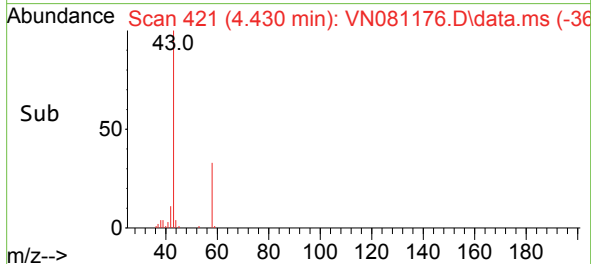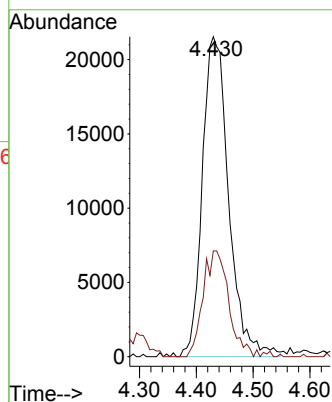

#17
Carbon Disulfide
Concen: 0.252 ug/l
RT: 4.724 min Scan# 471
Delta R.T. 0.012 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09

Tgt Ion: 76 Resp: 2220
Ion Ratio Lower Upper
76 100
78 0.0 6.3 9.5#


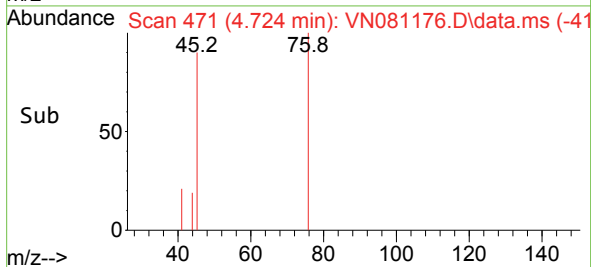
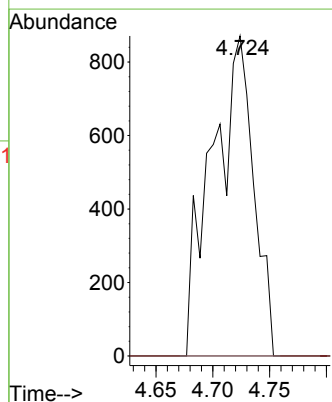
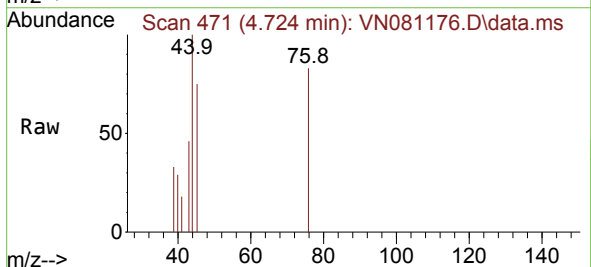




#18
Methyl Acetate
Concen: 2.162 ug/l
RT: 5.030 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09




Instrument :
MSVOA_N
ClientSampleId :
SB-6


Tgt Ion: 43 Resp: 7099
Ion Ratio Lower Upper
43 100
74 13.0 17.3 25.9#

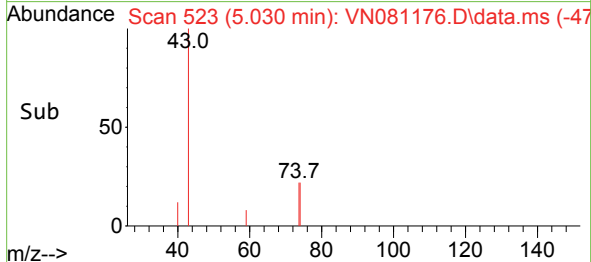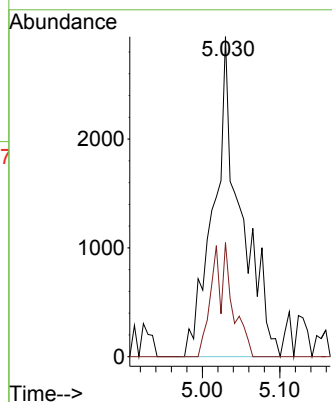

#20
Methylene Chloride
Concen: 4.841 ug/l
RT: 5.283 min Scan# 566
Delta R.T. 0.006 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09

Tgt Ion: 84 Resp: 19785
Ion Ratio Lower Upper
84 100
49 106.7 108.1 162.1#
51 29.4 32.9 49.3#
86 64.2 48.6 73.0

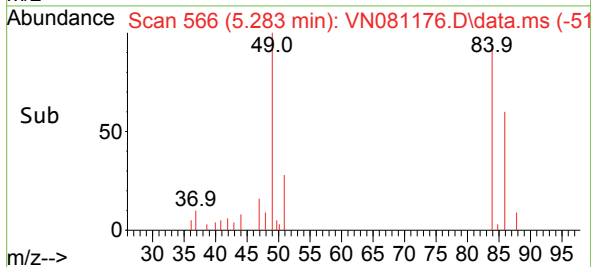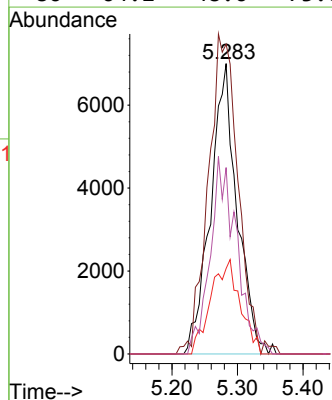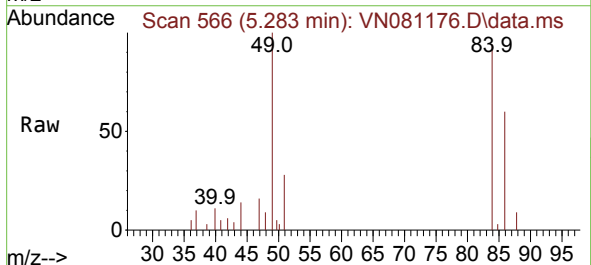

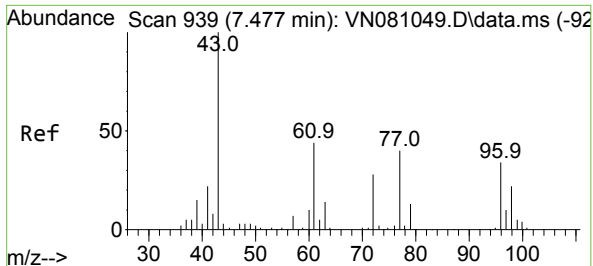

#25

2-Butanone

Concen: 2.790 ug/l

RT: 7.500 min Scan# 943

Delta R.T. 0.023 min

Lab File: VN081176.D

Acq: 23 Feb 2024 22:09

Instrument :

MSVOA_N

ClientSampleId :





SB-6

Tgt Ion: 43 Resp: 6068

Ion Ratio Lower Upper

43 100

72 17.8 19.5 29.3#

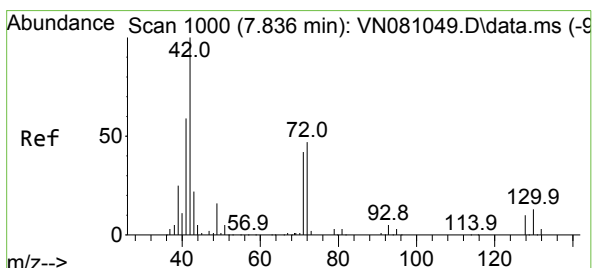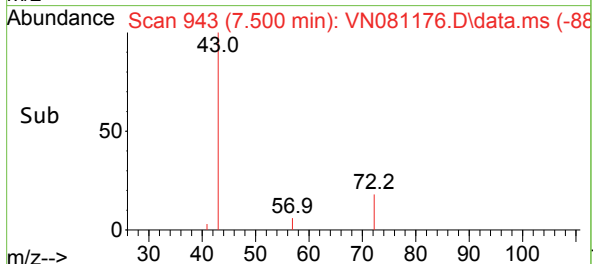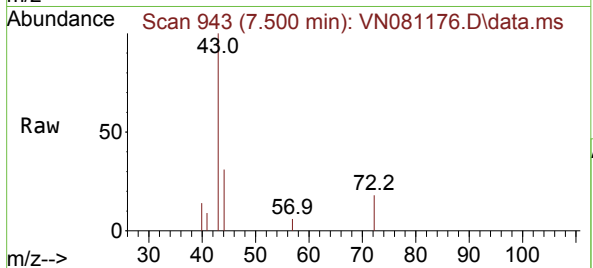

#29

Tetrahydrofuran

Concen: 3.834 ug/l

RT: 7.847 min Scan# 1002

Delta R.T. 0.012 min

Lab File: VN081176.D

Acq: 23 Feb 2024 22:09




Tgt Ion: 42 Resp: 5567


Ion Ratio Lower Upper

42 100

72 38.9 31.1 46.7

71 40.7 28.3 42.5

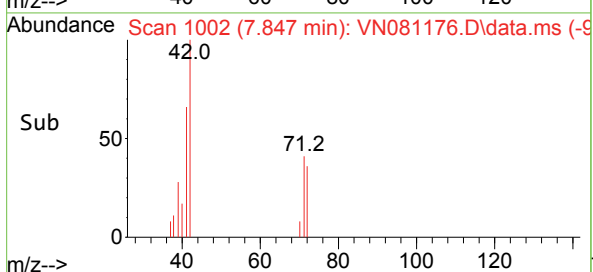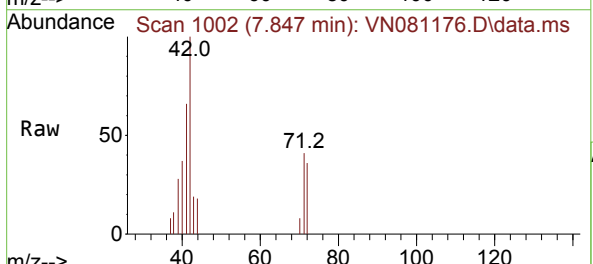



#31

Cyclohexane

Concen: 1.304 ug/l

RT: 8.230 min Scan# 1106

Delta R.T. -0.029 min

Lab File: VN081176.D

Acq: 23 Feb 2024 22:09

Instrument :

MSVOA_N

ClientSampleId :

SB-6





Tgt Ion: 56 Resp: 7706

Ion Ratio Lower Upper

56 100

69 148.4 20.1 30.1#

84 116.1 56.9 85.3#

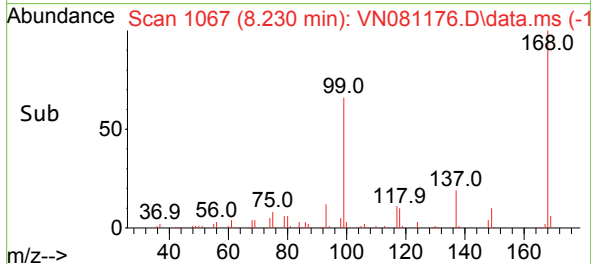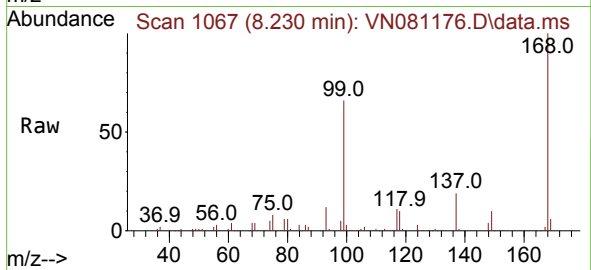

#33

1,2-Dichloroethane-d4

Concen: 51.188 ug/l

RT: 8.583 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VN081176.D




Acq: 23 Feb 2024 22:09


Tgt Ion: 65 Resp: 175140

Ion Ratio Lower Upper

65 100

67 53.0 0.0 102.4

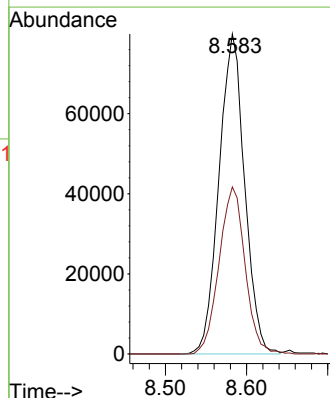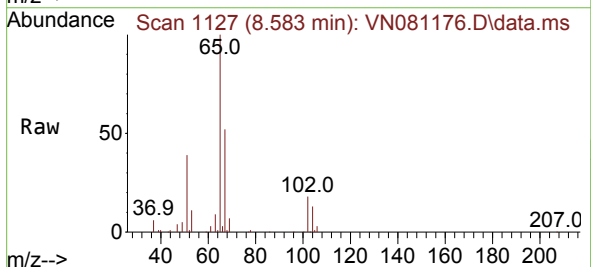



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN081176.D

Acq: 23 Feb 2024 22:09

Instrument :

MSVOA_N

ClientSampleId :

SB-6





Tgt Ion:114 Resp: 546519

Ion Ratio Lower Upper

114 100

63 19.7 0.0 48.0

88 14.4 0.0 34.8

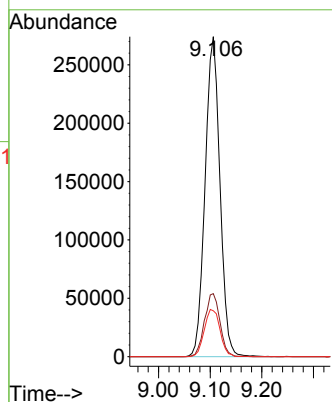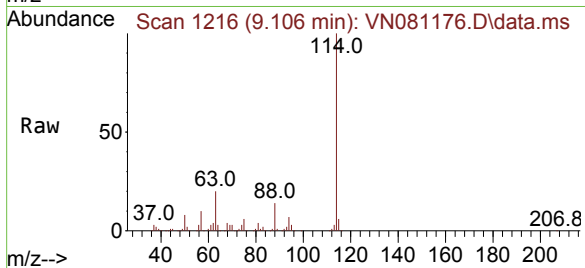

#35

Dibromofluoromethane

Concen: 48.327 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VN081176.D

Acq: 23 Feb 2024 22:09




Tgt Ion:113 Resp: 149351


Ion Ratio Lower Upper

113 100

111 103.0 82.2 123.4

192 16.2 12.5 18.7


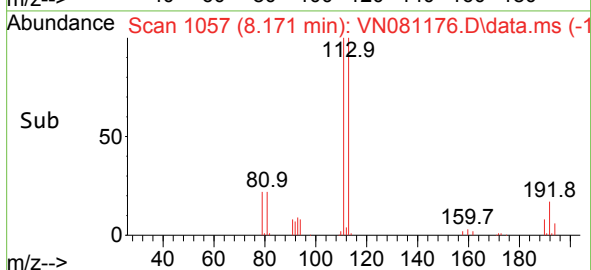
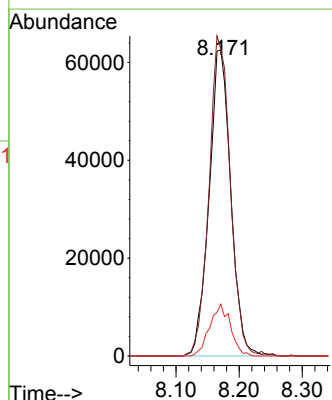
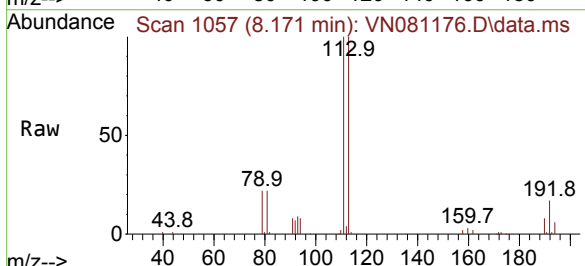




#36
1,1-Dichloropropene
Concen: 4.736 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.147 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09




Instrument :
MSVOA_N
ClientSampleId :
SB-6


Tgt Ion: 75 Resp: 25077
Ion Ratio Lower Upper
75 100
110 9.3 16.0 48.0#
77 0.0 25.8 38.6#

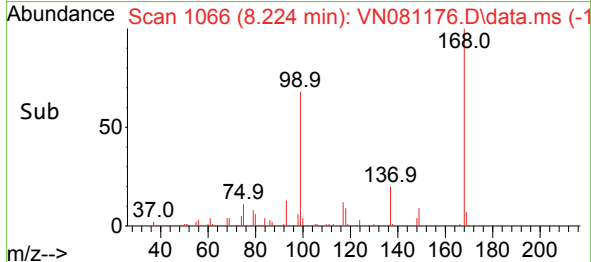

#37
Ethyl Acetate
Concen: 1.842 ug/l
RT: 7.559 min Scan# 953
Delta R.T. -0.000 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09

Tgt Ion: 43 Resp: 8803
Ion Ratio Lower Upper
43 100
61 14.9 10.6 15.8
70 11.5 8.0 12.0

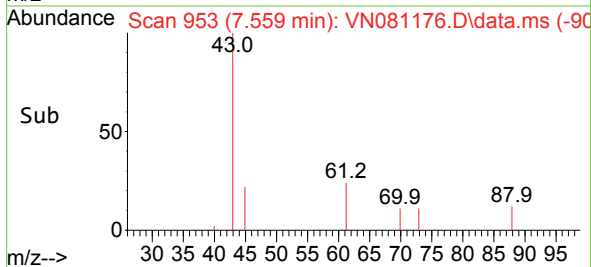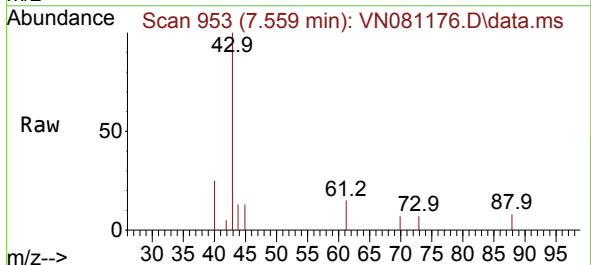



#38

Carbon Tetrachloride

Concen: 5.812 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.135 min

Lab File: VN081176.D

Acq: 23 Feb 2024 22:09

Instrument :

MSVOA_N

ClientSampleId :

SB-6





Tgt Ion:117 Resp: 31133

Ion Ratio Lower Upper

117 100

119 4.6 73.4 110.2#

121 0.0 24.4 36.6#

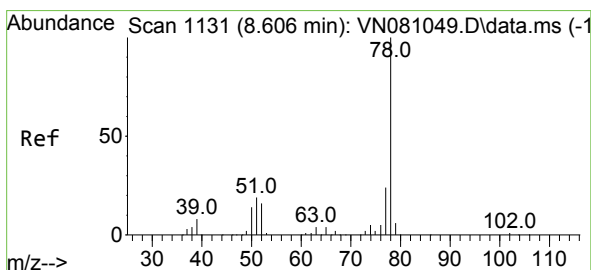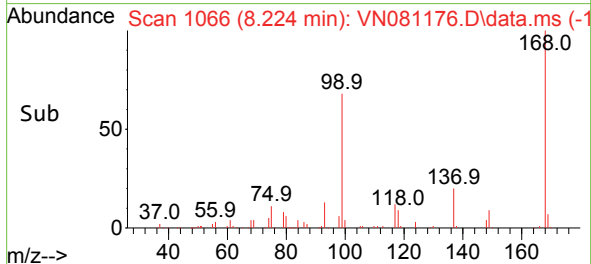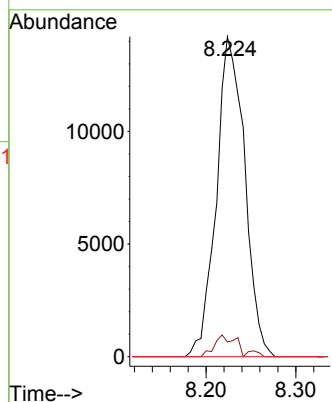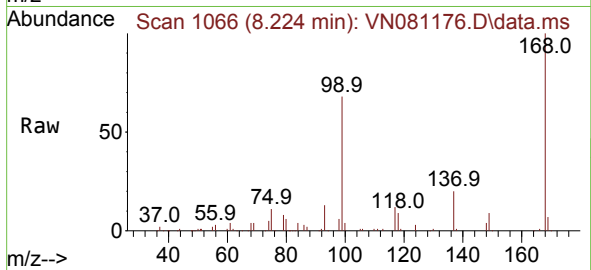

#40

Benzene

Concen: 0.344 ug/l

RT: 8.612 min Scan# 1132

Delta R.T. 0.006 min

Lab File: VN081176.D




Acq: 23 Feb 2024 22:09


Tgt Ion: 78 Resp: 5279

Ion Ratio Lower Upper

78 100

77 18.4 20.4 30.6#



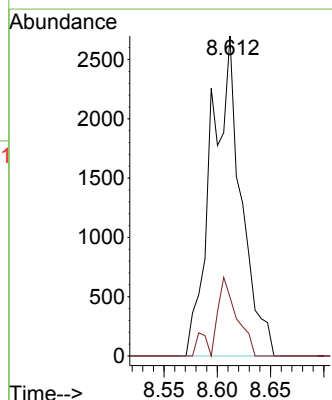
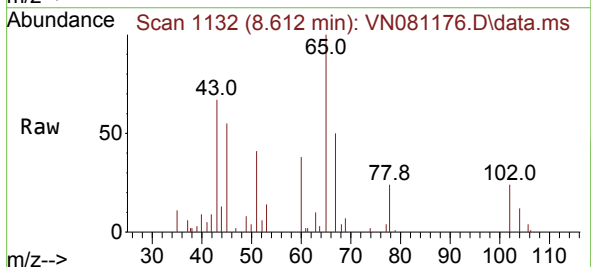




#41
Methacrylonitrile
Concen: 1.063 ug/l
RT: 7.847 min Scan# 1002
Delta R.T. 0.071 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09




Instrument :
MSVOA_N
ClientSampleId :
SB-6


Tgt Ion: 41	Resp: 2891
Ion Ratio	Lower Upper
41	100
39	65.1 48.4 72.6
67	0.0 56.8 85.2#
52	0.0 25.0 37.4#

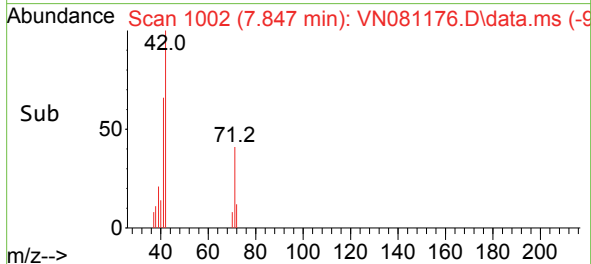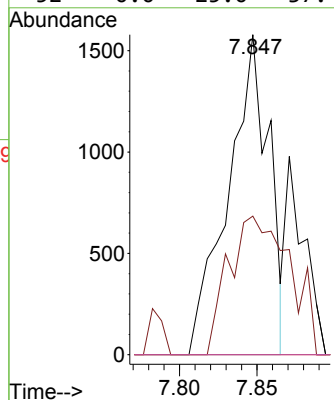

#42
1,2-Dichloroethane
Concen: 0.431 ug/l
RT: 8.682 min Scan# 1144
Delta R.T. 0.012 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09

Tgt Ion: 62	Resp: 2303
Ion Ratio	Lower Upper
62	100
98	0.0 0.0 18.0


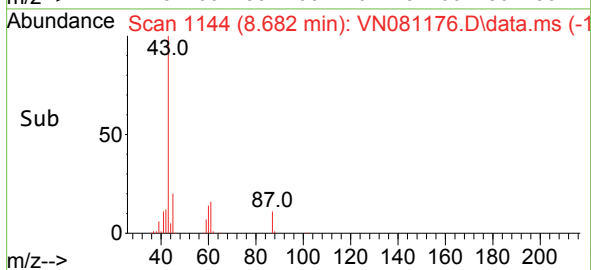
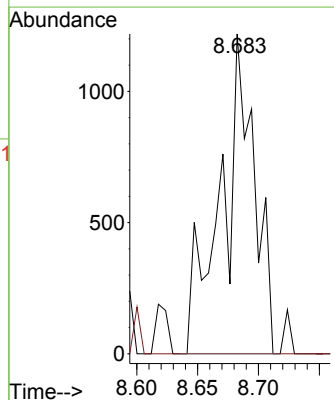
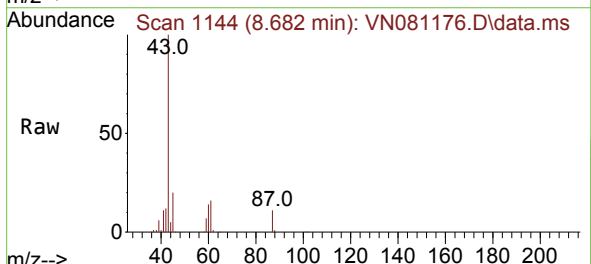


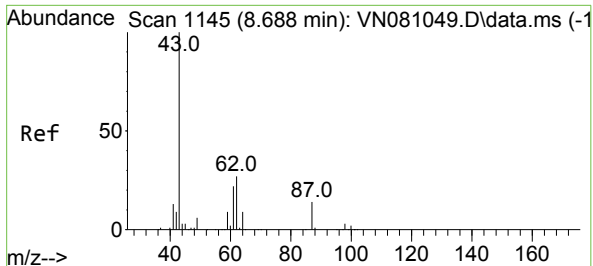

#43
Isopropyl Acetate
Concen: 68.522 ug/l
RT: 8.688 min Scan# 1145
Delta R.T. -0.000 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09




Instrument :
MSVOA_N
ClientSampleId :
SB-6


Tgt Ion: 43 Resp: 572637
Ion Ratio Lower Upper
43 100
61 10.4 19.9 29.9#
87 7.0 9.0 13.6#

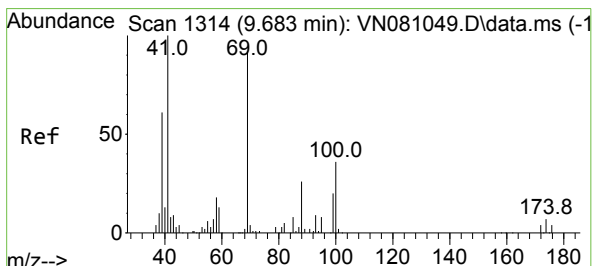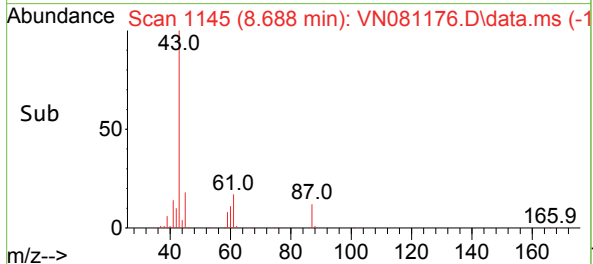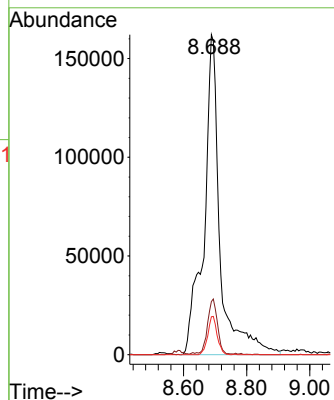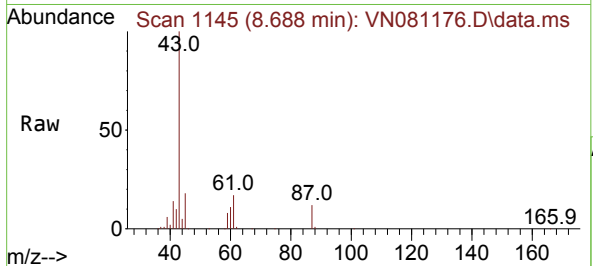

#48
Methyl methacrylate
Concen: 2.205 ug/l
RT: 9.665 min Scan# 1311
Delta R.T. -0.018 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09

Tgt Ion: 41 Resp: 8573
Ion Ratio Lower Upper
41 100
69 2.7 62.2 93.2#
39 58.7 47.6 71.4

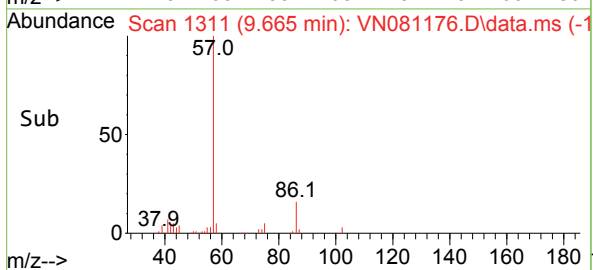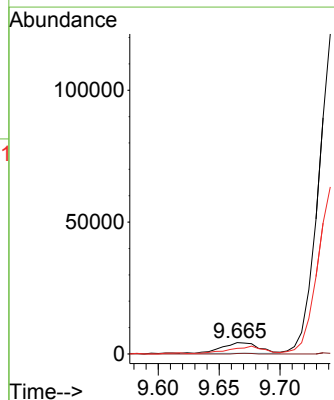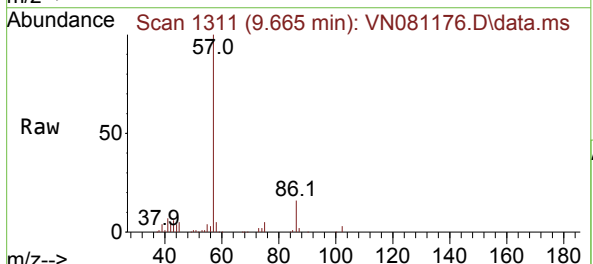



#49

1,4-Dioxane

Concen: Below Cal

RT: 9.694 min Scan# 11

Delta R.T. 0.000 min

Lab File: VN081176.D

Acq: 23 Feb 2024 22:09

Instrument :

MSVOA_N

ClientSampleId :

SB-6





Tgt Ion: 88 Resp: 101

Ion Ratio Lower Upper

88 100

43 0.0 30.1 45.1#

58 7611.9 63.9 95.9#

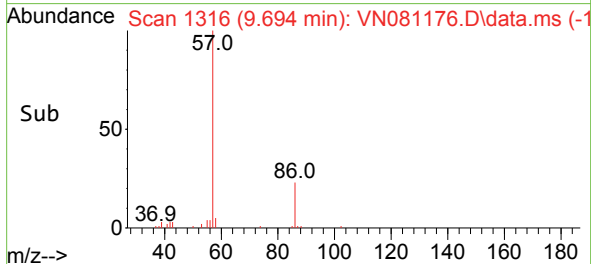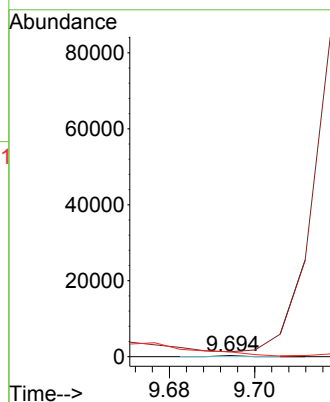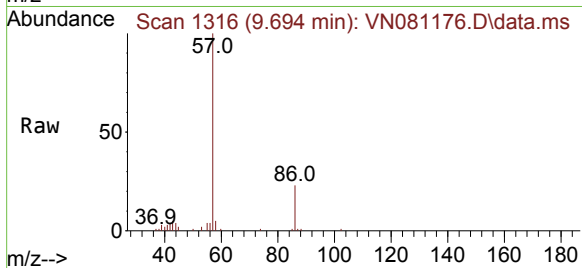

#50

Toluene-d8

Concen: 44.358 ug/l

RT: 10.571 min Scan# 1465

Delta R.T. 0.006 min

Lab File: VN081176.D




Acq: 23 Feb 2024 22:09


Tgt Ion: 98 Resp: 486881

Ion Ratio Lower Upper

98 100

100 66.1 51.4 77.0

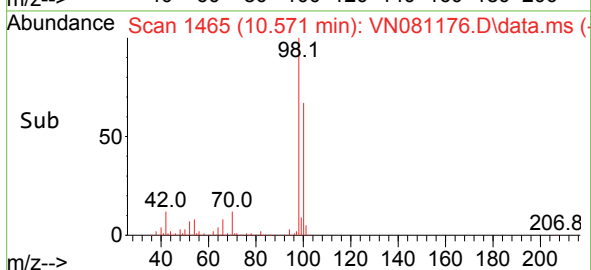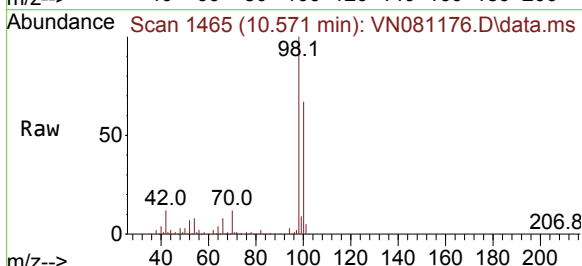



#51

4-Methyl-2-Pentanone

Concen: 4.959 ug/l

RT: 10.447 min Scan# 1444

Delta R.T. -0.000 min

Lab File: VN081176.D

Acq: 23 Feb 2024 22:09

Instrument :

MSVOA_N

ClientSampleId :





SB-6

Tgt Ion: 43 Resp: 23842

Ion Ratio Lower Upper

43 100

58 23.0 29.4 44.0#

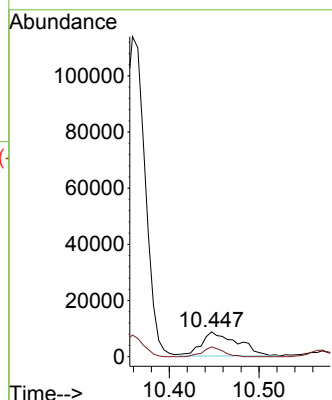

#52

Toluene

Concen: 0.316 ug/l

RT: 10.635 min Scan# 1476

Delta R.T. 0.006 min

Lab File: VN081176.D




Acq: 23 Feb 2024 22:09


Tgt Ion: 92 Resp: 3061

Ion Ratio Lower Upper

92 100

91 207.8 139.4 209.0


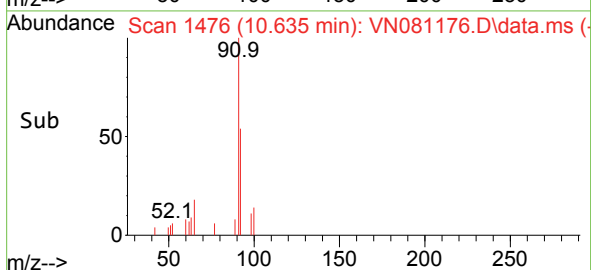
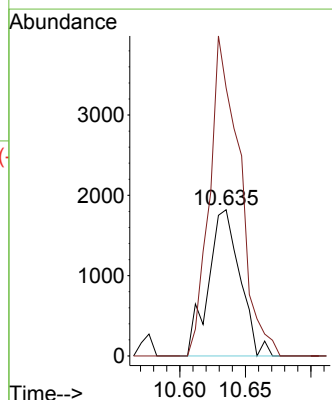



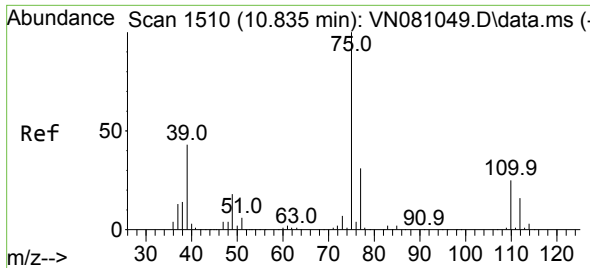

#53
 t-1,3-Dichloropropene
 Concen: 0.349 ug/l
 RT: 10.724 min Scan# 1491
 Delta R.T. -0.112 min
 Lab File: VN081176.D
 Acq: 23 Feb 2024 22:09




Instrument :
 MSVOA_N
 ClientSampleId :
 SB-6


Tgt Ion: 75 Resp: 2053
 Ion Ratio Lower Upper
 75 100
 77 22.1 25.5 38.3#

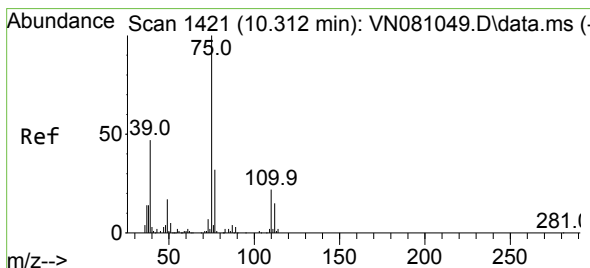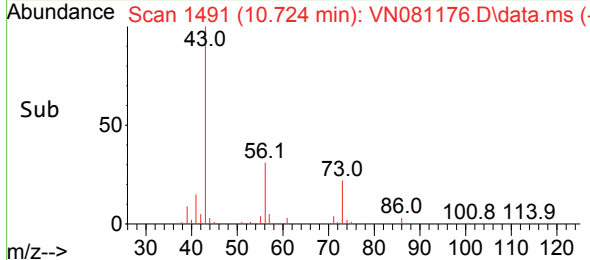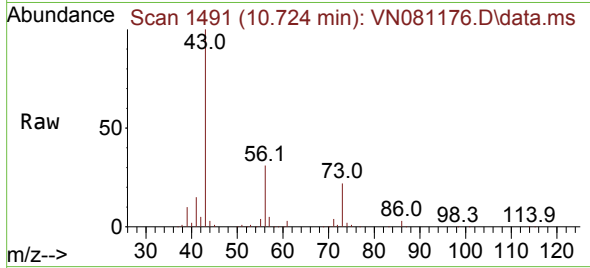

#54
 cis-1,3-Dichloropropene
 Concen: 15.741 ug/l
 RT: 10.359 min Scan# 1429
 Delta R.T. 0.047 min
 Lab File: VN081176.D
 Acq: 23 Feb 2024 22:09

Tgt Ion: 75 Resp: 99978
 Ion Ratio Lower Upper
 75 100
 77 0.5 23.3 34.9#
 39 32.6 44.6 66.8#


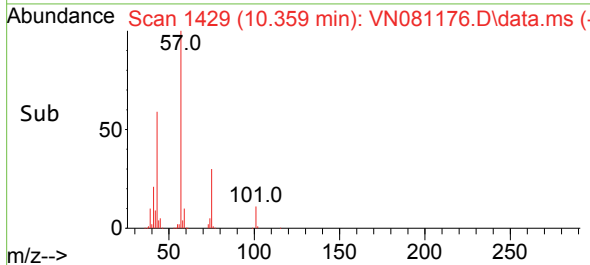

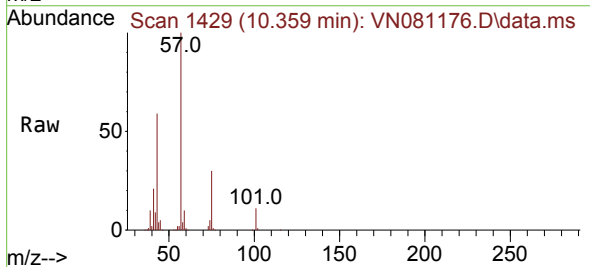


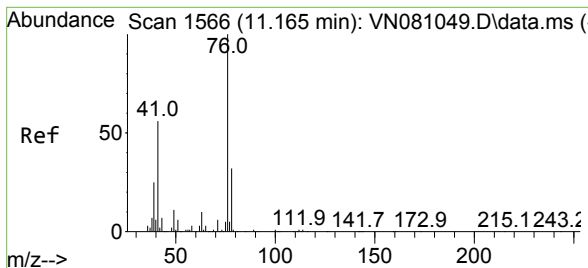

#57
1,3-Dichloropropane
Concen: 1.911 ug/l
RT: 11.200 min Scan# 11
Delta R.T. 0.035 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09




Instrument :
MSVOA_N
ClientSampleId :
SB-6


Tgt Ion: 76 Resp: 12327
Ion Ratio Lower Upper
76 100
78 0.0 25.5 38.3#

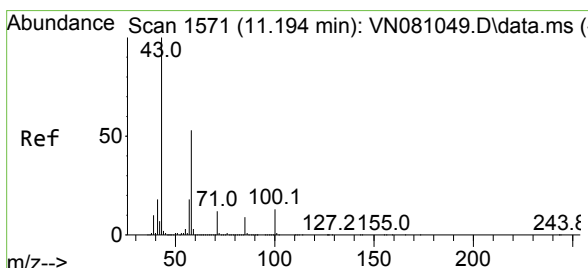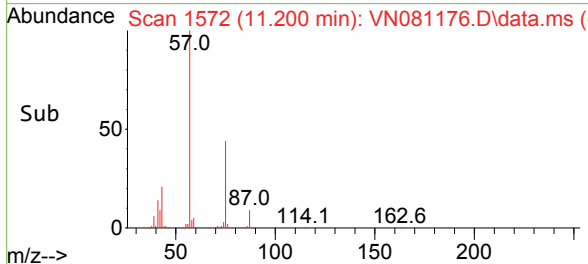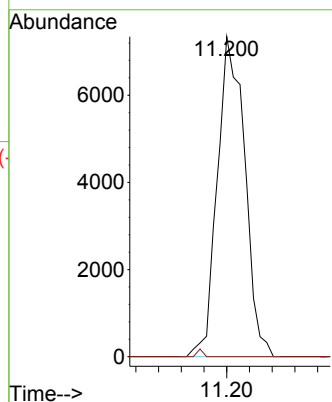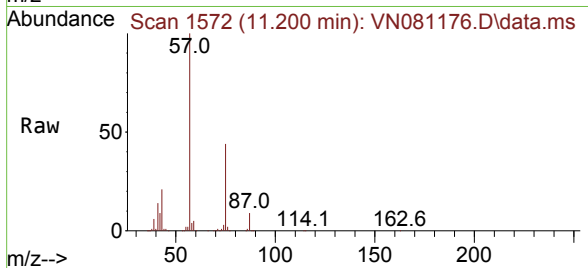

#59
2-Hexanone
Concen: 54.981 ug/l
RT: 11.171 min Scan# 1567
Delta R.T. -0.024 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09

Tgt Ion: 43 Resp: 209550
Ion Ratio Lower Upper
43 100
58 0.0 25.9 77.8#


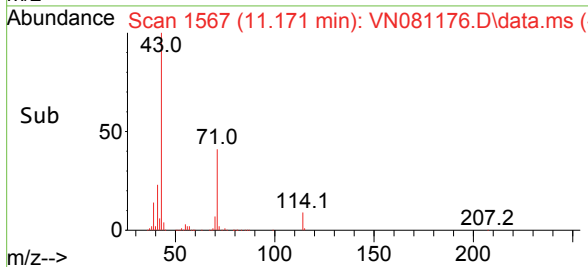
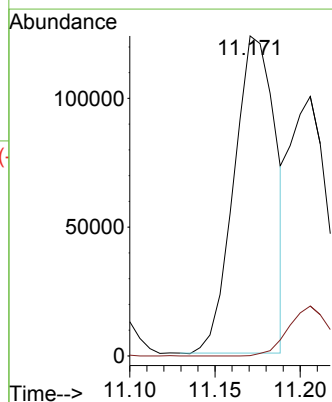
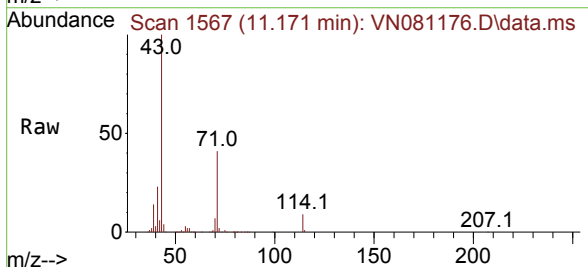


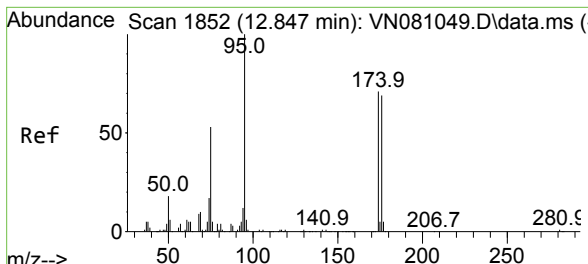

#62
4-Bromofluorobenzene
Concen: 43.052 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09




Instrument :
MSVOA_N
ClientSampleId :
SB-6


Tgt Ion:	95	Resp:	177564
Ion	Ratio	Lower	Upper
95	100		
174	71.1	0.0	120.4
176	67.2	0.0	121.0

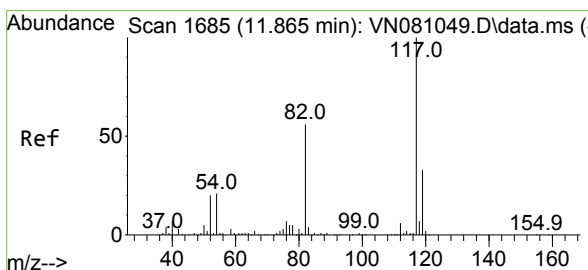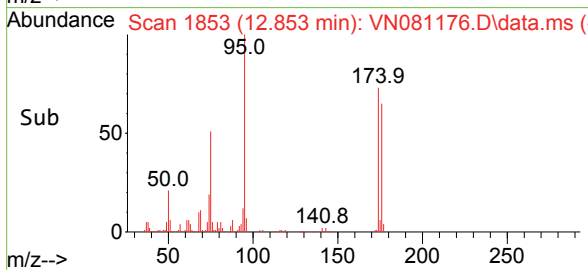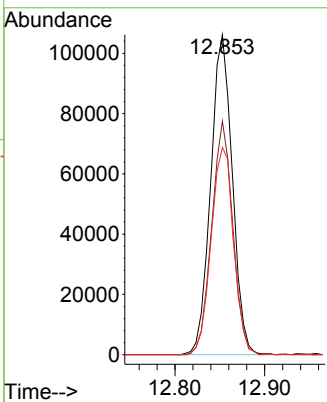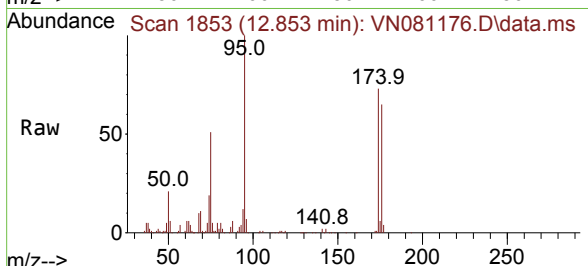

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. 0.006 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09

Tgt Ion:	117	Resp:	496145
Ion	Ratio	Lower	Upper
117	100		
82	55.3	52.7	79.1
119	33.8	25.3	37.9

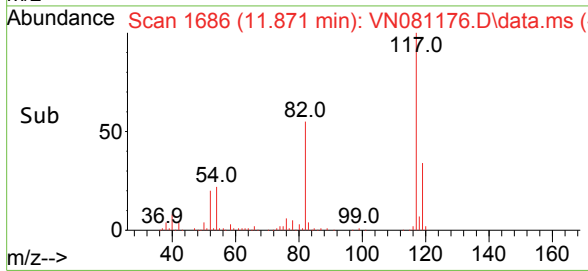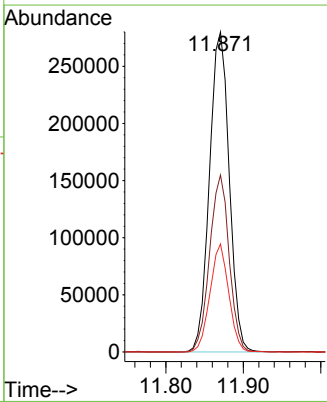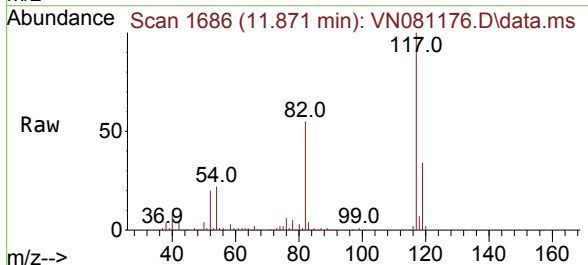



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. -0.000 min

Lab File: VN081176.D

Acq: 23 Feb 2024 22:09

Instrument :

MSVOA_N

ClientSampleId :

SB-6





Tgt Ion:152 Resp: 195836

Ion Ratio Lower Upper

152 100

115 64.3 32.3 96.8

150 155.4 0.0 339.8

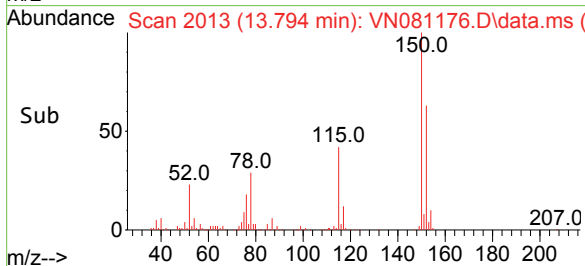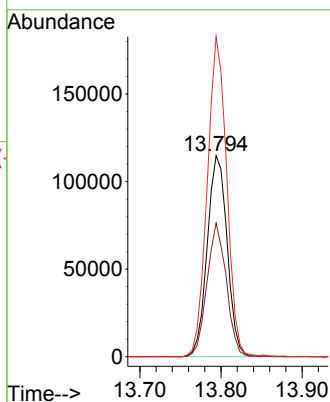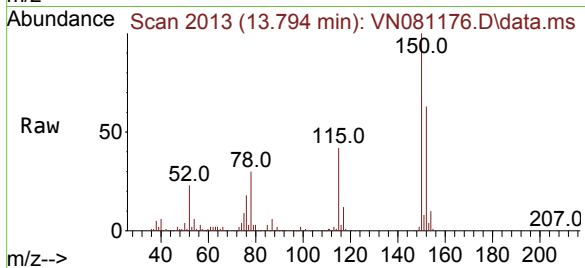

#74

N-ethyl acetate

Concen: 0.336 ug/l

RT: 12.494 min Scan# 1792

Delta R.T. -0.000 min

Lab File: VN081176.D

Acq: 23 Feb 2024 22:09

Tgt Ion: 43 Resp: 2435




Ion Ratio Lower Upper


43 100

70 0.0 30.1 45.1#

55 7.0 17.0 25.4#

61 0.0 17.5 26.3#


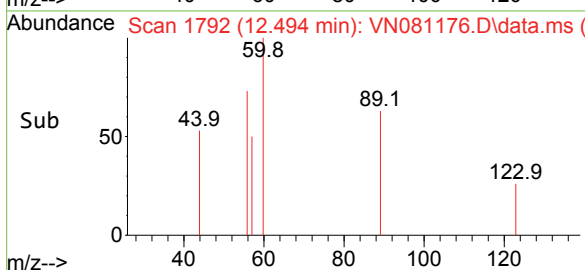

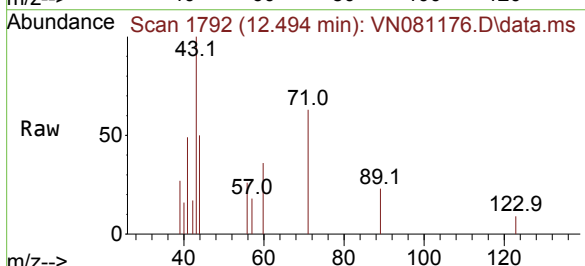




#76
1,2,3-Trichloropropane
Concen: 21.636 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.141 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09

Instrument :
MSVOA_N
ClientSampleId :
SB-6

Tgt Ion: 75 Resp: 96272
Ion Ratio Lower Upper
75 100
77 1.3 91.0 272.8#

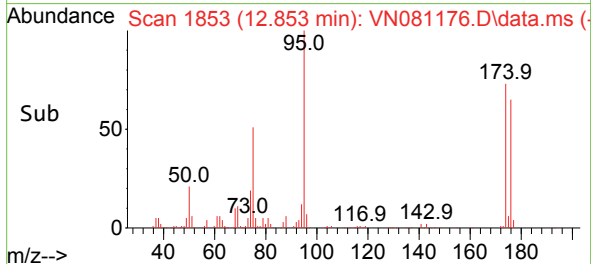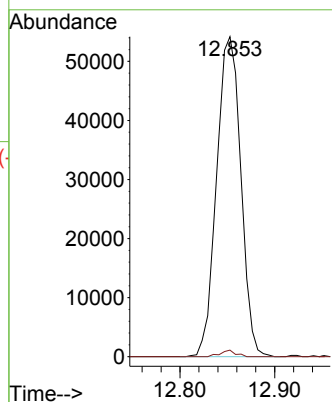

#81
trans-1,4-Dichloro-2-butene
Concen: 55.691 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.112 min
Lab File: VN081176.D
Acq: 23 Feb 2024 22:09

Tgt Ion: 75 Resp: 96272
Ion Ratio Lower Upper
75 100
53 0.0 71.4 107.2#
89 0.0 33.4 50.0#

