

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022421\
 Data File : VN065998.D
 Acq On : 24 Feb 2021 12:55
 Operator : JC/MD
 Sample : M1473-06
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FB-04-022321

Quant Time: Feb 25 02:12:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 17 15:48:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.631	168	135306	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.550	114	225367	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	203921	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.315	152	84099	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.991	65	89280	47.18	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	94.36%
35) Dibromofluoromethane	7.553	113	68617	49.20	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	98.40%
50) Toluene-d8	10.058	98	271072	47.35	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	94.70%
62) 4-Bromofluorobenzene	12.373	95	98496	45.83	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	91.66%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022421\
Data File : VN065998.D
Acq On : 24 Feb 2021 12:55
Operator : JC/MD
Sample : M1473-06
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FB-04-022321

Quant Time: Feb 25 02:12:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 17 15:48:13 2021
Response via : Initial Calibration




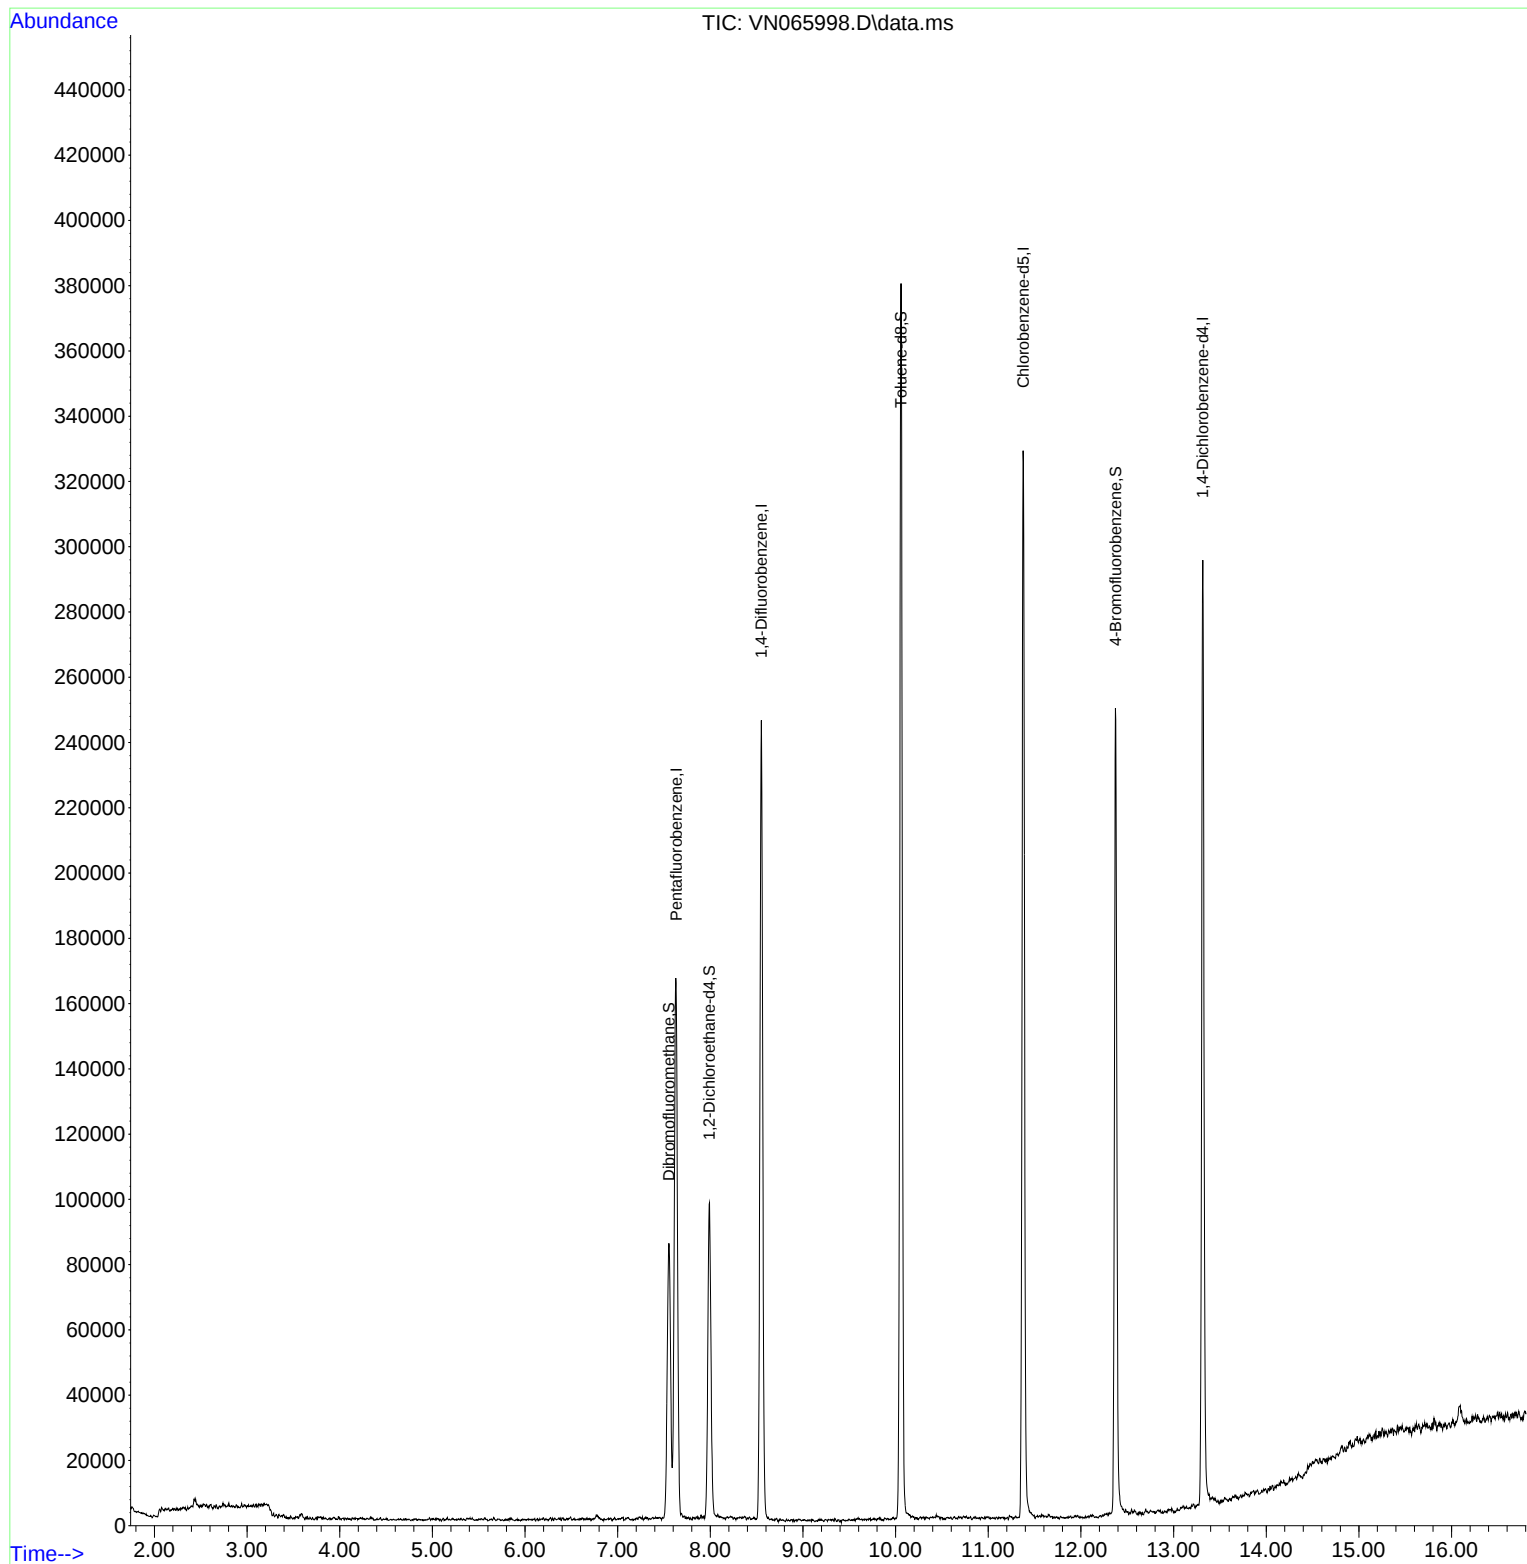


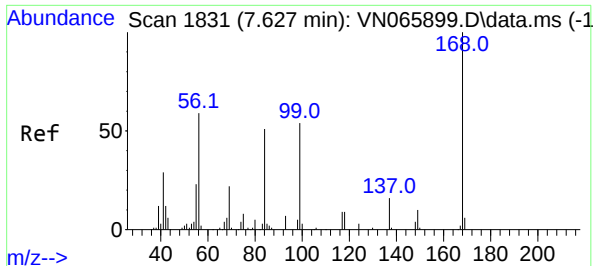

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.631 min Scan# 1832
Delta R.T. 0.004 min
Lab File: VN065998.D
Acq: 24 Feb 2021 12:55




Instrument :
MSVOA_N
ClientSampled :
FB-04-022321


Tgt Ion:168 Resp: 135306
Ion Ratio Lower Upper
168 100
99 60.0 42.6 63.8

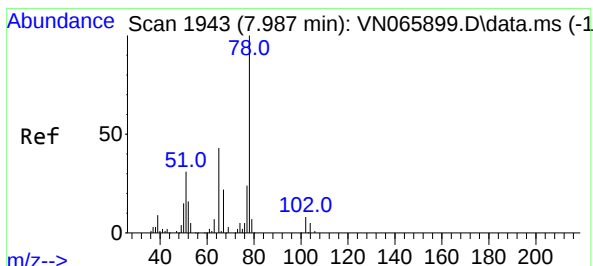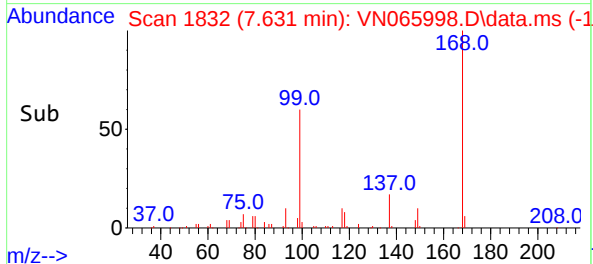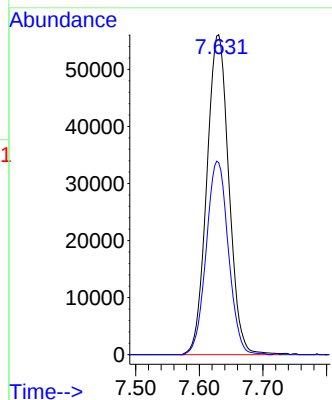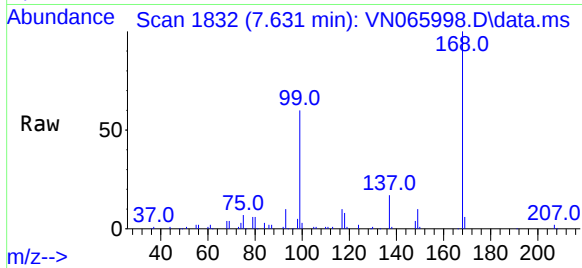

#33
1,2-Dichloroethane-d4
Concen: 47.18 ug/l
RT: 7.991 min Scan# 1944
Delta R.T. 0.004 min
Lab File: VN065998.D
Acq: 24 Feb 2021 12:55

Tgt Ion: 65 Resp: 89280
Ion Ratio Lower Upper
65 100
67 51.2 0.0 107.2

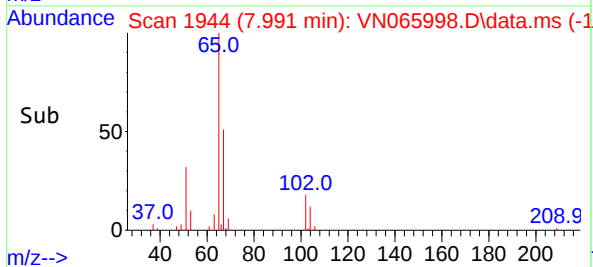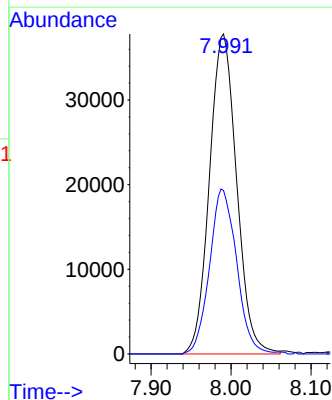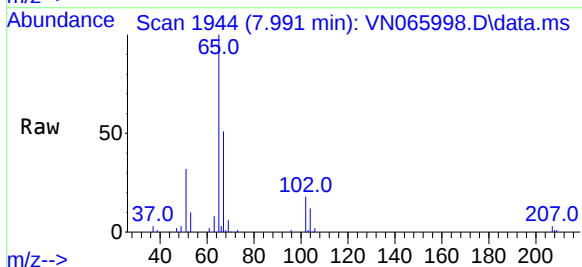




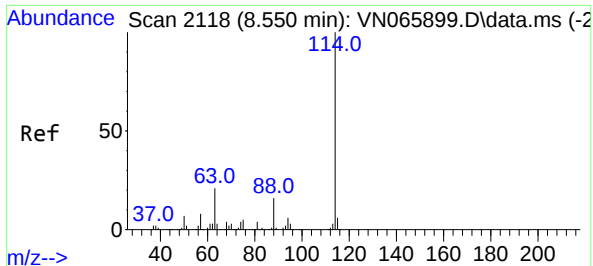


#34

1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.550 min Scan# 2118
Delta R.T. 0.000 min
Lab File: VN065998.D
Acq: 24 Feb 2021 12:55

Instrument :
MSVOA_N
ClientSampled :
FB-04-022321




Tgt Ion:	114	Resp:	225367
Ion	Ratio	Lower	Upper
114	100		
63	20.3	0.0	38.6
88	17.1	0.0	30.6

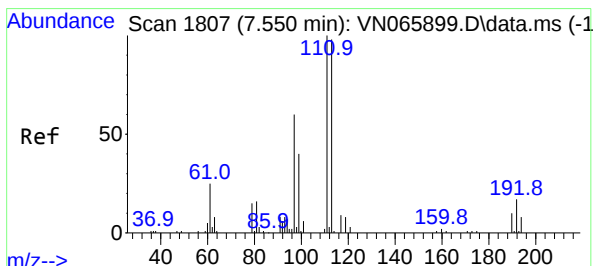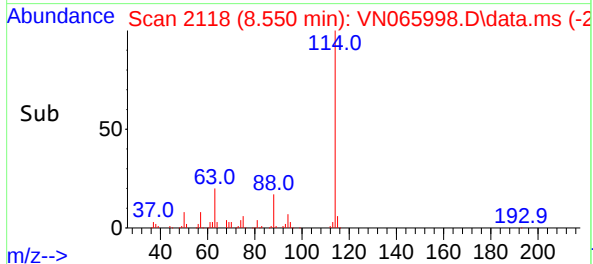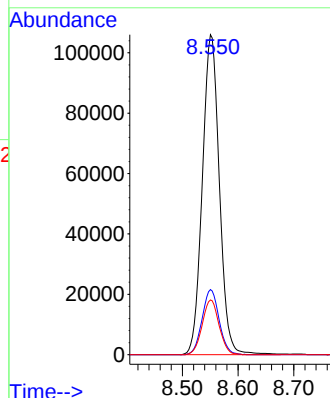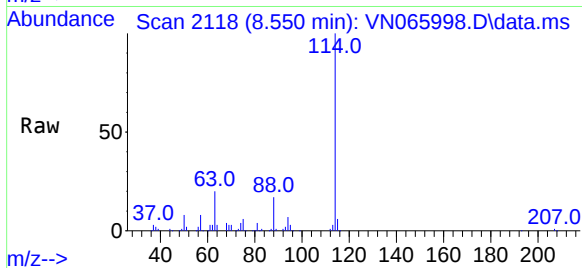


#35

Dibromofluoromethane
Concen: 49.20 ug/l
RT: 7.553 min Scan# 1808
Delta R.T. 0.003 min
Lab File: VN065998.D
Acq: 24 Feb 2021 12:55

Tgt Ion:	113	Resp:	68617
Ion	Ratio	Lower	Upper
113	100		
111	101.4	82.2	123.2
192	18.2	15.4	23.0


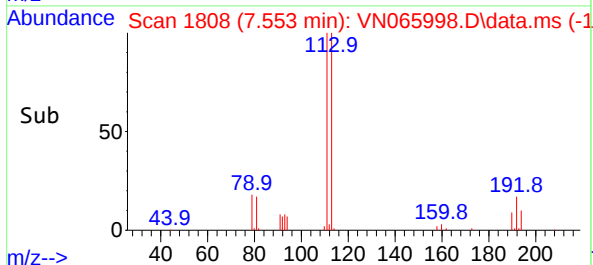
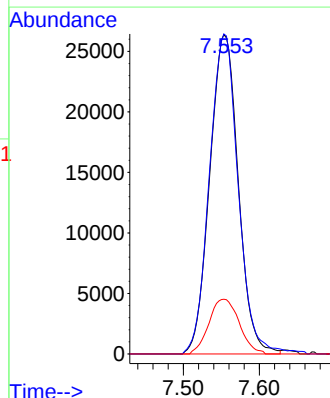
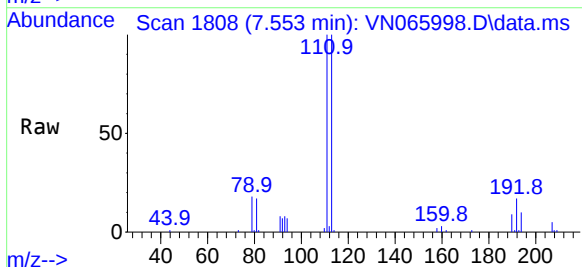


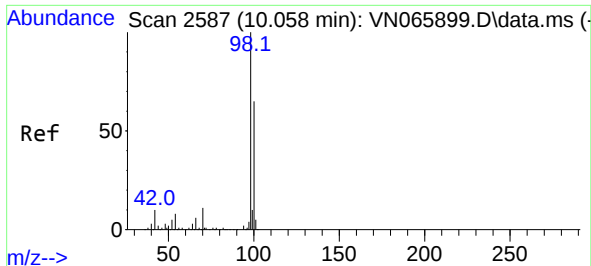

#50
Toluene-d8
Concen: 47.35 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. 0.000 min
Lab File: VN065998.D
Acq: 24 Feb 2021 12:55




Instrument :
MSVOA_N
ClientSampleId :
FB-04-022321


Tgt Ion: 98 Resp: 271072
Ion Ratio Lower Upper
98 100
100 66.2 50.5 75.7

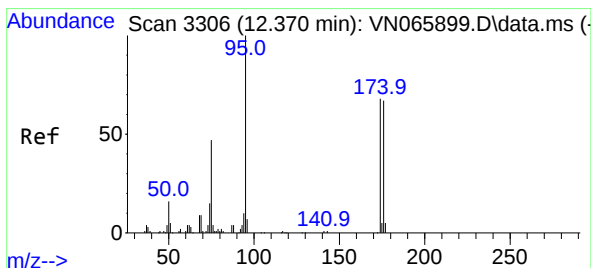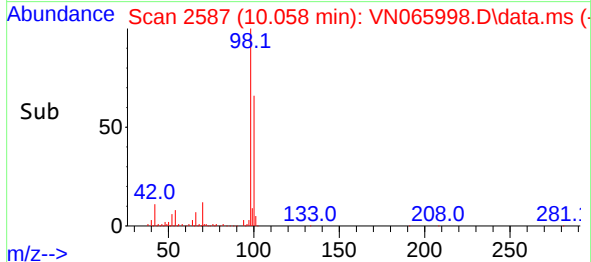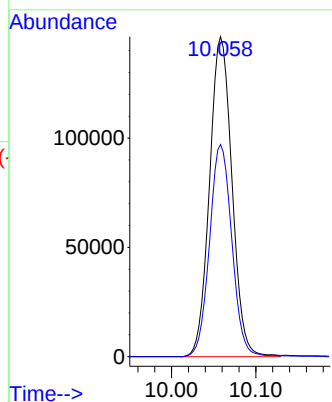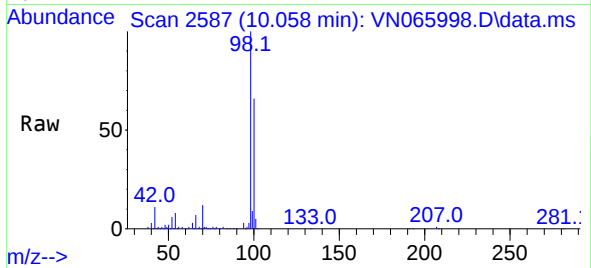

#62
4-Bromofluorobenzene
Concen: 45.83 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.003 min
Lab File: VN065998.D
Acq: 24 Feb 2021 12:55

Tgt Ion: 95 Resp: 98496
Ion Ratio Lower Upper
95 100
174 71.8 0.0 169.0
176 68.2 0.0 162.4


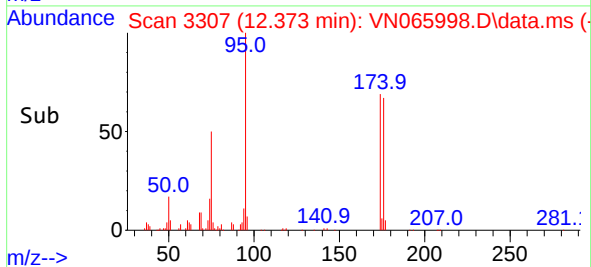
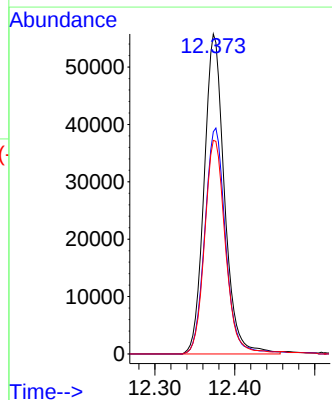
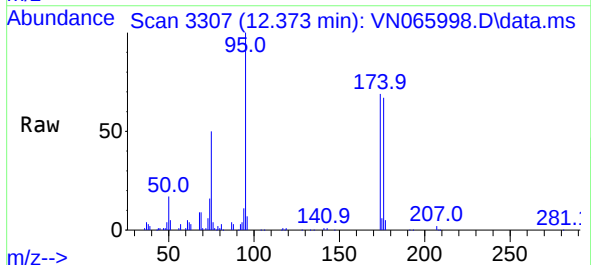


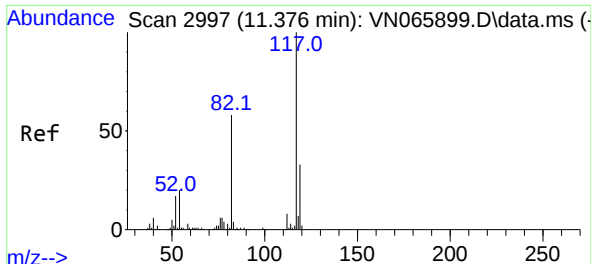

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN065998.D
Acq: 24 Feb 2021 12:55

Instrument :
MSVOA_N
ClientSampleId :
FB-04-022321

Tgt Ion:117 Resp: 203921
Ion Ratio Lower Upper
117 100
82 56.5 43.7 65.5
119 31.0 26.1 39.1

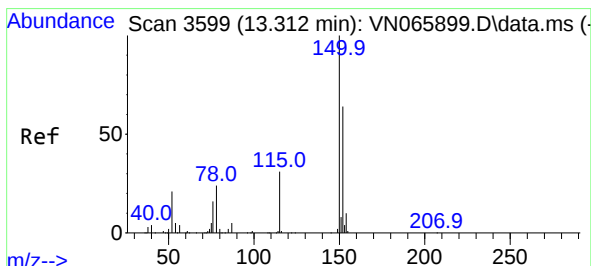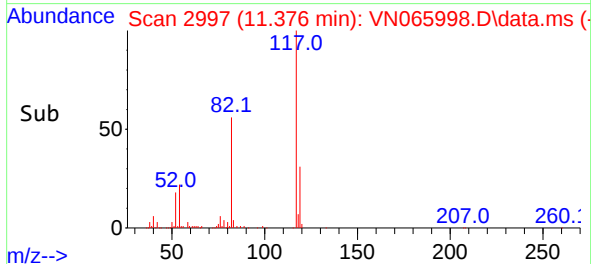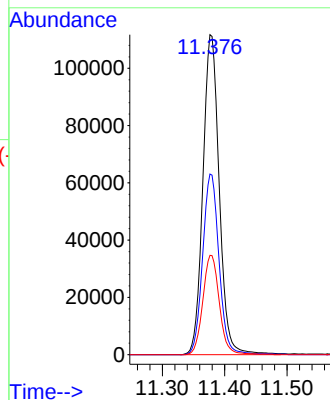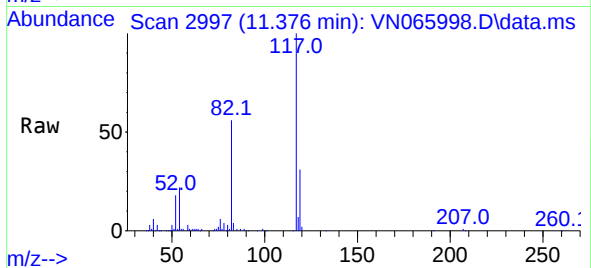

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.315 min Scan# 3600
Delta R.T. 0.003 min
Lab File: VN065998.D
Acq: 24 Feb 2021 12:55

Tgt Ion:152 Resp: 84099
Ion Ratio Lower Upper
152 100
115 62.0 28.5 85.6
150 160.2 0.0 347.6

